



Designation: D3697 – 07

Standard Test Method for Antimony in Water¹

This standard is issued under the fixed designation D3697; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method covers the determination of dissolved and total recoverable antimony in water by atomic absorption spectroscopy.²

1.2 This test method is applicable in the range from 1 to 15 $\mu\text{g/L}$ of antimony. The range may be extended by less scale expansion or by dilution of the sample.

1.3 The precision and bias data were obtained on reagent water, tap water, salt water, and two untreated wastewaters. The information on precision and bias may not apply to other waters.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*³

D1129 Terminology Relating to Water

D1193 Specification for Reagent Water

D2777 Practice for Determination of Precision and Bias of Applicable Test Methods of Committee D19 on Water

D3370 Practices for Sampling Water from Closed Conduits

D4691 Practice for Measuring Elements in Water by Flame Atomic Absorption Spectrophotometry

D4841 Practice for Estimation of Holding Time for Water Samples Containing Organic and Inorganic Constituents

D5847 Practice for Writing Quality Control Specifications for Standard Test Methods for Water Analysis

¹ This test method is under the jurisdiction of ASTM Committee D19 on Water and is the direct responsibility of Subcommittee D19.05 on Inorganic Constituents in Water.

Current edition approved Aug. 1, 2007. Published August 2007. Originally approved in 1978. Last previous edition approved in 2002 as D3697 – 02. DOI: 10.1520/D3697-07.

² Platte, J. A., and Marcy, V. M., "A New Tool for the Water Chemist," *Industrial Water Engineering*, IWEGA, May 1965.

³ For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

3. Terminology

3.1 *Definitions:* For definitions of terms used in this test method, refer to Terminology D1129.

3.2 *Definitions of Terms Specific to This Standard:*

3.2.1 *total recoverable antimony*—an arbitrary analytical term relating to forms of antimony that are determinable by the digestion method which is included in the procedure. Some organic compounds may not be completely recovered.

3.2.2 *laboratory control sample, n*—a solution with a certified concentration of the antimony.

4. Summary of Test Method

4.1 Organic antimony-containing compounds are decomposed by adding sulfuric and nitric acids and repeatedly evaporating the sample to fumes of sulfur trioxide. The antimony so produced, together with inorganic antimony originally present, is subsequently reacted with potassium iodide and stannous chloride, and finally with sodium borohydride to form stibine. The stibine is removed from solution by aeration and swept by a flow of nitrogen into a hydrogen flame where it is determined by atomic absorption at 217.6 nm.

5. Significance and Use

5.1 Because of the association with lead and arsenic in industry, it is often difficult to assess the toxicity of antimony and its compounds. In humans, complaints referable to the nervous system have been reported. In assessing human cases, however, the possibility of lead or arsenic poisoning must always be borne in mind. Locally, antimony compounds are irritating to the skin and mucous membranes.

6. Interference

6.1 Since the stibine is freed from the original sample matrix, interferences in the flame are minimized.

6.2 Selenium and arsenic, which also form hydrides, do not interfere at concentrations of 100 $\mu\text{g/L}$. Higher concentrations were not tested.

7. Apparatus

7.1 *Atomic Absorption Spectrophotometer*, for use at 217.6 nm with a scale expansion of approximately 3. A general guide for the use of flame atomic absorption applications is given in Practice D4691.

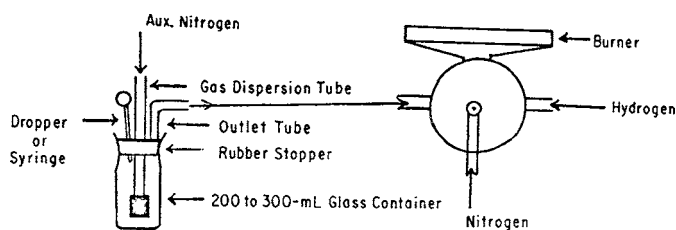


FIG. 1 Stibine Vapor Analyzer

NOTE 1—The manufacturer's instructions should be followed for all instrumental parameters.

7.1.1 Antimony Electrodeless Discharge Lamp.

7.2 Recorder or Digital Readout — Any multirange variable speed recorder or digital readout accessory, or both, that is compatible with the atomic absorption spectrophotometer is suitable.

7.3 Stibine Vapor Analyzer, assembled as shown in Fig. 1.

NOTE 2—A static system, such as one using a balloon, has been found to be satisfactory. See McFarren, E. F., "New, Simplified Method for Metal Analysis," *Journal of American Water Works Assoc.*, JAWWA, Vol 64, 1972, p. 28.

8. Reagents and Materials

8.1 Purity of Reagents— Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents shall conform to the specifications for the Committee on Analytical Reagents of the American Chemical Society, where such specifications are available.⁴ Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination.

8.2 Purity of Water— Unless otherwise indicated, references to water shall be understood to mean reagent water conforming to Specification D1193, Type I, II, or III water. Type I is preferred and more commonly used. Other reagent water types may be used provided it is first ascertained that the water is of sufficiently high purity to permit its use without adversely affecting the precision and bias of the test method. Type II water was specified at the time of round robin testing of these test methods.

NOTE 3—The user must ensure the type of reagent water chosen is sufficiently free of interferences. The water should be analyzed using the test method.

8.3 Antimony Solution, Stock (1.00 mL = 100 µg Sb)— Dissolve 274.3 mg of antimony potassium tartrate, $\text{KSbOC}_4\text{H}_4\text{O}_6 \cdot 1/2\text{H}_2\text{O}$, in water and dilute to 1000 mL with water. A purchased stock solution of adequate purity is also acceptable.

⁴ Reagent Chemicals, American Chemical Society Specifications, American Chemical Society, Washington, DC. For Suggestions on the testing of reagents not listed by the American Chemical Society, see *Annual Standards for Laboratory Chemicals*, BDH Ltd., Poole, Dorset, U.K., and the *United States Pharmacopeia and National Formulary*, U.S. Pharmacopeial Convention, Inc. (USPC), Rockville, MD.

8.4 Antimony Solution, Intermediate (1.00 mL = 10 µg Sb)—Dilute 50.0 mL of antimony stock solution to 500.0 mL with water.

8.5 Antimony Solution, Standard (1.0 mL = 0.10 µg Sb)— Dilute 5.0 mL of antimony intermediate solution to 500.0 mL with water. Prepare fresh before each use. This standard is used to prepare working standards at the time of analysis.

8.6 Hydrochloric Acid (sp gr 1.19)—Concentrated hydrochloric acid (HCl).

8.7 Nitric Acid (sp gr 1.42)—Concentrated nitric acid (HNO_3).

8.8 Nitric Acid (1 + 1)—Add 250 mL of concentrated nitric acid (sp gr 1.42) to 250 mL of water.

8.9 Potassium Iodide Solution (15 g/100 mL)—Dissolve 15 g of potassium iodide (KI) in 100 mL of water. This solution is stable when stored in an amber bottle or in the dark.

8.10 Sodium Borohydride Solution (4 g/100 mL)—Dissolve 4 g of sodium borohydride (NaBH_4) and 2 g of sodium hydroxide (NaOH) in 100 mL water. Prepare weekly.

8.11 Stannous Chloride Solution (4.6 g/100 mL of concentrated HCl)—Dissolve 5 g of stannous chloride ($\text{SnCl}_2 \cdot \text{H}_2\text{O}$) in 100 mL of concentrated HCl (sp gr 1.19). This solution is stable if a few small pieces of mossy tin are added to prevent oxidation.

8.12 Sulfuric Acid (1 + 1) **Cautiously**, and with constant stirring and cooling, add 250 mL of concentrated sulfuric acid (H_2SO_4 , sp gr 1.84) to 250 mL of water.

8.13 Hydrogen, commercially available. Set pressure on burner control box to 8 psig (55 KPa) and adjust flowmeter to approximately 6 L/min.

8.14 Nitrogen, commercially available. Set pressure on burner control box to 30 psig (206.8 KPa) and adjust flowmeter for maximum sensitivity by volatilizing standards. A flow of approximately 9 L/min has been found satisfactory. This will vary depending on the burner used.

9. Sampling

9.1 Collect the sample in accordance with Practices D3370. The holding time for the samples may be calculated in accordance with Practice D4841.

9.2 Immediately preserve samples with HNO_3 (sp gr 1.42) to a pH of 2 or less at the time of collection; normally about 2 mL/L is required. If only dissolved antimony is to be determined, filter the sample through a (No. 325) 0.45-µm membrane filter before acidification.

10. Standardization

10.1 Clean all glassware before use by rinsing first with HNO_3 (1 + 1) and then with water.

10.2 Prepare, in 200 to 300-mL wide-mouth glass containers, a blank and sufficient standards that contain from 0.0 to 1.5 µg of antimony by diluting 0.0 to 15.0-mL portions of the antimony standard solution to 100 mL with water.

10.3 Proceed as directed in 11.3 to 11.8.