

---

---

**Non-destructive testing — Measurement  
and evaluation of the X-ray tube  
voltage —**

**Part 1:  
Voltage divider method**

**iTeh STANDARD PREVIEW**  
*Essais non destructifs — Mesurage et évaluation de la tension des  
tubes radiogènes —  
(standards.iteh.ai)*  
*Partie 1: Méthode par diviseur de tension*

ISO 16526-1:2011

<https://standards.iteh.ai/catalog/standards/sist/3f63a61a-baef-4f74-b3a1-4889362fc07b/iso-16526-1-2011>



Reference number  
ISO 16526-1:2011(E)

## iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO 16526-1:2011

<https://standards.iteh.ai/catalog/standards/sist/3f63a61a-baef-4f74-b3a1-4889362fc07b/iso-16526-1-2011>



### **COPYRIGHT PROTECTED DOCUMENT**

© ISO 2011

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

## Contents

Page

Foreword . . . . .	iv
Introduction . . . . .	v
1 Scope . . . . .	1
2 Principle . . . . .	1
3 Measurement . . . . .	2
4 Test report . . . . .	2

## iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO 16526-1:2011

<https://standards.iteh.ai/catalog/standards/sist/3f63a61a-baef-4f74-b3a1-4889362fc07b/iso-16526-1-2011>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 16526-1 was prepared by CEN (as EN 12544-1:1999) and is submitted for approval under a special “fast-track procedure”, by Technical Committee ISO/TC 135, *Non-destructive testing*, Subcommittee SC 5, *Radiation methods*, in parallel with its approval by the ISO member bodies (see the *ISO/IEC Directives*, Part 1, “Fast-track procedure”).

ISO 16526 consists of the following parts, under the general title *Non-destructive testing — Measurement and evaluation of the X-ray tube voltage*:

- *Part 1: Voltage divider method*
- *Part 2: Constancy check by the thick filter method*
- *Part 3: Spectrometric method*

## Introduction

In order to cover the different requirements for the measurement of the X-ray tube voltage, three different methods are described in ISO 16526-1 to ISO 16526-3.

The voltage divider method (ISO 16526-1) enables a direct and absolute measurement of the average high voltage of constant potential X-ray systems on the secondary side of the high voltage generator.

The thick filter method (ISO 16526-2) describes a constancy check. This method is recommended for the regular stability check of an X-ray system.

The spectrometric method (ISO 16526-3) is a procedure for non-invasive measurement of the X-ray tube voltage using the energy spectrum of the X-rays. This method can be applied for all X-ray systems and is the recommended method whenever the voltage divider method is not applicable, e. g. in case of tank units where it is not possible to connect the voltage divider device.

## iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO 16526-1:2011

<https://standards.iteh.ai/catalog/standards/sist/3f63a61a-baef-4f74-b3a1-4889362fc07b/iso-16526-1-2011>

## **iTeh STANDARD PREVIEW** **(standards.iteh.ai)**

ISO 16526-1:2011

<https://standards.iteh.ai/catalog/standards/sist/3f63a61a-baef-4f74-b3a1-4889362fc07b/iso-16526-1-2011>

# Non-destructive testing — Measurement and evaluation of the X-ray tube voltage —

## Part 1: Voltage divider method

### 1 Scope

This part of ISO 16526 specifies a method for the direct and absolute measurement of the average high voltage of constant potential (DC) X-ray systems on the secondary side of the high voltage generator. The intention is to check the correspondence with the indicated high voltage value on the control unit of the X-ray system.


This method is applied to assure a reproducible operation of X-ray systems because the voltage influences particularly the penetration of materials and the contrast of X-ray images and also the requirements concerning the radiation protection.

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

### 2 Principle

The principle of the voltage divider method is presented in figure 1:

<https://standards.iteh.ai/catalog/standards/sist/3f63a61a-baef-4f74-b3a1-4889362fc07b/iso-16526-1-2011>

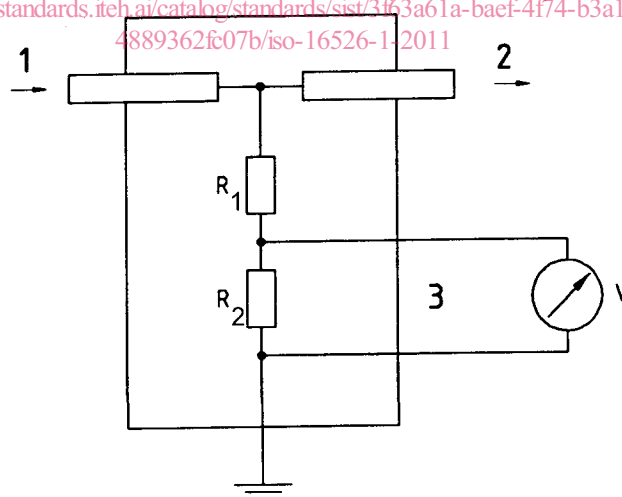

#### Key

- 1 from generator
- 2 to X-ray tube
- 3 analog exit

Figure 1 – Scheme of the voltage divider

The voltage divider system consists of

- a box with two high voltage connectors,
- a resistor chain  $R_1$ ,  $R_2$
- an analog exit for the voltage drop at  $R_2$ ,
- a measuring device, e. g. a voltmeter or an oscilloscope.

The value of the resistors should be chosen for a current of less than 10 % of the actual tube current.

The resistor chain shall have a temperature coefficient of  $\leq 50 \times 10^{-6}/^{\circ}\text{C}$  in relation to the resistor value.

The output voltage across the resistor  $R_2$  represents the value for the high voltage. The input resistance of the voltmeter shall be taken into account.

The required overall precision of the voltage divider method depends on the application, for example

- a) 1 % of the maximum voltage of the X-ray unit in case of highly stabilized constant potential systems for sophisticated applications like tomography or dosimetry, or
- b) 3 % for general radiographic and radiosopic applications.

### 3 Measurement

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

For measuring purposes the measuring device is connected between the high voltage generator and the X-ray tube. The high voltage is divided by means of the resistor chain, presented as  $R_1$  and  $R_2$  in figure 1, and the drop voltage is measured at  $R_2$  using a voltmeter or an oscilloscope.

<https://standards.iteh.ai/catalog/standards/sist/3f63a61a-baef-4f74-b3a1-4889362fc07b/iso-16526-1-2011>

### 4 Test report

The test report shall contain at least the following details:

- a) The X-ray system with type and serial number;
- b) the working conditions of the X-ray system, e. g. tube current, tube voltage, temperature;
- c) the accuracy of the measuring device;
- d) the date of measurement;
- e) a table with the result(s) and a comparison between the actual and the indicated values;
- f) name and signature of the operator.



## **iTeh STANDARD PREVIEW** **(standards.iteh.ai)**

ISO 16526-1:2011

<https://standards.iteh.ai/catalog/standards/sist/3f63a61a-baef-4f74-b3a1-4889362fc07b/iso-16526-1-2011>