
**Wheelchairs — Resistance to ignition
of non-integrated seat and back
support cushions —**

**Part 10:
Requirements and test methods**

iTeh STANDARD PREVIEW
(standards.iteh.ai)
*Fauteuils roulants — Résistance à l'inflammation des coussins de
sièges et de dossiers non intégrés —
Partie 10: Exigences et méthodes d'essai*

ISO 16840-10:2014

[https://standards.iteh.ai/catalog/standards/sist/29a0b4cd-0822-46a3-9769-
c448fd632fdc/iso-16840-10-2014](https://standards.iteh.ai/catalog/standards/sist/29a0b4cd-0822-46a3-9769-c448fd632fdc/iso-16840-10-2014)



iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 16840-10:2014
<https://standards.iteh.ai/catalog/standards/sist/29a0b4cd-0822-46a3-9769-c448fd632fdc/iso-16840-10-2014>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2014

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

	Page
Foreword.....	iv
Introduction.....	v
1 Scope.....	1
2 Normative references.....	1
3 Terms and definitions.....	2
4 Principle.....	2
5 Health and safety of test personnel.....	2
5.1 General.....	2
5.2 Enclosure.....	2
5.3 Extinguishers.....	2
6 Apparatus.....	3
6.1 Test rig.....	3
6.2 Test enclosure.....	3
6.3 Timer.....	3
6.4 Heat source.....	3
6.5 Conditioning environment.....	4
6.6 Test environment.....	5
6.7 Test sample.....	5
7 Test procedure.....	5
7.1 Preparation.....	5
7.2 Horizontal test.....	5
7.3 Vertical test.....	6
8 Requirements.....	6
9 Test report.....	6
10 Disclosure of results.....	6
Annex A (informative) Design of a heat source as a surrogate cigarette device.....	8
Annex B (normative) Conditioning of outer cover materials by washing and drying procedures.....	11
Bibliography.....	13

iTeh STANDARD PREVIEW

(standards.iteh.ai)

[ISO 16840-10:2014](https://standards.iteh.ai/catalog/standards/sist/29a0b4cd-0822-46a3-9769-c448fd632fd/iso-16840-10-2014)

[https://standards.iteh.ai/catalog/standards/sist/29a0b4cd-0822-46a3-9769-](https://standards.iteh.ai/catalog/standards/sist/29a0b4cd-0822-46a3-9769-c448fd632fd/iso-16840-10-2014)

[c448fd632fd/iso-16840-10-2014](https://standards.iteh.ai/catalog/standards/sist/29a0b4cd-0822-46a3-9769-c448fd632fd/iso-16840-10-2014)

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document can be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT), see the following URL: [Foreword — Supplementary information](#).

The committee responsible for this document is ISO/TC 173, *Assistive products for persons with disability*, Subcommittee SC 1, *Wheelchairs*.

ISO 16840 consists of the following parts, under the general title *Wheelchairs — Resistance to ignition of non-integrated seat and back support cushions*:

- *Part 1: Vocabulary, reference axis convention and measures for body segments, posture and postural support surfaces*
- *Part 2: Determination of physical and mechanical characteristics of devices intended to manage tissue integrity — Seat cushions*
- *Part 3: Determination of static, impact and repetitive load strengths for postural support devices*
- *Part 4: Seating systems for use in motor vehicles*
- *Part 6: Simulated use and determination of the changes in properties — Seat cushions*
- *Part 10: Resistance to ignition of non-integrated seat and back support cushions — Requirements and test methods*
- *Part 11: Determination of perspiration dissipation characteristics of seat cushions intended to manage tissue integrity [Technical Specification]*

The following parts are under preparation:

- *Part 9: Clinical interface pressure mapping guidelines for seating [Technical Report]*
- *Part 12: Apparatus and method for cushion envelopment testing*

Introduction

The ignition and subsequent burning of wheelchairs is very rare, but can occur as a result of

- being close to a burning object such as a fire beside the wheelchair,
- overheating of any electrical or electronic device on the wheelchair, and
- contact from sparks or flames (such as welding sparks, cigarettes, or matches).

Wheelchair occupants are at particular risk of injury or death from these fires and resulting fumes because they may not have the ability to move away from the wheelchair.

Wheelchairs can be considered to be comprised of the following components:

- a) structural components such as the frame, wheels, etc. which are essential to the mechanical integrity of the wheelchair;
- b) postural support devices, such as sling seats, sling back supports, arm supports, foot supports, etc., which are attached to the wheelchair and are primarily intended to give postural support to the wheelchair occupant (these can also be intended to aid in pressure redistribution);
- c) devices to manage tissue integrity, such as seat and back support cushions which are intended to have primarily a clinical function to minimize the risks of skin damage (these can also be intended to control or accommodate posture);
- d) power-related components such as motors, energy sources, controllers etc., which are required for the functioning of powered devices on wheelchairs.

Each of the above components has a different severity of risk associated with its likelihood of igniting and its resulting harm to the wheelchair occupant. ISO standards have been published or are in preparation to specify requirements and test methods for the above categories of components to help manufacturers and purchasers of wheelchairs to design and procure wheelchairs and their components which are appropriate for the risk of ignition balanced against the functional needs of the wheelchair occupant. The aim of these ISO standards is to provide appropriate alternatives to using furniture-based flammability standards, to reflect the uses and purposes of wheelchairs and their accessories.

The development of an ISO standard on the resistance to ignition of structural components [see list item a) above] has not yet commenced. The most likely sources of ignition are proximity to a heat source such as an electric radiator or domestic fire or a heat source such as a lighted match or cigarette falling onto the structure.

ISO 7176-16 is primarily concerned with the resistance to ignition of postural support device components of a wheelchair [see list item b) above]. These typically include arm supports, sling seats, sling back supports, lower leg supports, foot supports, lateral supports, head supports, etc. The most likely source of ignition is an open flame source falling onto the component's surface or into gaps between surfaces. Consequently that standard is written around resistance to a heat source equivalent to a lighted match in contact with a test sample of an assembly of the upholstered part's composite materials in both a vertical and horizontal orientation.

The power related components [see list item d) above] are the subject of ISO 7176-14 which specifies requirements to prevent overheating in electrical components that could lead to a fire.

The tissue integrity devices [see list item c) above] are the subject of this part of ISO 16840, and permit a less stringent resistance to ignition than in ISO 7176-16, based upon the priority of these components for their clinical function, which might override the need for a high resistance to ignitability.

The requirements of this part of ISO 16840 have been set at a basic minimum level and are less severe than mandatory requirements in some countries. This part of ISO 16840 has been produced to allow for the use of materials that would not meet the requirements of ISO 7176-16, but the manufacturer is required to make the case as to why ISO 7176-16 could not be employed. Good practice is also to use

ISO 16840-10:2014(E)

materials which minimize the risk of release of toxic substances as a result of ignition. Materials chosen are to comply also with biocompatibility requirements (ISO 10993-1 and ISO 10993-10).

The day to day usage of a wheelchair may affect its materials' resistance to ignition through cyclic loading, movement of materials, washing, cleaning, etc. Manufacturers will often take this effect into account as part of their risk assessment when selecting materials for their products to minimize the effects of this normal use. However, although this part of ISO 16840 can be used on parts that have been used, etc., the test samples specify new or unused parts.

Different environments commonly encountered by some wheelchair occupants may also affect the flammability of materials. For example, home oxygen systems, delivery systems for drugs carried in an inflammable medium, etc., can turn an inert material into a flammable one. Dust and other materials accumulated within the chair have also been found to be a source of readily ignitable material. Wheelchair manufacturers and occupants should be aware of these risks, and design and use wheelchairs accordingly as covered by ISO 14971.

This part of ISO 16840 describes testing an assembly of the composite of materials as used in the wheelchair component, because the resistance to ignition of these materials individually can be quite different from those when assembled as a composite. Hence, the results of this part of ISO 16840 do not give any indication of the resistance to ignition of any of the separate individual materials of the test sample.

iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO 16840-10:2014](https://standards.iteh.ai/catalog/standards/sist/29a0b4cd-0822-46a3-9769-c448fd632fdc/iso-16840-10-2014)

<https://standards.iteh.ai/catalog/standards/sist/29a0b4cd-0822-46a3-9769-c448fd632fdc/iso-16840-10-2014>

Wheelchairs — Resistance to ignition of non-integrated seat and back support cushions —

Part 10: Requirements and test methods

1 Scope

This part of ISO 16840 specifies requirements and test methods to assess the resistance to ignition by smouldering cigarette equivalent of non-integrated components of a wheelchair intended to protect tissue integrity.

The test measures only the resistance to ignition by smouldering cigarette equivalent of the items tested and not the ignitability of the complete wheelchair. It gives an indication, but cannot guarantee, the ignition behaviour of the assembled non-integrated devices of a complete wheelchair.

This part of ISO 16840 does not apply to resistance to ignition of structural parts of a wheelchair, nor does it cover postural support devices. This part of ISO 16840 does not cover changes in resistance to ignition as a result of regular washing or use.

This part of ISO 16840 allows for the separate testing of removable non-integrated components of a wheelchair which are normally used in the horizontal plane (e.g. a seat cushion) from those normally used in the vertical plane (e.g. a back support).

This part of ISO 16840 describes testing an assembly of the composite of materials as used in the removable non-integrated component. The results of this part of ISO 16840 do not give any indication of the resistance to ignition of any of the separate individual materials of the test sample.

NOTE 1 The intent of this part of ISO 16840 is primarily to cover removable cushions whose described purpose is that of protecting skin tissue against pressure, shear, and maceration related damage.

NOTE 2 The requirements of this part of ISO 16840 have been set at a basic minimal level and are less severe than mandatory requirements in some countries.

Where practical, it is advisable that manufacturers use materials with superior resistance to ignition. The manufacturer is required to make the case as to why ISO 7176-16 could not be employed rather than this part of ISO 16840.

NOTE 3 Requirements for the control of risks from sources of fire created by electrical and electronic components are included in ISO 7176-14

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 14971, *Medical devices — Application of risk management to medical devices*

ISO 554, *Standard atmospheres for conditioning and/or testing — Specifications*

EN 1021-1:2006, *Furniture — Assessment of the ignitability of upholstered furniture — Part 1: Ignition source smouldering cigarette*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 7176-26 and ISO 8191-1:1987 and the following apply.

3.1

flaming

undergoing combustion in the gaseous phase with the emission of light

[SOURCE: ISO 8191-1:1987, definition 3.2]

3.2

non-integrated

detachable without the use of tools

Note 1 to entry: Seat or back cushions held in place by hook and loop fastenings are also considered non-integrated.

Note 2 to entry: Other upholstered parts (such as padded seat or back canvasses) attached to the chair by hook and loop fastenings are regarded as wheelchair postural support devices as covered by ISO 7176-16.

3.3

progressive smouldering

exothermic oxidation, not accompanied by flaming, that is self-propagating i.e. independent of the ignition source

[SOURCE: ISO 8191-1:1987, definition 3.1]

Note 1 to entry: It may or may not be accompanied by incandescence.

iteh STANDARD PREVIEW
(standards.iteh.ai)

4 Principle

ISO 16840-10:2014

Test materials used in non-integrated seat and back support devices as used in wheelchairs are assembled in either horizontal or vertical samples and subjected to a heat source which is equivalent to a smouldering cigarette. The resulting effects on the test materials are observed and measured.

5 Health and safety of test personnel

5.1 General

WARNING — The following test requirements call for the use of procedures that may be hazardous to health if adequate precautions are not taken.

These precautions are drawn from ISO 8191-1:1987, Clause 6.

Ensure that there is no hidden smouldering of the sample before disposal.

5.2 Enclosure

For safety, the tests should be conducted in a non-combustible fume cupboard. If such a cupboard is not available, a test enclosure should be constructed (see 6.2) so that the operator is protected from the fumes.

5.3 Extinguishers

Adequate means of extinguishing the assembly should be provided, bearing in mind that some combinations may produce severe flaming during the test. A hand and/or a fixed water spray which can be directed over the burning area can be useful. Other means such as fire extinguishers (water and halogenated hydrocarbons), fire blankets, and a bucket of water will assist. In some cases smouldering may be difficult to extinguish completely and complete immersion in water may be necessary.

6 Apparatus

6.1 Test rig

The test rig in ISO 8191-1:1987 may be used as described.

NOTE The frame of the test rig described as the back frame with a width of 450 mm \pm 2 mm, but with a height of 450 mm \pm 2 mm can be used for both the horizontal and vertical tests.

6.2 Test enclosure

The test enclosure shall consist of either a room with a volume greater than 20 m³ (which contains adequate oxygen for testing) or a smaller enclosure with a through flow of air. Inlet and extraction systems providing air flows of 0,02 m/s to 0,2 m/s in the locality of the rig provide adequate oxygen without disturbing the burning behaviour.

NOTE This enclosure is the equivalent to that specified in ISO 8191-1:1987, 7.2.

6.3 Timer

A means of measuring time for a period of 5 s to 1 000 s with an accuracy of \pm 0,1 s.

6.4 Heat source

A temperature controlled heat source consisting of two separate parts.

- a) A heat source complying with the following:
- 8 mm \pm 0,5 mm diameter;
 - 75 mm \pm 5 mm heated length;
 - 100 W \pm 20 W heat output;
 - K-type thermocouple integrated in the centre of the heat source;
 - minimum wire length of 3 m;
 - heat resistant wire insulation;
 - a fixture to hold the heat source in place throughout the test, designed to avoid burns while handling the heat source.
- b) A temperature controller complying with the following:
- temperature controller with automatic identification of the control area or model based tuning of the controller parameters;
 - the test cycle commences when the temperature value of 150 °C has been reached;
 - the temperature values follow the temperature heating curve in [Figure 1](#) and [Table 1](#) automatically during the test cycle.

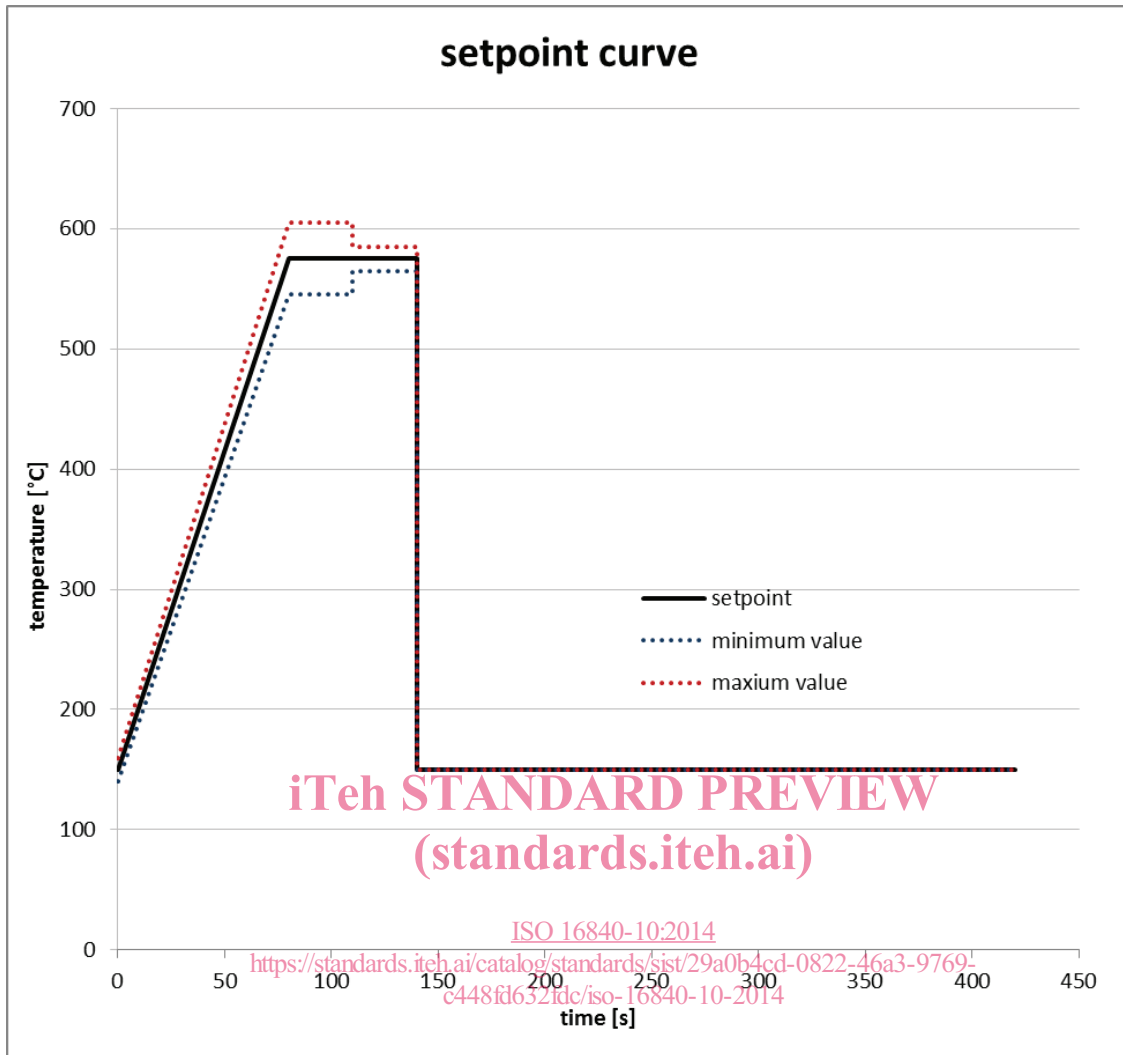


Figure 1 — Temperature-time-diagram of the test cycle with set point curve and allowed offset

Table 1 — Set point table for the test

	Duration	Initial set point	Final set point
Ramp	80 s ± 20 s	150 °C ± 10 °C	575 ± 30 °C
Plateau	30 s ± 1 s	575 °C ± 30 °C	575 °C ± 10 °C
Plateau	30 s ± 1 s	575 °C ± 10 °C	575 °C ± 10 °C
Cooling	Variable	575 °C ± 10 °C	150 °C ± 10 °C

NOTE 1 [Annex A](#) provides details of an apparatus that meets these specifications

NOTE 2 This source has been designed to give a calorific output approximating to that of a stabilized smouldering cigarette (ISO 8191-1:1987).

6.5 Conditioning environment

Prior to conditioning described below, all outer cover materials shall be subjected to the washing and drying procedures described in [Annex B](#).

An environment with an atmosphere which can be maintained for up to 20 h at a temperature of 23 °C ± 2 °C and relative humidity of 50 % ± 5 % as specified in ISO 554.

6.6 Test environment

An environment in which the test procedure in [Clause 7](#) can be conducted and which has an atmosphere with a temperature between 10 °C and 30 °C and a relative humidity between 15 % and 80 %.

In the area of the test rig within 100 mm ± 5 mm of the heat source, the airflow shall be less than 0,02 m/s

6.7 Test sample

A sample consisting of the materials assembled as used which shall be made up of cover, filling, and any other components, such as an interliner, which may be used in a real assembly. The sample shall have dimensions comprising of a minimum width of 300 mm and a maximum width of 450 mm, and a depth or length of a minimum of 300 mm and a maximum of 450 mm. A manufactured non-integrated seat or back support cushion provided that it is no smaller than the minimum dimensions or no larger than the maximum dimensions specified above may be used.

Spray-on flame retardant substances shall not be relied on unless the durability of their effectiveness for the life of the manufactured part is confirmed.

NOTE 1 If the cushion is designed to be used only with its cover, then the test sample shall include that cover.

NOTE 2 If the cushion is designed to be used only with its cover from a choice of covers, each cover option shall be tested separately in combination with that cushion.

NOTE 3 If the cushion is designed to be used either with or without its cover, then the cushion shall be tested with and without its cover.

STANDARD PREVIEW
(standards.iteh.ai)

7 Test procedure

7.1 Preparation

ISO 16840-10:2014

<https://standards.iteh.ai/catalog/standards/sist/29a0b4cd-0822-46a3-9769->

[0448f632f1c/iso-16840-10-2014](https://standards.iteh.ai/catalog/standards/sist/29a0b4cd-0822-46a3-9769-0448f632f1c/iso-16840-10-2014)

- a) Identify the removable seat or back support cushion.
- b) If testing items which are intended to be used only in the range of the horizontal plane ± 30°, use the horizontal test, and for all other supports use the vertical test. If the part is intended for use in either plane, then use both tests.
- c) Attach the test sample(s) to the test rig(s).
- d) Place the test rig and sample in the conditioning environment for a minimum of 16 h.
- e) Ensure the heat source is below 50 °C.

7.2 Horizontal test

- a) Set up the test sample mounted in the test rig in a horizontal orientation (of the contact surface) in the test environment.
- b) Apply the heat source specified in [6.4](#) within 50 mm of the centre of the top surface as possible and parallel to the top surface of the test sample with no pressure from the heat source, nor a gap between the heat source and the sample.
- c) Switch on the heat source and make sure the actual temperature value of the heat source is 150 °C ± 30 °C before starting the test cycle.
- d) Start the test cycle. Observe the subsequent progress of combustion, and record any evidence of progressive smouldering, or flaming in the interior and/or surface. Disregard any afterglow, smoking, or smouldering that ceases within 10 s of the end of the plateau of the heat temperature curves. Allow the heat source to cool down to 150 °C or less before removing it from the sample.