



Designation: D1500 – 07



Designation: 196/97

## Standard Test Method for ASTM Color of Petroleum Products (ASTM Color Scale)<sup>1</sup>

This standard is issued under the fixed designation D1500; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

*This standard has been approved for use by agencies of the Department of Defense.*

### 1. Scope\*

1.1 This test method covers the visual determination of the color of a wide variety of petroleum products, such as lubricating oils, heating oils, diesel fuel oils, and petroleum waxes.

NOTE 1—Test Method D156 is applicable to refined products that have an ASTM color lighter than 0.5. IP Method 17 includes a procedure for measuring the color of undyed, refined products such as gasoline, white spirit, and kerosine by comparison with a series of IP Standard glasses. It also includes a procedure by which petroleum products, except black oils and bitumens, may be measured for tint and depth of color in terms of Lovibond units by a series of red, yellow, and blue glasses.

1.2 This test method reports results specific to the test method and recorded as “ASTM Color.”

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

### 2. Referenced Documents

#### 2.1 ASTM Standards:<sup>2</sup>

D156 Test Method for Saybolt Color of Petroleum Products (Saybolt Chromometer Method)

D938 Test Method for Congealing Point of Petroleum Waxes, Including Petrolatum

D2500 Test Method for Cloud Point of Petroleum Products

D4057 Practice for Manual Sampling of Petroleum and Petroleum Products

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee D02 on Petroleum Products and Lubricants and is the direct responsibility of Subcommittee D02.05 on Properties of Fuels, Petroleum Coke and Carbon Material.

Current edition approved Dec. 1, 2007. Published January 2008. Originally approved in 1957. Last previous edition approved in 2004 as D1500–04a.

This is also a standard of Energy Institute issued under the fixed designation IP 196. The final number indicates the year of last revision. This test method was adopted as a joint ASTM-IP standard in 1966. In the IP, this test method is under the jurisdiction of the Standardization Committee. DOI: 10.1520/D1500-07.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

#### 2.2 Energy Institute Standard:<sup>3</sup>

IP 17 Color by the Lovibond Tintometer

### 3. Summary of Test Method

3.1 Using a standard light source, a liquid sample is placed in the test container and compared with colored glass disks ranging in value from 0.5 to 8.0. When an exact match is not found and the sample color falls between two standard colors, the higher of the two colors is reported.

### 4. Significance and Use

4.1 Determination of the color of petroleum products is used mainly for manufacturing control purposes and is an important quality characteristic, since color is readily observed by the user of the product. In some cases, the color may serve as an indication of the degree of refinement of the material. When the color range of a particular product is known, a variation outside the established range may indicate possible contamination with another product. However, color is not always a reliable guide to product quality and should not be used indiscriminately in product specifications.

### 5. Apparatus

5.1 *Colorimeter*, consisting of light source, glass color standards, sample container housing with cover, and viewing piece as listed in Annex A1.

5.2 *Sample Container*—For referee work, use the glass sample jar as shown in Fig. 1. For routine tests, it is permissible to use a cylindrical, clear glass jar with a flat bottom of 30 to 32.4 mm internal diameter, 115 to 125 mm in external height, and a wall thickness no greater than 1.6 mm as specified in Test Method D2500, or an ordinary 125-mL oil sample bottle if it meets these requirements.

### 6. Sampling

6.1 Samples shall be taken in accordance with the instructions in Practice D4057.

<sup>3</sup> “Methods for Analysis and Testing,” available from Energy Institute, 61 New Cavendish St., London, WIG 7AR, U.K.

\*A Summary of Changes section appears at the end of this standard

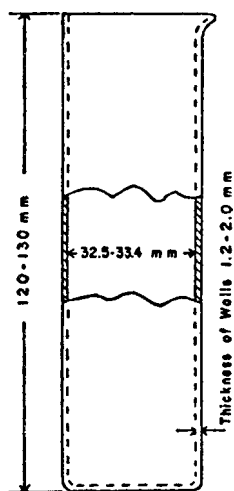


FIG. 1 Standard Glass Sample Jar

## 7. Diluent

7.1 *Solvent Kerosine*— (**Warning**—Combustible. Vapor harmful.) Having a color lighter than +21 Saybolt color by Test Method **D156** or 1.5 by Method B of IP 17, this material is used for diluting dark samples for the test. As an alternative, other solvents, such as white oil or solvent neutral 100 of satisfactory purity that meet the color requirements specified here in **7.1**, are also acceptable.

NOTE 2—Solvent kerosine complies with this requirement if it is lighter in color than potassium dichromate ( $K_2Cr_2O_7$ ) solution formed by dissolving 4.8 mg of pure anhydrous  $K_2Cr_2O_7$  in 1 L of distilled water.

## 8. Preparation of Sample

8.1 *Liquid Petroleum Products such as Lubricating Oils*— Fill the sample container to a depth of 50 mm or more and observe the color. When the sample is not clear, heat it just sufficiently enough to make it clear to perform the color measurement at that temperature. A sample heated to a temperature of 6°C (10°F) above its cloud point (see Test Method **D2500**) has been found suitable to test samples using this test method. When the sample is darker than 8 color, one may either stop the test and report “D8 ASTM Color” (see **10.2**) or continue the test and mix 15 volumes of sample into 85 volumes of solvent kerosine or alternative material (see **7.1**) and observe the color of the mixture.

8.2 *Petroleum Waxes, Including Petrolatum*—Heat the sample just sufficiently enough to make it fluid and clear to perform the color measurement at that temperature without heating the wax excessively, because oxidation can occur, along with consequent discoloration of the test specimen. A sample heated to a temperature of 11 to 17°C (20 to 30°F) above its congealing point, as determined in accordance with Test Method **D938**, has been found suitable to test samples using this test method. When the sample is darker than 8 color, one may either stop the test and report “D8 ASTM Color” (see **10.2**) or continue the test and mix 15 volumes of melted sample with 85 volumes of solvent kerosine or alternative material (see **7.1**) brought to the same temperature and test the mixture at that temperature.

## 9. Procedure

9.1 Place a sample container or containers, filled to a depth of at least 50 mm with distilled or deionized water, in the compartment or compartments of the colorimeter through which the standard glasses will be observed. Place the sample in its container in the other compartment. (When using a three-field comparator, this will be the middle compartment.) Cover the containers to exclude all exterior light.

9.2 Switch on the light source and compare the color of the sample with that of the standard glasses. When using a three-field comparator, the sample must be bracketed by darker and lighter discs or by an exact match and a darker disc. Determine for two-field comparators which glass matches the color of the sample; or if an exact match is not possible, then use that glass which possesses the next darker color.

## 10. Report

10.1 Report as the color of the sample, the designation of the glass producing a matching color (for example, “7.5 ASTM Color.”)

10.2 If the color of the sample is intermediate between those of two standard glasses, report that the sample is less than the darker glass designation. As an example, report the designation of the darker glass preceded by the letter “L” (for example, “L7.5 ASTM Color”) or with a “<” symbol (for example, “<7.5 ASTM Color”). Never report the color as being darker than a given standard except those darker than 8 (for example, “D8 ASTM Color” or “>8 ASTM Color.”)

10.2.1 If the color of the sample is less than the 0.5 glass color standard, report that the sample is less than the 0.5 glass color standard. As an example, report the designation as “L0.5 ASTM Color” or “<0.5 ASTM Color.”

10.3 If the sample has been diluted in accordance with **7.1**, report the color of the mixture followed by the abbreviation “Dil” (for example, “L7.5 Dil ASTM Color” or “<7.5 Dil ASTM Color”). See **Note 3**.

NOTE 3—For samples that are diluted in **10.3**, it is permissible for the laboratory to annotate the report in any suitable manner, provided that the information clearly conveys to the data recipient that the sample analyzed was diluted.

## 11. Precision and Bias<sup>4</sup>

11.1 *Precision*—The precision of this test method as obtained by statistical examination of interlaboratory test results is as follows:

11.1.1 *Repeatability*—The difference between successive test results obtained by the same operator with the same apparatus under constant operating conditions on identical test material would, in the long run, in the normal and correct operation of the test method, exceed the following value only in one case in twenty: 0.5 color units.

11.1.2 *Reproducibility*— The difference between two single and independent test results obtained by different operators working in different laboratories on identical test material

<sup>4</sup> Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D02-1234.