

SLOVENSKI STANDARD
SIST EN 60601-1:2007/A1:2014/AC:2015
01-maj-2015

Medicinska električna oprema - 1. del: Splošne zahteve za osnovno varnost in bistvene lastnosti (IEC 60601-1:2005/AMD1:2012)

Medical electrical equipment - Part 1: General requirements for basic safety and essential performance

Medizinische elektrische Geräte - Teil 1: Allgemeine Festlegungen für die Sicherheit einschließlich der wesentlichen Leistungsmerkmale

STANDARD PREVIEW

(standards.iteh.ai)

Appareils électromédicaux - Partie 1: Exigences générales pour la sécurité de base et les performances essentielles

[SIST EN 60601-1:2007/A1:2014/AC:2015](#)

<https://standards.iteh.ai/catalog/standards/sist/17cf8992-761d-4eca-943e-8eefa3d86fef/sist-en-60601-1-2007-a1-2014-ac-2015>

Ta slovenski standard je istoveten z: [EN 60601-1:2006/A1:2013/AC:2014](#)

ICS:

11.040.01 Medicinska oprema na splošno Medical equipment in general

SIST EN 60601-1:2007/A1:2014/AC:2015 en,fr,de

iTeh STANDARD PREVIEW (standards.iteh.ai)

[SIST EN 60601-1:2007/A1:2014/AC:2015](#)

<https://standards.iteh.ai/catalog/standards/sist/17cf8992-761d-4eca-943e-8eefa3d86fef/sist-en-60601-1-2007-a1-2014-ac-2015>


**IEC 60601-1:2005/AMD1:2012
(Amendment 1 to the third edition)**

**Medical electrical equipment –
Part 1: General requirements for basic safety and essential performance**

C O R R I G E N D U M 1

Figure 12 – Example of a measuring device and its frequency characteristics

Replace, in the text of the vertical axis of b) Frequency characteristics, "dB: 20" by "(dB):20 log" as follows:

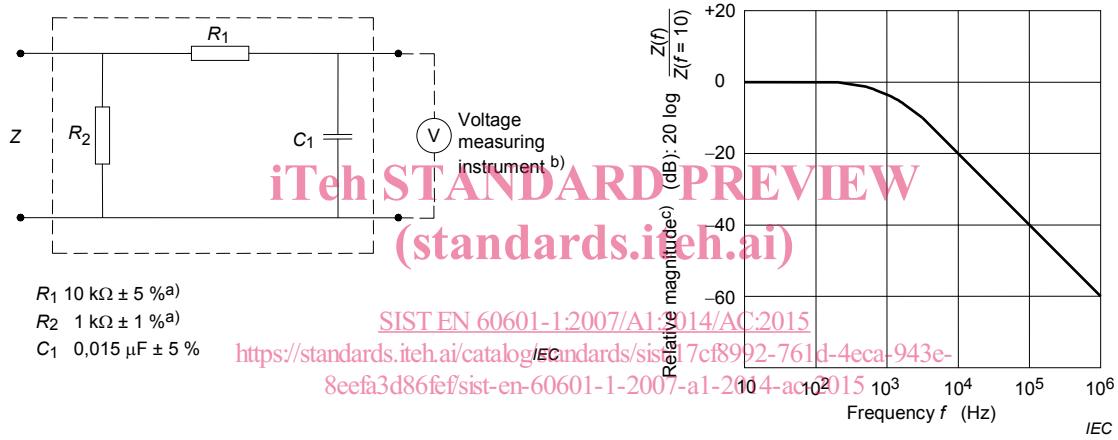

NOTE The network and voltage measuring instrument above are replaced by the symbol  in the following figures.

a) Non-inductive components

b) Resistance $\geq 1 \text{ M}\Omega$ and capacitance $\leq 150 \text{ pF}$

c) $Z(f)$ is the transfer impedance of the network, i.e. $V_{\text{out}}/I_{\text{in}}$, for a current of frequency f .

Figure 12 – Example of a measuring device and its frequency characteristics