
**Fine ceramics (advanced ceramics,
advanced technical ceramics) —
Ceramic composites — Determination
of the degree of misalignment in
uniaxial mechanical tests**

*Céramiques techniques — Céramiques composites — Détermination
du degré de non-alignement lors des essais mécaniques uniaxiaux*

(standards.iteh.ai)

[ISO 17161:2014](https://standards.iteh.ai/catalog/standards/sist/9323ce9d-ecb7-41f1-bcb4-87d921e2eb9e/iso-17161-2014)

<https://standards.iteh.ai/catalog/standards/sist/9323ce9d-ecb7-41f1-bcb4-87d921e2eb9e/iso-17161-2014>



iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 17161:2014

<https://standards.iteh.ai/catalog/standards/sist/9323ce9d-ecb7-41f1-bcb4-87d921e2eb9e/iso-17161-2014>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2014

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
3.1 General	1
3.2 Type of defects	2
4 Principle	2
5 Apparatus	3
5.1 Test machine	3
5.2 Load train	4
5.3 Strain gauges	4
5.4 Data recording system	4
5.5 Micrometers	4
6 Reference test specimens	4
7 Reference test specimen preparation	6
7.1 Adhesion of strain gauges	6
7.2 Reference test specimen validity	6
8 Test procedure	6
8.1 General	6
8.2 Correction of the torsion defect	6
8.3 Correction of the C defect	7
8.4 Correction of the S defect	8
8.5 Final verification before starting a series of measurements on CMCs	9
9 Test report	9
Bibliography	10

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: Foreword - Supplementary information

The committee responsible for this document is ISO/TC 206, *Fine ceramics*.

[ISO 17161:2014](https://standards.iteh.ai/catalog/standards/sist/9323ce9d-ccb7-41f1-bcb4-87d921e2eb9e/iso-17161-2014)

<https://standards.iteh.ai/catalog/standards/sist/9323ce9d-ccb7-41f1-bcb4-87d921e2eb9e/iso-17161-2014>

Fine ceramics (advanced ceramics, advanced technical ceramics) — Ceramic composites — Determination of the degree of misalignment in uniaxial mechanical tests

1 Scope

This International Standard describes a procedure

- to verify the degree of misalignment of the load train of the test machines using a reference test specimen uniformly loaded in tension or in compression, and
- to give indications in order to correct defects such as torsion and bending.

This International Standard is not intended to provide a quantitative and acceptable limit before the testing of ceramic matrix composites with a fibre reinforcement: unidirectional (1D), bidirectional (2D), and tridirectional (x D, with $2 < x \leq 3$) loaded along one principal axis of reinforcement. This limit depends on the sensitivity of each type of composite to the misalignment defect.

NOTE 1 This limit is to be defined between the testing establishment and the customer.

NOTE 2 Monolithic ceramics are very sensitive to misalignment defects while CMCs (ceramic matrix composite) in general are moderately sensitive to them.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3611, *Geometrical product specifications (GPS) — Dimensional measuring equipment: Micrometers for external measurements — Design and metrological characteristics*

ISO 7500-1, *Metallic materials — Verification of static uniaxial testing machines — Part 1: Tension/compression testing machines — Verification and calibration of the force-measuring system*

ISO/IEC 17025, *General requirements for the competence of testing and calibration laboratories*

CEN/TR 13233:2007, *Advanced technical ceramics — Notations and symbols* (to be replaced by future ISO NP 19634)

3 Terms and definitions

For the purposes of this document, the terms and definitions given in CEN/TR 13233:2007 (to be replaced by future ISO NP 19634) and the following apply.

3.1 General

3.1.1 calibrated length

l

part of the reference test specimen which has a uniform and minimum cross-section area

3.1.2
width

b
width of the reference test specimen in the calibrated length

3.1.3
thickness

h
thickness of the reference test specimen in the calibrated length

3.2 Type of defects

3.2.1
C-type magnitude

θ
angle between the loading axis of each of the two grips

Note 1 to entry: See [Figure 1](#).

3.2.2
S-type magnitude

d
distance between the loading axis when they are parallel

Note 1 to entry: See [Figure 2](#).

3.2.3
torsion defect magnitude

ϕ
angle between the gripping planes

Note 1 to entry: See [Figure 3](#).

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 17161:2014

<https://standards.iteh.ai/catalog/standards/sist/9323ce9d-ecb7-41f1-bcb4-87d921e2eb9e/iso-17161-2014>

4 Principle

A rectangular cross section of a reference test specimen ([Clause 7](#)) equipped with 10 strain gauges is loaded in tension or in compression, up to a load corresponding to 10 % of the nominal load capacity of the load cell used for the tests of CMCs. The stress corresponding to this value shall not exceed 50 % of the elasticity limit of the material used for the reference test specimen. The readings obtained from the strain gauges bonded on the calibrated length of the reference test specimen allow the determination of the degree of misalignment.

The positioning of strain gauges is such that it indicates the magnitude of defects. These magnitudes allow the correction, in a practical manner, of the different types of defects:

- bending defects, either C ([Figure 1](#)) or S ([Figure 2](#));
- torsion ([Figure 3](#)).

The indications for correction are obtained by comparing the experimental readings of the strain gauges to values from charts established from numerical simulations.



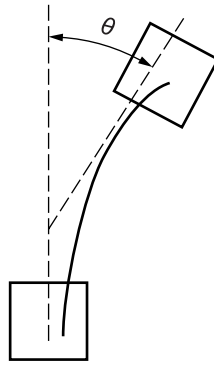


Figure 1 — C defect magnitude

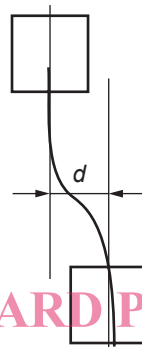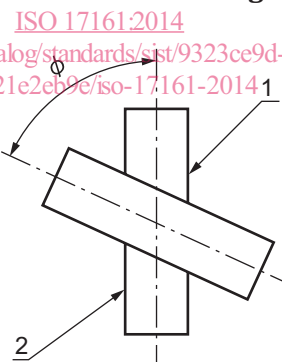

iTeh STANDARD PREVIEW
(standards.iteh.ai)

Figure 2 — S defect magnitude

**Key**

- 1 lower grip
- 2 upper grip

Figure 3 — Torsion defect magnitude

5 Apparatus**5.1 Test machine**

The configuration of the test machine, including the load train and load cell, shall be identical to the test machine used for the tests on the CMCs and shall be in accordance with ISO 7500-1.

5.2 Load train

The load train configuration shall ensure that the load indicated by the load cell and the load experienced by the test specimen are the same.

The grip design shall prevent the test specimen from slipping. The choice of gripping system will depend on material, on test specimen design, and on alignment requirements.

5.3 Strain gauges

The principle of this method requires the use of strain gauges with an active surface equal to or smaller than $4 \times 2,5 \text{ mm}^2$.

Furthermore, the distance between the edge of the test reference specimen and the longitudinal axis of the strain gauge shall be such as to avoid edge effects. A minimum distance of 2 mm is required.

Care shall be taken to ensure that the strain gauge readings are not influenced by the surface preparation and the adhesive used.

5.4 Data recording system

A calibrated recorder can be used to record load/strain curves. The use of a data recording system combined with an analogue recorder is recommended.

All strain measuring equipment and data acquisition systems shall be calibrated as appropriate. Typically they shall have an accuracy to within $\pm 0,5 \%$ of indicated reading or ± 3 microstrain, whichever is greater, and a resolution of 1 microstrain.

5.5 Micrometers

Micrometers used for the measurement of the dimensions of the reference test specimen shall be in accordance with ISO 3611.

6 Reference test specimens

The degree of misalignment of the load train of the test machine is verified by performing tests at room temperature with the following reference test specimen:


- dimensions: see [Figure 4](#) and [Table 1](#);
- material: steel ISO reference;
- location of the strain gauges: see [Figure 4](#).

If another reference test specimen is used, it is necessary to establish a new series of charts.

Plan parallelism of the faces: $\pm 0,02 \text{ mm}$.

Dimensions of the strain gauges, in millimetres: $\begin{matrix} 2,5 \\ \square \\ 4 \end{matrix}$.

Dimensions in millimetres

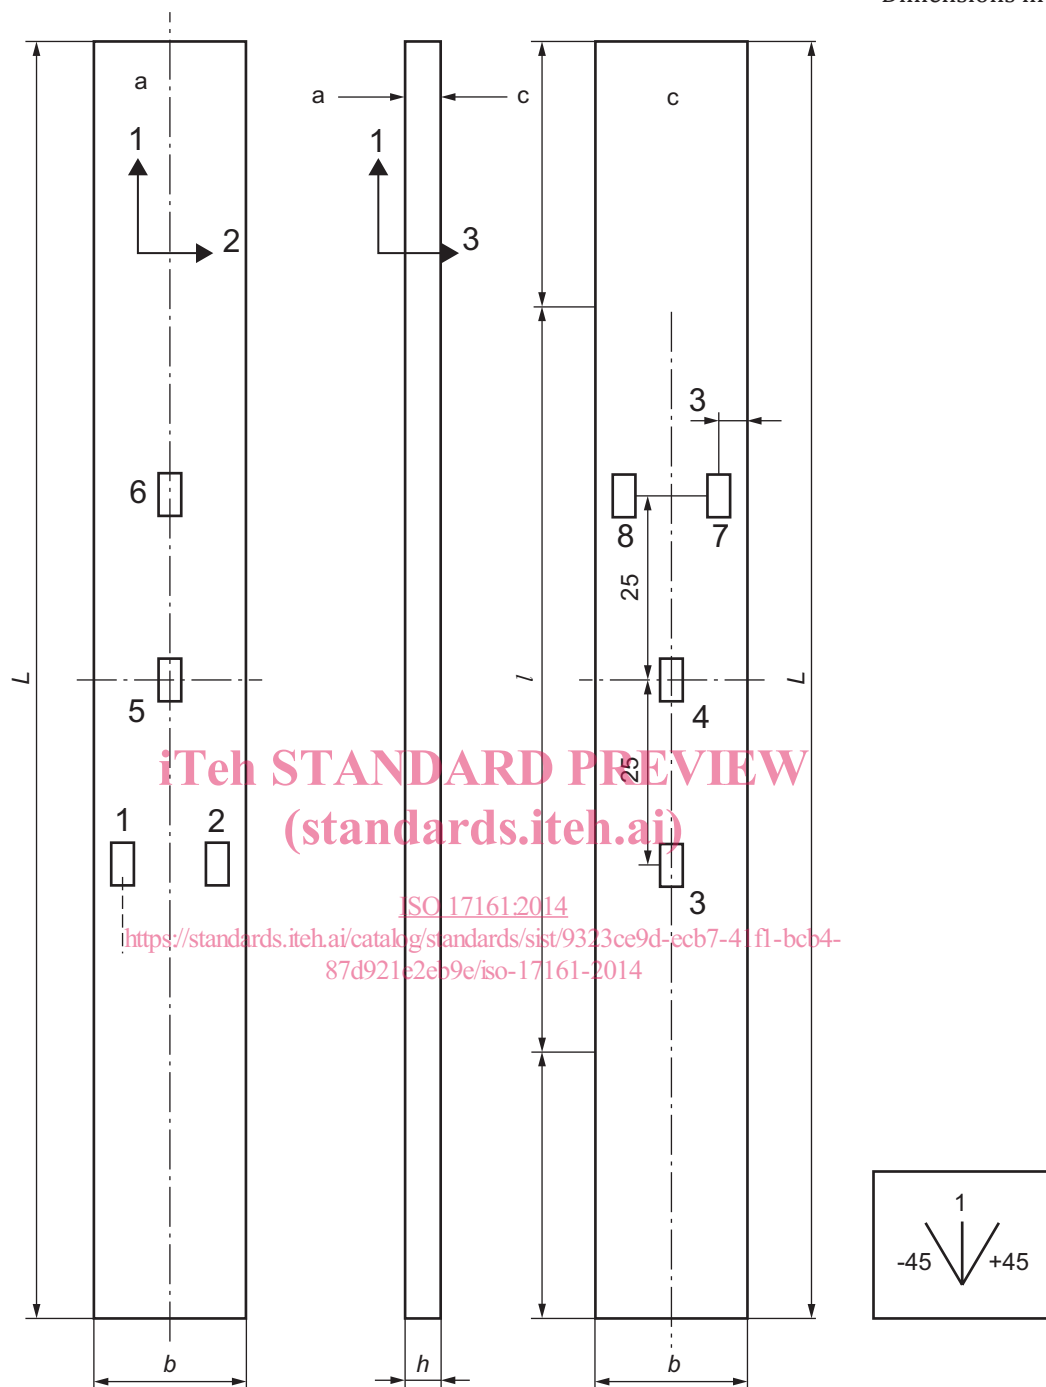

NOTE 1 Gauge n° 5 is a rosette allowing measurements of strains parallel to 1 and to $\pm 45^\circ$.

NOTE 2 Keys a and c indicate each surface.

Figure 4 — Dimensions of the reference test specimen and location of the strain gauges