
**Sterile acupuncture needles for single
use**

Aiguilles d'acupuncture stériles à usage unique

**iTeh STANDARD PREVIEW
(standards.iteh.ai)**

[ISO 17218:2014](https://standards.iteh.ai/catalog/standards/sist/ff2ea673-db69-4871-8322-838776fc598f/iso-17218-2014)

<https://standards.iteh.ai/catalog/standards/sist/ff2ea673-db69-4871-8322-838776fc598f/iso-17218-2014>



iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 17218:2014

<https://standards.iteh.ai/catalog/standards/sist/ff2ea673-db69-4871-8322-838776fc598f/iso-17218-2014>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2014

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Configuration	2
4.1 Acupuncture needle configuration.....	2
4.2 Acupuncture needle types.....	2
4.3 Types of needle handles.....	3
5 Requirements	5
5.1 Materials.....	5
5.2 Dimensions.....	5
5.3 Performance requirements.....	7
5.4 Sterility assurance.....	9
6 Package	9
6.1 Primary package.....	9
6.2 Secondary package.....	10
7 Labelling	10
7.1 General.....	10
7.2 Primary package.....	10
7.3 Secondary package.....	10
8 Transit and storage	11
Annex A (informative) Test methods for the intensity and sharpness of the tip of the needle	12
Annex B (informative) Test methods for the puncture performance of the tip of the needle	16
Annex C (informative) Test method for resistance to corrosion	21
Bibliography	23

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: Foreword - Supplementary information

The committee responsible for this document is ISO/TC 249, *Traditional Chinese medicine*.

[ISO 17218:2014](https://standards.iteh.ai/catalog/standards/sist/ff2ea673-db69-4871-8322-838776fc598f/iso-17218-2014)

<https://standards.iteh.ai/catalog/standards/sist/ff2ea673-db69-4871-8322-838776fc598f/iso-17218-2014>

Introduction

This International Standard applies to sterile acupuncture needles for single use (specialized for filiform needles) used by professional acupuncturists for acupuncture treatment. Sterile acupuncture needles for single use are sterilized by the manufacturer, and the healthcare professional can open the sealed package and use the needle immediately.

In order to encourage innovation, this International Standard does not enforce the combination of the needle diameter and length. However, considering the clinical usage requirements, the standard provides the specifications for the needle diameter and length.

The sharpness and puncture performance of the needle tip are of very important clinical significance. [Annex A](#) states the guidelines and the evaluation methods for the intensity and the sharpness of the needle tip, while [Annex B](#) provides two qualitative and quantitative evaluation methods to determine the puncture performance of the needle tip.

The qualitative methods to evaluate the puncture performance of needle tip are described in [Annex B](#). The methods are simple, direct and practical. It makes them especially suitable for routine inspection and for cross-comparison of the acupuncture needles' clinical applications. They also play a very important role in the enhancement of the quality of the needle tip. The methods to evaluate the puncture performance of the needle tip can be used to further evaluate the puncture and puncture performance of the acupuncture needle. Currently, the more appropriate method is to use the needle tip to pierce through polyurethane material; however, this method has not yet been implemented internationally.

Considering the consistency of standards in the future, this standard provides the methods to evaluate the puncture performance of the needle tip and ranks [5.3.5.2](#) as recommended. The standard does not provide the sharpness index of the piercing through polyurethane material by the needle tip. This index will be added to the standard when it becomes appropriate. To improve product quality, all inspection reports should include the inspection information as well as the results of the performance evaluation.

Since every manufacturer's design, production, and sterilization methods are different, no regulations exist for the materials of the acupuncture needle handle. Still, the needle body and the needle handle of acupuncture needle should have good biocompatibility.

In order to ensure product safety and efficacy, the manufacturer should perform risk analysis and enforce risk management in addition to adhering to the requirements of local rules and regulations, the relevant background data of the medical devices and clinical practice throughout the entire duration of the product's life cycle. ISO 14971 has provided manufacturers a framework for the effective management of hazards associated with the use of medical devices.

In some countries, the requirements proposed here are subject to legal sanctions. Such rules and regulations should take precedence over the standards set forth in this document.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 17218:2014

<https://standards.iteh.ai/catalog/standards/sist/ff2ea673-db69-4871-8322-838776fc598f/iso-17218-2014>

Sterile acupuncture needles for single use

1 Scope

This International Standard specifies the requirements for the sterile acupuncture needles for single use (specialized for filiform needles).

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 6507-1:2005, *Metallic materials — Vickers hardness test — Part 1: Test method*

ISO 10993-1, *Biological evaluation of medical devices — Part 1: Evaluation and testing within a risk management process*

ISO 15223-1, *Medical devices — Symbols to be used with medical device labels, labelling and information to be supplied — Part 1: General requirements*

iTeh STANDARD PREVIEW

3 Terms and definitions (standards.iteh.ai)

For the purposes of this document, the following terms and definitions apply.

3.1 <https://standards.iteh.ai/catalog/standards/sist/ff2ea673-db69-4871-8322-838776fc598f/iso-17218-2014>
body of the needle

part of the acupuncture needle that is inserted into the human body

Note 1 to entry: See [Figure 1](#).

3.2
handle of the needle

part of the acupuncture needle that is not inserted into the human body

Note 1 to entry: See [Figure 1](#).

3.3
tip of the needle

sharp apex at the end of the acupuncture needle body that is inserted into the human body

Note 1 to entry: See [Figure 1](#).

3.4
root of the needle

part of the acupuncture needle that connects the needle body to the needle handle

Note 1 to entry: See [Figure 1](#).

3.5
tail of the needle

end part of the needle handle at the opposite side of the tip of the needle

Note 1 to entry: See [Figure 1](#).

3.6 sterile acupuncture needle
acupuncture needle that has been sterilized

3.7 guide tube
assistant tool in the shape of a slender, long tube into which the needle is placed and used for easy insertion

3.8 hardness of the needle body
measure of resistance of the acupuncture needle body to permanent deformation

3.9 primary package
sealed or closed packaging system that forms a microbial barrier, directly enclosing the acupuncture needle

Note 1 to entry: The primary package is usually the smallest unit package of use and the package that is in direct contact with one or more acupuncture needles.


3.10 secondary package
package containing one or more primary packages for distribution and storage

4 Configuration

iTeh STANDARD PREVIEW
(standards.iteh.ai)

4.1 Acupuncture needle configuration

The configuration of the acupuncture needle and the name of each of its parts are shown in [Figure 1](#).

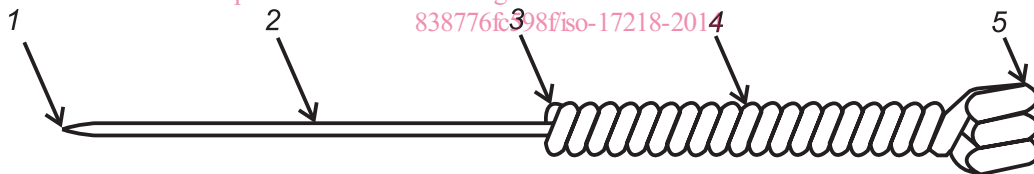

- Key**
- 1 tip of the needle
 - 2 body of the needle
 - 3 root of the needle
 - 4 handle of the needle
 - 5 tail of the needle


Figure 1 — Example of typical structure of acupuncture needle

4.2 Acupuncture needle types

The acupuncture needle includes two types:

- acupuncture needle with a guide tube; and
- acupuncture needle without a guide tube.

The acupuncture needle with guide tube is shown in [Figure 2](#). However, no uniform requirement is provided for the fixing method of the needle tube.

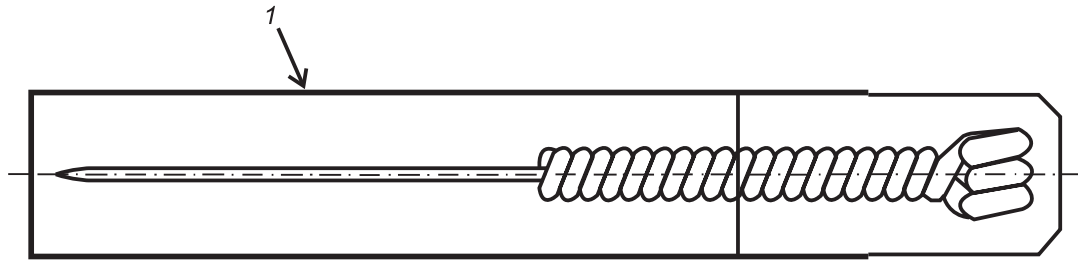**Key**

1 guide tube


Figure 2 — The acupuncture needle with a guide tube**4.3 Types of needle handles**

The types of needle handles include the ring handle, the plain handle, the flower handle, the metal tube handle, and the plastic handle, etc. The types of needle handles are not limited to those shown in the [Figure 3](#).

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[ISO 17218:2014](#)

<https://standards.iteh.ai/catalog/standards/sist/ff2ea673-db69-4871-8322-838776fc598f/iso-17218-2014>

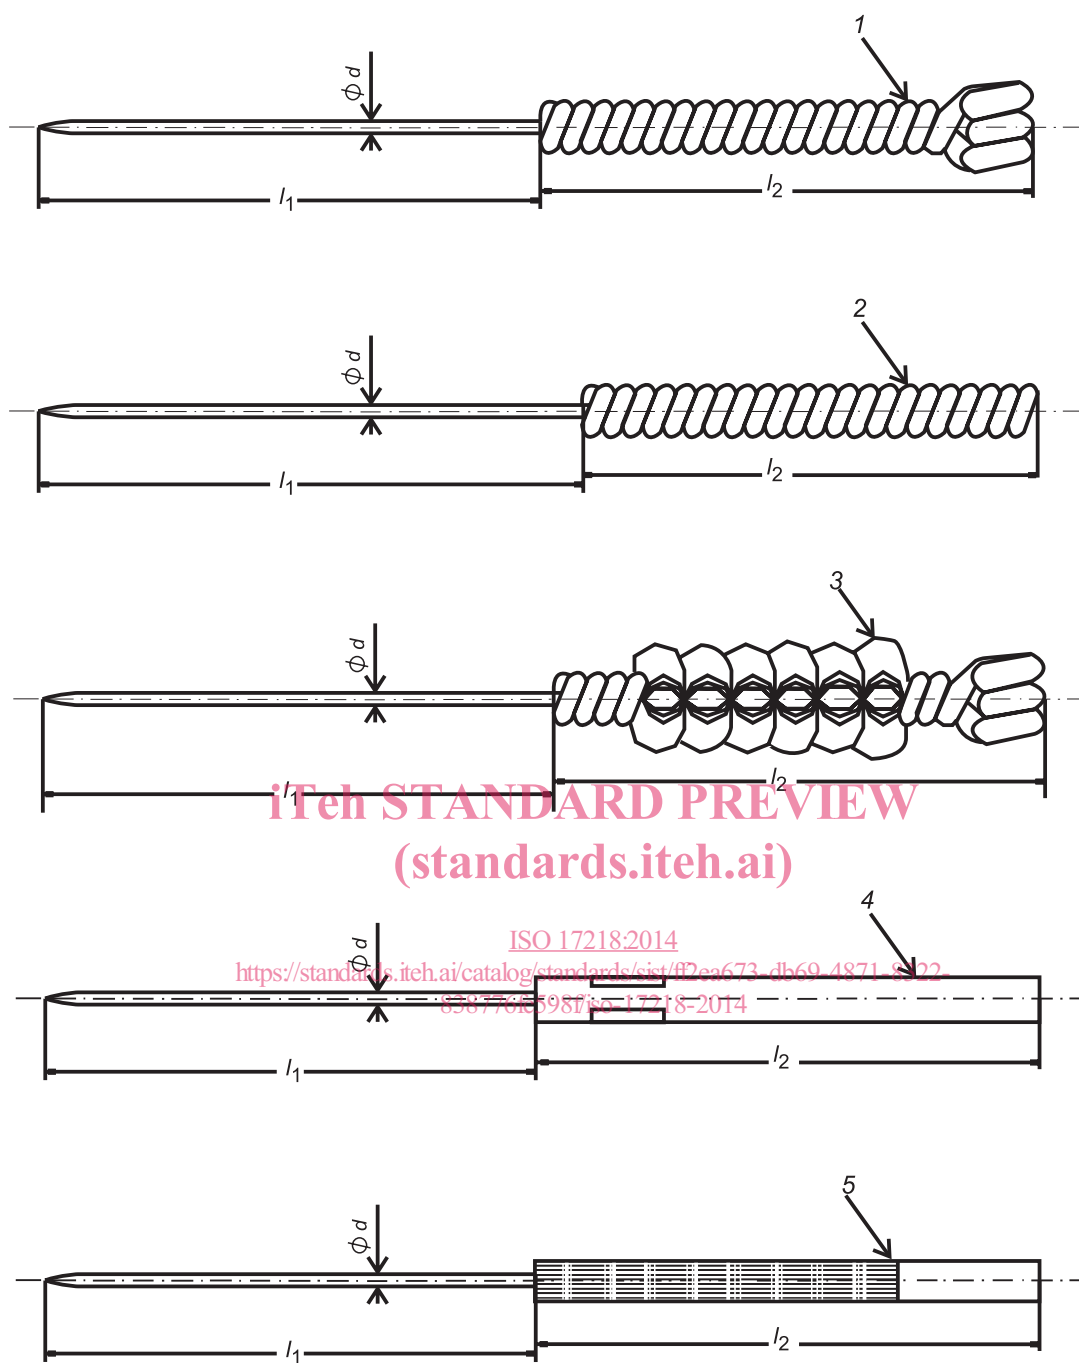

STANDARD PREVIEW
(standards.iteh.ai)

ISO 17218:2014

<https://standards.iteh.ai/catalog/standards/cist/f2ea673-db69-4871-8222-8587761598f/iso-17218-2014>

Key

- | | | | |
|---|-------------------|-----------------|-----------------------------|
| 1 | ring handle | l_1 | length of the needle body |
| 2 | plain handle | l_2 | length of the needle handle |
| 3 | flower handle | $\varnothing d$ | diameter of the needle body |
| 4 | metal tube handle | | |
| 5 | plastic handle | | |

Figure 3 — Example of types of handles of acupuncture needles

5 Requirements

5.1 Materials

The biocompatibility of the body of the needle shall be assessed and documented according to the guidance and principles given in ISO 10993-1.

Compliance is demonstrated by:

- a) analogy with published data; or
- b) the selection of materials already shown to be biocompatible by proven clinical use in a similar application; or
- c) experience with similar devices already on the market together with evidence of traceability to the materials used in the acupuncture needle; or
- d) compliance with published procedures for biological evaluation of:
 - 1) Cytotoxicity;
 - 2) Sensitization;
 - 3) Intracutaneous reactivity;
 - 4) Ethylene oxide sterilization residuals (if using EO. to sterilize).

If the material of the body of the needle is changed and/or if there is a new coating on the surface of the needle body, and if there is risk indicating that these may cause side-effects to the human body, then testing should be in accordance with ISO 10993 series.

NOTE There is no uniform regulation regarding materials of the needle handle and body. Currently, the popularly used material of the needle body is made of X5CrNi18-9, X7CrNi18-9 Austenite Stainless Steel, etc. which are given in ISO 15510:2010.

5.2 Dimensions

5.2.1 Size designation

The size of the acupuncture needle shall be designated by the following:

- a) the nominal diameter of the body of acupuncture needle, expressed in millimetres; and
- b) the nominal length of the body of acupuncture needle, expressed in millimetres.

The size of acupuncture needle shall be referred to as “the designated metric size” and specified as the diameter of the needle body × the length of the needle body.

EXAMPLE $\varnothing 0,30 \times 40$ mm

5.2.2 Tolerance of dimensions

5.2.2.1 Diameter of the needle body

When measured by a micrometer or similar equipment, the nominal diameter of the body of acupuncture needle shall comply with [Table 1](#).

Table 1 — Nominal diameter of needle body

Dimensions in millimetres

Nominal diameter of needle body d	Tolerance
$0,10 \leq d < 0,25$	$\pm 0,008$
$0,25 \leq d \leq 0,45$	$\pm 0,015$
$0,45 < d \leq 0,80$	$\pm 0,020$

5.2.2.2 Length of body of the needle

When measured by vernier calipers or similar equipment, the nominal length of the body of acupuncture needle shall comply with [Table 2](#).

Table 2 — Nominal length of needle body

Dimensions in millimetres

Nominal length of needle body l_1	Tolerance
$5 \leq l_1 \leq 25$	$\pm 0,50$
$25 < l_1 \leq 60$	$\pm 1,00$
$60 < l_1 \leq 100$	$\pm 2,00$
$100 < l_1 \leq 200$	$\pm 3,00$

iteh STANDARD PREVIEW
(standards.iteh.ai)

5.2.3 Dimensions of needle handle

The handle of acupuncture needles shall be of suitable diameter and length for the intended purpose or manipulation.

The length of the handle of acupuncture needles (l_2) shall be no less than 13 mm.

The dimensions of the coiling handle wire used in the manufacturing of ring handles, plain handles and flower handles should comply with [Table 3](#). The diameter of the plastic handle and the metal tube handle should comply with [Table 4](#).

Table 3 — Diameter of the coiling handle wire

Dimensions in millimetres

Nominal diameter of needle body d	Diameter of the coiling handle wire
$0,10 \leq d < 0,20$	0,30
$0,20 \leq d < 0,30$	0,35
$0,30 \leq d < 0,40$	0,40
$0,40 \leq d < 0,50$	0,45
$0,50 \leq d \leq 0,80$	0,50