
**Textiles — Determination of
deodorant property —
Part 4:
Condensation sampling analysis**

*Textiles — Détermination des propriétés du déodorant —
Partie 4: Analyse par condensation d'échantillonnage*

**iTeh STANDARD PREVIEW
(standards.iteh.ai)**

[ISO 17299-4:2015](https://standards.iteh.ai/catalog/standards/sist/ba0b2d09-2722-4ad1-8b1f-93fb6d3622ab/iso-17299-4-2015)

<https://standards.iteh.ai/catalog/standards/sist/ba0b2d09-2722-4ad1-8b1f-93fb6d3622ab/iso-17299-4-2015>



iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 17299-4:2015

<https://standards.iteh.ai/catalog/standards/sist/ba0b2d09-2722-4ad1-8b1f-93fb6d3622ab/iso-17299-4-2015>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2015

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

	Page
Foreword.....	iv
Introduction.....	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	1
5 Reagents	1
6 Apparatus and materials	2
7 Test method	3
7.1 Sampling of test specimen.....	3
7.2 Preparation of container.....	4
7.3 Preparation of odour chemical solution or master gas.....	4
7.4 Testing procedure.....	4
7.4.1 Take three specimens from the sample for one test as shown in Table 1	4
7.5 Measurement of odour gas concentration.....	6
7.5.1 General.....	6
7.6 Testing without specimen.....	6
8 Calibration	6
9 Test result	6
9.1 Calculation of the concentration of the odour chemical.....	6
9.2 Calculation of reduction rate for odour chemical.....	7
10 Test report	7
Annex A (informative) Actual application of the thermal desorption GC-MS to the measurement of indole, isovaleric acid, and nonenal	8
Annex B (informative) Actual application of ion chromatography to the measurement of hydrogen sulfide	15
Annex C (informative) Actual application of ion chromatography to the measurement of methyl mercaptan	19
Annex D (informative) Practical example	22

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT), see the following URL: [Foreword — Supplementary information](#).

The committee responsible for this document is ISO/TC 38, *Textiles*.

ISO 17299 consists of the following parts, under the general title of *Textiles — Determination of deodorant property*

- *Part 1: General principle*
- *Part 2: Detector tube method*
- *Part 3: Gas chromatography method*
- *Part 4: Condensation sampling analysis*
- *Part 5: Metal-oxide semiconductor sensors method*

Introduction

This part of ISO 17299 describes condensation sampling analyses to measure the very low concentration of the odour chemicals which is assumed at the level of human olfactory perception threshold.

iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO 17299-4:2015](https://standards.iteh.ai/catalog/standards/sist/ba0b2d09-2722-4ad1-8b1f-93fb6d3622ab/iso-17299-4-2015)

<https://standards.iteh.ai/catalog/standards/sist/ba0b2d09-2722-4ad1-8b1f-93fb6d3622ab/iso-17299-4-2015>

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 17299-4:2015

<https://standards.iteh.ai/catalog/standards/sist/ba0b2d09-2722-4ad1-8b1f-93fb6d3622ab/iso-17299-4-2015>

Textiles — Determination of deodorant property —

Part 4: Condensation sampling analysis

1 Scope

This part of ISO 17299 specifies a deodorant testing method using analytical instruments after using condensation sampling methods for all textile products. This method is applicable to gaseous odour chemicals, such as indole, methyl mercaptan, hydrogen sulfide, isovaleric acid, and nonenal.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 17299-1, *Textiles — Determination of deodorant property — Part 1: General principle*

iTeh STANDARD PREVIEW

3 Terms and definitions (standards.iteh.ai)

For the purpose of this document, the following terms and definitions apply.

3.1

condensation sampling

method for collecting gaseous odour chemicals at very low concentration levels, which are then condensed by analytical methods to higher concentration levels to facilitate detections of the chemicals

4 Principle

The concentration of a gaseous odour chemical in a container with or without a textile specimen after a designated elapsed time is measured by instrumental devices. The reduction rate of concentration of gaseous odour chemicals is calculated from the difference of average concentration data obtained from the container with specimen and from that without specimen. The test shall be done for each chemical individually.

5 Reagents

Unless otherwise specified, analytical grade reagents are used.

5.1 **Ethanol**, reagent with concentration of 99,5 %.

5.2 **Odour chemicals**.

5.2.1 **Indole (C₈H₇N)**, reagent.

5.2.2 **Methyl mercaptan**, at a certified concentration of 2,0 µl/l ± 3 % in nitrogen diluent.

5.2.3 **Hydrogen sulfide (H₂S)**, at a certified concentration of 2,0 µl/l ± 3 % in nitrogen diluent.

5.2.4 **Isovaleric acid** [(CH₃)₂CHCH₂COOH], reagent with a purity of 98,0 %.

5.2.5 **Nonenal** (C₉H₁₆O), reagent with a concentration of 95,0 % in ethanol solution.

5.3 **Diluent gas**, nitrogen gas from nitrogen gas cylinder with a purity of at least 99,99 %.

6 Apparatus and materials

6.1 **Plastic bags**, with a volume of 3 l, at least six plastic bags for one test (see ISO 17299-1).

6.2 **Micro syringe**, capable of delivering 10 µl of solution by an accuracy of ±0,1 µl.

6.3 **Heat sealer**, used to seal open edge of plastic bag. The adhesive tape can be used as an alternative.

NOTE A sealing attachment such as a linear binder can be used.

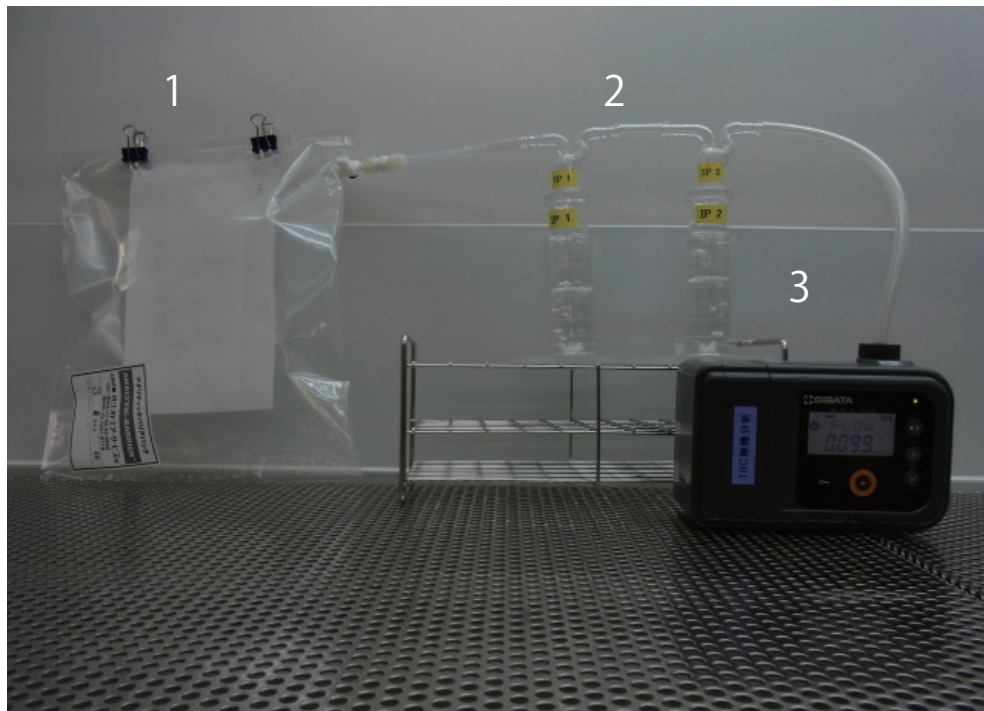
6.4 **Aspirator or vacuum pump**, capable of evacuating remaining air from 3 l sealed plastic bag (refer to [Figure 1](#), item 1).

6.5 **Adsorption tube**, capable of being mounted on a thermal desorption instrument, and absorbing condensed samples of testing chemicals.

6.6 **Thermal desorption instrument**, capable of mounting an adsorption tube and baking it for cleaning at a temperature over 280 °C with flow of inert gas.

6.7 **Impinger**, capable of putting absorbing solution and condensing odour chemical of the gas sample supplied from the plastic bag (refer to [Figure 1](#), item 2).

6.8 **Air pump**, capable of drawing approximately 0,2 l per minute of a sample gas from a plastic bag into adsorption tube, impinger, etc. (refer to [Figure 1](#), item 3).

**Key**

- 1 plastic bag with specimen
- 2 impinger
- 3 air pump

iTech STANDARD PREVIEW
(standards.iteh.ai)

ISO 17299-4:2015
Figure 1 — Sampling set-up
<https://standards.iteh.ai/catalog/standards/sist/ba0b2d09-2722-4ad1-8b1f-93fb6d3622ab/iso-17299-4-2015>

6.9 Thermal desorption gas chromatography (GC) equipment, coupled with a thermal desorption instrument which can be heated up a temperature higher than 280 °C and equipped with a flame photometer detector (FPD), a flame ionization detector (FID), or mass spectrometer (MS).

6.10 Ion chromatography (IC) equipment, to analyse the testing solution of condensed sample in impinger. The detectors used are Conductivity Detector (CD).

7 Test method

7.1 Sampling of test specimen

The dimension or mass of specimen for textile products is shown in [Table 1](#).

Table 1 — Dimension or mass of specimen

Kind	Dimension or mass
Fabrics (woven, knit, non-woven, and tapes)	250 cm ² ± 12,5 cm ²
Yarns, fibres, and feather	2,5 g ± 0,125 g

For multi-layer products, the edge and the untreated layer (or the “not targeted” layer) may be covered with an aluminium sheet or the test specimen may be folded in two with the untreated layers inward, in order to avoid contact of untreated layer with odorous atmosphere.

Condition the specimen as specified in ISO 17299-1.

7.2 Preparation of container

7.2.1 Prepare six plastic bags with the capacity of 3 l, three plastic bags for testing with a specimen and three plastic bags for the control test without a specimen. Place adhesive tape on the plastic bag at the insertion point of the odour chemical.

NOTE The capacity of plastic bag is 3 l for all testing methods.

7.2.2 Clean the plastic bags used in this test using nitrogen gas or clean air, more than five times of taking gas in and out by filling gas of the plastic bag volume just before testing.

7.3 Preparation of odour chemical solution or master gas

Perform the test for each odour chemical independently. Prepare the odour chemical solutions for the testing as indicated below.

7.3.1 Indole solution.

Dissolve 0,6 g of the indole reagent (5.2.1) in 100 ml of ethanol (5.1).

7.3.2 Methyl mercaptan

Prepare the master gas with 1 µl/l of methyl mercaptan concentration by using the standard methyl mercaptan gas (5.2.2) and diluent gas (5.3).

7.3.3 Hydrogen sulfide

Prepare the master gas with 0,2 µl/l of hydrogen sulfide concentration by using the standard hydrogen sulfide gas (5.2.3) and diluent gas (5.3).

7.3.4 Isovaleric acid.

7.3.4.1 Dilute isovaleric acid reagent (5.2.4) of 5 ml and make up to 100 ml by ethanol (5.1).

7.3.4.2 Dilute the diluted solution of 1 ml and make up to 100 ml by ethanol (5.1).

7.3.5 Nonenal.

7.3.5.1 Dilute nonenal reagent (5.2.5) of 3,5 ml and make up to 100 ml by ethanol (5.1).

7.3.5.2 Dilute the diluted solution of 0,6 ml and make up to 100 ml by ethanol (5.1).

Perform the test for each odour chemical separately.

7.4 Testing procedure

This is a test with specimens.

7.4.1 Take three specimens from the sample for one test as shown in [Table 1](#).

7.4.2 Place the specimens in the plastic bag one by one, so as to spread them out as much as possible. See [Figure 2](#).

NOTE Curling and creasing of specimen might be unavoidable.



Figure 2 — Specimen in a plastic bag

7.4.3 Hold the specimen by clips from outside of bag to make easier operation. Then, seal the opened edge of the bag for insertion of specimen by using heat sealer (6.3).

7.4.4 Deaerate from the plastic bag as much as possible by using an aspirator or a vacuum pump (6.4).

7.4.5 Insert 2,5 l of nitrogen gas or the odour testing gas prepared. Then, add the odour testing solution by using micro syringe into the dilution nitrogen gas. The injection needle is stung at the point of the attached adhesive tape. The insertion quantity is indicated in Table 2.

7.4.6 When inserting the solution or gas, be careful not to touch the specimen. After inserting the chemical, close the hole of the needle with adhesive tape.

Table 2 — Insertion quantity of odour testing solution or gas

	Indole	Methyl mercaptan	Hydrogen sulfide	Isovaleric acid	Nonenal
Odour testing solution	2,5 µl	—	—	2,5 µl	2,5 µl
Odour testing gas	-	2,5 l (1 µl/l)	2,5 l (0,2 µl/l)	—	—

7.4.7 Knead the bag 20 times.

7.4.8 Place the plastic bag still for 2 h as a reaction time.

7.4.9 After 2 h have elapsed, knead the bag 20 times.

7.4.10 Connect the outlet of the testing bag to either

- a plug of adsorption tube, or
- an impinger.

7.4.11 Extract 2 l of the testing gas from the plastic bag using the air pump (6.8) at a rate of 0,2 l/min and deliver the testing gas into a condensation sampling device as shown in Table 3.

Lie the testing bag sprawled during delivery of the testing gas.

Table 3 — Testing gas sampling method and amount

	Indole	Methyl mercaptan	Hydrogen sulfide	Isovaleric acid	Nonenal
Gas condensation sampling method	adsorption tube	impinger	impinger	adsorption tube	adsorption tube
Testing gas amount	2,0 l				

If using the activated carbon type adsorption tube, clean the tube by baking prior to testing.

7.5 Measurement of odour gas concentration

7.5.1 General

Mount an adsorption tube after sampling of the odour chemical on a thermal-desorption GC, then measure the gas concentration of the odour chemical. FID, FPD, or MS are available as the detector of GC.

If using methyl mercaptan and hydrogen sulfide, the absorbing solution after sampling by impinger could be measured by an ion chromatography.

ITeH STANDARD PREVIEW

7.6 Testing without specimen (standards.iteh.ai)

This is a control test which is performed following the instructions in 7.4 and 7.5 without a specimen. The number of tests shall be same as that for the testing with specimen, i.e. three.

ISO 17299-4:2015
<https://standards.iteh.ai/catalog/standards/sist/ba0b2d09-2722-4ad1-8b1f-93fb6d3622ab/iso-17299-4-2015>

8 Calibration

Prepare three different concentration gases from the standard solution or master gas.

Measure the standard solutions or gases using either thermal-desorption GC or ion chromatography. Then, plot the peak area data on a graph against the inserted quantity of the odour chemical which is calculated from the concentration. More than three points of concentration are required and the coefficient of correlation shall be higher than 0,99.

9 Test result

9.1 Calculation of the concentration of the odour chemical

The peak area value from a gas chromatography is obtained for testing with or without the specimen.

The absolute amount (ng) of the odour chemical is obtained from the coefficient of the calibration curve, and the concentration of the odour chemical (ng/l) is calculated as follows:

The concentration of the odour chemical (ng/l) is equal to the odour component chemical amount (ng) divided by the sampling gas amount (l).