



Designation: ~~D6239-02~~ Designation: **D 6239 – 03^{€1}**

Standard Test Method for Uranium in Drinking Water by High-Resolution Alpha-Liquid-Scintillation Spectrometry¹

This standard is issued under the fixed designation D 6239; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

^{€1} NOTE—Added research report reference to Section 14 editorially in March 2008.

1. Scope

1.1 This test method covers determining the total soluble uranium activity in drinking water in the range of 0.037 Bq/L (1 pCi/L) or greater by selective solvent extraction and high-resolution alpha-liquid-scintillation spectrometry. The energy resolution obtainable with this technique also allows estimation of the ^{238}U to ^{234}U activity ratio.

1.2 This test method was tested successfully with reagent water and drinking water. It is the user's responsibility to ensure the validity of this test method for waters of untested matrices.

1.3 The values stated in SI units are to be regarded as standard. The values given in parentheses are for information only.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.* For specific hazard statements, see Section 9.

2. Referenced Documents

2.1 *ASTM Standards:*²

D 1129 Terminology Relating to Water

D 1193 Specifications for Reagent Water

D 2777 Practice for Determination of Precision and Bias of Applicable Methods of Committee D19 on Water

D 3370 Practices for Sampling Water from Closed Conduits

D 3648 Practices for the Measurement of Radioactivity

3. Terminology

3.1 *Definitions:*

3.1.1 For definitions of terms used in this test method, refer to Terminology D 1129. For terms not included in this reference, refer to other published glossaries (I)³

4. Summary of Test Method

4.1 This test method is based on solvent extraction technology to isolate and concentrate uranium in drinking water for counting via a high-resolution alpha-liquid-scintillation spectrometer.

4.2 To determine total uranium, as well as limited isotopic uranium (^{238}U and ^{234}U) by activity in drinking water, a 200-mL acidified water sample is first spiked with ^{232}U as an isotopic tracer, boiled briefly to remove radon, and evaporated until less than 50 mL remain. The solution is then made approximately 0.01 M in diethylenetriaminepentaacetic acid (DTPA) and the pH is adjusted to between 2.5 and 3.0. The sample is transferred to a separatory funnel and equilibrated with 1.50 mL of an extractive scintillator containing a dialkyl phosphoric acid extracting agent. Under these conditions only uranium is quantitatively transferred to the organic phase while the extraction of undesired ions is masked by the presence of DTPA. Following phase separation, 1.00 mL of the organic phase is sparged with dry argon gas to remove oxygen, a chemical quench agent, and counted on a high-resolution alpha-liquid-scintillation spectrometer and multichannel analyzer (MCA).

¹ This test method is under the jurisdiction of ASTM Committee D19 on Water and is the direct responsibility of Subcommittee D19.04 on Methods of Radiochemical Analysis.

Current edition approved August 10, 2002. Published September 2002. Originally published as D 6239-98. Last previous edition D 6239-98a.

Current edition approved June 10, 2003. Published August 2003. Originally approved in 1998. Last previous edition approved in 2002 as D 6239-02.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards*, Vol 11.01, volume information, refer to the standard's Document Summary page on the ASTM website.

³ *Annual Book of ASTM Standards*, Vol 11.02.

³ The boldface numbers in parenthesis refer to the list of references at the end of the text.

4.3 The alpha spectrum of a sample that contains natural uranium and that is analyzed with an internal ^{232}U tracer will appear similar to the spectrum in Fig. 1. An approximate resolution of 250 keV FWHM for ^{238}U (4.2 MeV) allows resolution and analysis of the ^{238}U , ^{234}U , and ^{232}U energy spectrum peaks when their activities are of the same order of magnitude. Resolution of the ^{235}U (4.4 MeV) alpha peak is not possible, but its activity, which accounts for approximately 2.2 % of the total natural uranium activity, is included in the total uranium activity calculated when the ^{238}U and ^{234}U peaks are in the region of interest (ROI). When the ^{238}U and ^{234}U peaks are integrated separately, a portion of the ^{235}U activity will be included in the ^{238}U activity and the rest in the ^{234}U activity, depending on the exact ROIs selected. Likewise, if present, ^{236}U and ^{233}U will not be resolved by the spectrometer; however, their activity will be included in the total uranium ROI.

5. Significance and Use

5.1 This test method is a fast, cost-effective method that can yield limited isotopic activity levels for ^{238}U and ^{234}U , as well as total uranium activity. Although ^{232}U is incorporated as a tracer, uranium recoveries for this test measured during the developmental work on this test method were usually between 95 and 105%.

5.2 The high-resolution alpha-liquid-scintillation spectrometer offers a constant 99.6 ± 0.1 % counting efficiency and instrument backgrounds as low as 0.001 counts per minute (cpm) over a 4 to 7 MeV energy range according to McDowell and McDowell (2). Count rates for extractive scintillator blanks and reagent blanks usually range from 0.01 cpm to 0.1 cpm.

6. Interferences

6.1 During the development work on this method, less than 1% of ^{241}Am , ^{238}Pu , ^{210}Po , ^{226}Ra , ^{222}Rn , and ^{230}Th present in the original sample were found to extract under the conditions described for the extraction of uranium by this procedure. Uranium extraction is quantitative at pH values from 1.0 to 5.0 but extraction of ^{230}Th and ^{238}Pu increased slightly at pH values below 2.5 and phase separation was slower and less complete at pH values above 3.5. DTPA concentration is not critical in the range of 0.001 *M* to 0.1 *M* as long as a stoichiometric excess relative to the concentration of interfering ions, especially ferric ion (Fe^{3+}), is maintained. As much as 30 mg of Fe^{3+} did not interfere with the extraction of uranium when the DTPA concentration was 0.010 *M*, and as much as 250 mg of Fe^{3+} did not interfere when the DTPA concentration was increased to 0.10 *M*. As much as 2000 mg of calcium ion (Ca^{2+}) did not present an interference in a 0.010 *M* DTPA solution. Sulfate ion (SO_4^{2-}) did not interfere with the extraction of uranium at concentrations as high as 1 *M*, but hydrogen oxalate (HC_2O_4^-) concentrations greater than 0.001 *M* and dihydrogen phosphate (H_2PO_4^-) concentrations greater than 0.2 *M* resulted in decreased uranium recovery. These concentrations, however, are several orders of magnitude higher than the normal concentration of these ions in drinking water.

6.2 Beta- and gamma-emitting radionuclide interference is minimized (typically 99.95 % rejection of beta/gamma pulses) according to McDowell and McDowell (2) by the pulse-shape discrimination of the high-resolution alpha-liquid-scintillation spectrometer.

6.3 Quenching, often a problem with liquid scintillation counting, is significantly reduced by the use of extractive scintillator technology and will only result in a normally insignificant spectral energy shift with this procedure. No alpha counts will be lost due to quenching.

6.4 ^{234}U and ^{238}U may exist in the ^{232}U tracer. The extent of the positive bias should be determined periodically.

7. Apparatus

7.1 Caps, vinyl or cork for culture tubes.

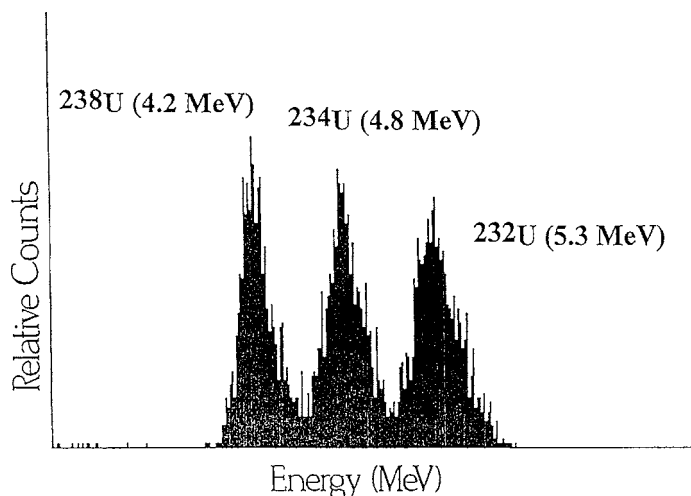


FIG. 1 Alpha Energy Spectrum of Natural Uranium and ^{232}U Tracer Measured on a High-Resolution Alpha-Liquid-Scintillation Spectrometer

- 7.2 *Funnels*, separatory, 125-mL, pear-shaped, polytetrafluoroethylene or polypropylene.
- 7.3 *Meter*, pH, with gel electrode or low leak-rate reference electrode.
- 7.4 *Multichannel Analyzer (MCA)*, 512 channels or more, ADC/memory or better.
- 7.5 *NIM Bin and Power Supply*.
- 7.6 *Power Supply*, high voltage (+1000 volt @ 1 ma), or integral to the spectrometer, see item 7.10.
- 7.7 *Sample*, counting reference, normal uranium.⁴ This counting reference sample is an approximately 50/50 mix of ²³⁸U and ²³⁴U by activity in 1.00 mL of the extractive scintillator solution and enclosed in a 10 by 75 mm glass culture tube and is for standardization purposes only.
- 7.8 *Source*, ¹³⁷Cs, approximately 1.85×10^5 Bq (5 microcuries). This item is for standardization purposes only.
- 7.9 *Sparging Gas Conditioner*⁵—This apparatus provides conditioned argon gas to remove oxygen, a chemical quench agent, from the sample, thus improving pulse shape discrimination and energy resolution. It consists of a specially-made glass tube, partially filled with silicone oil, that serves as a pressure-limiter, a gas drying tower filled with CaSO₄ (6 to 8 mesh) for additional drying of the argon gas, a gas washing bottle containing toluene and molecular sieve to saturate the argon with toluene and prevent sample evaporation while deoxygenating, and plastic tubing of various lengths to serve as connections between the pieces. The inlet from the compressed argon cylinder is connected to one side arm of the pressure limiter; the opposite side arm of the pressure limiter is connected to the inlet (bottom) of the gas drying tower. The outlet (top) of the drying tower is connected to the inlet (dispersion tube) of the gas washing bottle. The outlet of the gas washing bottle is connected to a disposable Pasteur pipet that serves as the sparging lance for the sample. For further information, consult the spectrometer (see 7.10) instruction manual.
- 7.10 *Spectrometer*, high-resolution pulse-shape discriminating alpha-liquid-scintillation spectrometer. Typical performance specifications include greater than 99 % alpha counting efficiency, 99.95 % beta/gamma rejection, energy resolution of 200 to 250 keV FWHM for the 4.78 MeV ²²⁶Ra spectrum peak and instrument backgrounds of 0.001 counts per minute over a 4 to 7 MeV energy range.⁶
- 7.11 *Tubes*, 10 by 75 mm borosilicate glass. These tubes serve as sample-counting cells for the spectrometer (see 7.10).

8. Reagents and Materials

- 8.1 *Purity of Reagents*—Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents shall conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society (3). Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination.
- 8.2 *Purity of Water*— Unless otherwise indicated, references to water shall be understood to mean reagent water conforming to Specification D 1193, Type III, or better.
- 8.3 *Argon Gas, Compressed*—99.999 % pure, with two-stage pressure regulator.
- 8.4 *Ascorbic Acid*— Reagent grade, solid ascorbic acid (C₆H₈O₆).
- 8.5 *Dialkyl Phosphoric Acid Extractive Scintillator*—See Ref (4).⁷
- 8.6 *Diethylenetriaminepentaacetic Acid (DTPA)(0.1 M)*—Add 3.93 g of solid DTPA (C₁₄H₂₃N₃O₁₀) to 50 mL of water. Adjust the pH approximately 7 by the dropwise addition of 6 M sodium hydroxide (NaOH) while stirring to complete dissolution. Dilute to 100 mL with water.
- 8.7 *Hydrochloric Acid (sp gr 1.19)* —Concentrated hydrochloric acid (HCl).
- 8.8 *Molecular Sieve*— Type 4A, activated, indicating, 4-8 mesh (Na₁₂[AlO₂]₁₂(SiO₂)₁₂·xH₂O).
- 8.9 *Nitric Acid (sp gr 1.42)*—Concentrated nitric acid (HNO₃).
- 8.10 *Sodium Hydroxide (6 M)*—Slowly and with cooling add 240 g sodium hydroxide (NaOH) pellets to 500 mL of water and stir to dissolve. Dilute to 1 L with water.
- 8.11 *Toluene*—Reagent grade (C₆H₅CH₃).
- 8.12 *²³²U Solution, Standard* —Nominally 0.04 Bq/mL activity and standardized as per Practice D 3648.

9. Hazards

- 9.1 Use extreme caution when handling all acids and bases. They are extremely corrosive and skin contact could result in severe burns.

⁴ The boldface numbers in parenthesis refer to the list of references at the end of the text.

⁴ The sole source of supply of the ²³⁸U and ²³⁴U normal uranium counting reference sample known to the committee at this time is from ORDELA, Inc., 1009 Alvin Weinberg Drive, Oak Ridge, TN, 37830. If you are aware of alternative suppliers, please provide this information to ASTM Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee that you may attend.

⁵ The sole source of supply of the ²³⁸U and ²³⁴U normal uranium counting reference sample sparging gas conditioner known to the committee at this time is from ORDELA, Inc., 1009 Alvin Weinberg Drive, Oak Ridge, TN, 37830. If you are aware of alternative suppliers, please provide this information to ASTM Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee that you may attend.

⁶ The sole source of supply of the sparging gas conditioner spectrometer known to the committee at this time is ORDELA, Inc., 1009 Alvin Weinberg Drive, Oak Ridge, TN, 37830. If you are aware of alternative suppliers, please provide this information to ASTM Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee that you may attend.

⁷ The sole source of supply of the spectrometer extractive scintillator known to the committee at this time is ORDELA, Inc., 1009 Alvin Weinberg Drive, Oak Ridge, TN, 37830, and may be prepared as in Ref (4). If you are aware of alternative suppliers, please provide this information to ASTM Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee that you may attend.

9.2 When diluting concentrated acids, always use safety glasses and protective clothing, and add the acid to the water.

9.3 Toluene is flammable. Avoid breathing vapors. Use with adequate ventilation and avoid open flames.

10. Sampling

10.1 Collect the sample in accordance with the applicable methods as described in Practice D 3370.

11. Calibration and Standardization

11.1 Use a normal uranium counting reference sample (that consists of an approximate 50/50 mixture of ²³⁸U and ²³⁴U, by activity) to establish an initial region of interest (ROI) on the multichannel analyzer (MCA).

NOTE 1—The actual ROI for any given sample may differ slightly from this initial ROI setting depending on the nature of the sample and the extractive scintillator used. This reference sample may be made using the techniques cited in Burnett and Tai (5). Set the pulse shape discriminator (PSD) of the high-resolution alpha-liquid-scintillation spectrometer prior to counting each individual sample. A 1.85×10^5 Bq (5 microcurie) ¹³⁷Cs gamma source may be used to aid in setting the PSD by quickly inducing a beta/gamma peak (4). For additional information, refer to the instrument instruction manual.

NOTE 2—Setting the pulse shape discriminator (PSD) is a quick, but critical procedure. Inaccurate activity determinations will result if the PSD is set improperly.

11.2 A reagent blank, without tracer, must be made in exactly the same way as the sample determination.

11.3 For general guidance on calibration and standardization, refer to Practice D 3648.

12. Procedure

NOTE 3—This procedure applies to analysis of water samples, whether preserved with HNO₃ or HCl or unpreserved.

12.1 Measure 200 mL of a water sample into a 400-mL borosilicate glass beaker.

12.2 Acidify the sample with 0.5 mL of concentrated nitric acid (HNO₃) and 0.5 mL of concentrated hydrochloric acid (HCl).

12.3 Add an accurately measured activity (depending on the expected uranium activity of the sample) of ²³²U tracer solution.

NOTE 4—It is recommended that the tracer activity corresponds roughly (0.75 to 1.25 times the expected ²³⁴U activity) to the ²³⁴U activity so as to minimize uncertainties in determining the integral peak areas. If the approximate level of uranium activity in the sample is not known it may be estimated by the following simple screening technique: Add 40 mL of the water sample to a 100 mL beaker, boil for 5 min and let cool to room temperature. Then, follow 12.6-12.16. Calculate the ²³⁴U activity (Bq/L) as in 12.18 by integrating the right-hand peak and assuming chemical recovery equals 100 % (recovery/efficiency (R) equals 0.667). Add ²³²U tracer solution to each subsequent 200 mL sample such that the added tracer activity is equal to approximately one-fifth the activity calculated in 12.18. This amount of tracer activity should result in an energy spectrum having ²³⁴U and ²³²U peaks of approximately the same magnitude. Analyzing the sample without tracer will also show any potentially interfering radionuclides in the ²³²U tracer ROI (such as ²¹⁰Po) that may result in a high yield bias and therefore a corresponding low uranium activity analysis.

12.4 Place the beaker on a hot plate, cover with a ribbed watch glass, and heat to boiling. Boil for approximately 5 min to remove radon.

12.5 Reduce the temperature and evaporate until approximately 40 mL of solution remains. Remove from heat and cool to room temperature.

12.6 Make the solution approximately 0.01 M in DTPA by adding 5 mL of 0.1 M DTPA solution.

12.7 Adjust the pH to between 2.5 and 3.0 with 6 M NaOH added dropwise while swirling the beaker. Rinse the pH electrode back into the solution with several milliliters of water.

12.8 Transfer the sample to a 125-mL, pear-shaped, polytetrafluoroethylene or polypropylene separatory funnel. Rinse the beaker twice with 5 to 10 mL of water delivered from a plastic wash bottle and transfer both rinses to the separatory funnel.

12.9 Add 200 mg of ascorbic acid and agitate to dissolve.

12.10 Using a calibrated pipet, add 1.50 mL of dialkyl phosphoric acid extractive scintillator to the separatory funnel and cap tightly. Agitate by inverting about once every second for five minutes.

12.11 Allow the phases to separate for at least 15 to 20 min, or longer if necessary. Proper phase separation is evidenced by two distinct, clear phases; the organic phase will be on top. Discard the aqueous phase.

12.12 Carefully transfer 1.00 mL of the organic phase to a 10 by 75 mm culture tube using a calibrated pipet, ensuring no water is transferred along with the organic.

12.13 Sparge the sample for three minutes with dry, oxygen-free, toluene-saturated argon (at a flow rate of approximately 10 mL/min) supplied by the sparging gas conditioner (see 7.9) using a Pasteur pipet as a sparging lance.

12.14 Cap the tube with a vinyl cap or close the tube with a cork stopper or other suitable device.

12.15 Place the counting cell in a high-resolution alpha-liquid-scintillation spectrometer. Set the instrument to acquire a pulse-shape (time) spectrum and begin acquiring a spectrum on the multichannel analyzer (MCA). Set the pulse-shape discriminator (PSD) three to five channels to the left of the minimum point between the beta/gamma peak (left) and the alpha peak (right) appearing on the MCA display. Especially on low level samples, it is sometimes helpful to use an external gamma source such as ¹³⁷Cs to identify the beta/gamma peak. For very low-level samples, set the PSD a few channels to the right of the beta/gamma peak.

NOTE 5—If the PSD is set too far to the left, the pulse-height spectrum will record beta/gamma pulses resulting in high background values. If the PSD is set too far to the right, some of the alpha pulses will not be recorded in the pulse-height spectrum resulting in low values for sample activity. For additional information refer to the instrument instruction manual.