
**Petroleum and related products —
Determination of the ageing
behaviour of inhibited oils and fluids
using the TOST test —**

Part 3:

**Anhydrous procedure for synthetic
hydraulic fluids**

iTeh STANDARD PREVIEW
(standards.iteh.ai)

*Pétrole et produits connexes — Détermination du comportement au
vieillessement des fluides et huiles inhibés au moyen de l'essai TOST —*

<https://standards.iteh.ai/catalog/standards/sist/ba3176ff-37d0-4336-bbf2-8583acdcada0/iso-4263-3-2015>

Partie 3: Méthode anhydre pour les fluides hydrauliques synthétiques



iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 4263-3:2015

<https://standards.iteh.ai/catalog/standards/sist/ba3176ff-37d0-4336-bfb2-8583acdcada0/iso-4263-3-2015>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2015, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

	Page
Foreword.....	iv
1 Scope.....	1
2 Normative references.....	1
3 Principle.....	1
4 Reagents and materials.....	2
5 Apparatus.....	3
6 Sampling.....	11
7 Preparation of materials and apparatus.....	12
7.1 Cleaning the catalyst wire.....	12
7.2 Preparation of catalyst coil.....	12
7.3 Storage of the catalyst coil.....	12
7.4 Cleaning new glassware.....	12
7.5 Cleaning used glassware.....	12
7.6 Cleaning aliquot-removal device.....	12
8 Procedure.....	13
9 Calculation.....	14
10 Expression of results.....	15
11 Precision.....	15
11.1 General.....	15
11.2 Repeatability, r	15
11.3 Reproducibility, R	16
11.4 Reproducibility with duplicate tests.....	16
12 Test report.....	16
Annex A (normative) Liquid-in-glass thermometer specifications.....	17
Annex B (normative) Procedure for packaging and storage of catalyst coils.....	18
Annex C (informative) Method for the determination of the insolubles content of mineral oils and anhydrous synthetic fluids.....	19
Annex D (informative) Appearance rating of catalyst coil wires.....	22
Annex E (informative) Determination of metals content.....	23
Bibliography.....	24

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](http://standards.iteh.ai)

The committee responsible for this document is ISO/TC 28, *Petroleum products and related products of synthetic or biological origin*.

This third edition cancels and replaces the second edition (ISO 4263-3:2010). The main change is the revision of the calculation in [Clause 9](#) to include calculations for both a test oil reaching a TAN of 2,0 mg KOH per gram and for a test oil reaching an increase of TAN of 2,0 mg KOH per gram. In addition, the inclusion of HETG and exclusion of HFDR from the scope have been adopted.

ISO 4263 consists of the following parts, under the general title *Petroleum and related products — Determination of the ageing behaviour of inhibited oils and fluids using the TOST test*:

- Part 1: Procedure for mineral oils
- Part 2: Procedure for category HFC hydraulic fluids
- Part 3: Anhydrous procedure for synthetic hydraulic fluids
- Part 4: Procedure for industrial gear oils

NOTE As of the date of publication of this part of ISO 4263, the titles of parts 1, 2 and 4 started with *Petroleum and related products – Determination of the ageing behaviour of inhibited oils and fluids — TOST test*.

Petroleum and related products — Determination of the ageing behaviour of inhibited oils and fluids using the TOST test —

Part 3: Anhydrous procedure for synthetic hydraulic fluids

WARNING — The use of this part of ISO 4263 can involve hazardous materials, operations and equipment. This part of ISO 4263 does not purport to address all of the safety problems associated with its use. It is the responsibility of the user of this part of ISO 4263 to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.

1 Scope

This part of ISO 4263 specifies a method for the determination of the ageing behaviour of synthetic hydraulic fluids of categories HFDU, HEES, HEPG and HETG as defined, for example, in ISO 12922[1] and ISO 15380[2]. The ageing is accelerated by the presence of oxygen and metal catalysts at elevated temperature, and the degradation of the fluid is followed by changes in acid number. Other parts of ISO 4263 specify similar procedures for the determination of ageing behaviour of mineral oils and specified categories of fire-resistant fluids used in hydraulic and other applications.

NOTE Other signs of fluid deterioration, such as the formation of insoluble sludge, catalyst coil corrosion or change in viscosity, can occur which indicate oxidation of the fluid, but are not reflected in the calculated oxidation lifetime. The correlation of these occurrences with field service is under investigation. This test method may be used to compare the oxidation stability of fluids that are not prone to contamination with water. However, because of the large number of individual field-service applications, the correlation between the results of this test and actual service performance can vary markedly, and is best judged on experience. The precision of this test method for synthetic hydraulic fluids is not known because interlaboratory data are not available. This method might not be suitable for use in specifications or in the event of disputed results as long as these data are not available.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3170, *Petroleum liquids — Manual sampling*

ISO 3696:1987, *Water for analytical laboratory use — Specification and test methods*

ISO 7537, *Petroleum products — Determination of acid number — Semi-micro colour-indicator titration method*

EN 10130:2007, *Cold rolled low carbon steel flat products for cold forming — Technical delivery conditions*

3 Principle

A test portion is reacted, in the absence of light, at 95 °C with oxygen and a steel and copper catalyst coil. Small aliquots of the fluid are withdrawn at regular intervals and the acid number is measured (see the Note in [Clause 1](#)). The test is continued until either an acid number of 2,0 mg of potassium hydroxide

(KOH) per gram is reached or until an increase of 2,0 mg of potassium hydroxide (KOH) per gram of test portion is reached and the number of hours is recorded as the oxidation lifetime. For some requirements, the test may be discontinued at a fixed number of hours (e.g. 500 h or 1 000 h) when the value of the acid number has still not either reached or increased by 2,0 mg of KOH per gram of test portion.

4 Reagents and materials

4.1 Water, unless otherwise specified, in accordance with the requirements of grade 2 of ISO 3696. Potable water means tap water, unless normal piped supplies are contaminated with particulate or high levels of soluble mineral content.

4.2 Heptane, (C₇H₁₆), of minimum purity 99,75 %.

4.3 Acetone, (CH₃COCH₃), of general purpose reagent grade (GPR).

4.4 Propan-2-ol, (CH₃CHOHCH₃), of general purpose reagent grade (GPR).

4.5 Oxygen, of minimum purity 99,5 %, supplied through a pressure regulation system adequate to maintain the specified flow rate throughout the test duration.

Supply from an oxygen cylinder should be via a two-stage regulation system and a needle valve to improve the consistency of gas-flow regulation.

WARNING — Use oxygen only with equipment validated for oxygen service. Do not allow oil or grease to come into contact with oxygen and clean and inspect all regulators, gauges and control equipment. Check the oxygen-supply system regularly for leaks. If a leak is suspected, turn off immediately and seek qualified assistance. <https://standards.iteh.ai/catalog/standards/sist/ba3176ff-37d0-4336-bfb2-8583acdcada0/iso-4263-3-2015>

4.6 Cleaning solutions.

4.6.1 Strong oxidizing acid solution.

The reference strong oxidizing cleaning solution on which precision was based, is chromosulfuric acid (see the following warning), but alternative non-chromium containing solutions, such as ammonium persulfate in concentrated sulfuric acid (8 g/l), have been found to give satisfactory cleanliness. A 10 % solution of three parts of hydrochloric acid (1 mol/l) and one part of orthophosphoric acid (concentrated GPR grade) removes iron oxide deposits.

WARNING — Chromosulfuric acid is a health hazard. It is toxic, a recognized carcinogen as it contains Cr (VI) compounds, highly corrosive and potentially hazardous in contact with organic materials. When using a chromosulfuric acid cleaning solution, eye protection and protective clothing are essential. Never pipette the cleaning solution by mouth. After use, do not pour cleaning solution down the drain, but neutralize it with great care owing to the concentrated sulfuric acid present, and dispose of it in accordance with standard procedures for toxic laboratory waste (chromium is highly dangerous to the environment).

Strongly oxidizing acid cleaning solutions that are chromium-free are also highly corrosive and potentially hazardous in contact with organic materials, but do not contain chromium which has special disposal problems.

4.6.2 Surfactant cleaning fluid.

A proprietary strong surfactant cleaning fluid is a preferred alternative for example a combination of non-ionic with anionic detergent pH of 9,5 to 11,0.

4.7 Catalyst wires.

4.7.1 Low-metalloid steel wire, of diameter 1,60 mm \pm 0,05 mm, made of low carbon steel to EN 10130 DC04, soft bright annealed and free from rust.

4.7.2 Copper wire, of diameter 1,63 mm \pm 0,05 mm, made of electrolytic copper wire of 99,9 % minimum purity, conforming to EN 13601^[3]. Soft copper wire of an equivalent grade may also be used.

4.8 Abrasive cloth, made of silicon carbide of 150 μ m (100 grit) with cloth backing, or an equivalent grade of abrasive cloth.

4.9 Absorbent cotton.


5 Apparatus

5.1 Oxidation cell, consisting of a large test tube of borosilicate glass. A mushroom condenser and oxygen-delivery tube, also of borosilicate glass, fit into the test tube. The design and dimensions shall be as illustrated in [Figure 1](#). The stages of preparation of the oxygen-delivery tube are illustrated in [Figure 2](#).

5.2 Heating bath, consisting of a thermostatically controlled bath capable of maintaining the hydraulic fluid test portion in the oxidation cell at 95,0 $^{\circ}$ C \pm 0,2 $^{\circ}$ C. It shall be large enough to hold the required number of oxidation cells ([5.1](#)) immersed in the heat transfer medium to a depth of 355 mm \pm 10 mm. It shall be constructed to ensure that light is excluded from the test portions during the test. If a fluid bath is used, it shall be fitted with a suitable stirring system to provide a uniform temperature throughout the bath. If the fluid bath is fitted with a top, the total length of the oxidation cell within the bath shall be 390 mm \pm 10 mm. If a metal-block bath is used, the heaters shall be distributed so as to produce a uniform temperature throughout the bath, and the holes in the block shall have a minimum diameter of 50 mm and a depth, including any insulating cover, of 390 mm \pm 10 mm.

5.3 Flowmeter, capable of measuring 3,0 l/h with an accuracy of \pm 0,1 l/h.

Dimensions in millimetres (unless otherwise indicated)

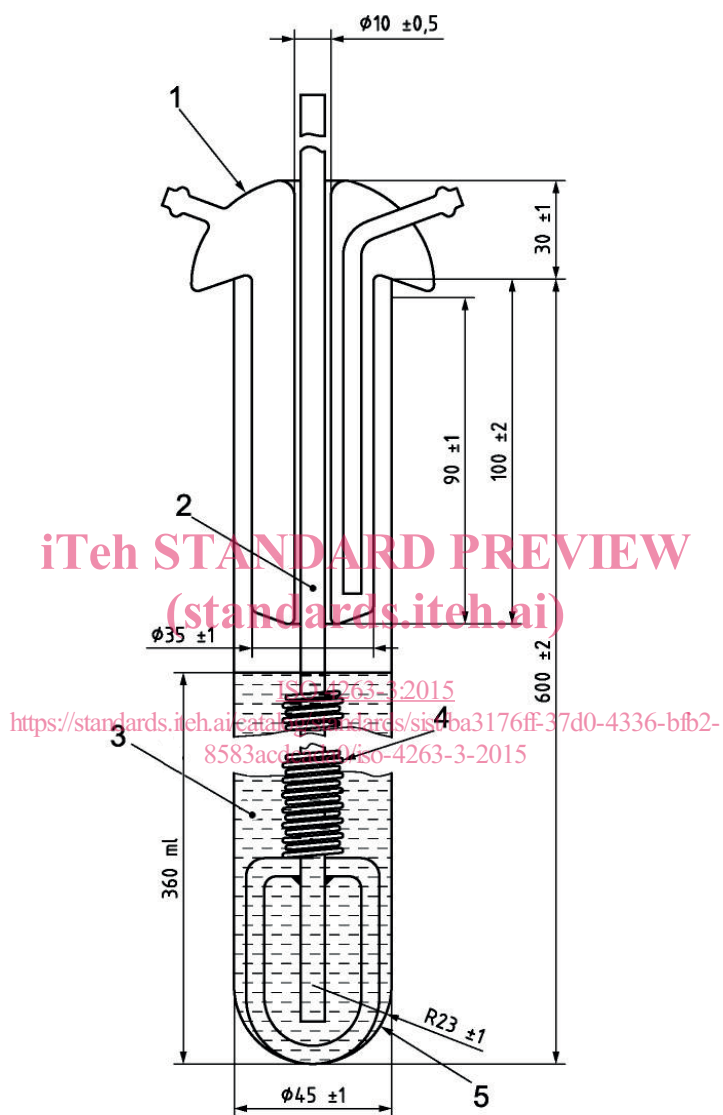


Key


- 1 glass condenser
- 2 oxygen delivery tube
- 3 fluid sample
- 4 catalyst coil
- 5 radius of bottom cell

Figure 1 — Oxidation cell

Dimensions in millimetres

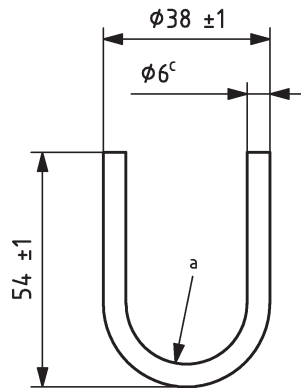


a) First stage — Delivery tube base preparation

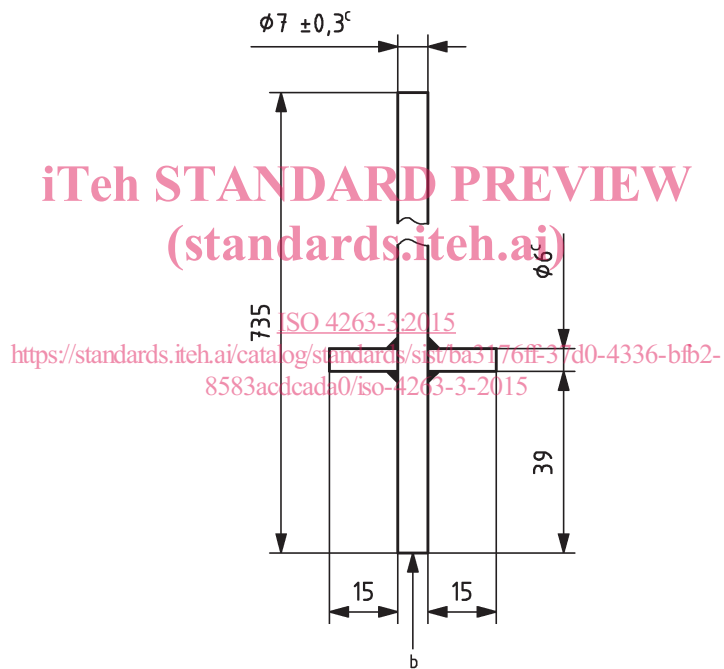

b) Second stage — Delivery tube middle section preparation

Figure 2 — Construction of the oxygen delivery lead-in tube (continued on the next page)

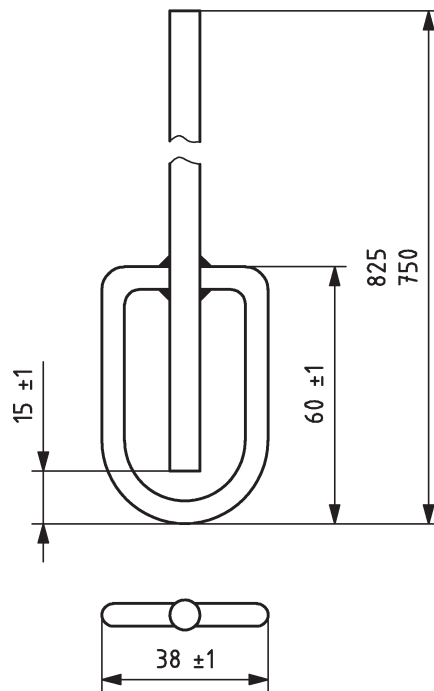

c) Third stage — Delivery tube final assembly

Key

- a Bend over mandrel of diameter 26 mm.
- b Grind end of tube flat.
- c Refers to the outer diameter.

(standards.iteh.ai)

ISO 4263-3:2015

<https://standards.iteh.ai/catalog/standards/sist/ba3176ff-37d0-4336-bfb2-8583acdcada0/iso-4263-3-2015>

Figure 2 — Construction of the oxygen delivery lead-in tube


5.4 Temperature-measurement devices.

5.4.1 Heating bath, the temperature in liquid heating baths shall be measured by either a liquid-in-glass thermometer meeting the requirements of the specification given in [Annex A](#), or an equivalent temperature-measurement system readable to $\pm 0,1$ °C and graduated in 0,1 °C increments. For metal-block heating baths, a temperature-measurement system, with possibly more than one device of the same readability and accuracy, is required.

5.4.2 Oxidation cell, the temperature in the oxidation cell shall be measured by either a liquid-in-glass thermometer meeting the requirements of the specification given in [Annex A](#), or an equivalent temperature-measurement system readable to $\pm 0,1$ °C and calibrated to better than $\pm 0,1$ °C.

5.4.3 Thermometer bracket, if a liquid-in-glass thermometer is used in the oxidation cell, it shall be suspended by means of a bracket as illustrated in [Figure 3](#). The thermometer is held in the bracket by either two fluoro-elastomer O-rings of approximately 5 mm diameter, or by the use of thin, stainless steel wire.

Dimensions in millimetres

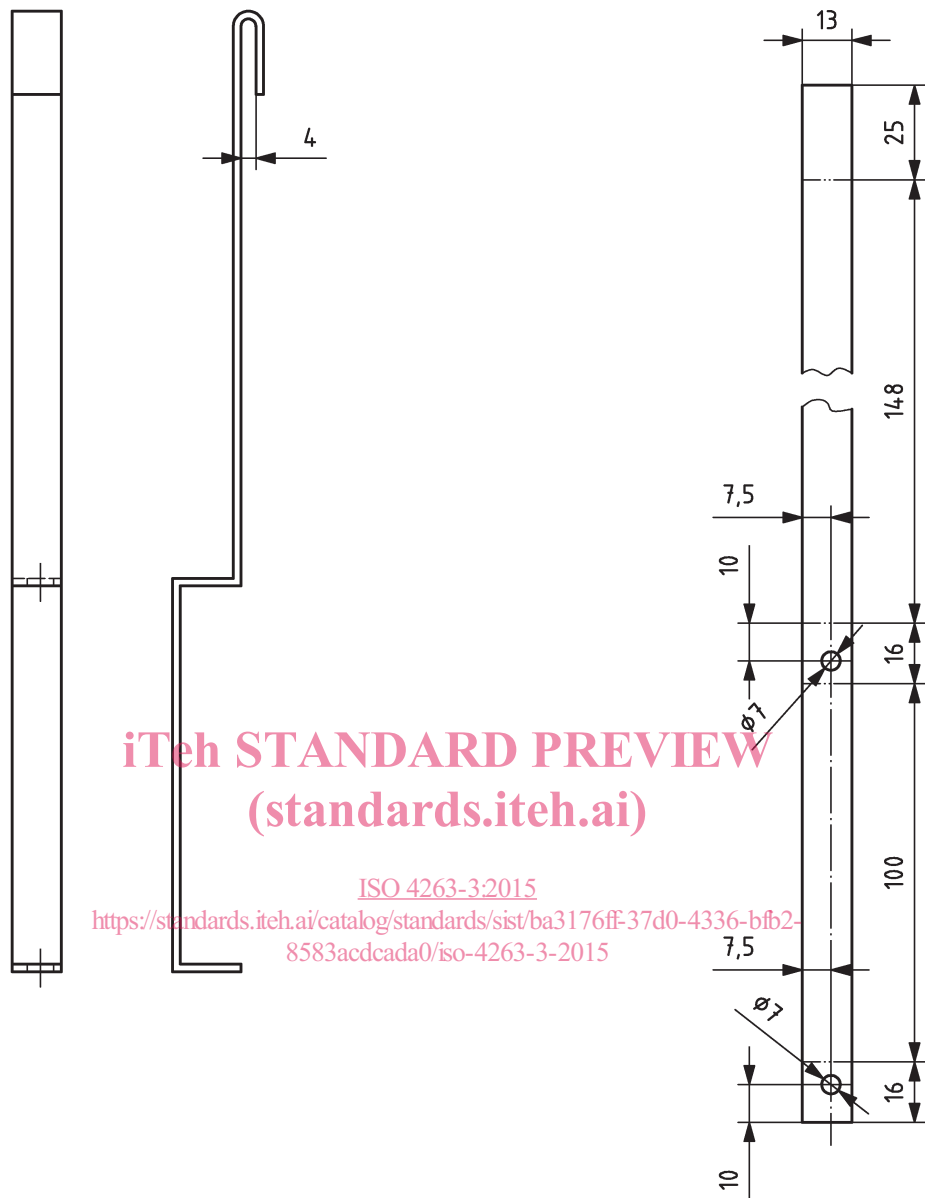

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 4263-3:2015

<https://standards.iteh.ai/catalog/standards/sist/ba3176ff-37d0-4336-bfb2-8583acdcada0/iso-4263-3-2015>

a) Bracket (finished)

b) Development of bracket

Material: Thickness 0,792 mm, stainless steel

Figure 3 — Thermometer bracket

5.5 **Wire-coiling mandrel**, as illustrated in [Figure 4](#), is used to produce the double spiral of copper and steel wire. The mandrel is included in a suitable winding device.

Dimensions in millimetres

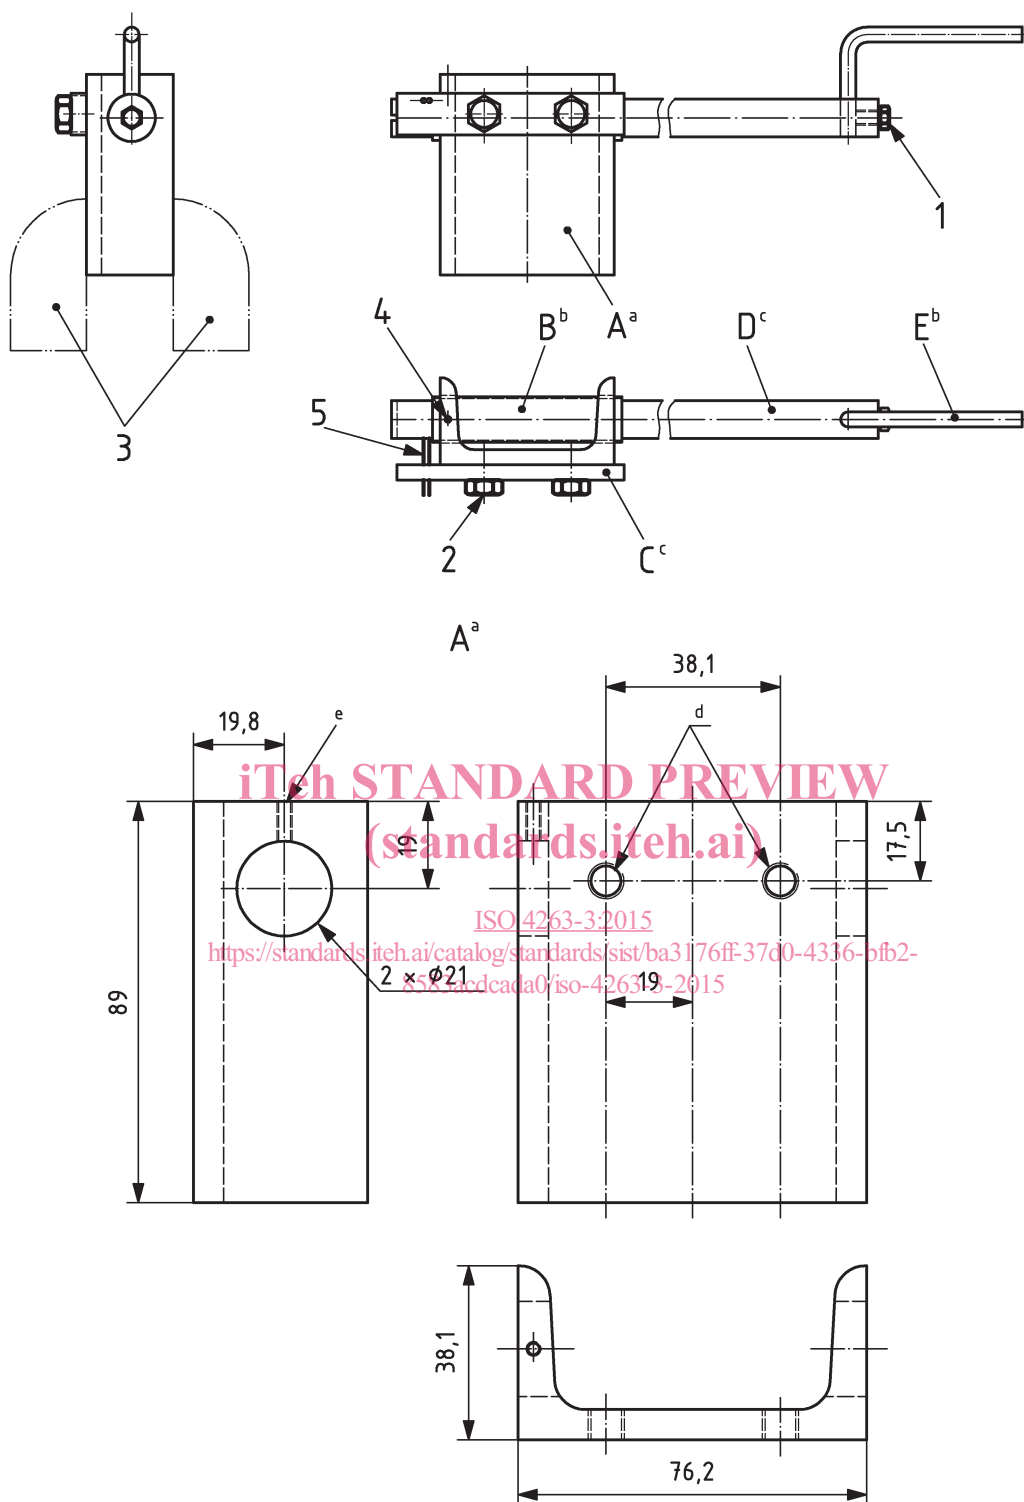


Figure 4 — Catalyst coil mandrel (continued on the next page)

Dimensions in millimetres