



~~Designation: D3908-99~~ Designation: D 3908 – 03 (Reapproved 2008)

~~Standard Test Method for Hydrogen Chemisorption on Supported Platinum on Alumina Catalysts and Catalyst Carriers by Volumetric Vacuum Method~~ Hydrogen Chemisorption on Supported Platinum Catalysts by Volumetric Vacuum Method¹

This standard is issued under the fixed designation D 3908; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method covers the determination of the chemisorption of hydrogen at 298 K (25°C) on supported platinum catalysts that have been reduced in flowing hydrogen at 723 K (450°C). It incorporates a static volumetric vacuum technique at constant volume.

1.2 The test method is intended for use on unused supported platinum on alumina catalysts of loadings greater than 0.3 weight %. Data on other supports and lower platinum loadings were not tested.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*²

D 3766 Terminology Relating to Catalysts and Catalysis

E 177 Practice for Use of the Terms Precision and Bias in ASTM Test Methods

E 456 Terminology Relating to Quality and Statistics

E 691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method

3. Symbols

~~3.1 The following symbols are used: Terminology~~

3.1 *Definitions*—See Terminology D 3766.

3.2 *Quality and Statistics*—See Terminology E 456.

3.3 *Precision and Bias*—See Practice E 177.

3.4 *Symbols*—The following symbols are used:

P_c	= pressure of gas in calibrated bulb, torr
P_{mc}	= pressure of gas in calibrated bulb and manifold, torr
P_m	= pressure in manifold, torr
P_{md}	= pressure in manifold and dead space, torr
P_{m_x}	= pressure in manifold prior to expansion into sample tube for X equilibration point, torr
P_{e_x}	= equilibrium pressure after expansion for generating X equilibrium point, torr
V_c	= volume of calibrated bulb, cm ³
V_m	= volume of manifold between stopcocks 12 and 2 with only 4 and 1 open, cm ³
V_d	= volume of dead space in sample cell containing catalyst (volume between 2 and 3), cm ³
$V_{ads}(STP)_x$	= volume of gas adsorbed at STP, cm ³
$V_{ads}(STP)_{cx}$	= cumulative volume of gas adsorbed through X, cm ³

¹ This test method is under the jurisdiction of ASTM Committee D32 on Catalysts and is the direct responsibility of Subcommittee D32.01 on Physical-Chemical Properties.

Current edition approved April 10, 1999; 1, 2008. Published June 1999; May 2008. Originally published as D3908-80; approved in 1980. Last previous edition D3908-88 (1993)¹ approved in 2003 as D 3908-03.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards*, Vol 14.02, volume information, refer to the standard's Document Summary page on the ASTM website.

V_S	= monolayer volume of gas adsorbed at STP, cm^3
$T_{m_{Ax}}$	= temperature representative of the manifold prior to expansion into the sample cell, K
$T_{m_{Bx}}$	= temperature representative of the entire system after equilibrium pressure (P_e) has been established, K
T_m	= temperature of manifold prior to expansion into sample cell for dead space determination, K
T_{m_D}	= temperature of entire system after equilibrium pressure has been established for dead space determination, K
T	= average manifold temperature for a given dose, K
	= $(T_{m_{Ax}} + T_{m_{Bx}})/2$
W_{cat}	= weight of catalyst, g/mass of catalyst, g
X	= weight percent of platinum
$\%D$	= percent platinum atoms on the surface

4. Significance and Use

4.1 This test method sets forth a procedure by which duplicate catalyst samples can be compared either on an interlaboratory or intralaboratory basis. It is anticipated that catalyst producers and users will find this test method of value.

4.2 Discrimination of the samples for which this procedure is recommended must be exercised when considering carrier (support) materials that adsorb or absorb appreciable quantities of hydrogen or could cause an alteration of the state of the catalyst during pretreatment, or both, (that is, sintering or metal occlusion). These materials must be identified by the user and experimented with to determine the most significant conditions of measurement.

4.3 This test method provides a measure of the total hydrogen uptake ($\text{mL (at standard conditions (STP)) H}_2$ (volume of hydrogen at STP, cm^3/g of catalyst)) without specifying the nature of the hydrogen-platinum interaction. Persons interested in using hydrogen uptake data to calculate percent platinum (dispersion) in a specific catalyst should be aware of carrier (support) interactions, spill-over effects, and other phenomena related to the hydrogen uptake capabilities of the catalyst in question.

5. Apparatus

5.1 *Gas-Handling System* as shown in, as shown in Fig. 1. The components may be either glass or metal. Commercial metal instruments are available. The following components are to be included in the glass system:

5.1.1 *Vacuum System*, capable of attaining pressures below 1 mPa (1×10^{-5} torr). The vacuum can be monitored with any suitable vacuum gage. A diffusion pump backed by a mechanical pump must be isolated from the system by a trap held at liquid nitrogen temperature. High-vacuum stopcocks using a low-vapor pressure grease can be employed.

5.1.2 *Pressure-Measuring Device* that, that operates at constant volume and that is capable of reading in the range from 0 to 66.7 kPa (0 to 500 torr) to the nearest 0.01 kPa (0.1 torr).

5.1.3 *Calibration Bulb*, whose volume has been carefully determined to within 0.1 % prior to attachment to the main manifold. Typically one fills the bulb and stopcock bore with mercury, weighs it, and calculates the volume of the bulb from the density of mercury at the temperature of the measurement. Following careful cleaning, the bulb is attached to the main manifold. One should make sure that the glass blowing is sufficiently far removed from the calibrated volume to avoid distortion.

5.1.4 *Flow-Through Cell* that, that can be evacuated and that can be detached from the main manifold as, for example, see Fig. 2. This is accomplished by including a removeable joint, if glass, a male cone joint, on the manifold end of the tube. (Other types of joints, that is, Swagelok with TFE-fluorocarbon fittings, etc., and so forth, are suitable.) Its mate is attached to the main manifold by a glass vacuum stopcock. A stopcock is also included on the vent side of the cell to allow for vacuum and flow-through procedures.

5.1.5 *Catalyst Sample*, secured by a quartz wool plug upstream of the catalyst and another quartz wool plug downstream (Fig. 2). The sample should be in the form of an extrudate, pellets, or powder greater than 20 mesh.

5.1.6 *Furnace* capable, capable of maintaining a heating rate of 5 deg/min 5 K/min and a temperature-control mechanism capable of maintaining the furnace at temperatures in the range from 673 to 773 ± 10 K (400 to 500°C).

5.1.7 *Thermometer or Thermocouple* to, to monitor the furnace temperature to within ± 5 K and two thermometers to register the temperature of the manifold system and sample cell during uptake determination to the nearest ± 0.1 K.

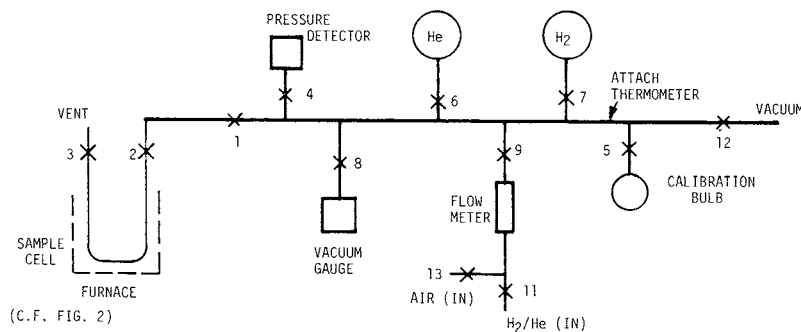


FIG. 1 Schematic: Static Vacuum System

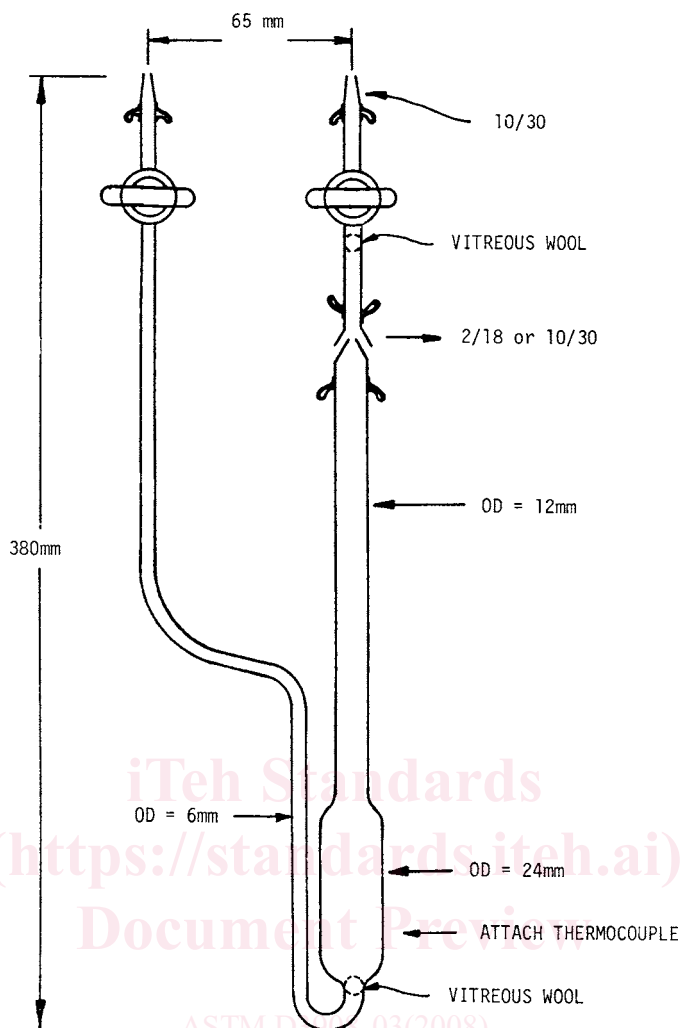


FIG. 2 A Suitable Sample Cell

5.1.8 *Balance*, measuring to the nearest 1 mg (± 0.001 g).

5.1.9 *Flowmeter* for, for hydrogen capable of measuring a flow rate of between 10 and 25 ± 3 cm³ (STP) gas per gram of catalyst per minute.

5.2 *Gas Purification Facilities* for helium and hydrogen, for helium and hydrogen.

6. Reagents

6.1 *High-Purity Helium* purified, purified by passing through a trap containing activated (Note 1) molecular sieve of the A type or 13X type, maintained at liquid nitrogen temperature.

NOTE 1—Activation as suggested by manufacturer.

6.2 *High-Purity Hydrogen* purified, purified by passing first through an oxygen removal catalyst or palladium thimble and then through a trap containing activated molecular sieve of the A type or 13X type maintained at liquid nitrogen temperature.

6.3 *High-Purity Cylinder Air* purified, purified by passing through a trap containing activated molecular sieve of the A series.

7. Safety Hazards

7.1 Follow the usual precautions associated with handling hydrogen gas. Adequately vent the hydrogen flow at the roughing pump discharge and vent the sample (stopcock 3). A flash arresting check valve and pressure relief valves or safety manometers should be incorporated into the design of the apparatus.

7.2 Adequately tape or otherwise shield glass reservoirs to avoid unrestricted explosion in the event of an over-fill and to avoid flying glass in the event of an implosion during evacuation.

7.3 Eye protection is essential when operating the vacuum system.

7.4 Avoid accidental formation of mixtures of hydrogen and air at all times.

8. Volume Calibrations

8.1 The reliability of any gas adsorption measurement is naturally dependent on the accuracy with which the system volume