

---

---

**Rubber — Determination of  
5-ethylidenenorbornene (ENB) or  
dicyclopentadiene (DCPD) in ethylene-  
propylene-diene (EPDM) terpolymers**

*Caoutchouc — Détermination du 5-éthylidènenorbornène (ENB)  
ou du dicyclopentadiène (DCPD) dans les terpolymers d'éthylène-  
propylène-diène (EPDM)*

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

ISO 16565:2013

<https://standards.iteh.ai/catalog/standards/sist/4e3873c5-c93c-4e47-85ff-76200184c6d2/iso-16565-2013>



**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

ISO 16565:2013

<https://standards.iteh.ai/catalog/standards/sist/4e3873c5-c93c-4e47-85ff-76200184c6d2/iso-16565-2013>



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2013

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

	Page
Foreword .....	iv
<b>1 Scope</b> .....	<b>1</b>
<b>2 Principle</b> .....	<b>1</b>
<b>3 Apparatus</b> .....	<b>1</b>
<b>4 Test specimen preparation</b> .....	<b>2</b>
4.1 Primary method .....	2
4.2 Alternative method .....	2
4.3 Alternative method for liquid polymer film preparation .....	2
<b>5 Acquisition of spectra</b> .....	<b>3</b>
5.1 With a specimen shuttle .....	3
5.2 Without a specimen shuttle .....	3
<b>6 Calibration of the spectrophotometer</b> .....	<b>3</b>
<b>7 Diene determination</b> .....	<b>4</b>
7.1 Preparation .....	4
7.2 Single absorbance spectrum .....	4
7.3 Determination of film thickness .....	4
7.4 Determination of diene content .....	4
<b>8 Precision</b> .....	<b>8</b>
<b>9 Test report</b> .....	<b>9</b>
<b>Annex A (normative) Procedure for spectral subtraction of water vapour</b> .....	<b>10</b>
<b>Annex B (informative) Precision and bias</b> .....	<b>12</b>
<b>Bibliography</b> .....	<b>14</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2. [www.iso.org/directives](http://www.iso.org/directives)

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received. [www.iso.org/patents](http://www.iso.org/patents)

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

The committee responsible for this document is ISO/TC 45, *Rubber and rubber products*, Subcommittee SC 2, *Testing and analysis*.

This third edition cancels and replaces the second edition (ISO 16565:2008), of which it constitutes a minor revision. The main changes are: a correction to the Scope concerning the range of termonomer content (either ENB or DCPD) to be determined and the locations of points A and B on [Figure 1](#).

<https://standards.iteh.ai/catalog/standards/sist/4e3873c5-c93c-4e47-85ff-76200184c6d2/iso-16565-2013>

# Rubber — Determination of 5-ethylidenenorbornene (ENB) or dicyclopentadiene (DCPD) in ethylene-propylene-diene (EPDM) terpolymers

**WARNING** — Persons using this International Standard should be familiar with normal laboratory practice. This International Standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this International Standard to establish appropriate safety and health practices and to ensure compliance with any national regulatory conditions.

## 1 Scope

This International Standard specifies the methods to be used to determine the content of 5-ethylidenenorbornene (ENB) or dicyclopentadiene (DCPD) in ethylene-propylene-diene (EPDM) terpolymers in the 0,1 % to 10 % range.

ENB and DCPD are dienes introduced into ethylene-propylene rubbers to generate specific cure properties. Since high precision for diene content determination is important, a Fourier transform infrared spectroscopic (FT-IR) method is utilized.

**NOTE** The procedures for the mass fraction of ENB and the mass fraction of DCPD differ only in the location in the infrared (IR) of the peak being quantified.

## 2 Principle

A test specimen is moulded between two PTFE-coated aluminium or mylar sheets. The ENB content is determined from its infrared absorbance at 1 681  $\text{cm}^{-1}$  to 1 690  $\text{cm}^{-1}$  (a measure of the exocyclic double bond in ENB). The DCPD content is determined from its infrared absorbance at 1 605  $\text{cm}^{-1}$  to 1 610  $\text{cm}^{-1}$  (a measure of the monocyclic double bond in DCPD).

The second derivative of the absorbance is calculated and ratioed to an internal standard. For ENB, the resulting second-derivative peak near 1 690  $\text{cm}^{-1}$  is related to the ENB mass fraction by calibrating the instrument with known EPDM standards. For DCPD, the resulting second-derivative peak near 1 610  $\text{cm}^{-1}$  is related to the DCPD mass fraction in the same way.

For oil-extended polymers, the oil shall be extracted before the diene content is determined.

## 3 Apparatus

**3.1 Carver-type press**, capable of compressing films at 150 °C and 10 MPa.

**3.2 Mould.**

**3.2.1** The mould primarily used is made of a stainless-steel strip 400  $\mu\text{m}$  thick with an opening, which gives a specimen of the appropriate size for the specimen-film holder described in 3.4 (2 cm by 2 cm). The mould shall have approximately the same dimensions as the press platens.

**3.2.2** Alternatively, a thinner mould plate may be used. However, precision can be adversely affected at low diene levels. The precision of the method shall be determined when thinner films are utilized. For example, 127  $\mu\text{m}$ -thick stainless-steel foil with a 15 mm by 35 mm opening may be used for the simultaneous determination of ethylene and diene.

**3.2.3** For liquid EPDMs, a ring washer of 22 mm outer diameter by 16 mm inner diameter and 400 µm-thick is used as a spacer between salt plates (NaBr, NaCl) to set a fixed path length. The spacer is sized to cover only the outer edge of the salt plates.

**3.3 PTFE-coated aluminium moulding sheets**, type A, 36 µm thick, or **silicone release sheeting**.

**3.4 Specimen-film holders:** films may be moulded, cut out and transferred to a film holder. Magnetic-film holders are ideal. Alternatively, a mould sized to fit in the spectrophotometer specimen compartment, with an appropriate-sized opening, may be used to support the film without removal after compressing. A standard salt plate support is used for liquid samples prepared between salt plates.

**3.5 Infrared Fourier transform spectrophotometer**, capable of measuring absorbances in the range of 4 000 cm<sup>-1</sup> to 600 cm<sup>-1</sup> with a transmittance specification (accuracy) of ±1 % T or better. The instrument shall be capable of spectral resolution of 2 cm<sup>-1</sup>. A deuterated triglycine sulfate (DTGS) or, as an alternative, a mercury cadmium telluride (MCT) detector shall be used.

NOTE A specification for the evaluation of the analysis of infrared spectra is given in Reference.<sup>[1]</sup>

The instrument shall be capable of spectral accumulation, averaging and subtracting. Water is the primary source of interference in this method. Methods, physical and electronic, which minimize the moisture level and moisture-level variation are required to obtain the highest precision. The preferred method is to use an instrument equipped with a dry-gas purge and specimen shuttle, which permits alternating and repetitive collection of single-beam specimen and background spectra (see [Clause 5](#)). Alternatively, should a specimen shuttle be unavailable, careful purging of the specimen compartment with dry nitrogen can yield satisfactory results. High precision of calibration-standard data is indicative of adequate purging. When moisture interference is not removed by purging, spectral subtraction of water vapour may be used. A procedure for further development of the method is described in [Annex A](#).

## 4 Test specimen preparation

ISO 16565:2013  
www.iso.org/catalog/standards/sist/4e3873c5-c93c-4e47-85ff-76200184c6d2/iso-16565-2013

### 4.1 Primary method

Place 0,20 g ± 0,05 g of the material to be analysed between two sheets (see [3.3](#)) in the mould (see [3.2.1](#)). Place the mould between the press platens heated to 125 °C ± 5 °C and apply 4 MPa pressure for 60 s ± 10 s.

Should the material be highly viscous, the mould may be heated to 175 °C ± 5 °C.

Cool the material to ambient temperature. Cut out a piece of film of approximately 15 mm by 50 mm. Detach the specimen film from the sheets (see [3.3](#)), and position it on the spectrophotometer specimen compartment window.

### 4.2 Alternative method

When using the thinner mould described in [3.2.2](#), place a small piece (0,04 g to 0,06 g) of the material to be analysed in the mould opening between two sheets (see [3.3](#)) and compress as in [4.1](#). Remove the mould from the press, turn it over and compress it again. Then, remove the mould from the press and allow it to cool to ambient temperature. When cool, carefully remove the sheets (see [3.3](#)), allowing the specimen film to remain attached to the mould.

### 4.3 Alternative method for liquid polymer film preparation

Place a washer (see [3.2.3](#)) on top of a salt plate. Place a small amount (about 0,3 g) of the liquid EPDM polymer to be analysed in the centre of the washer, filling the hole completely. Place a second salt plate on top of the filled washer. Gently place a 1 kg weight on top of the salt plate/washer assembly and allow the weighted assembly to sit for 2 min to 3 min. (For viscous samples, it may be necessary to warm the sample prior to compressing.) Remove the 1 kg weight and, if necessary, allow to cool. Wipe off any excess material that might have been pressed out of the assembly. Hold the assembly up to the light and

inspect for bubbles and/or voids. Should there be imperfections, repeat the preparation with a larger amount of material.

## 5 Acquisition of spectra

### 5.1 With a specimen shuttle

5.1.1 The data-acquisition parameters shall be:

- resolution: 2 cm<sup>-1</sup>;
- scans/scan time: total scan time, split between specimen scans and background scans, about 90 s.

5.1.2 Place the test specimen in the specimen compartment, allow purge to be re-established and, in alternating fashion, collect single-beam specimen and empty specimen compartment spectra. Eight passes of the shuttle shall be made (eight specimen and eight empty-compartment collections), collecting four scans at each position.

5.1.3 Calculate the specimen absorbance spectrum as  $-\log_{10}$  of the ratio of the accumulated single-beam specimen to the empty-compartment spectrum using Formula (1):

$$A = -\log_{10}(P/P_0) \quad (1)$$

**iTeh STANDARD PREVIEW**  
(standards.iteh.ai)

where

$A$  is the absorbance of the specimen at a given wavelength;

$P_0$  is the empty specimen compartment light-beam intensity at that wavelength;

$P$  is the single-beam specimen light-beam intensity at that wavelength.

### 5.2 Without a specimen shuttle

5.2.1 The data-acquisition parameters shall be:

- resolution: 2 cm<sup>-1</sup>;
- scans/scan time: background scans: 32 scans, 120 s total; specimen scans: 32 scans, 120 s total.

5.2.2 Establish a dry atmosphere inside the empty specimen compartment and collect the empty specimen compartment spectra.

5.2.3 Place the test specimen in the specimen compartment and re-establish a dry atmosphere inside the compartment. Collect the single-beam specimen spectra and calculate the specimen absorption spectrum as described in [5.1.3](#).

## 6 Calibration of the spectrophotometer

6.1 Obtain a series of known standards covering the diene content range 0 % to 10 %. Calibration may be based on secondary standards qualified by other laboratories using this method or, more generally, by primary standards whose diene content is well known. Primary standards may be established via use of proton nuclear magnetic resonance (<sup>1</sup>H-NMR), in conjunction with other techniques. The ENB

calibration standards<sup>1)</sup> employed in the development of this method were determined by a combination of refractive index and H-NMR (utilizing samples dissolved in deuterated *o*-dichlorobenzene at 120 °C; the ENB assignment was based exclusively on the exocyclic olefinic protons of ENB). The DCPD standards<sup>1)</sup> were determined by a similar H-NMR technique involving the cyclic olefinic protons of DCPD. The use of four standards at the (copolymer) 2 %, 5 % and 10 % levels is the minimum recommended.

**6.2** Using the procedure in [Clause 5](#), acquire a minimum of five absorbance spectra for each of the calibration standards described in [6.1](#). Several repetitions on separate specimens of each standard may be averaged to improve the accuracy of the calibration.

**6.3** Using the procedure in [Clause 7](#), calculate the ratio of the second-derivative diene peak height to the internal thickness gauge for each of the spectra acquired.

**6.4** Calculate a linear calibration line (diene peak ratio versus assigned values of the standards as mass fraction in per cent of diene) by computing a slope and intercept using standard least-squares linear-regression techniques.

## 7 Diene determination

### 7.1 Preparation

Prepare the specimen film as described in [Clause 4](#).

### 7.2 Single absorbance spectrum

Collect a single absorbance spectrum based on the procedure in [Clause 5](#).

### 7.3 Determination of film thickness

**7.3.1** Normalize the spectrum by bringing the lowest point of the spectrum to zero (that is, determine the minimum absorbance in the spectrum and offset the spectrum to bring the minimum absorbance to zero).

**7.3.2** To determine the film thickness automatically, subtract the absorbance at 2 750 cm<sup>-1</sup> from the absorbance at 2 703 cm<sup>-1</sup>. If the result is positive, the sample belongs to group 1. Otherwise, it belongs to group 2 (see [Figure 1](#)).

**Group 1:** the thickness gauge is the net absorbance difference between 2 708 cm<sup>-1</sup> (isooptic point) and 2 450 cm<sup>-1</sup> (anchor point) (see [Figure 2](#)).

**Group 2:** the thickness gauge is the net absorbance difference between 2 668 cm<sup>-1</sup> (isooptic point) and 2 450 cm<sup>-1</sup> (anchor point) (see [Figure 3](#)).

### 7.4 Determination of diene content

**7.4.1** Normalize the total spectrum to one optical density (OD) unit by multiplying the total spectrum by 1/*A*, where *A* is the net absorbance at thickness gauge.

**7.4.2** Calculate the ENB content, as a mass fraction, in per cent, using Formula (2):

---


1) The ENB standards are supplied by Exxon Chemical Polymer Laboratories (the sole source), P.O. Box 5200, Baytown, TX 77522, USA. DCPD standards are supplied by Uniroyal Chemical Company (the sole source), World Headquarters, Chemical Characterization Laboratory, Benson Road, Middlebury, CT 06749, USA. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of the products/standards named. Equivalent products/standards may be used if they can be shown to lead to the same results.



$$\text{Peak ht} = A_{1\,681} - (0,75A_{1\,688} + 0,25A_{1\,689}) \quad (2)$$

This is subsequently referred to as the ENB peak height. [Figure 4](#) shows a typical second-derivative spectrum for EPDM.


Use the calibration procedure described in [Clause 6](#) to compute a mass fraction of ENB for the sample, using only interpolation (and not extrapolation). If the ENB peak height is lower than the ENB peak height of the lowest, or higher than the ENB peak height of the highest, calibration standard, then report the ENB content as out of range for the calibration standards employed.

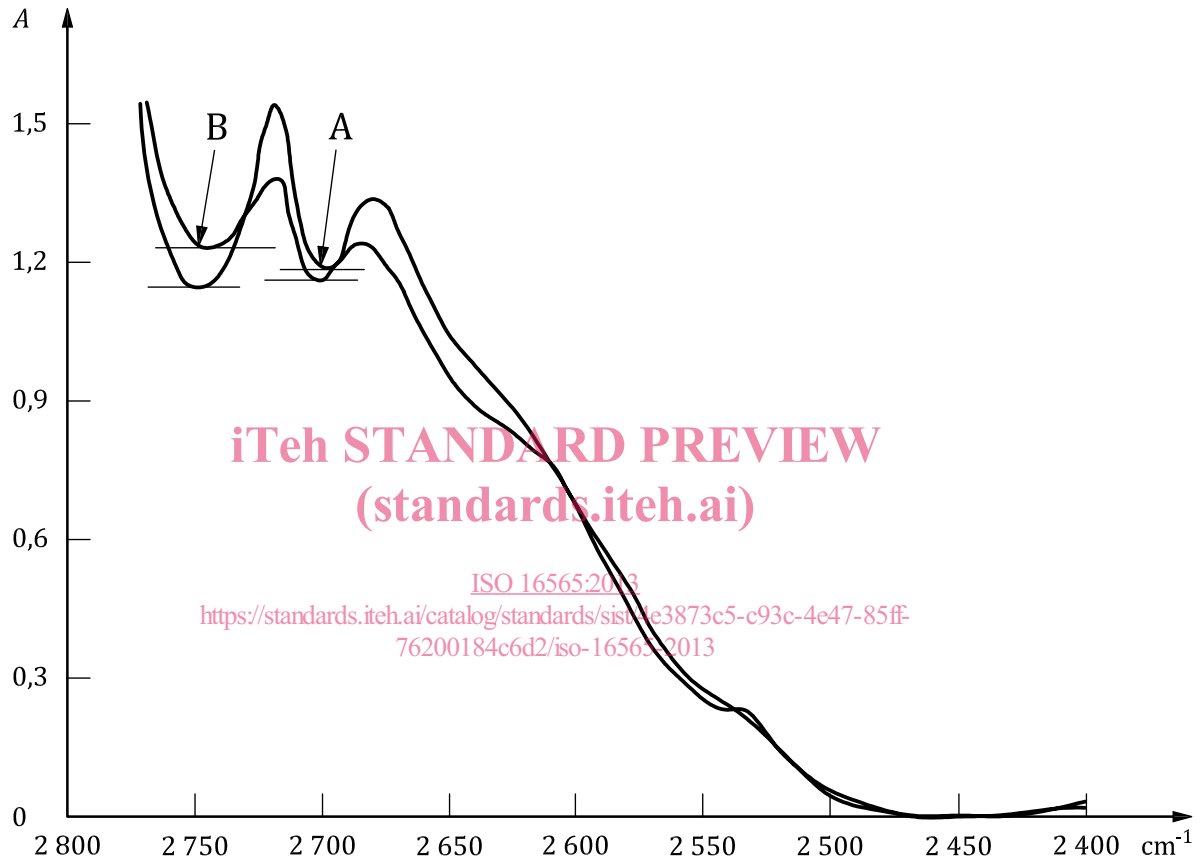


If  $A_{\text{Point A}} - A_{\text{Point B}} > 0$ , the sample belongs to group 1.

If  $A_{\text{Point A}} - A_{\text{Point B}} < 0$ , the sample belongs to group 2.

**Figure 1 — FT-IR thickness gauge — Determination of group**

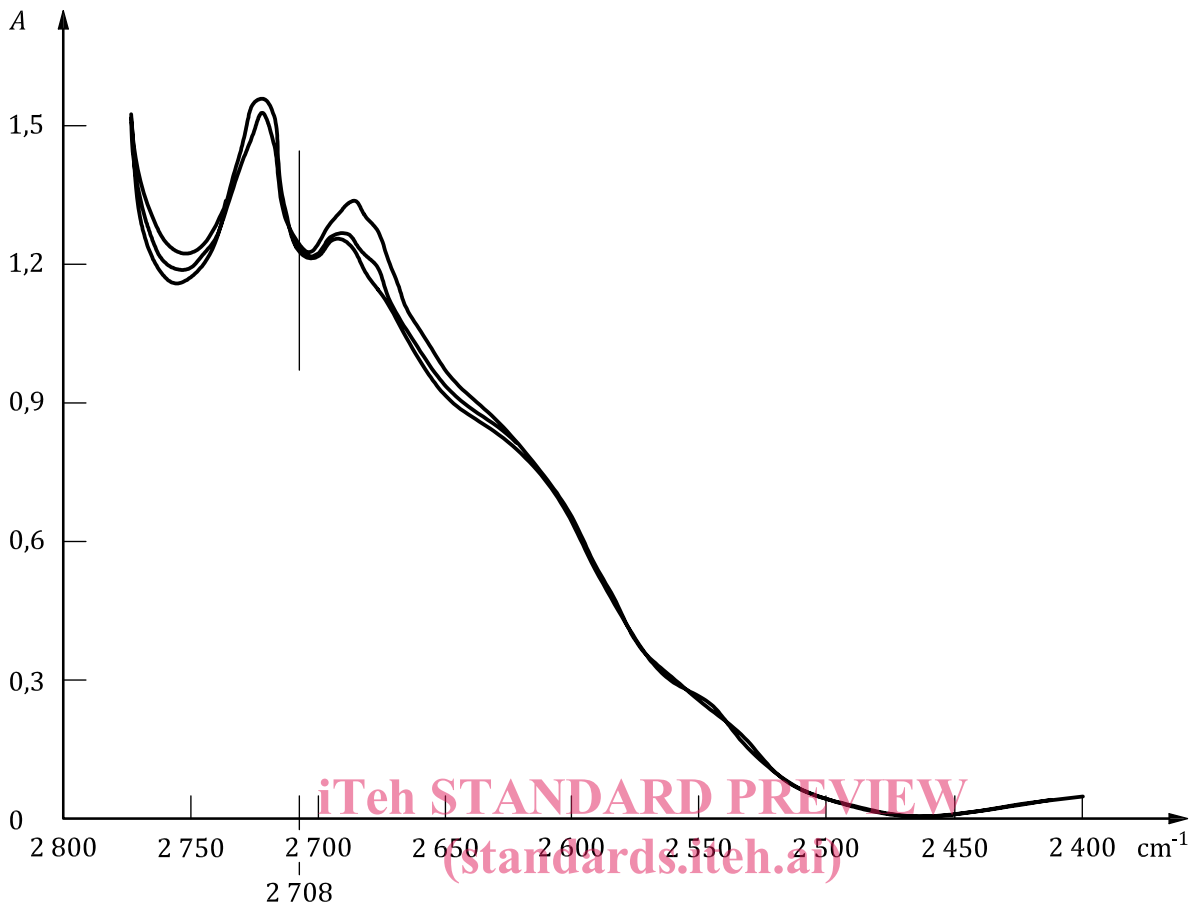

ISO 16565:2013  
**Figure 2 — FT-IR thickness gauge — Group 1**  
<http://standards.iteh.ai/catalog/standards/sist/23675300-2013-0447-85ff-76200184c6d2/iso-16565-2013>

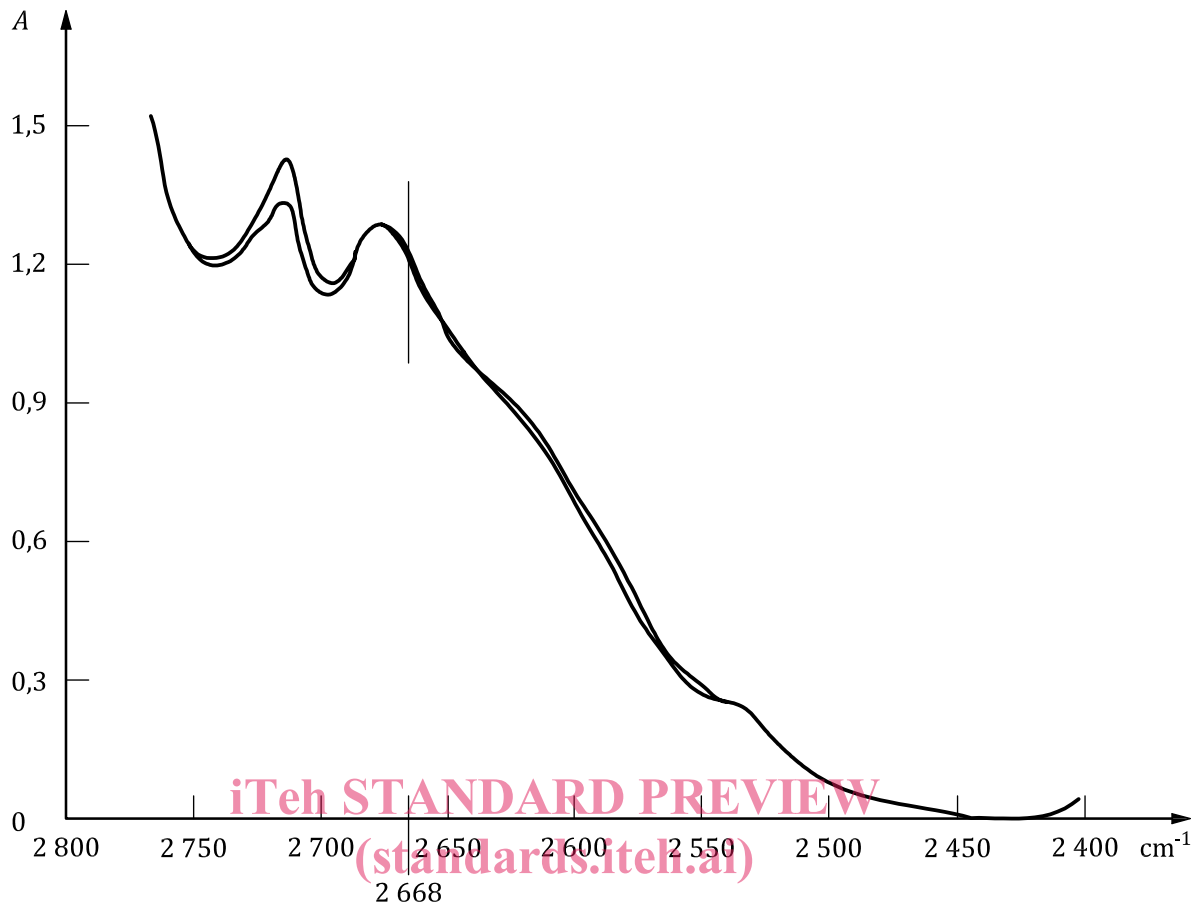

ISO 16565:2013  
**Figure 3 — FT-IR thickness gauge — Group 2**  
<https://standards.iteh.ai/catalog/standards/sist/95c410-0154-76200184c6d2/iso-16565-2013>