
**Copper, lead, zinc and nickel sulfide
concentrates — Determination of
hygroscopic moisture content of the
analysis sample — Gravimetric method**

*Éléments concentrés sulfurés de cuivre, de plomb et de zinc —
Détermination de l'humidité hygroscopique dans l'échantillon pour
analyse — Méthode gravimétrique*

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 9599:2015

<https://standards.iteh.ai/catalog/standards/sist/09cf8945-f557-4544-85f7-1e9127faaba2/iso-9599-2015>



Reference number
ISO 9599:2015(E)

© ISO 2015

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 9599:2015

<https://standards.iteh.ai/catalog/standards/sist/09cf8945-f557-4544-85f7-1e9127faaba2/iso-9599-2015>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2015, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Principle	1
4 Reagents	1
5 Apparatus	1
6 Sampling and samples	2
6.1 General.....	2
6.2 Laboratory sample.....	2
6.3 Preparation of the test sample	2
7 Procedure	2
7.1 Preparation of the weighing vessel.....	2
7.2 Test portion.....	2
7.3 Determination	2
8 Expression of results	3
9 Test report (for internal laboratory use only)	3
Annex A (normative) Method for samples susceptible to oxidation — Drying in nitrogen	4

ITih STANDARD PREVIEW
(standards.itech.ai)

[ISO 9599:2015](https://standards.itech.ai/catalog/standards/sist/09cf8945-f557-4544-85f7-1e9127faaba2/iso-9599-2015)

<https://standards.itech.ai/catalog/standards/sist/09cf8945-f557-4544-85f7-1e9127faaba2/iso-9599-2015>

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#)

ISO 9599 was prepared by Technical Committee ISO/TC 183, *Copper, lead, zinc and nickel ores and concentrates*.

This second edition cancels and replaces the first edition (ISO 9599:1991), which has been technically revised.

Copper, lead, zinc and nickel sulfide concentrates — Determination of hygroscopic moisture content of the analysis sample — Gravimetric method

WARNING — Any chemical-reagent waste must be disposed of in an environmentally sound manner that does not injure the health or welfare of the environment, people, animals, vegetation, etc.

1 Scope

This International Standard specifies a gravimetric loss-in-mass method for the determination of the hygroscopic moisture content in analysis samples of copper, lead, zinc, and nickel sulfide concentrates.

The method is applicable to copper, lead, zinc, and nickel sulfide concentrates free from volatile organic flotation reagents, for example kerosene, and with hygroscopic moisture contents between 0,05 % (m/m) and 2 % (m/m). The hygroscopic moisture content is used to correct the analysis results from the equilibrated moisture level to the dry basis.

NOTE The result of the determination of hygroscopic moisture content using this International Standard should not be reported as part of the analysis of a concentrate sample. Whenever the bulk moisture content of a commercial shipment of concentrate is required, ISO 10251 should be used. The determination of hygroscopic moisture content and the determination of bulk moisture content are connected with each other. In both determinations, the same state of dryness has to be achieved, in order to ascertain the correct metal content of a lot.

This method is not applicable to sulfide concentrates that are susceptible to oxidation (see 6.3, note 2). [Annex A](#) sets out a modified procedure, which can be used for sulfide concentrates that are susceptible to oxidation.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 10251, *Copper, lead, zinc and nickel concentrates — Determination of mass loss of bulk material on drying*

ISO 12743, *Copper, lead, zinc and nickel concentrates — Sampling procedures for determination of metal and moisture content*

3 Principle

Drying of a weighed test portion in air in an oven maintained at $105\text{ °C} \pm 5\text{ °C}$ and calculation of the percentage moisture content from the loss in mass.

4 Reagents

4.1 Desiccant, such as self-indicating silica gel or anhydrous magnesium perchlorate.

5 Apparatus

Ordinary laboratory equipment, and the following.

5.1 Analytical balance, sensitive to 0,1 mg.

5.2 Laboratory oven, capable of maintaining a temperature of $105\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$.

5.3 Weighing vessel, shallow, of glass or silica or corrosion-resistant metal, with an externally fitting air-tight cover of approximately 50 mm diameter.

5.4 Flat dish, or tray.

6 Sampling and samples

6.1 General

Sampling and sample preparation shall be according to ISO 12743.

6.2 Laboratory sample

Use a sample of minus 150 μm particle size.

6.3 Preparation of the test sample

Take a sufficient mass of the laboratory sample for the required chemical analysis and moisture determination and transfer to a flat dish or tray (5.4). Spread the sample evenly into a thin layer about 3 mm to 5 mm thick. Cover the dish to protect the sample from dust, but allowing a free flow of air across the top of the sample. Allow the test sample to equilibrate with the laboratory atmosphere for 2 h or for long enough to achieve equilibration.

Equilibration is achieved whenever the change in mass of the test sample over a 2 h period of exposure is less than 0,1 %.

7 Procedure

7.1 Preparation of the weighing vessel

Dry a weighing vessel and cover (5.3) by heating in the laboratory oven (5.2) at $105\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ for 1 h. Transfer the weighing vessel and cover to a desiccator containing a suitable fresh desiccant (4.1), and allow to cool to ambient temperature. Remove the weighing vessel and cover from the desiccator and weigh to the nearest 0,1 mg (mass m_1), after slightly lifting the weighing vessel cover and quickly replacing it.

7.2 Test portion

Transfer approximately 10 g of the equilibrated test sample (6.2) directly to the dried and tared weighing vessel (7.1), spreading in an even layer about 3 mm to 5 mm thick. Record the mass of the weighing vessel and cover plus test portion to the nearest 0,1 mg (mass m_2). Within the following 5 min, also weigh the test portions required for the determination of constituents for which correction of the analytical values to a dry basis is required and transfer such test portions to the appropriate receptacles required for subsequent testing.

7.3 Determination

Transfer the uncovered weighing vessel containing the test portion and the vessel cover to the laboratory oven (5.2) and dry at $105\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ for 2 h. After the 2 h period, remove the weighing vessel containing the dry test portion from the oven, replace the cover and allow cooling to ambient temperature in the desiccator. Whenever cool, remove the weighing vessel containing the dry test portion and the vessel

cover from the desiccator and reweigh to the nearest 0,1 mg, after slightly lifting the weighing vessel cover and quickly replacing it.

Repeat the drying at $105\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ for another 2 h, cool to ambient temperature in the desiccator and weigh to determine if constant mass ($\pm 1\text{ mg}$) has been achieved. If constant mass has not been achieved, repeat the drying and weighing steps described above. Record the constant mass (m_3).

NOTE If constant mass ($\pm 1\text{ mg}$) is not achieved after three drying periods of 2 h, then the method specified in [Annex A](#) should be used.

8 Expression of results

The hygroscopic moisture content, H , expressed as a percentage by mass, is calculated from the formula

$$H = \frac{m_2 - m_3}{m_2 - m_1} \times 100$$

where

m_1 is the mass, in grams, of the dried weighing vessel plus cover;

m_2 is the mass, in grams, of the weighing vessel plus cover plus test portion before drying;

m_3 is the mass, in grams, of the weighing vessel plus cover plus test portion after drying.

Calculate the hygroscopic moisture content of the sample to the second decimal place.

9 Test report (for internal laboratory use only)

The test report shall contain the following information:

- identification of the sample;
- reference to this International Standard;
- hygroscopic moisture content of the sample;
- date on which the test was carried out.

Annex A (normative)

Method for samples susceptible to oxidation — Drying in nitrogen

A.1 Principle

Drying of a weighed test portion in oxygen-free, dry nitrogen in an oven maintained at $105\text{ °C} \pm 5\text{ °C}$ and calculation of the percentage moisture content from the loss in mass.

A.2 Reagents

A.2.1 Nitrogen, dry gas containing less than 30 µl of oxygen per litre.

A.2.2 Desiccant, such as self-indicating silica gel or anhydrous magnesium perchlorate.

A.3 Apparatus

Ordinary laboratory equipment, and the following.

A.3.1 Analytical balance, sensitive to 0,1 mg.

A.3.2 Minimum-free-space oven, capable of maintaining a temperature of $105\text{ °C} \pm 5\text{ °C}$, with provision for pre-heated nitrogen (A.2.1) to pass through the oven at 15 to 20 oven-volumes per hour. A suitable oven is shown in Figure A.1.

A.3.3 Weighing vessel, shallow, of glass or silica or corrosion-resistant metal, with an externally fitting air-tight cover of approximately 50 mm diameter.

A.3.4 Flowmeter, capable of measuring the rate of flow of nitrogen (A.2.1) through the oven (A.3.2).

A.3.5 Drying tower, of approximately 250 ml capacity, packed with anhydrous magnesium perchlorate (A.2.2) for drying the nitrogen (A.2.1).

A.4 Procedure

A.4.1 Preparation of the weighing vessel

Raise the temperature of the oven (A.3.2) to $105\text{ °C} \pm 5\text{ °C}$ while passing nitrogen (A.2.1) through the oven at the rate of 15 to 20 oven-volumes per hour.

Dry a weighing vessel and cover (A.3.3) by heating in the oven at $105\text{ °C} \pm 5\text{ °C}$ for 1 h. Transfer the weighing vessel and cover to a desiccator containing a suitable fresh desiccant (A.2.2), and allow to cool to ambient temperature. Remove the weighing vessel and cover from the desiccator and weigh to the nearest 0,1 mg (mass m_1), after slightly lifting the weighing vessel cover and quickly replacing it.

Dimensions in millimetres

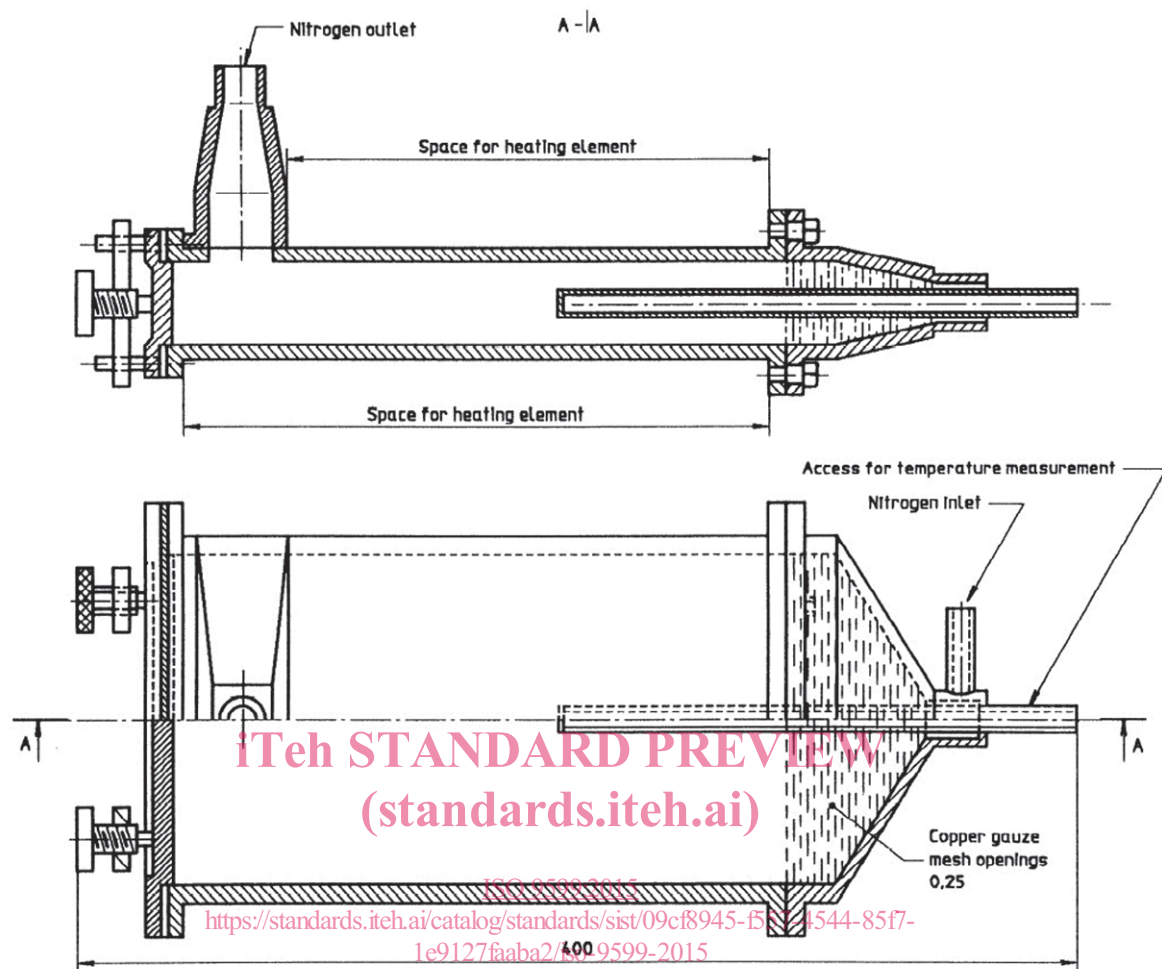


Figure A.1 — Suitable nitrogen oven

A.4.2 Test portion

Transfer approximately 10 g of the equilibrated test sample (5.2) directly into the dried and tared weighing vessel (A.4.1), spreading the sample in an even layer about 3 mm to 5 mm thick. Record the mass of the weighing vessel and cover plus test portion to the nearest 0,1 mg (mass m_2).

A.4.3 Determination

Transfer the uncovered weighing vessel containing the test portion and the vessel cover to the oven (A.3.2) and dry at $105\text{ °C} \pm 5\text{ °C}$ until constant mass ($\pm 1\text{ mg}$) is achieved (see Note).

NOTE Under the conditions described above, drying should be complete in between 1,5 h and 3 h. Constancy in mass ($\pm 1\text{ mg}$) should be established by reheating at $105\text{ °C} \pm 5\text{ °C}$ for a further period of 30 min, followed by cooling and weighing as described.

Remove the weighing vessel containing the dry test portion from the oven, replace the cover and allow cooling to ambient temperature in the desiccator. Whenever cool, remove the weighing vessel containing the test portion and the vessel cover from the desiccator and reweigh to the nearest 0,1 mg (mass m_3), after slightly lifting the weighing vessel cover and quickly replacing it.