



Designation: E526 – 08

# Standard Test Method for Measuring Fast-Neutron Reaction Rates by Radioactivation of Titanium<sup>1</sup>

This standard is issued under the fixed designation E526; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 This test method covers procedures for measuring reaction rates by the activation reactions  $^{46}\text{Ti}(n,p)^{46}\text{Sc} + ^{47}\text{Ti}(n,np)^{46}\text{Sc}$ .

NOTE 1—Since the cross section for the (n,np) reaction is relatively small for energies less than 12 MeV and is not easily distinguished from that of the (n,p) reaction, this test method will refer to the (n,p) reaction only.

1.2 The reaction is useful for measuring neutrons with energies above approximately 4.4 MeV and for irradiation times up to about 250 days (for longer irradiations, see Practice E261).

1.3 With suitable techniques, fission-neutron fluence rates above  $10^9 \text{ cm}^{-2}\cdot\text{s}^{-1}$  can be determined. However, in the presence of a high thermal-neutron fluence rate,  $^{46}\text{Sc}$  depletion should be investigated.

1.4 Detailed procedures for other fast-neutron detectors are referenced in Practice E261.

1.5 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.6 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

## 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

E170 Terminology Relating to Radiation Measurements and Dosimetry

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee E10 on Nuclear Technology and Applications and is the direct responsibility of Subcommittee E10.05 on Nuclear Radiation Metrology.

Current edition approved July 1, 2008. Published September 2008. Originally approved in 1976. Last previous edition approved in 2002 as E526 – 97 (2002). DOI: 10.1520/E0526-08.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

E181 Test Methods for Detector Calibration and Analysis of Radionuclides

E261 Practice for Determining Neutron Fluence, Fluence Rate, and Spectra by Radioactivation Techniques

E262 Test Method for Determining Thermal Neutron Reaction Rates and Thermal Neutron Fluence Rates by Radioactivation Techniques

E844 Guide for Sensor Set Design and Irradiation for Reactor Surveillance, E 706 (IIC)

E944 Guide for Application of Neutron Spectrum Adjustment Methods in Reactor Surveillance, E 706 (IIA)

E1005 Test Method for Application and Analysis of Radiometric Monitors for Reactor Vessel Surveillance, E 706 (IIIA)

E1018 Guide for Application of ASTM Evaluated Cross Section Data File, Matrix E706 (IIB)

## 3. Terminology

3.1 *Definitions:*

3.1.1 Refer to Terminology E170.

## 4. Summary of Test Method

4.1 High-purity titanium is irradiated in a fast-neutron field, thereby producing radioactive  $^{46}\text{Sc}$  from the  $^{46}\text{Ti}(n,p)^{46}\text{Sc}$  activation reaction.

4.2 The gamma rays emitted by the radioactive decay of  $^{46}\text{Sc}$  are counted in accordance with Methods E181 and the reaction rate, as defined by Test Method E261, is calculated from the decay rate and the irradiation conditions.

4.3 The neutron fluence rate above about 4.4 MeV can then be calculated from the spectral-weighted neutron activation cross section as defined by Test Method E261.

## 5. Significance and Use

5.1 Refer to Guide E844 for the selection, irradiation, and quality control of neutron dosimeters.

5.2 Refer to Test Method E261 for a general discussion of the determination of fast-neutron fluence rate with threshold detectors.

5.3 Titanium has good physical strength, is easily fabricated, has excellent corrosion resistance, has a melting temperature of 1675°C, and can be obtained with satisfactory purity.

5.4  $^{46}\text{Sc}$  has a half-life of 83.79 days.<sup>3</sup> The  $^{46}\text{Sc}$  decay<sup>4</sup> emits a 0.8893 MeV gamma 99.984 % of the time and a second gamma with an energy of 1.1205 MeV 99.987 % of the time.

5.5 The isotopic content of natural titanium recommended for  $^{46}\text{Ti}$  is 8.25 %.<sup>3</sup>

5.6 The radioactive products of the neutron reactions  $^{47}\text{Ti}(n,p)^{47}\text{Sc}$  ( $\tau_{1/2} = 3.3492$  d) and  $^{48}\text{Ti}(n,p)^{48}\text{Sc}$  ( $\tau_{1/2} = 43.67$  h), might interfere with the analysis of  $^{46}\text{Sc}$ .

5.7 Contaminant activities (for example,  $^{65}\text{Zn}$  and  $^{182}\text{Ta}$ ) might interfere with the analysis of  $^{46}\text{Sc}$ . See Sections 7.1.2 and 7.1.3 for more details on the  $^{182}\text{Ta}$  and  $^{65}\text{Zn}$  interference.

5.8  $^{46}\text{Ti}$  and  $^{46}\text{Sc}$  have cross sections for thermal neutrons of 0.59 and 8 barns, respectively<sup>5</sup>; therefore, when an irradiation exceeds a thermal-neutron fluence greater than about  $2 \times 10^{21} \text{ cm}^{-2}$ , provisions should be made to either use a thermal-neutron shield to prevent burn-up of  $^{46}\text{Sc}$  or measure the thermal-neutron fluence rate and calculate the burn-up.

5.9 Fig. 1 shows a plot of cross section versus neutron energy for the fast-neutron reactions of titanium which produce  $^{46}\text{Sc}$  [that is,  $^{46}\text{Ti}(n,p)^{46}\text{Sc}$ ]. Included in the plot is the

$^{46}\text{Ti}(n,p)$  reaction<sup>6</sup> and the  $^{47}\text{Ti}(n,np)$  contribution to the  $^{46}\text{Sc}$  production,<sup>7</sup> normalized (at 14.7 MeV)<sup>8</sup> per  $^{46}\text{Ti}$  atom. This figure is for illustrative purposes only to indicate the range of response of the  $^{46}\text{Ti}(n,p)$  reaction. Refer to Guide E1018 for descriptions of recommended tabulated dosimetry cross sections.

## 6. Apparatus

6.1 *Nal(Tl) or High Resolution Gamma-Ray Spectrometer.* Because of its high resolution, the germanium detector is useful when contaminant activities are present. See Methods E181 and E1005.

6.2 *Precision Balance,* able to achieve the required accuracy.

6.3 *Digital Computer,* useful for data analysis (optional).

## 7. Materials

7.1 *Titanium Metal*—High-purity titanium metal in the form of wire or foil is available.

7.1.1 The metal should be tested for impurities by a neutron activation technique. If the measurement is to be made in a thermal-neutron environment, scandium impurity must be low because of the reaction,  $^{45}\text{Sc}(n,\gamma)^{46}\text{Sc}$ . To reduce this interference, the use of a thermal-neutron shield during irradiation would be advisable if scandium impurity is suspected. As an example, when a titanium sample containing 6 ppm scandium has been irradiated in a neutron field with equal thermal and fast-neutron fluence rates about 1 % of the  $^{46}\text{Sc}$  in the sample is due to the reaction  $^{45}\text{Sc}(n,\gamma)^{46}\text{Sc}$ .

7.1.2 Tantalum impurities can also cause a problem. The low-energy response of the  $^{181}\text{Ta}(n,\gamma)^{182}\text{Ta}$  reaction produces gamma activity that interferes with the measurement of  $^{46}\text{Sc}$  radioactivity produced from the  $^{46}\text{Ti}(n,p)^{46}\text{Sc}$  high-energy threshold reaction. The radioactive  $^{182}\text{Ta}$  isotope has a half-life of  $\tau_{1/2} = 114.43$  d and emits a 1121.302 keV photon 34.7 % of the time. This photon is very close in energy to one of the two photons emitted by  $^{46}\text{Sc}$  (889.3 keV and 1120.5 keV). Moreover, during the  $^{46}\text{Sc}$  decay, the 1120.5 keV and 889.3 keV photons are emitted in true coincidence and the random coincidence between the 1121.302 keV photons from  $^{182}\text{Ta}$  and the 889.3 keV photons from  $^{46}\text{Sc}$  can affect the application of summing corrections when the counting is done in a close geometry and the  $^{46}\text{Sc}$  activity is being monitored with 889.3 keV photon.

7.1.3 Zinc contamination can lead to the production of  $^{65}\text{Zn}$  via the  $^{64}\text{Zn}(n,\gamma)^{65}\text{Zn}$  reaction. The radioactive  $^{65}\text{Zn}$  isotope has a half-life of  $\tau_{1/2} = 243.66$  d and emits a 1115.518 keV photon 50.75 % of the time. These 1115.518 keV photons can

<sup>6</sup> "International Reactor Dosimetry File (IRDF-2002)," International Atomic Energy Agency, Nuclear Data Section, Technical Reports Series No. 452, 2006, Document available from URL <http://www-nds.iaea.org/irdf2002/docs/irdf-2002.pdf>.

<sup>7</sup> Zolotarev, K. I., Ignatyuk, A. V., Mahokhin, V. N., Pashchenko, A. B., RRDF-98, Russian Reactor Dosimetry File, Rep. IAEA-NDS-193, Rev. 1, IAEA, Vienna, 2005. URL is <http://www-nds.ipen.br/ndspub/libraries2/rdf98/>

<sup>8</sup> Meadows, J. W., Smith, D. L., Bretscher, M. M., and Cox, S. A., "Measurement of 14.7 MeV Neutron-Activation Cross Sections for Fusion," *Annals of Nuclear Energy*, Vol 1, No. 9, 1987 .

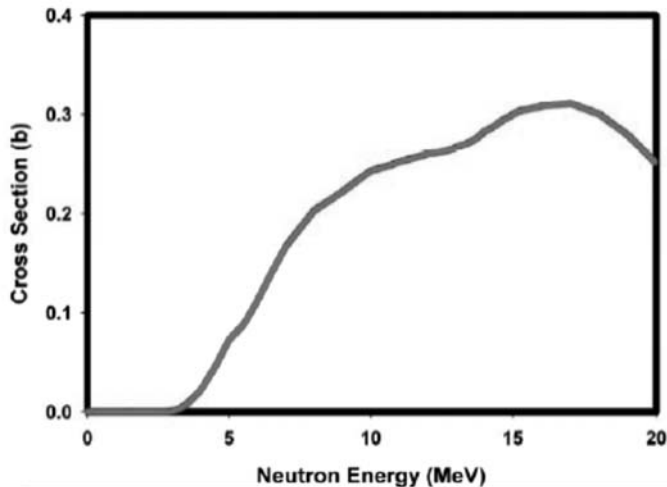


FIG. 1  $^{46}\text{Ti}(n,p)^{46}\text{Sc}$  Cross Section (Normalized per Ti-46 Atom)