

First edition
2018-10

Corrected version
2019-03

Indoor air —

Part 36:

**Standard method for assessing the
reduction rate of culturable airborne
bacteria by air purifiers using a test
chamber**

Air intérieur —

*Partie 36: Méthode normalisée d'évaluation du taux d'abattement
de bactéries cultivables aéroportées par des purificateurs d'air en
utilisant une chambre d'essai*

ISO 16000-36:2018

<https://standards.iteh.ai/catalog/standards/iso/84bef033-15cb-4877-a826-943dbf6ad56a/iso-16000-36-2018>



Reference number
ISO 16000-36:2018(E)

© ISO 2018

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

ISO 16000-36:2018

<https://standards.iteh.ai/catalog/standards/iso/84bef033-15cb-4877-a826-943dbf6ad56a/iso-16000-36-2018>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2018

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Fax: +41 22 749 09 47
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	2
5 Apparatus and materials	2
5.1 Apparatus	2
5.2 Materials	5
5.2.1 Test bacteria	5
5.2.2 Culture media and reagents	5
6 Preparation of the stock cultures and working cultures of the test bacteria	6
6.1 Preparation and maintenance of stock culture	6
6.2 Preparation and maintenance of working cultures of the test bacteria on agar plates	6
6.3 Preparation of working culture suspensions	6
7 Procedures	6
7.1 General	6
7.2 Step 1 — Measurement of the concentration of culturable test bacteria, c_i , without operating the air purifier	7
7.2.1 General	7
7.2.2 Preparation of the air purifier and the test chamber	7
7.2.3 Measurement of bacterial background concentration in the test chamber	7
7.2.4 Nebulizing test bacterial suspension	7
7.2.5 Measurement of the initial concentration of culturable bacteria inside the test chamber after nebulizing	7
7.2.6 Measurement of the concentration of culturable bacteria inside the test chamber after a defined time	8
7.2.7 Post-test actions	8
7.3 Step 2 — Measurement of the concentration of culturable test bacteria, c_t , after operating the air purifier	8
8 Calculation and expression of results	8
8.1 Calculation of the concentration of airborne culturable bacteria	8
8.2 Conditions for a valid test	9
8.3 Reduction rate of bacteria	9
9 Test report	9
10 Quality assurance	10
Annex A (informative) Test chamber	11
Annex B (informative) Natural decay rate according to the operating mode of air purifier	14
Annex C (informative) Homogeneity of airborne culturable bacteria in the test chamber	16
Bibliography	17

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 146, *Air quality*, Subcommittee SC 6, *Indoor air*.

A list of all parts in the ISO 16000 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

This corrected version of ISO 16000-36:2018 incorporates the following corrections:

- In 6.3, the values $1,0 \times 10^3$ to $3,5 \times 10^3$ have been changed to $1,0 \times 10^9$ to $9,0 \times 10^9$;
- In 7.2.5, the values $1,0 \times 10^3$ and $3,2 \times 10^3$ have been changed to $1,0 \times 10^4$ and $3,2 \times 10^4$;
- In 8.2, the values $1,0 \times 10^3$ to $3,2 \times 10^3$ have been changed to $1,0 \times 10^4$ to $3,2 \times 10^4$.

Introduction

An indoor microbial environment is important to the health of occupants, particularly with regard to increased time spent indoors.

Air purifiers are used to reduce the concentration of microorganisms in indoor air.

The efficiency of such air purifiers to reduce airborne microorganisms can be investigated in test chambers at constant temperature and relative air humidity.

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

[ISO 16000-36:2018](https://standards.iteh.ai/catalog/standards/iso/84bef033-15cb-4877-a826-943dbf6ad56a/iso-16000-36-2018)

<https://standards.iteh.ai/catalog/standards/iso/84bef033-15cb-4877-a826-943dbf6ad56a/iso-16000-36-2018>

Indoor air —

Part 36:

Standard method for assessing the reduction rate of culturable airborne bacteria by air purifiers using a test chamber

WARNING — The test given in this document shall be performed by expert staff trained and certified to handle microorganism-related techniques. The test bacterium *Staphylococcus aureus* is a facultative pathogen for human and animals. National and international safety procedures for working with infectious biomaterials shall be followed to prevent any contamination of apparatus, working place or environment. The examination and preparation of the cultures should be carried out in a microbiological safety cabinet class II.

1 Scope

This document specifies a method to evaluate the capacity of air purifiers to reduce the concentration of airborne culturable bacteria.

The test is applicable to air purifiers commonly used in single room spaces.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 16000-9:2006, *Indoor air — Part 9: Determination of the emission of volatile organic compounds from building products and furnishing — Emission test chamber method*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

3.1

air purifier

electrically-powered device that is basically built of a fan and a set of components possessing the ability to capture and/or (partially or totally) destroy air pollutants

3.2

colony forming unit

cfu

unit by which the number of culturable *bacteria* (3.3) is expressed

[SOURCE: EN 13098:2000, modified]

3.3

bacteria

procaryotic, single-celled, microscopic organism with peptidoglycan cell wall

3.4

background concentration

concentration of culturable airborne *bacteria* (3.3) inside the test chamber prior to testing

3.5

natural decay rate

reduction rate of culturable *bacteria* (3.3), which is measured by comparing the concentration of bacteria immediately after nebulizing a bacterial suspension inside the chamber with the concentration counted after a defined time (testing time) without running the *air purifier* (3.1)

Note 1 to entry: Natural decay rate is expressed in per cent.

3.6

bacterial reduction rate

reduction rate of culturable *bacteria* (3.3), which is measured by comparing the concentration of bacteria immediately after nebulizing a bacterial suspension inside the chamber with the concentration counted after a defined running time (testing time) of the *air purifier* (3.1)

Note 1 to entry: Bacterial reduction rate is expressed in per cent.

3.7

impaction

sampling of airborne culturable *bacteria* (3.3) by inertial separation on a solid agar surface

4 Principle

The efficiency of air purifiers is tested using nebulized bacterial suspensions inside a test chamber at constant temperature and relative air humidity. The efficiency is calculated by the reduction rate of culturable airborne bacteria in a defined period of time, considering homogeneity and natural decay rate of the bacteria.

5 Apparatus and materials

5.1 Apparatus

5.1.1 Test chamber.

The chamber shall be made from suitable material, i.e. one that emits minimal pollutant is corrosion proof, such as stainless steel. It shall maintain sufficient airtight capacity.

The volume of the chamber should reflect the later application of the air purifier. The minimum volume shall not be below be 8 m³ and is typically between 15 m³ and 30 m³.


Install a HEPA filter unit for cleaning air by removing particles, an air conditioning unit to control the temperature and humidity, and a system to decontaminate the air inside the test chamber. Particularly for larger test chambers, a fan is needed for homogenous distribution of the bacteria.

The test environment shall be kept clean and free from microbial contamination. It shall have a suitable environmental control system to maintain a constant temperature and humidity. To achieve this, the test chamber should include the following:

- a system capable of removing contamination and maintaining aseptic condition inside the chamber, such as an UV lamp;

- a facility to transfer items into and out of the chamber without cross-contamination (this can include a special system, such as a glove box);
- a facility to control power inside the chamber from outside;
- a facility to generate an aerosol of test bacteria inside the chamber and to ensure its homogeneity (this can be achieved by using a spray inlet through which bacteria are nebulised connected to a spray nozzle in the chamber, with a fan to ensure homogeneous distribution of the bacteria inside the chamber);
- an air conditioning system inside the chamber capable of controlling temperature and relative humidity in a stable and precise manner; the air conditioning system shall be switched off during the test;
- a facility to use negative pressure air flow to flush the chamber post-testing;
- an indicator to display main environmental factors of the test, including flow rate, temperature and relative humidity;
- a filter to prevent contamination from the outside during ventilation.

A test system using a test chamber is shown in [Figure 1](#).

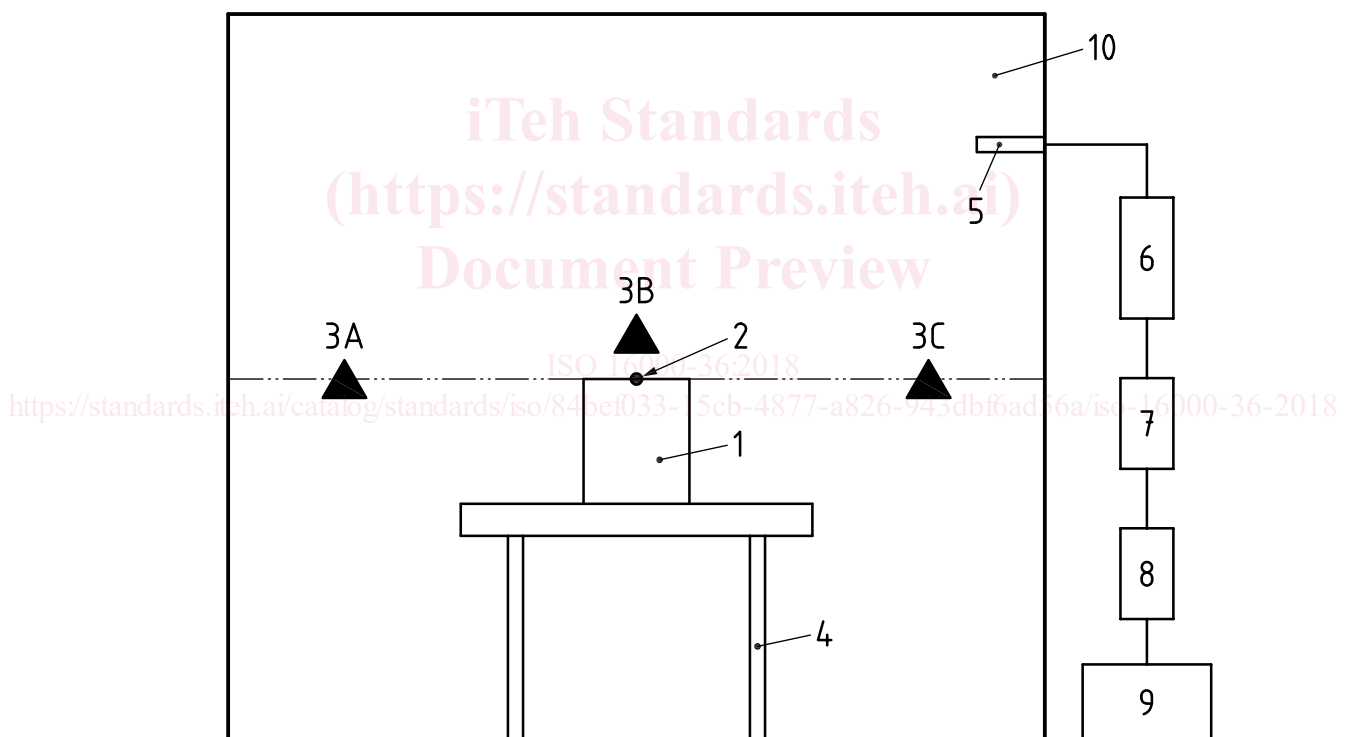

Key

- | | | | |
|---|----------------------------------|----|------------------------------|
| 1 | air purifier | 6 | dehumidifier |
| 2 | air intake of air purifier | 7 | nebulizer |
| 3 | 3A, 3B, 3C position of impactors | 8 | filter (to supply clean air) |
| 4 | stand for the air purifier | 9 | pressure pump |
| 5 | the inlet of spray | 10 | test chamber |

Figure 1 — Schematic diagram of test system using a test chamber

Example photos of a test chamber are given in [Annex A](#).

In accordance with ISO 16000-9:2006, 8.1:

- the test temperature and acceptable range of variation shall be $(23 \pm 2) ^\circ\text{C}$;
- the test humidity and acceptable range of variation shall be $(50 \pm 5) \%$.

In addition, the test may be performed under other conditions. These conditions shall be documented.

After each test, the interior space of the test chamber is decontaminated using an UV lamp, 70 % ethanol (5.1.12) or adopting other decontamination methods in order to prevent contamination after a test.

5.1.2 Nebulizer.

The nebulizer shall be capable of nebulizing culture medium into particles ($0,05 \mu\text{m}$ to $5 \mu\text{m}$) to produce, as far as possible, individual bacterial particles. It typically comprises a pump to generate a defined air pressure to nebulize, a clean air supplying unit and a dehumidifier to remove excess water from the generated culture medium.

5.1.3 Impactor for sampling of bacteria.

The impaction method described in this document is only applicable for relatively low concentrations of culturable bacteria and small chambers, e.g. 8 m^3 .

The initial concentration shall be below the upper detection limit of the sampling method. For impaction with a 300 holes sampler and a sampling volume of 100 l or 50 l, the upper detection limit is approximately $1,6 \times 10^4 \text{ cfu/m}^3$ or approximately $3,2 \times 10^4 \text{ cfu/m}^3$, respectively (299 of 300 possible colonies).

5.1.4 **Stand**, to position the impactor at the sampling height needed.

5.1.5 **Autoclave**, thermostatically controlled at $(121 \pm 3) ^\circ\text{C}$ and a pressure of $(103 \pm 5) \text{ kPa}$.

5.1.6 **Incubator**, thermostatically controlled at $(36 \pm 2) ^\circ\text{C}$.

5.1.7 **Deep freezer**, thermostatically controlled at $(-70 \pm 10) ^\circ\text{C}$.

5.1.8 **Microbiological safety cabinet class II**.

5.1.9 **Balance**, capable of weighing to $\pm 0,01 \text{ g}$.

5.1.10 **Inoculating loop**, 4 mm in ring diameter, sterile.

5.1.11 **Petri dishes**, vented, sterile, 90 mm to 100 mm diameter.

5.1.12 **Disinfectant**, isopropanol or ethanol (70 % volume fraction).

5.1.13 **pH-meter**, capable of measuring to $\pm 0,2$ unit.

5.1.14 **Timer**.