



Designation: ~~D 1429-03~~ Designation: D 1429 - 08

## Standard Test Methods for Specific Gravity of Water and Brine<sup>1</sup>

This standard is issued under the fixed designation D 1429; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

### 1. Scope <sup>\*</sup>

1.1 These test methods cover the determination of the specific gravity of water and brine free of separable oil, as follows:

	Sections
<del>Test Method A—Pycnometer</del>	<del>7 to 11, 21</del>
<del>Test Method A—Pycnometer</del>	<del>7 to 11, 21</del>
<del>Test Method B—Balance</del> <sup>12 to 16, 21</sup>	<del>12 to 16, 21</del>
<del>Test Method B—Balance</del>	<del>12 to 16, 21</del>
Test Method C—Erlenmeyer Flask	17 to 21
Test Method D—Hydrometer	22 to 27

1.2 Test Methods A and B are applicable to clear waters or those containing only a moderate amount of particulate matter. Test Method B is preferred for samples of sea water or brines and is more sensitive than Test Method D which has the same general application. Test Method C is intended for samples of water containing mud or sludge.

1.3 It is the user's responsibility to ensure the validity of these test methods for waters of untested matrices.

1.4 The test method was tested at 22°C over a range, shown in Tables 1-4, of 1.0252 through 1.2299; all data were corrected to 15.6°C (60°F).

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

### 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

D 1066 Practice for Sampling Steam

D 1129 Terminology Relating to Water

D 1193 Specification for Reagent Water

D 2777 Practice for Determination of Precision and Bias of Applicable Test Methods of Committee D19 on Water

D 3370 Practices for Sampling Water from Closed Conduits

D 5847 Practice for Writing Quality Control Specifications for Standard Test Methods for Water Analysis

E 1 Specification for ASTM Liquid-in-Glass Thermometers

### 3. Terminology

3.1 *Definitions:*

3.1.1 *brine*—water that contains dissolved matter at an approximate concentration of more than 30 000 mg/L.

3.1.2 For definitions of terms used in these test methods, refer to Terminology D 1129.

### 4. Significance and Use

4.1 Specific gravity is an important property of fluids being related to density and viscosity. Knowing the specific gravity will allow determination of a fluid's characteristics compared to a standard, usually water, at a specified temperature. This will allow the user to determine if the test fluid will be heavier or lighter than the standard fluid.

### 5. Reagents

5.1 *Purity of Water*— Unless otherwise indicated, reference to water shall be understood to mean reagent water conforming to

<sup>1</sup> These test methods are under the jurisdiction of ASTM Committee D19 on ~~Water~~<sup>Water</sup> and are the direct responsibility of Subcommittee D19.05 on Inorganic Constituents in Water.

Current edition approved Aug. 10, 2003; Nov. 15, 2008. Published September 2003; November 2008. Originally approved in 1956. Last previous edition approved in 1999; 2003 as ~~D 1429-95 (1999)~~; D 1429 - 2003.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* Vol. 11.01, volume information, refer to the standard's Document Summary page on the ASTM website.

\*A Summary of Changes section appears at the end of this standard.

Specification D 1193, Type I. Other reagent water types may be used provided it is first ascertained that the water is of sufficiently high purity to permit its use without adversely affecting the precision and bias of the test method. Type III water was specified at the time of round robin testing of this test method.

**6. Sampling**

- 6.1 Collect the samples in accordance with Practices D 3370 and Practice D 1066.
- 6.2 In view of the lack of a standard test method for sampling mud or sludge, no instructions are given for sampling this type of material.

**TEST METHOD A—PYCNOMETER**

**7. Summary of Test Method**

7.1 The sample is introduced into a pycnometer, stabilized at the desired temperature, and weighed. The specific gravity is calculated from this weight and the previously determined weight of reagent water that is required to fill the pycnometer at the same temperature.


**8. Apparatus**

8.1 *Bath*—Constant-temperature bath designed to maintain a temperature of  $15.6 \pm 1^\circ\text{C}$  ( $60 \pm 1.8^\circ\text{F}$ ). If any other temperature must be used due to local conditions, appropriate corrections shall be made.

8.2 *Pycnometer*—Cylindrical or conical glass vessel carefully ground to receive an accurately fitting 24/12 standard taper glass stopper provided with a hole approximately 1.0 to 2.0 mm in diameter, centrally located in reference to the vertical axis. The top surface of the stopper shall be smooth and substantially plane, and the lower surface shall be concave in order to allow all air to escape through the bore. The height of the concave section shall be approximately 5 mm at the center. The stoppered pycnometer shall have a capacity of about 24 to 30 mL, and shall weigh not more than 40 g. Suitable pycnometers are shown in Fig. 1.

**TABLE 1 Determination of Bias, Pycnometer Method**

Calculated Specific Gravity	Specific Gravity Experimentally Determined	± %Bias	Statistically Significant (95 % Confidence Level)
1.0247	1.0262	-0.049	yes
1.0648	1.0665	+ 0.16	yes
1.1100	1.1119	+ 0.17	yes
1.2299	1.2235	-0.52	yes

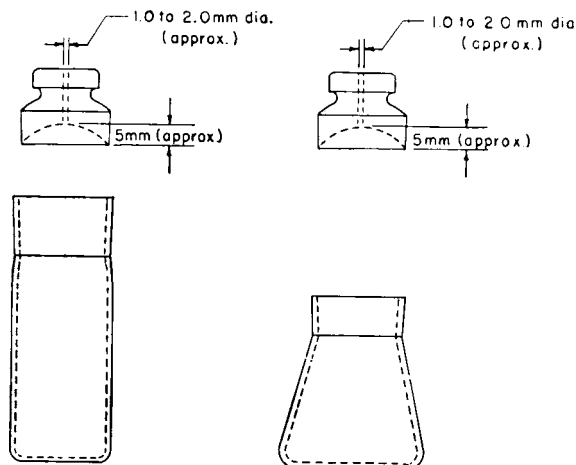

**FIG. 1 Suitable Pycnometers**