



Designation: D189 – 06<sup>ε2</sup>

British Standard 4380



Designation: 13/94

## Standard Test Method for Conradson Carbon Residue of Petroleum Products<sup>1</sup>

This standard is issued under the fixed designation D189; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

*This standard has been approved for use by agencies of the Department of Defense.*

<sup>ε1</sup> NOTE—Removed “asbestos” from 6.4 and reinstated original research report footnote editorially in October 2007.

<sup>ε2</sup> NOTE—Updated Summary of Changes and added to research report footnote editorially in December 2008.

### 1. Scope\*

1.1 This test method covers the determination of the amount of carbon residue (Note 1) left after evaporation and pyrolysis of an oil, and is intended to provide some indication of relative coke-forming propensities. This test method is generally applicable to relatively nonvolatile petroleum products which partially decompose on distillation at atmospheric pressure. Petroleum products containing ash-forming constituents as determined by Test Method D482 or IP Method 4 will have an erroneously high carbon residue, depending upon the amount of ash formed (Note 2 and Note 4).

NOTE 1—The term *carbon residue* is used throughout this test method to designate the carbonaceous residue formed after evaporation and pyrolysis of a petroleum product under the conditions specified in this test method. The residue is not composed entirely of carbon, but is a coke which can be further changed by pyrolysis. The term *carbon residue* is continued in this test method only in deference to its wide common usage.

NOTE 2—Values obtained by this test method are not numerically the same as those obtained by Test Method D524. Approximate correlations have been derived (see Fig. X1.1), but need not apply to all materials which can be tested because the carbon residue test is applied to a wide variety of petroleum products.

NOTE 3—The test results are equivalent to Test Method D4530, (see Fig. X1.2).

NOTE 4—In diesel fuel, the presence of alkyl nitrates such as amyl

nitrate, hexyl nitrate, or octyl nitrate causes a higher residue value than observed in untreated fuel, which can lead to erroneous conclusions as to the coke forming propensity of the fuel. The presence of alkyl nitrate in the fuel can be detected by Test Method D4046.

1.2 The values stated in SI units are to be regarded as the standard. The values given in parentheses are for information only.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

### 2. Referenced Documents

#### 2.1 ASTM Standards:<sup>2</sup>

D482 Test Method for Ash from Petroleum Products

D524 Test Method for Ramsbottom Carbon Residue of Petroleum Products

D4046 Test Method for Alkyl Nitrate in Diesel Fuels by Spectrophotometry

D4057 Practice for Manual Sampling of Petroleum and Petroleum Products

D4175 Terminology Relating to Petroleum, Petroleum Products, and Lubricants

D4177 Practice for Automatic Sampling of Petroleum and Petroleum Products

D4530 Test Method for Determination of Carbon Residue (Micro Method)

E1 Specification for ASTM Liquid-in-Glass Thermometers

E133 Specification for Distillation Equipment

### 3. Terminology

#### 3.1 Definitions:

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

\*A Summary of Changes section appears at the end of this standard.

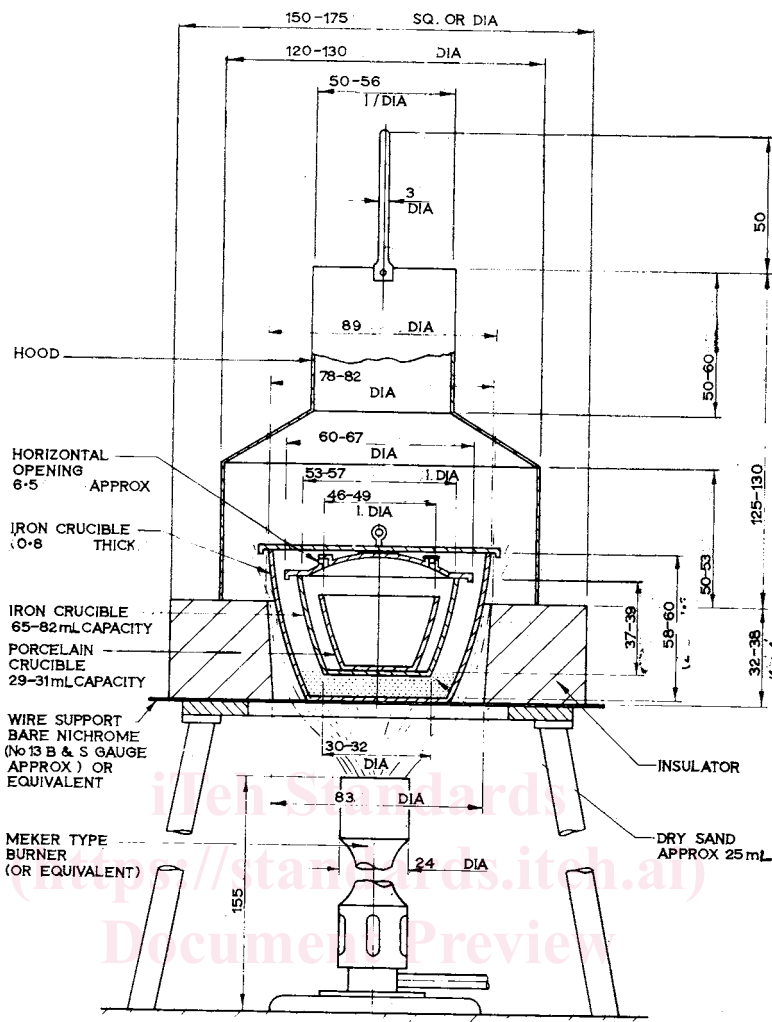


FIG. 1 Apparatus for Determining Conradson Carbon Residue

3.1.1 *carbon residue, n*—the residue formed by evaporation and thermal degradation of a carbon containing material.

3.1.2 *Discussion*—The residue is not composed entirely of carbon but is a coke that can be further changed by carbon pyrolysis. The term carbon residue is retained in deference to its wide common usage.

D4175

#### 4. Summary of Test Method

4.1 A weighed quantity of sample is placed in a crucible and subjected to destructive distillation. The residue undergoes cracking and coking reactions during a fixed period of severe heating. At the end of the specified heating period, the test crucible containing the carbonaceous residue is cooled in a desiccator and weighed. The residue remaining is calculated as a percentage of the original sample, and reported as Conradson carbon residue.

#### 5. Significance and Use

5.1 The carbon residue value of burner fuel serves as a rough approximation of the tendency of the fuel to form deposits in vaporizing pot-type and sleeve-type burners. Similarly, provided alkyl nitrates are absent (or if present, provided the test is performed on the base fuel without additive) the

carbon residue of diesel fuel correlates approximately with combustion chamber deposits.

5.2 The carbon residue value of motor oil, while at one time regarded as indicative of the amount of carbonaceous deposits a motor oil would form in the combustion chamber of an engine, is now considered to be of doubtful significance due to the presence of additives in many oils. For example, an ash-forming detergent additive may increase the carbon residue value of an oil yet will generally reduce its tendency to form deposits.

5.3 The carbon residue value of gas oil is useful as a guide in the manufacture of gas from gas oil, while carbon residue values of crude oil residuums, cylinder and bright stocks, are useful in the manufacture of lubricants.

#### 6. Apparatus (see Fig. 1)

6.1 *Porcelain Crucible*, wide form, glazed throughout, or a silica crucible; 29- to 31-mL capacity, 46 to 49 mm in rim diameter.

6.2 *Iron Crucible*—Skidmore iron crucible, flanged and ringed, 65- to 82-mL capacity, 53 to 57 mm inside and 60- to 67-mm outside diameter of flange, 37 to 39 mm in height supplied with a cover without delivery tubes and having the

vertical opening closed. The horizontal opening of about 6.5 mm shall be kept clean. The outside diameter of the flat bottom shall be 30 to 32 mm.

6.3 *Iron Crucible*—Spun sheet-iron crucible with cover; 78 to 82 mm in outside diameter at the top, 58 to 60 mm in height, and approximately 0.8 mm in thickness. Place at the bottom of this crucible, and level before each test, a layer of about 25 mL of dry sand, or enough to bring the Skidmore crucible, with cover on, nearly to the top of the sheet-iron crucible.

6.4 *Wire Support*—Triangle of bare Nichrome wire of approximately No. 13 B & S gage having an opening small enough to support the bottom of the sheet-iron crucible at the same level as the bottom of the heat-resistant block or hollow sheet-metal box (6.6).

6.5 *Hood*—Circular sheet-iron hood from 120 to 130 mm in diameter the height of the lower perpendicular side to be from 50 to 53 mm; provided at the top with a chimney 50 to 60 mm in height and 50 to 56 mm in inside diameter, which is attached to the lower part having the perpendicular sides by a cone-shaped member, bringing the total height of the complete hood to 125 to 130 mm. The hood can be made from a single piece of metal, provided it conforms to the foregoing dimensions. As a guide for the height of the flame above the chimney, a bridge made of approximately 3-mm iron or Nichrome wire, and having a height of 50 mm above the top of the chimney, shall be attached.

6.6 *Insulator*—Heat-resistant block, refractory ring, or hollow sheet-metal box, 150 to 175 mm in diameter if round, or on a side if square, 32 to 38 mm in thickness, provided with a metal-lined, inverted cone-shaped opening through the center; 83 mm in diameter at the bottom, and 89 mm in diameter at the top. In the case of the refractory ring no metal lining is necessary, providing the ring is of hard, heat-resistant material.

NOTE 5—It is not known what type of insulators were used in the round robin conducted for obtaining the precision given in Section 13.

6.7 *Burner*, Meker type, having an orifice approximately 24 mm in diameter.

## 7. Sampling

7.1 For sampling techniques see Practices D4057 and D4177.

## 8. Procedure

8.1 Shake thoroughly the sample to be tested, first heating to  $50^{\circ} \pm 10^{\circ}\text{C}$  for 0.5 h when necessary to reduce its viscosity. Immediately following the heating and shaking, filter test portion through a 100 mesh screen. Weigh to the nearest 5 mg a 10-g sample of the oil to be tested, free of moisture and other suspended matter, into a tared porcelain or silica crucible containing two glass beads about 2.5 mm in diameter. Place this crucible in the center of the Skidmore crucible. Level the sand in the large sheet-iron crucible and set the Skidmore crucible on it in the exact center of the iron crucible. Apply covers to both the Skidmore and the iron crucible, the one on the latter fitting loosely to allow free exit to the vapors as formed.

8.2 On a suitable stand or ring, place the bare Nichrome wire triangle and on it the insulator. Next center the sheet-iron

crucible in the insulator with its bottom resting on top of the triangle, and cover the whole with the sheet-iron hood in order to distribute the heat uniformly during the process (see Fig. 1).

8.3 Apply heat with a high, strong flame from the Meker-type gas burner, so that the pre-ignition period will be  $10 \pm 1.5$  min (a shorter time can start the distillation so rapidly as to cause foaming or too high a flame). When smoke appears above the chimney, immediately move or tilt the burner so that the gas flame plays on the sides of the crucible for the purpose of igniting the vapors. Then remove the heat temporarily, and before replacing adjust by screwing down the pinch-cock on the gas tubing so that the ignited vapors burn uniformly with the flame above the chimney but not above the wire bridge. Heat can be increased, if necessary, when the flame does not show above the chimney. The period of burning the vapors shall be  $13 \pm 1$  min. If it is found impossible to meet the requirements for both flame and burning time, the requirement for burning time is the more important.

8.4 When the vapors cease to burn and no further blue smoke can be observed, readjust the burner and hold the heat as at the beginning so as to make the bottom and lower part of the sheet-iron crucible a cherry red, and maintain for exactly 7 min. The total period of heating shall be  $30 \pm 2$  min, which constitutes an additional limitation on the tolerances for the pre-ignition and burning periods. There should be no difficulty in carrying out the test exactly as directed with the gas burner of the type named, using city gas ( $20$  to  $40$  MJ/m<sup>3</sup>), with the top of the burner about 50 mm below the bottom of the crucible. The time periods shall be observed with whatever burner and gas is used.

8.5 Remove the burner and allow the apparatus to cool until no smoke appears, and then remove the cover of the Skidmore crucible (about 15 min). Remove the porcelain or silica crucible with heated tongs, place in the desiccator, cool, and weigh. Calculate the percentage of carbon residue on the original sample.

## 9. Procedure for Residues Exceeding 5 %

9.1 This procedure is applicable to such materials as heavy crude oils, residuums, heavy fuel oils, and heavy gas oils.

9.2 When the carbon residue as obtained by the procedure described in Section 8 (using a 10-g sample) is in excess of 5 %, difficulties can be experienced due to boiling over of the sample. Trouble also can be encountered with samples of heavy products which are difficult to dehydrate.

9.3 For samples showing more than 5.0 and less than 15.0 % carbon residue by the procedure described in Section 8, repeat the test using a  $5 \pm 0.5$  g sample weighed to the nearest 5 mg. In event that a result greater than 15.0 % is obtained, repeat the test, reducing the sample size to  $3 \pm 0.1$  g, weighed to the nearest 5 mg.

9.4 If the sample boils over, reduce the sample size first to 5 g and then to 3 g as necessary to avoid the difficulty.

9.5 When the 3-g sample is used, it can be impossible to control the preignition and vapor burning times within the limits specified in 8.3. However, in such cases, the results shall be considered as valid.