



Designation: **C 770 – 98 (Reapproved 2003)2008)**

## Standard Test Method for Measurement of Glass Stress—Optical Coefficient<sup>1</sup>

This standard is issued under the fixed designation C 770; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

### 1. Scope

1.1 This test method covers procedures for determining the stress-optical coefficient of glass, which is used in photoelastic analyses. In Procedure A the optical retardation is determined for a glass fiber subjected to uniaxial tension. In Procedure B the optical retardation is determined for a beam of glass of rectangular cross section when subjected to four-point bending. In Procedure C, the optical retardation is measured for a beam of glass of rectangular cross-section when subjected to uniaxial compression.

1.2 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

### 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

C 336 [Test Method for Annealing Point and Strain Point of Glass by Fiber Elongation](#)

C 598 [Test Method for Annealing Point and Strain Point of Glass by Beam Bending](#)

~~FE 218 [Test Method for Analyzing Stress in Glass](#)~~<sup>2</sup> [Method for Radiochemical Determination of Cesium-137 in Aqueous Solutions \(Chloroplatinate Method\)](#)<sup>3</sup>

### 3. Significance and Use

3.1 Stress-optical coefficients are used in the determination of stress in glass. They are particularly useful in determining the magnitude of thermal residual stresses for annealing or pre-stressing (tempering) glass. As such, they can be important in specification acceptance.

### 4. Apparatus

4.1 *Stressing Equipment and Polarimeter :*

4.1.1 *Procedure A*— Figs. 1 and 2 illustrate a polarimeter employing a quarter-wave plate and rotatable analyzer,<sup>4</sup> described in Test Method F 218. The quarter-wave plate shall be designed for the wavelength of the light being used. The polarizing axes of the polarizer and analyzer shall be set at right angles to each other with each being located at an angle of 45° with the horizontal and vertical. The analyzer, however, shall be mounted in a rotatable mount having a scale graduated on either side from 0 to 180°. The quarter-wave plate shall be fixed to give maximum extinction when the polarizer and analyzer are crossed at right angles; that is, when its polarizing axes are set at 45° and 135° to the horizontal and vertical. In place of the immersion cell *E*, a means of supporting and loading a glass specimen shall be provided, either in air (Fig. 3(a)) or in an immersion liquid (Fig. 3(b)). In this arrangement the optical elements of the polarimeter between light source and telescope have been reversed and a large scale graduated in 2-nm divisions is employed with the rotatable analyzer *I*.

4.1.1.1 Fig. 3 illustrates the fiber-stressing and optical arrangement used in Procedure A. Figure 3(a) shows the fiber mounted vertically, positioned, and supported by two brass collars with swivel handles so that the kilogram weight may be applied to load the fiber. A light shield having entrance and exit slits surrounds the fiber providing a degree of collimation to the light passing

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee C14 on Glass and Glass Products and is the direct responsibility of Subcommittee C14.04 on Physical and Mechanical Properties.

Current edition approved April 10, 2003; 1, 2008. Published January 1999; December 2008. Originally approved in 1973. Last previous edition approved in 1995; 2003 as C 770 – 95 (2003).

<sup>2</sup> Annual Book of ASTM Standards, Vol 15.02.

<sup>3</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

<sup>4</sup> Goranson and Adams, "Measurement of Optical Path Differences," *Journal of Franklin Institute*, Vol 216, 1933, p. 475.

<sup>5</sup> Withdrawn. The last approved version of this historical standard is referenced on [www.astm.org](http://www.astm.org).

<sup>6</sup> Working drawings of test frames are available from Strainoptic Technologies, Inc., North Wales, PA.

<sup>7</sup> Goranson and Adams, "Measurement of Optical Path Differences," *Journal of Franklin Institute*, Vol 216, 1933, p. 475.

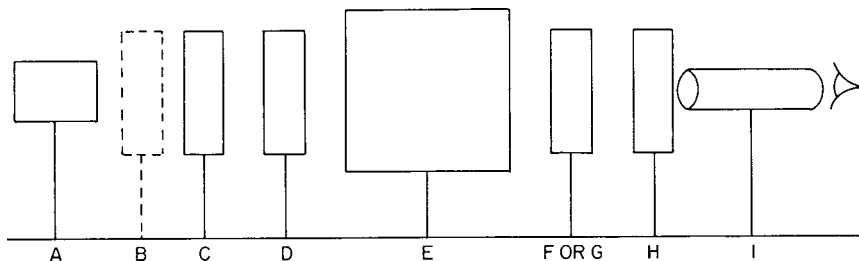


FIG. 1 Polarimeter

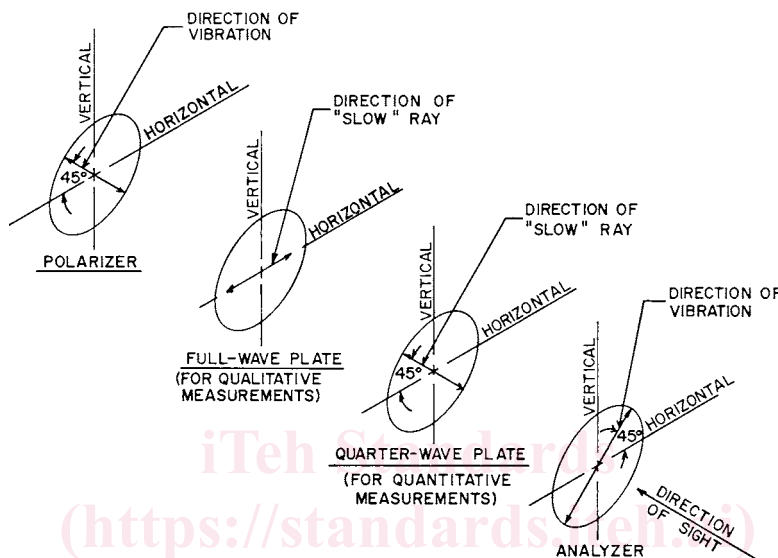


FIG. 2 Orientation of Polarimeter in Standard Position

through the fiber and also helping to eliminate stray light.

4.1.1.2 In Fig. 3(b) the fiber is stressed while immersed in a liquid which matches the refractive index of the fiber. This arrangement provides more satisfactory viewing of the fiber. (C770-98(2008))

#### 4.1.2 Procedure B:

4.1.2.1 The apparatus for the beam-bending procedure is shown in Fig. 4(a). Radiation from a white-light source passes through the following components and in this sequence: a diffusing plate, an adjustable aperture, a polarizer whose axis is at  $45^\circ$  to the vertical, the glass specimen, a Babinet compensator, a polarizer whose axis is at  $90^\circ$  to that of the first polarizer, and a telescope of modest power.

4.1.2.2 The loading scheme is shown in Fig. 4(b). Metal fixtures shall be provided to subject the specimen to four-point bending. A support span of 115 mm and a moment arm,  $a$ , of 45 mm are recommended. Dimensions within 5 % of these values are acceptable. Symmetrical loading is essential, and requires careful centering of the upper loading block. The knife edges shall be finished to approximately 5-mm radius. Loading can be accomplished through a yoke, which rests in a V-groove in the upper loading block, and a weight pan as shown. However, any convenient loading scheme at the center of the upper block may be used.

4.1.2.3 A Babinet compensator is positioned so as to produce vertical fringes (Fig. 4(c)). The neutral fringe must fall near the center of the support span. Recommended fringe spacing is  $1000 \pm 200$  nm of retardation per centimeter. In actual practice the compensator is placed very close to the specimen inside the loading yoke.

4.1.2.4 A telescope is mounted in a rotating collar equipped with an angular scale which can be read to  $0.1^\circ$  by a vernier. The cross hairs in the eyepiece are used to measure the tilt angle of the neutral fringe as shown in Fig. 4(c). An 80-mm objective lens and  $10\times$  eyepiece are adequate components for the telescope.

4.1.2.5 The adjustable aperture is set at the smallest diameter that permits suitable viewing. As with the fiber apparatus, this provides some collimation and helps to eliminate stray light.

#### 4.1.3 Procedure C:

4.1.3.1 Polarimeter as described in Test Method F 218.

4.1.3.2 Force application frame, shown in Fig. 5 must include:

- A strain-gage load cell and load cell indicator, capable of measuring the force applied within 1 % accuracy.
- Hydraulic or mechanical means of applying constant force and maintaining the force during the measuring time.
- Swivel-mounted loading blocks, offering at least two degrees of swivel freedom, to avoid the loading on the edge.

4.2 *Micrometer Caliper*, for measuring specimen dimensions to 0.0025 mm (0.0001 in.).

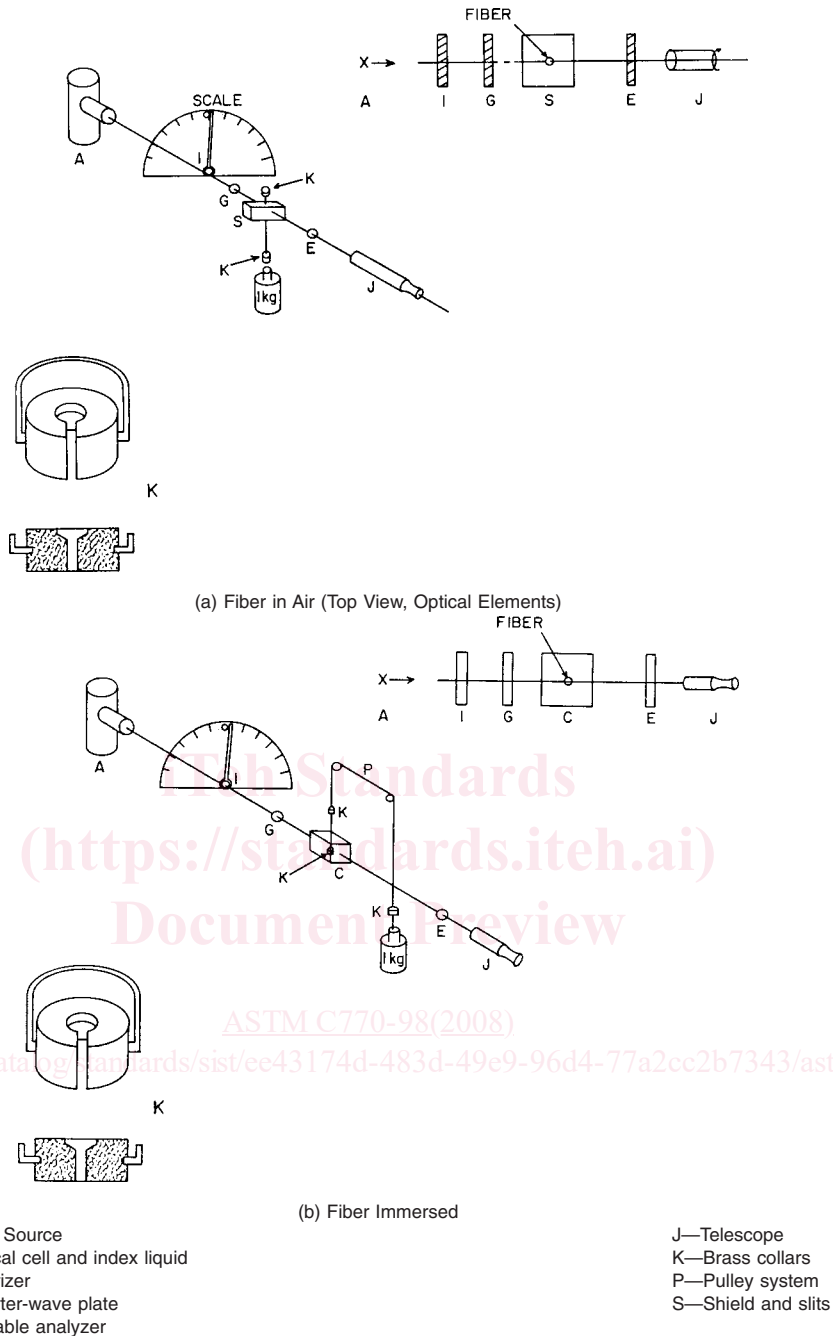


FIG. 3 Optical and Fiber-Stressing Polarimeter Arrangement

4.3 Weights that are known to an accuracy of  $\pm 1\%$ .

**5. Test Specimen**

5.1 Procedure A:

5.1.1 Select a mass of the glass to be tested that has good optical quality with no heavy cords or striae. By conventional lamp-working methods, draw 0.6 to 0.9 m (2 to 3 ft) of fiber from the glass, sufficient to provide five specimens 76 to 102 mm (3 to 4 in.) long with taper (variation in diameter along the length) less than 0.025 mm (0.001 in.) and diameters in the range 0.635 mm (0.025 in.) to 0.760 mm (0.030 in.). The difference in mutually perpendicular diameters at any point along the specimen length shall be less than 0.0076 mm (0.0003 in.).

5.1.2 Bead both ends of each specimen by holding the end in a flame with the fiber vertical until a bead of two to three fiber diameters forms.

5.1.3 Anneal the specimens together so as to remove most of the lamp-working stress (Annex A2).

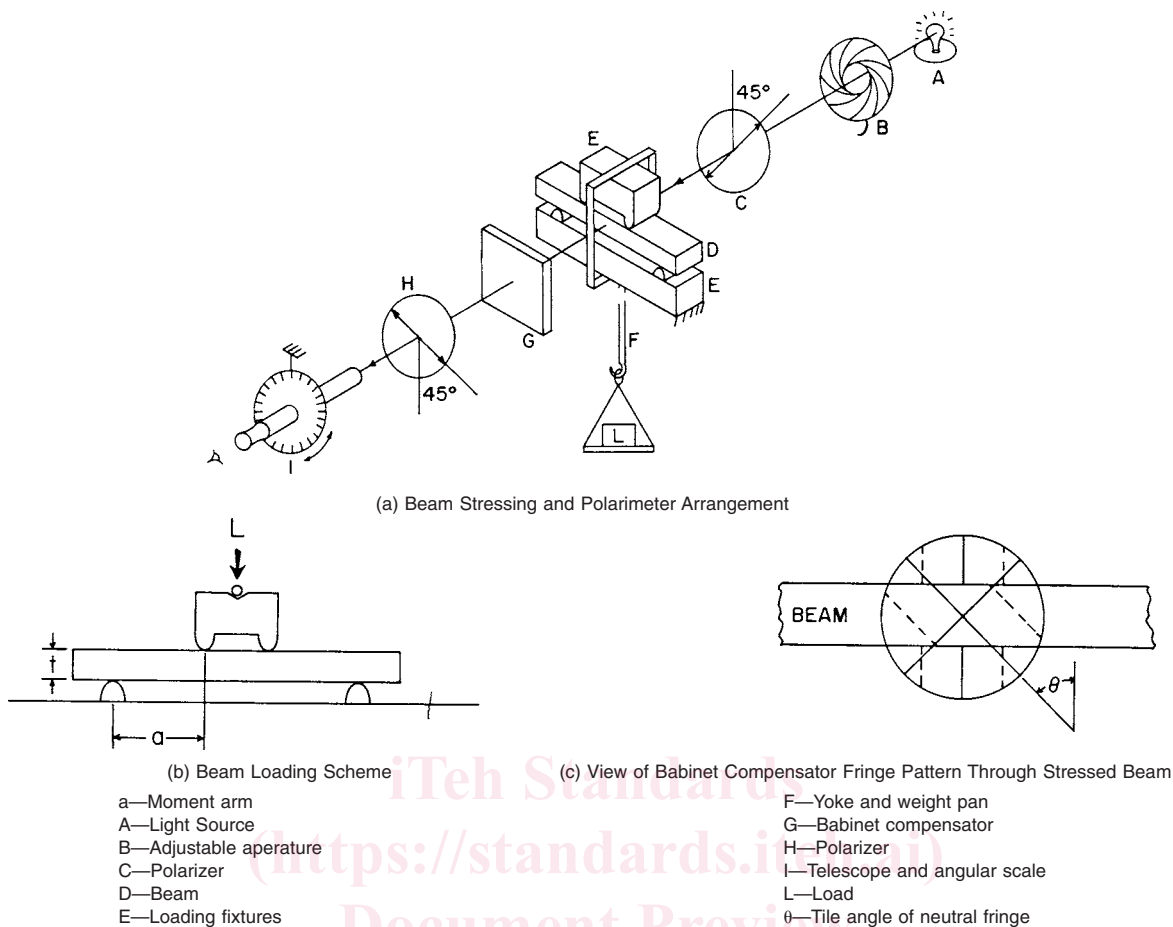


FIG. 4 Optical and Mechanical Details for Beam Method

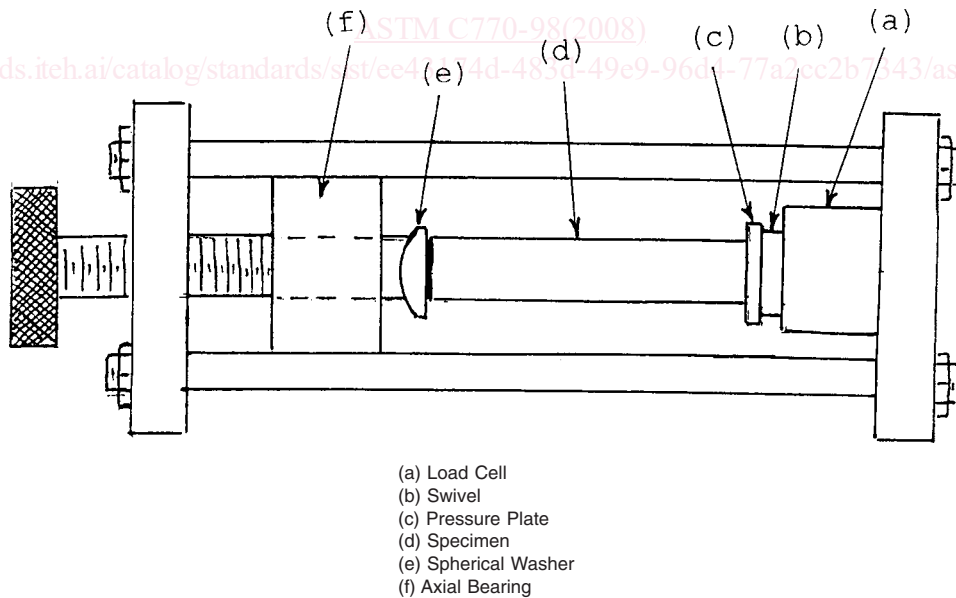


FIG. 5 Force Application Frame

5.2 Procedure B:

5.2.1 Select a mass of glass to be tested that has good optical quality with no heavy cords or striae. By conventional grinding methods, prepare a beam of rectangular cross section. The width of the beam shall be within the range 20 to 30 mm (0.8 to 1.2 in.), the thickness within the range 6 to 10 mm (0.25 to 0.40 in.), and the length within the range 120 to 130 mm (4.75 to 5.10