

DRAFT INTERNATIONAL STANDARD

ISO/DIS 18898

ISO/TC 45/SC 2

Secretariat: JISC

Voting begins on:
2015-05-20

Voting terminates on:
2015-08-20

Rubber — Calibration and verification of hardness testers

Caoutchouc — Étalonnage et vérification des duromètres

ICS: 83.060

iTeh STANDARD PREVIEW
(standards.iteh.ai)
Full standard:
<https://standards.iteh.ai/catalog/standards/sist/51d14e34-65ec-4b95-a304-2f6bdd42f5c6/iso-18898-2016>

THIS DOCUMENT IS A DRAFT CIRCULATED FOR COMMENT AND APPROVAL. IT IS THEREFORE SUBJECT TO CHANGE AND MAY NOT BE REFERRED TO AS AN INTERNATIONAL STANDARD UNTIL PUBLISHED AS SUCH.

IN ADDITION TO THEIR EVALUATION AS BEING ACCEPTABLE FOR INDUSTRIAL, TECHNOLOGICAL, COMMERCIAL AND USER PURPOSES, DRAFT INTERNATIONAL STANDARDS MAY ON OCCASION HAVE TO BE CONSIDERED IN THE LIGHT OF THEIR POTENTIAL TO BECOME STANDARDS TO WHICH REFERENCE MAY BE MADE IN NATIONAL REGULATIONS.

RECIPIENTS OF THIS DRAFT ARE INVITED TO SUBMIT, WITH THEIR COMMENTS, NOTIFICATION OF ANY RELEVANT PATENT RIGHTS OF WHICH THEY ARE AWARE AND TO PROVIDE SUPPORTING DOCUMENTATION.



Reference number
ISO/DIS 18898:2015(E)

© ISO 2015

iTeh STANDARD PREVIEW
(standards.iteh.ai)
Full standard:
<https://standards.iteh.ai/catalog/standards/sist/51d14e34-65ec-4b95-a304-2f6bdd42f5c6/iso-18898-2016>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2015

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Measurands and metrological requirements for calibration and verification	1
4.1 Environmental conditions.....	1
4.2 Metrological requirements.....	1
5 Calibration and verification methods	10
5.1 Requirements to be met by the measuring instruments used for the calibration and verification methods.....	10
5.2 Outline of the calibration and verification methods to be used.....	11
5.2.1 Indentors.....	11
5.2.2 Geometry of the pressure foot.....	11
5.2.3 Depth of indentation.....	12
5.2.4 Contact force of the pressure foot.....	17
5.2.5 Spring force.....	17
5.2.6 Contact and total force of IPHD dead-load instruments.....	20
5.2.7 Duration of force application.....	21
6 Calibration and verification certificate	21

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2. www.iso.org/directives

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received. www.iso.org/patents

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT), see the following URL: [Foreword - Supplementary information](#)

The committee responsible for this document is ISO/TC 45, *Rubber and rubber products*, Subcommittee SC 2, *Testing and analysis*.

This third edition cancels and replaces the second edition (ISO 18898:2012), which has been technically revised as follows:

Calibration and verification for determination of dead load hardness using the Very Low Rubber hardness scale (VLRH) has been incorporated.

Rubber — Calibration and verification of hardness testers

1 Scope

This International Standard specifies procedures for the calibration and verification of durometers of types A, D, AO and AM (see ISO 7619-1), IRHD pocket meters (see ISO 7619-2), IRHD dead-load instruments (see ISO 48) and dead load instruments using the Very Low Rubber Hardness scale (see ISO 27588).

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 48, *Rubber, vulcanized or thermoplastic — Determination of hardness (hardness between 10 IRHD and 100 IRHD)*

ISO 7619-1, *Rubber, vulcanized or thermoplastic — Determination of indentation hardness — Part 1: Durometer method (Shore hardness)*

ISO 7619-2, *Rubber, vulcanized or thermoplastic — Determination of indentation hardness — Part 2: IRHD pocket meter method*

ISO/IEC 17025, *General requirements for the competence of testing and calibration laboratories*

ISO 18899:2004, *Rubber — Guide to the calibration of test equipment*

ISO 27588, *Rubber, vulcanized or thermoplastic — Determination of dead-load hardness using the very low rubber hardness (VLRH) scale*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 48 and ISO 18899 apply.

4 Measurands and metrological requirements for calibration and verification

4.1 Environmental conditions

The ambient temperature of the measurement room in which the calibration or verification is carried out shall be 18 °C to 25 °C.

4.2 Metrological requirements

The measurands of indenter and pressure foot for the instrument to be calibrated are depicted in [Figures 1 to 7](#) and requirements are specified in [Tables 1 to 10](#).

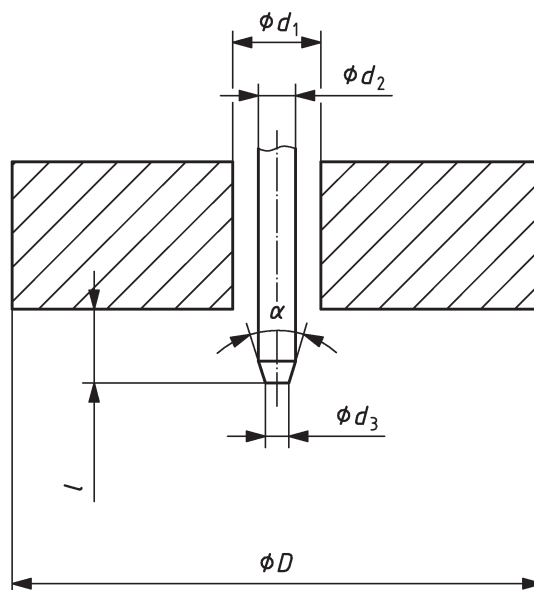


Figure 1 — Indentor and pressure foot for type A durometer

Table 1 — Type A durometer

Measurand		Unit	Metrological requirement	Calibration and verification instructions
Shaft diameter of indenter	d_2	mm	$1,25 \pm 0,15$	5.2.1.2
Cone frustum top diameter	d_3	mm	$0,79 \pm 0,01$	5.2.1.2
Cone angle of indenter	α	°	$35,00 \pm 0,25$	5.2.1.2
Centrality of pressure foot			Central	
Diameter of pressure foot	D	mm	$18,0 \pm 0,5$	5.2.2.1
Hole diameter of pressure foot	d_1	mm	$3,0 \pm 0,1$	5.2.2.2
Mass on pressure foot	m	kg	$1,0^{+0,1}_{0,0}$	5.2.4.1
Depth of indentation	l	mm	$0,00$ to $2,50$; $\Delta l = \pm 0,02$	5.2.3.1
Spring force on indenter	F	mN	$F = 550,0 + 75,0H_A$; $\Delta F = \pm 37,5^a$ where H_A = hardness reading on type A durometer	5.2.5.1
Duration of force application	t	s	3 or 15	5.2.7

^a For hand-held durometers, the tolerance may be doubled.

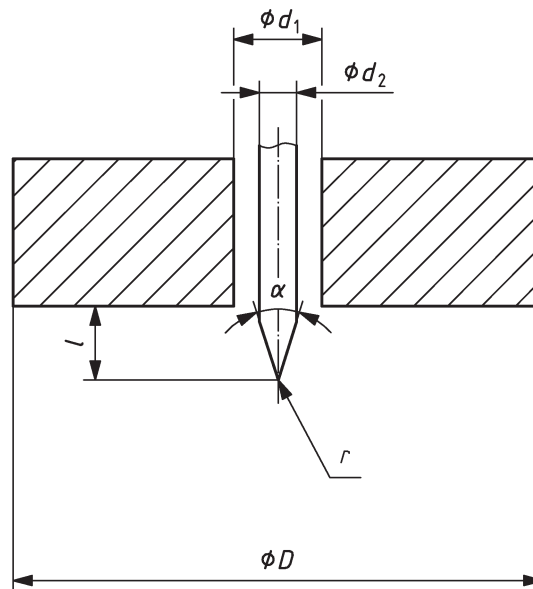


Figure 2 — Indentor and pressure foot for type D durometer

Table 2 — Type D durometer

Measurand	Unit	Metrological requirement	Calibration and verification instructions
Shaft diameter of indentor	d_2 mm	$1,25 \pm 0,15$	5.2.1.3
Radius of indentor	r mm	$0,10 \pm 0,01$	5.2.1.3
Cone angle of indentor	α °	$30,00 \pm 0,25$	5.2.1.3
Centrality of pressure foot		Central	
Diameter of pressure foot	D mm	$18,0 \pm 0,5$	5.2.2.1
Hole diameter of pressure foot	d_1 mm	$3,0 \pm 0,1$	5.2.2.2
Mass on pressure foot	m kg	$5,0^{+0,5}_{0,0}$	5.2.4.1
Depth of indentation	l mm	$0,00$ to $2,50$; $\Delta l = \pm 0,02$	5.2.3.2
Spring force on indentor	F mN	$F = 445,0H_D$; $\Delta F = \pm 222,5^a$ where H_D = hardness reading on type D durometer	5.2.5.2
Duration of force application	t s	3 or 15	5.2.7

^a For hand-held durometers, the tolerance may be doubled.

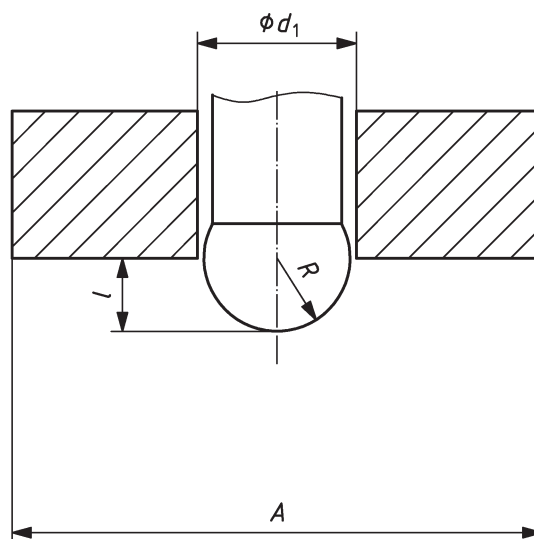


Figure 3 — Indentor and pressure foot for type AO durometer

Table 3 — Type AO durometer

Measurand		Unit	Metrological requirement	Calibration and verification instructions
Radius of indenter	R	mm	$2,50 \pm 0,02$	5.2.1.4
Centrality of pressure foot			Central	
Area of pressure foot	A	mm ²	500 minimum	5.2.2.1
Hole diameter of pressure foot	d_1	mm	$5,4 \pm 0,2$	5.2.2.2
Mass on pressure foot	m	kg	$1,0^{+0,1}_{0,0}$	5.2.4.1
Depth of indentation	l	mm	0,00 to 2,50; $\Delta l = \pm 0,02$	5.2.3.3
Spring force on indenter	F	mN	$F = 550,0 + 75,0H_{AO}$; $\Delta F = \pm 37,5^a$ where H_{AO} = hardness reading on type AO durometer	5.2.5.3
Duration of force application	t	s	3 or 15	5.2.7

^a For hand-held durometers, the tolerance may be doubled.

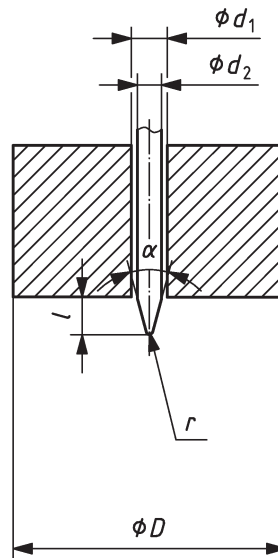


Figure 4 — Indenter and pressure foot for type AM durometer

Table 4 — Type AM durometer

Measurand	Unit	Metrological requirement	Calibration and verification instructions
Shaft diameter of indenter	d_2 mm	$0,790 \pm 0,025$	5.2.1.5
Radius of indenter	r mm	$0,10 \pm 0,01$	5.2.1.5
Cone angle of indenter	α °	$30,00 \pm 0,25$	5.2.1.5
Centrality of pressure foot		Central	
Diameter of pressure foot	D mm	$9,0 \pm 0,3$	5.2.2.1
Hole diameter of pressure foot	d_1 mm	$1,19 \pm 0,03$	5.2.2.2
Mass on pressure foot	m kg	$0,25^{+0,05}_{-0,00}$	5.2.4.1
Depth of indentation	l mm	$0,00$ to $1,25$; $\Delta l = \pm 0,01$	5.2.3.4
Spring force on indenter	F mN	$F = 324,0 + 4,4H_{AM}$; $\Delta F = \pm 8,8$ where H_{AM} = hardness reading on type AM durometer	5.2.5.4
Duration of force application	t s	3 or 15	5.2.7

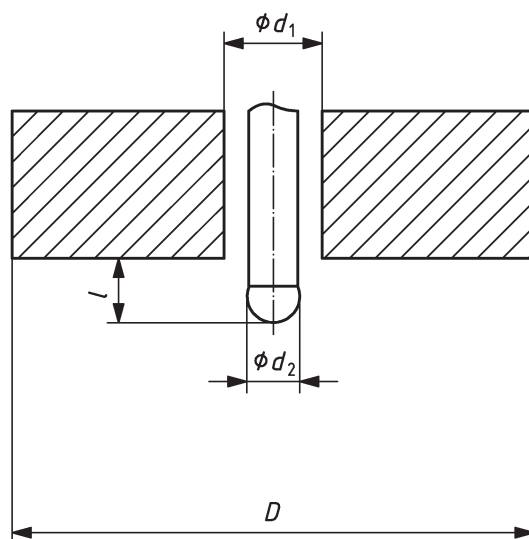


Figure 5 — Indenter and pressure foot for IRHD dead-load tester

Table 5 — IRHD dead-load method N

Measurand		Unit	Metrological requirement	Calibration and verification instructions
Ball diameter of indenter	d_2	mm	$2,50 \pm 0,01$	5.2.1.6
Centrality of pressure foot			Central	
Diameter of pressure foot	D	mm	20 ± 1	5.2.2.1
Hole diameter of pressure foot	d_1	mm	6 ± 1	5.2.2.2
Force on pressure foot	F_f	N	$8,3 \pm 1,5$	5.2.4.2
Incremental indentation depth	l	mm	$l = f(\text{IRHD})$ (see Table 15) $\Delta l = \pm 0,01$	5.2.3.5
Contact force on indenter	F_c	N	$0,30 \pm 0,02$	5.2.6.1
Total force on indenter	F_t	N	$5,70 \pm 0,03$	5.2.6.1
Duration of application of total force t_t and contact force t_c		s	$t_t = 30; t_c = 5$	5.2.7