



Designation: A 957/A 957M – 09

Standard Specification for Investment Castings, Steel and Alloy, Common Requirements, for General Industrial Use¹

This standard is issued under the fixed designation A 957/A 957M; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reappraisal.

1. Scope*

1.1 This specification covers a group of requirements that are mandatory for castings produced by the investment casting process to meet the metallurgical requirements of the following steel casting specifications issued by ASTM.

ASTM Designation	Title of Specification
A 27/A 27M A27/A27M	Steel Castings, Carbon, for General Application
A 148/A 148M A148/A148M	Steel Castings, High-Strength, for Structural Purposes
A 297/A 297M A297/A297M	Steel Castings, Iron-Chromium and Iron-Chromium-Nickel, Heat-Resistant, for General Application
A 447/A 447M A447/A447M	Steel Castings, Chromium-Nickel-Iron Alloy (25-12 Class), for High-Temperature Service
A 494/A 494M A494/A494M	Castings, Nickel and Nickel Alloy
A 560/A 560M A560/A560M	Castings, Chromium-Nickel Alloy
A 732/A 732M A732/A732M	Castings, Investment, Carbon and Low Alloy Steel for General Application, and Cobalt Alloy for High Strength at Elevated Temperatures
A 743/A 743M A743/A743M	Castings, Iron-Chromium, Iron-Chromium-Nickel, Corrosion-Resistant, for General Application
A 744/A 744M A744/A744M	Castings, Iron-Chromium-Nickel, Corrosion Resistant, for Severe Service
A 747/A 747M A747/A747M	Steel Castings, Stainless, Precipitation Hardening
A 890/A 890M A890/A890M	Castings, Iron-Chromium-Nickel-Molybdenum Corrosion-Resistant, Duplex (Austenitic/Ferritic) for General Application
A 915/A 915M A915/A915M	Steel Castings, Carbon and Alloy, Chemical Requirements Similar to Standard Wrought Grades

1.2 This specification also covers a group of supplementary requirements that may be applied to the above specifications as indicated therein. These are provided for use when additional testing or inspection is desired and apply only when specified individually by the purchaser in the order.

1.3 When investment castings are ordered, the requirements stated in this specification form an integral part of the material specification. In cases of conflict, the requirements of this

specification shall take precedence over the individual material specification requirements.

1.4 The values stated in either SI units or inch-pound units are to be regarded separately as standard. The values stated in each system may not be exact equivalents; therefore, each system shall be used independently of the other. Combining values from the two systems may result in non-conformance with the standard.

2. Referenced Documents

2.1 ASTM Standards:²

- A27/A27M** Specification for Steel Castings, Carbon, for General Application
- A148/A148M** Specification for Steel Castings, High Strength, for Structural Purposes
- A297/A297M** Specification for Steel Castings, Iron-Chromium and Iron-Chromium-Nickel, Heat Resistant, for General Application
- A370** Test Methods and Definitions for Mechanical Testing of Steel Products
- A380** Practice for Cleaning, Descaling, and Passivation of Stainless Steel Parts, Equipment, and Systems
- A447/A447M** Specification for Steel Castings, Chromium-Nickel-Iron Alloy (25-12 Class), for High-Temperature Service
- A488/A488M** Practice for Steel Castings, Welding, Qualifications of Procedures and Personnel
- A494/A494M** Specification for Castings, Nickel and Nickel Alloy
- A560/A560M** Specification for Castings, Chromium-Nickel Alloy
- A609/A609M** Practice for Castings, Carbon, Low-Alloy, and Martensitic Stainless Steel, Ultrasonic Examination Thereof
- A732/A732M** Specification for Castings, Investment, Carbon and Low Alloy Steel for General Application, and Cobalt Alloy for High Strength at Elevated Temperatures
- A743/A743M** Specification for Castings, Iron-Chromium,

¹ This specification is under the jurisdiction of ASTM Committee A01 on Steel, Stainless Steel and Related Alloys and is the direct responsibility of Subcommittee A01.18 on Castings.

Current edition approved Jan. 1, 2009. Published January 2009. Originally approved in 1996. Last previous edition approved in 2008 as A 957/A 957M – 08.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

*A Summary of Changes section appears at the end of this standard.

Iron-Chromium-Nickel, Corrosion Resistant, for General Application

A744/A744M Specification for Castings, Iron-Chromium-Nickel, Corrosion Resistant, for Severe Service

A747/A747M Specification for Steel Castings, Stainless, Precipitation Hardening

A751 Test Methods, Practices, and Terminology for Chemical Analysis of Steel Products

A800/A800M Practice for Steel Casting, Austenitic Alloy, Estimating Ferrite Content Thereof

A890/A890M Specification for Castings, Iron-Chromium-Nickel-Molybdenum Corrosion-Resistant, Duplex (Austenitic/Ferritic) for General Application

A903/A903M Specification for Steel Castings, Surface Acceptance Standards, Magnetic Particle and Liquid Penetrant Inspection

A915/A915M Specification for Steel Castings, Carbon, and Alloy, Chemical Requirements Similar to Standard Wrought Grades

A941 Terminology Relating to Steel, Stainless Steel, Related Alloys, and Ferrous Alloys

A967 Specification for Chemical Passivation Treatments for Stainless Steel Parts

A991/A991M Test Method for Conducting Temperature Uniformity Surveys of Furnaces Used to Heat Treat Steel Products

A997 Practice for Investment Castings, Surface Acceptance Standards, Visual Examination

E29 Practice for Using Significant Digits in Test Data to Determine Conformance with Specifications

E94 Guide for Radiographic Examination

E125 Reference Photographs for Magnetic Particle Indications on Ferrous Castings

E165 Practice for Liquid Penetrant Examination for General Industry

E 186 Reference Radiographs for Heavy-Walled (2 to 4 ½ in. [51 to 114-mm]) Steel Castings

E192 Reference Radiographs of Investment Steel Castings for Aerospace Applications

E 280 Reference Radiographs for Heavy-Walled (4 ½ to 12-in. [114 to 305-mm]) Steel Castings

E340 Test Method for Macroetching Metals and Alloys

E353 Test Methods for Chemical Analysis of Stainless, Heat-Resisting, Maraging, and Other Similar Chromium-Nickel-Iron Alloys

E354 Test Methods for Chemical Analysis of High-Temperature, Electrical, Magnetic, and Other Similar Iron, Nickel, and Cobalt Alloys

E446 Reference Radiographs for Steel Castings Up to 2 in. (50.8 mm) in Thickness

E709 Guide for Magnetic Particle Testing

2.2 *SAE Aerospace Recommended Practice*:³

ARP 1341 Determining Decarburization and Carburization in Finished Parts of Carbon and Low-Alloy Steel

3. Terminology

3.1 *Definitions*—The definitions in Test Methods and Definitions A 370**A370**, Test Methods, Practices, and Terminology A 751**A751**, and Terminology A 941**A941** are applicable to this specification and to those listed in 1.1.

3.2 *Definitions of Terms Specific to This Standard*:

3.2.1 *investment casting, n*—a metal casting that is produced in a mold obtained by investing (surrounding) an expendable pattern with a ceramic slurry that is allowed to solidify. The expendable pattern may consist of wax, plastic, or other material and is removed prior to filling the mold with liquid metal.

3.2.2 *master heat, n*—a quantity of metal processed in a single furnace or refining vessel at one time in such a manner as to produce the desired composition and properties.

3.2.3 *sub-heat, n*—a portion of a master heat remelted without additional processing for pouring into castings. Synonyms: melt, production heat.

4. Materials and Manufacture

4.1 *Melting Process*—Master heats shall be made by the electric furnace process with or without separate refining such as argon-oxygen-decarburization (AOD), vacuum-oxygen-degassing (VOD), vacuum-induction-melting (VIM), and so forth, unless otherwise specified in the individual specification or agreed upon between the customer and producer. Master heats may be used directly for producing castings or converted into ingot, bar, shot, or other suitable form, not including gates and risers from casting production, for later remelting as a sub-heat.

4.2 *Re-Melting Process*—Sub-heats shall be produced from master heat metal in suitable batch sizes by electric induction furnace with or without atmosphere protection such as vacuum or inert gas unless otherwise specified in the individual specification or agreed upon between the customer and producer. Revert (gates, sprues, risers, and rejected castings) shall not be re-melted except in master heats.

4.3 *Sampling*:

4.3.1 If castings are poured directly from one or more master heats, then the samples for chemical and other required testing shall also be poured directly from each of the master heats.

4.3.2 If castings are poured from a sub-heat, then the samples for chemical and other required testing shall also be poured from a sub-heat of that same master heat, but not necessarily from the same sub-heat as the castings. The sub-heat used for the test samples shall be produced using the same practices and additions as used for the castings.

³ Available from Society of Automotive Engineers (SAE), 400 Commonwealth Dr., Warrendale, PA 15096-0001, <http://www.sae.org>.

4.3.3 Unless otherwise specified by the purchaser, test specimens may be taken from castings or from coupons cast integrally with the castings, in the same molds as the castings, or in separate molds.

4.4 *Heat Treatment:*

4.4.1 Castings shall be heat treated in the working zone of a furnace that has been surveyed in accordance with Test Method A 991/A 991M **A991/A991M**.

4.4.2 When castings are heat treated at temperatures above 2000°F (1100°C), then the working zone shall have been established by a survey performed at not more than 25°F (15°C) below nor more than 200°F (110°C) above the minimum heat treatment temperature specified for the grade. If a minimum heat treatment temperature is not specified for the grade, then the survey temperature shall be not more than 50°F (30°C) below nor more than 175°F (100°C) above the furnace set point used.

4.4.3 The maximum variation in measured temperature as determined by the difference between the highest temperature and the lowest temperature shall be as agreed between the purchaser and producer except that during production heat treatment, no portion of the furnace shall be below the minimum specified temperature nor above the maximum specified temperature for the grade being processed.

5. Chemical Composition

5.1 *Chemical Analysis*—Chemical analysis of materials covered by this specification shall be in accordance with Test Methods, Practices, and Terminology A 751 **A751**.

5.2 *Heat Analysis*—An analysis of samples obtained in accordance with 4.3 or Supplementary Requirement S17 as appropriate, shall be made by the manufacturer to determine the percentages of the elements specified in the individual specification for the grade being poured. When drillings are used, they shall be taken not less than 1/16 in. [1.6 mm] beneath the surface. The chemical composition thus determined shall conform to the requirements in the individual specification for the grade being poured.

5.3 *Product Analysis*—A product analysis may be made by the purchaser from material representing each master heat, sub-heat, lot, or casting. The analysis shall be made on representative material. Samples for carbon analysis of carbon and alloy steel shall be taken no closer than 1/16 in. [1.6 mm] to a cast surface, except that castings too thin for this shall be analyzed on representative material. The chemical composition thus determined shall meet the requirements specified in the applicable specification for the grade involved, or shall be subject to rejection by the purchaser, except that the chemical composition determined for carbon and low alloy steel castings may vary from the specified limits by the amounts shown in **Table 1**. The product analysis tolerances of **Table 1** are not applicable as acceptance criteria for heat analysis by the casting manufacturer. When comparing product and heat analysis for other than carbon and low alloy steels, the reproducibility Data R2, in Test Methods E 353 or E 354 **E353E354**, as applicable, shall be taken into consideration.

TABLE 1 Product Analysis Tolerances

Element	Range, % ^A	Tolerances ^{B,C} Over Maximum or Under Minimum Limit, %
C	up to 0.65 above 0.65	0.03 × % C _L + 0.02 0.04
Mn	up to 1 above 1	0.08 × % Mn _L + 0.01 0.09
Si	up to 0.60 above 0.60	0.22 × % Si _L - 0.01 0.15
P	all	0.13 × % P _L + 0.005
S	all	0.36 × % S _L + 0.001
Ni	up to 2 above 2	0.10 × % Ni _L + 0.03 0.25
Cr	up to 2 above 2	0.07 × % Cr _L + 0.04 0.18
Mo	up to 0.6 above 0.6	0.04 × % Mo _L + 0.03 0.06
V	up to 0.25 above 0.25	0.23 × % V _L + 0.004 0.06
W	up to 0.10 above 0.10	0.08 × % W _L + 0.02 0.02
Cu	up to 0.15 above 0.15	0.18 × % Cu _L + 0.02 0.05
Al	up to 0.10 above 0.10	0.08 × % Al _L + 0.02 0.03

^A The range denotes the composition limits up to which tolerances are computed by the equation, and above which the tolerances are given by a constant.

^B The subscript L for the elements in each equation indicates that the limits of the element specified by the applicable specification are to be inserted into the equation to calculate the tolerance for the upper limit and the lower limit (if applicable), respectively. Examples of computing tolerances are presented in footnote C.

^C To illustrate the computation of the tolerance, consider the manganese maximum of 0.70 for an 0.30 carbon grade 65-35 in Specification A 27/A 27M **A27/A27M**. The maximum permissible deviation is (0.08 × 0.70 + 0.01) = 0.066. Therefore, the highest acceptable product analysis is 0.766. Similarly, for an 0.20 carbon grade 70-40 in Specification A 27/A 27M **A27/A27M**, the maximum manganese content is 1.40; thus, the highest acceptable product analysis is (1.40 + 0.09) = 1.49.

5.4 *Unspecified Elements*—When chemical analysis for elements not specified for the grade ordered is desired, Supplementary Requirement S13 may be specified.


NOTE 1—All commercial metals contain small amounts of various elements in addition to those that are specified. It is neither practical nor necessary to specify limits for every unspecified element that might be present, despite the fact that the presence of many of these elements is often routinely determined by the producer.

5.5 The substitution of a grade or composition different from that specified by the purchaser is prohibited.

6. Mechanical Requirements

6.1 The individual product specifications vary as to whether mechanical tests are required; for this reason, and to determine specific test requirements, the individual product specification should be reviewed. If mechanical testing is required by the product specification, sampling shall be in accordance with 4.3 or with Supplementary Requirement S18 as appropriate.

6.2 Unless otherwise specified by the purchaser, when mechanical properties are required by the product specification, test coupons may be taken from castings, may be cast integrally with the castings, or may be cast in separate molds of the same type and material as those used for the castings, in accordance with Fig. 1, Fig. 2, Fig. 3, or Fig. 4, except when Supplementary Requirement S15 is specified. The test coupon

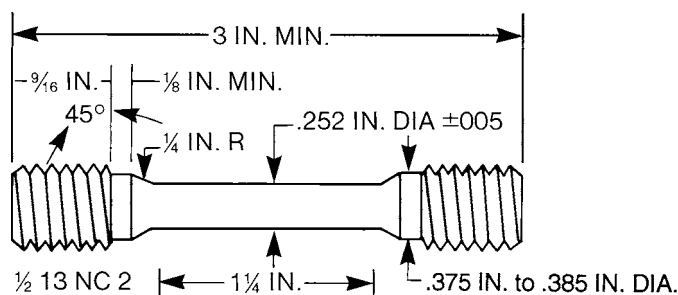

In.	SI Equivalents	[mm]
1/8 *		[3*]
1/4		[5]
.252 ± .005		[6.40 ± 0.15]
.375 to .385*		[9.50-9.75*]
9/16 *		[15*]
1 1/4		[30]
3*		[75*]
1/2 13 NC 2*		[as needed to fit machine]

*Suggested dimension

FIG. 1 Design and Dimensions of the ICI Test Bar

in Fig. 4 shall be employed only for austenitic alloy castings with cross sections less than 2 1/2 in. [65 mm].⁴

6.3 The coupon from which the test specimen is taken shall be heat treated in production furnaces to the same procedure as the castings it represents.

6.4 The specimens may be cast to shape or machined from coupons to dimensions in accordance with Test Methods and Definitions A 370A370 or the ICI bar shown in Fig. 1.

6.5 If any specimen shows defective machining or develops flaws, it may be discarded and another substituted from the same master heat.

6.6 To determine conformance with the tension test requirements, an observed value or calculated value shall be rounded off in accordance with Practice E 29E29 to the nearest 500 psi [5 MPa] for yield and tensile strength and to the nearest 1 % for elongation and reduction of area.

7. Workmanship, Finish, and Appearance

7.1 All castings shall be made in a workmanlike manner and shall conform to the dimensions on drawings furnished by the

⁴ Information on the relationship of mechanical properties determined on test coupons obtained as specified in 6.2 with those obtained from the casting may be found in "The Steel Casting Handbook," Fifth Edition, Steel Founders' Society of America, 1980, pp. 15-35 through 15-43.

purchaser before manufacture is started. If the pattern is supplied by the purchaser or is produced using a die supplied by the purchaser, the dimensions of the casting shall be as predicated by the pattern or die.

8. Quality

8.1 The surface of the casting shall be free of adhering ceramic, scale, cracks, and hot tears as determined by visual examination. Other surface discontinuities shall meet the visual acceptance standards specified in the order. Practice A 997A997 or other visual standards may be used to define acceptable surface discontinuities and finish. Unacceptable visual surface discontinuities shall be removed and their removal verified by visual examination of the resultant cavities.

8.2 When additional inspection is desired, Supplementary Requirements S1, S2, S3, S4, or S5 may be specified.

9. Repair

9.1 Repair by welding shall be in accordance with the requirements of the individual specification using procedures and welders qualified in accordance with Practice A 488/A 488MA488/A488M.

10. Inspection


10.1 The manufacturer shall afford the purchaser's inspector all reasonable facilities necessary to satisfy that the material is being produced and furnished in accordance with the applicable specification. Foundry inspection by the purchaser shall not interfere unnecessarily with the manufacturer's operations. All tests and inspections, with the exception of product analysis (5.3), are the responsibility of the manufacturer.

11. Rejection

11.1 Subsequent to acceptance at the manufacturer's works, material that is found to be unacceptable as determined by requirements specified in the order may be rejected by the purchaser. The manufacturer should be notified of such rejection. If the manufacturer is dissatisfied with the results of any tests performed by the purchaser, he may make claim for a reheating.

12. Keywords

12.1 casting; investment casting; master heat; steel; sub-heat

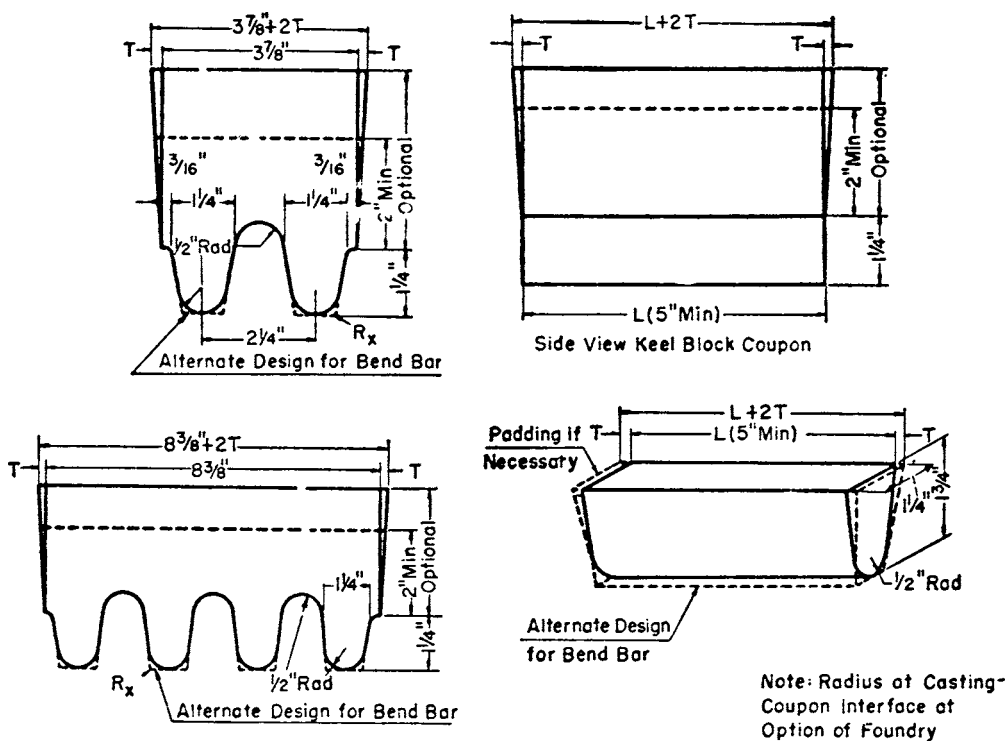


Metric Equivalents

in. [mm]	3/16 [4.8]	1/2 [13]	1 1/4 [32]	1 3/4 [45]	2 [51]	2 1/4 [57]	3 3/8 [98]	5 [127]	8 3/8 [213]
			Leg Design [125 mm]					Riser Design	
1. L (length)			A 5 in. [125 mm] minimum length will be used. This length may be increased at the option of the foundry to accommodate additional test specimens (see Note 1).			1. L (length)	The length of the riser at the base will be the same as the top length of the leg. The length of the riser at the top therefore depends on the amount of taper added to the riser.		
2. End Taper			Use of and size of end taper is at the option of the foundry.			2. Width	The width of the riser at the base of a multiple-leg coupon shall be $n(2\frac{1}{4}) - \frac{5}{8}$ where n equals the number of legs attached to the coupon. The width of the riser at the top is therefore dependent on the amount of taper added to the riser.		
3. Height			1 1/4 in. [32 mm]						
4. Width (at top)			1 1/4 [32 mm] (see Note 1).						
5. Radius (at bottom)			1/2 in. [13 mm], max						
6. Spacing between legs			A 1/2-in. [13-mm] radius will be used between the legs.			3. T (riser taper) Height	Use of and size is at the option of the foundry. The minimum height of the riser shall be 2 in. [51 mm]. The maximum height is at the option of the foundry for the following reasons: (a) many risers are cast open, (b) different compositions may require variation in risering for soundness, and (c) different pouring temperatures may require variation in risering for soundness.		
7. Location of test specimens			The tensile, bend, and impact specimens will be taken from the lower portion of the leg (see Note 2).						
8. Number of legs			The number of legs is at the option of the foundry providing they are equi-spaced according to Item 6.						
9. R _s			Radius from 0 to approximately 1/16 in. [2 mm].						

NOTE 1—*Test Coupons for Large and Heavy Steel Castings*—The test coupons in Fig. 2 are to be used for large and heavy steel castings. However, at the option of the foundry the cross-sectional area and length of the standard coupon may be increased as desired.

NOTE 2—*Bend Bar*—If a bend bar is required, an alternate design (as shown by dotted lines in Fig. 2) is indicated.

FIG. 2 Test Coupons for Castings with Details of Design

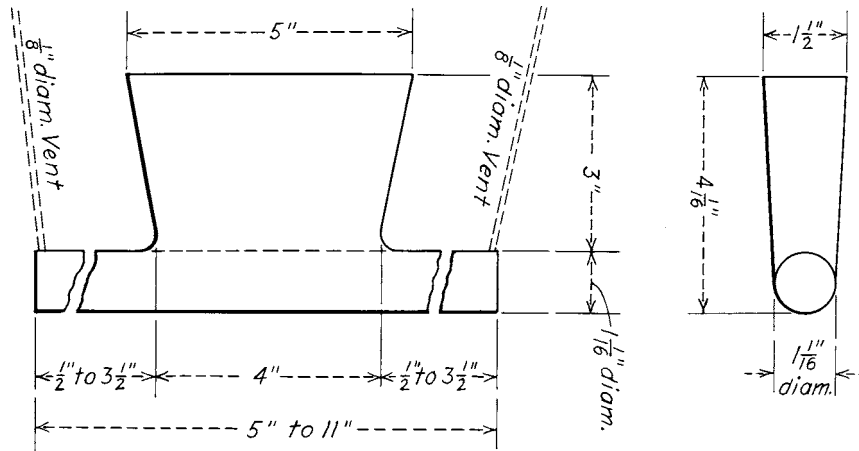

Metric Equivalents

in.	[mm]	in.	[mm]
1/8	[3.2]	3 1/2	[88.9]
1/2	[12.7]	4	[101.6]
1 1/16	[27.0]	4 1/16	[103.2]
1 1/2	[38.1]	5	[127.0]
3	[76.2]	11	[279.4]

NOTE—Pour through head; cover molten head with powdered charcoal, coke dust, and so forth, immediately after pouring, in order to keep head fluid as long as possible.

FIG. 3 Test Block for Tension Test Specimen

iteh standards
<https://standards.iteh.ai>
 Document Preview

[ASTM A957/A957M-09](https://standards.iteh.ai/catalog/standards/sist/246cd6eb-327b-45a7-a5cf-0d881cc6c886/astm-a957-a957m-09)

<https://standards.iteh.ai/catalog/standards/sist/246cd6eb-327b-45a7-a5cf-0d881cc6c886/astm-a957-a957m-09>