

SLOVENSKI STANDARD
oSIST prEN ISO 12800:2019
01-januar-2019

Tehnologija jedrskih goriv - Smernice za merjenje specifične površine prahu uranovega oksida po metodi BET (ISO 12800:2017)

Nuclear fuel technology - Guidelines on the measurement of the specific surface area of uranium oxide powders by the BET method (ISO 12800:2017)

Kernbrennstofftechnologie - Leitlinien für die Messung des spezifischen Oberflächenbereiches von Uranoxid-Pulvern mittels der BET-Methode (ISO 12800:2017)

Technologie du combustible nucléaire - Lignes directrices pour le mesurage de l'aire massique (surface spécifique) des poudres d'oxyde d'uranium par la méthode BET (ISO 12800:2017)

Ta slovenski standard je istoveten z: prEN ISO 12800

ICS:

27.120.30

Cepljivi materiali in jedrska
gorivna tehnologija

Fissile materials and nuclear
fuel technology

oSIST prEN ISO 12800:2019

en,fr,de

INTERNATIONAL STANDARD

ISO
12800

Second edition
2017-06

Nuclear fuel technology — Guidelines on the measurement of the specific surface area of uranium oxide powders by the BET method

*Technologie du combustible nucléaire — Lignes directrices pour le
mesurage de l'aire massique (surface spécifique) des poudres d'oxyde
d'uranium par la méthode BET*

iTeh STANDARD REVIEW
(standards.iteh.ai)

SIST EN ISO 12800:2019

<https://standards.iteh.ai/catalog/standards/sist/4a5e60b1-f2c7-4c39-9cef-285b264f05a9/sist-en-iso-12800-2019>



Reference number
ISO 12800:2017(E)

© ISO 2017

iTeh STANDARD PREVIEW (standards.iteh.ai)

SIST EN ISO 12800:2019

<https://standards.iteh.ai/catalog/standards/sist/4a5e60b1-f2c7-4c39-9cef-285b264f05a9/sist-en-iso-12800-2019>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2017, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	1
4.1 Summary of the BET method	1
4.2 Isothermal adsorption curves.....	1
4.3 Conditions and assumptions.....	2
5 Procedure	3
5.1 Sample preparation	3
5.2 Volumetric measurement	3
5.3 Gravimetric measurement	3
5.4 Original and single-point methods	3
5.5 Dynamic method (carrier gas method)	4
5.6 Alternative methods	4
6 Expression of results	4
6.1 Methods of calculation	4
6.1.1 Multipoint determination	4
6.1.2 Single-point determination	7
6.2 Precision and accuracy.....	7
7 Test report	7
Bibliography	8

SIST EN ISO 12800:2019

<https://standards.itech.ai/catalog/standards/sist/4a5e60b1-f2c7-4c39-9cef-285b264f05a9/sist-en-iso-12800-2019>

ISO 12800:2017(E)

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 85, *Nuclear energy, nuclear technologies, and radiological protection*, Subcommittee SC 5, *Nuclear installations, processes and technologies*.

This second edition cancels and replaces the first edition (ISO 12800:2003), which has been technically revised.

Nuclear fuel technology — Guidelines on the measurement of the specific surface area of uranium oxide powders by the BET method

1 Scope

This document gives guidelines on the determination of the specific surface area of as-fabricated uranium dioxide powder by volumetric or gravimetric determination of the amount of nitrogen adsorbed on the powder, and can be applied to other similar materials, e.g. U_3O_8 , $\text{UO}_2\text{-PuO}_2$ powders, and other bodies with similar surface areas, e.g. powder granules or green pellets, provided that the conditions described are fulfilled. Modifications using other adsorbing gases are included.

The method is relevant as long as the expected value is in the range between $1 \text{ m}^2/\text{g}$ and $10 \text{ m}^2/\text{g}$.

2 Normative references

There are no normative references in this document.

3 Terms and definitions

No terms and definitions are listed in this document.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <http://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

4 Principle

4.1 Summary of the BET method

The BET method is based on the determination of the amount of gas necessary to cover the surface by a monomolecular layer. This amount is determined from the isothermal adsorption curve of nitrogen (N_2) at the temperature of liquid nitrogen (77,4 K) according to Reference [2]. The amount of N_2 adsorbed at a given pressure is determined by volumetric or gravimetric measurement[6]. In order to remove surface contamination of the adsorbent, the sample has to be evacuated and heated under appropriate conditions before the measurement is performed.

4.2 Isothermal adsorption curves

The isothermal adsorption curve describes the relationship between the mass of the adsorbate, m_A (N_2), adsorbed per gram of adsorbent (e.g. UO_2 powder) at an equilibrium pressure of p at constant temperature T , as shown in [Formula \(1\)](#):

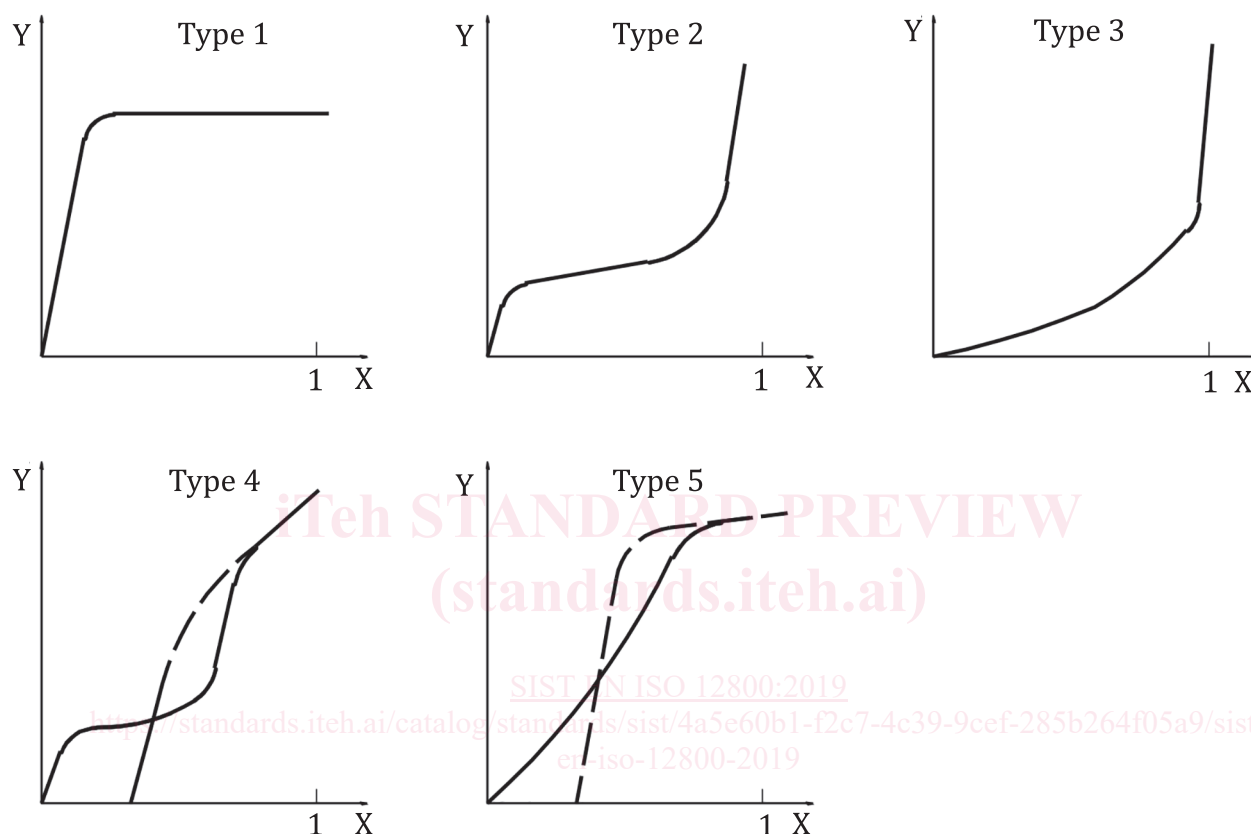
$$m_A = f(p, T) \quad (1)$$

Generally, the relative pressure p/p_0 is introduced instead of the absolute pressure p , where p_0 is the saturation vapour pressure which is $1,013 \times 10^5 \text{ Pa}$ for nitrogen at 77,4 K.

ISO 12800:2017(E)

Most isothermal adsorption curves can be classified according to Reference [3] to be one of the five common types (see Figure 1).

Materials with pure micropores (<2 nm diameter) result in a type 1 adsorption curve. Most frequently, types 2 and 4 adsorption curves are observed where the adsorption energy of the first layer, E_1 , is much higher than that of subsequent layers, E_n . When $E_1 \approx E_n$, type 3 or type 5 adsorption curves result. The BET method can be applied to type 2 and type 4 curves only. The practice shows that the UO_2 , U_3O_8 and PuO_2 powders meet this condition.

**Key**

X	relative pressure
Y	specific amount adsorbed
Type 1	Langmuir type
Type 2	adsorption followed by condensation
Type 3	condensation type
Type 4	two-fold adsorption
Type 5	condensation followed by adsorption

Figure 1 — Classification of adsorption isotherms

4.3 Conditions and assumptions

The method can only be applied to materials where

- nitrogen is not absorbed by the material,
- nitrogen does not react chemically with the adsorbent,
- all pores can be reached by the nitrogen molecule, and

d) a type 2 or type 4 adsorption curve is observed.

The BET theory includes the following assumptions.

- The adsorption energy of the first layer is independent of the degree of occupation. The adsorption energy as well as the kinetic parameters and condensation/evaporation equilibrium conditions for the second and higher layers are equal.
- The probability of adsorption at a vacant site is independent of the occupation of the neighbouring sites.
- Horizontal interactions between the adsorbed N₂ molecules can be neglected.
- The heterogeneity of the adsorbent surface can be neglected.

5 Procedure

5.1 Sample preparation

Impurities on the sample surface, especially water vapour, shall be removed before the adsorption measurement. Conditions for removing impurities (vacuum, temperature, time) have to be found which are compatible with the powder type. Chemical reactions (decomposition), sintering, change of crystal structure and other processes on the surface shall be avoided. Long evacuation periods are needed for highly porous powders. In order to shorten the heating time, the optimum temperature should be determined. In most cases, the measured specific surface area first increases with an increase in the heating temperature and then decreases, e.g. by sintering of the powder.

The optimum pre-treatment of hyperstoichiometric UO₂ powder depends on its specific surface area, intra-particle open pore size, and stoichiometry. For powders with a specific surface area between 2 m²/g and 8 m²/g, evacuation down to 2 mPa to 10 mPa (10⁻⁵ Torr to 10⁻⁴ Torr) followed by heating for 2,5 h at (150 °C ± 10 °C) is sufficient. Equivalent conditions, like 1,5 h at (180 °C ± 10 °C) or others, can be utilized as well. To prevent sintering, heating temperatures higher than 350 °C should be avoided if the O to U ratio exceeds 2,10. Shorter heating times to 20 min are possible. Instead of evacuation, the powder can be purged with purified inert gas at the temperatures and for the times mentioned above after having verified that there is no deleterious effect on characteristics of powders.

Mass of sample required depends upon material density and expected specific surface area.

5.2 Volumetric measurement

The pre-treated sample of known mass is placed in a bulb of calibrated volume, which is filled with nitrogen at a defined temperature and pressure. At ambient temperature and pressure, measurable adsorption does not occur. The closed bulb is cooled to the temperature of liquid nitrogen. The adsorbed amount of nitrogen can be calculated from the amount of nitrogen enclosed in the bulb, the volume, the temperature, and the pressure drop. Accurate volumetric measurements^{[4][5]} can be obtained by measuring the difference in pressure between the sample-containing bulb and an empty reference bulb.

5.3 Gravimetric measurement

In this case, the nitrogen is adsorbed at constant temperature and pressure. The amount of nitrogen adsorbed is directly measured by means of a microbalance.

5.4 Original and single-point methods

The determination of the specific surface area requires the static volumetric or gravimetric measurement of at least three data points of the adsorption curve in the relative pressure region 0,05 < p/p_0 < 0,35. The measurements shall be made under equilibrium conditions.

ISO 12800:2017(E)

If less accuracy is acceptable, the determination can be made easier by application of the single-point method, taking only one point of the adsorption curve in the relative pressure range $0,05 < p/p_0 < 0,35$ ("single-point method").

5.5 Dynamic method (carrier gas method)

The BET method may also be applied in a dynamic, flowing gas system. The relative pressure of the adsorbing gas (p/p_0) is obtained by mixing with an inert gas, usually helium. A stream of this gas mixture is passed over the sample which is cooled to 77,4 K in liquid nitrogen. Nitrogen from the gas stream is adsorbed on the sample.

On warming the sample to ambient temperature, the adsorbed nitrogen is desorbed into the gas stream. The amount of nitrogen desorbed is detected using a katharometer coupled to an integrator. The katharometer is calibrated by an injection of pure nitrogen.

5.6 Alternative methods

Modified methods use other adsorptives and other temperatures (see [Table 1](#)). The occupied areas per adsorbed molecule (or atom in the case of argon, krypton, and xenon) are also reported in [Table 1](#).

Another indirect method is the tracer method^{[8][9]}, where the amount of a radioactive adsorbed gas is determined by activity measurements.

Table 1 — Occupied areas per adsorbed molecule

Gas	Temperature K	Saturation pressure, p_0 Pa	Occupied area ^a per molecule nm ²
Nitrogen	77,4	$1,01 \times 10^5$	0,162
Argon	77,4	$2,58 \times 10^4$	0,138
Argon	87,3	$1,33 \times 10^5$	0,142
Krypton	77,4	$2,66 \times 10^2$	0,202
Krypton	90,2	$2,27 \times 10^2$	0,214
Xenon	90,2	8,00	0,232
^a Standard values.			

6 Expression of results

6.1 Methods of calculation

6.1.1 Multipoint determination

The so-called BET equation is given by [Formula \(2\)](#):

$$V_A = \frac{V_m \cdot C \cdot p_r}{(1 - p_r)(1 - p_r + C \cdot p_r)} \quad (2)$$