

SLOVENSKI STANDARD oSIST prEN ISO 12183:2019

01-januar-2019

Tehnologija jedrskih goriv - Kulometrična analiza plutonija z nadzorovanim potencialom (ISO 12183:2016)

Nuclear fuel technology - Controlled-potential coulometric assay of plutonium (ISO 12183:2016)

Kernbrennstofftechnologie - Coulometrische Bestimmung von Plutonium mit kontrolliertem Potential (ISO 12183:2016)

Technologie du combustible nucléaire - Dosage du plutonium par coulométrie à potentiel imposé (ISO 12183:2016)

Ta slovenski standard je istoveten z: prEN ISO 12183

ICS:

27.120.30 Cepljivi materiali in jedrska

gorivna tehnologija

Fissile materials and nuclear

fuel technology

oSIST prEN ISO 12183:2019 en,fr,de

oSIST prEN ISO 12183:2019

iTeh STANDARD PREVIEW (standards.iteh.ai)

SIST EN ISO 12183:2019

https://standards.iteh.ai/catalog/standards/sist/33947a1b-41a8-454d-921c-b82df74b9df5/sist-en-iso-12183-2019

oSIST prEN ISO 12183:2019

INTERNATIONAL STANDARD

ISO 12183

Third edition 2016-08-15

Nuclear fuel technology — Controlledpotential coulometric assay of plutonium

Technologie du combustible nucléaire — Dosage du plutonium par coulométrie à potentiel imposé

iTeh STANDARD PREVIEW (standards.iteh.ai)

<u>SIST EN ISO 12183:2019</u> https://standards.iteh.ai/catalog/standards/sist/33947a1b-41a8-454d-921c



Reference number ISO 12183:2016(E)

iTeh STANDARD PREVIEW (standards.iteh.ai)

SIST EN ISO 12183:2019
https://standards.iteh.ai/catalog/standards/sist/33947a1b-41a8-454d-921c-b82df74b9df5/sist-en-iso-12183-2019



COPYRIGHT PROTECTED DOCUMENT

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office Ch. de Blandonnet 8 • CP 401 CH-1214 Vernier, Geneva, Switzerland Tel. +41 22 749 01 11 Fax +41 22 749 09 47 copyright@iso.org www.iso.org

| Contents | | | Page |
|---|---|--|----------------------|
| Fore | Foreword | | |
| 1 | Scope | | 1 |
| 2 | Norm | native references | 1 |
| 3 | Terms and definitions | | |
| | | | |
| 4 | | iple | |
| 5 | _ | ents | |
| 6 | Appa | Apparatus | |
| 7 | Proce 7.1 | edure Plutonium determination 7.1.1 Weighing the test sample, with an uncertainty of ±0,01 %, K = 1 | 8 9 |
| | | 7.1.3 Electrode pre-treatment 7.1.4 Electrical calibration of the current integration system 7.1.5 Formal potential determination 7.1.6 Coulometric blank determination 7.1.7 Plutonium measurement | 10 11 12 |
| | 7.2 | Analysis of subsequent test samples | |
| 8 | 8.1 8.2 8.3 8.4 8.5 | Calculation of the electrical calibration factor Calculation of the blank Fraction of electrolysed plutonium Plutonium content Quality control | 14 15 16 |
| 9 | Characteristics of the method | | 16 |
| | 9.1 9.2 9.3 | Repeatability Confidence interval Analysis time | 17 |
| 10 | Inter | ferences | 17 |
| 11 | Proce 11.1 11.2 11.3 11.4 11.5 11.6 11.7 11.8 11.9 | Accountability measurements and reference material preparation Process control measurements Measurement cell design Electrolyte and electrode options Test sample size Background current corrections Correction for iron Control-potential adjustment Calibration methodologies | 21 21 22 22 22 23 24 |
| Annex A (normative) Purification by anion-exchange separation | | | 25 |
| Annex B (normative) Determination of formal potential, E ₀ | | | 27 |
| Rihliogranhy | | | 28 |

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html.

The committee responsible for this document is Technical Committee ISO/TC 85, *Nuclear energy, nuclear technologies, and radiological protection*, Subcommittee SC 5, *Nuclear fuel cycle*.

This third edition cancels and replaces the second edition (ISO 12183:2005), which has been technically revised.

h82df74h9df5/sist-en-iso-12183-2019

Nuclear fuel technology — Controlled-potential coulometric assay of plutonium

1 Scope

This document describes an analytical method for the electrochemical assay of pure plutonium nitrate solutions of nuclear grade, with a total uncertainty not exceeding $\pm 0.2\%$ at the confidence level of 0.95 for a single determination (coverage factor, K = 2). The method is suitable for aqueous solutions containing more than 0.5 g/L plutonium and test samples containing between 4 mg and 15 mg of plutonium. Application of this technique to solutions containing less than 0.5 g/L and test samples containing less than 4 mg of plutonium requires experimental demonstration by the user that applicable data quality objectives will be met.

For some applications, purification of test samples by anion exchange is required before measurement to remove interfering substances when present in significant amounts. Refer to <u>Clause 10</u> for a discussion of interferences and corrective actions. Purification is also appropriate in situations where the purity of the test sample is unknown or when it may fluctuate unpredictably in a manufacturing process.

<u>Clause 11</u> discusses the changes in application of the method and methodology that can be applied and important considerations when selecting measurement parameters, while still remaining within the intended scope of this document.

2 Normative references tandards.iteh.ai)

There are no normative references in this document.

https://standards.iteh.ai/catalog/standards/sist/33947a1b-41a8-454d-921c-

3 Terms and definitions df74b9df5/sist-en-iso-12183-2019

No terms and definitions are listed in this document.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- IEC Electropedia: available at http://www.electropedia.org/
- ISO Online browsing platform: available at http://www.iso.org/obp

4 Principle

The key steps and their purposes are outlined below:

- test samples are prepared by weighing and then fuming to dryness with sulphuric acid to achieve a
 consistent and stable anhydrous plutonium sulphate salt that is free from chloride, fluoride, nitrate,
 nitrite, hydroxylamine, and volatile organic compounds;
- if needed to remove interferences, dissolve test samples and purify by anion exchange, then fume
 the eluted plutonium solution in the presence of sulphuric acid to obtain the dry plutonium sulphate
 chemical form;
- measure a blank of the nitric acid supporting electrolyte and calculate the background current correction applicable to the electrolysis of the test sample from charging, faradaic, and residual current[1];
- dissolve the dried test sample in the previously measured supporting electrolyte (the blank);

- reduce the test sample at a controlled potential that electrolyses the plutonium to greater than 99,8 % Pu³⁺ and measure the equilibrium solution potential at the end of this step by control-potential adjustment^[2];
- oxidize the test sample at a controlled potential that electrolyses the plutonium to greater than 99,8 % Pu⁴⁺ and measure the equilibrium solution potential at the end of this electrolysis by controlpotential adjustment;
- correct the result for the background current and the fraction of plutonium not electrolysed;
- calibrate the coulometer using traceable electrical standards and Ohm's Law;
- use the measured value of the coulometer calibration factor and the Faraday constant to convert the coulombs of integrated current from the electrolyses to moles of plutonium;
- use traceable quality-control plutonium standards to demonstrate independently the performance of the measurement system;
- periodically measure the formal potential of the plutonium couple, E_{0} , which is user-specific based on the cell design, connections, reference electrode type, and the acid-type and molarity of the supporting electrolyte.

These steps ensure that representative, reproducible, and stable test samples are prepared for measurement. The test samples are measured using a protocol that is based upon first principles and is consistent with a traceable, electrical calibration of the coulometer. Additional details are provided in Clauses 10 and 11.

5 Reagents

Use only analytical grade reagents.

All aqueous solutions shall be prepared with double-distilled or distilled, demineralized water with a resistivity greater than $10 \text{ M}\Omega \cdot \text{cm}$, i.e. ISO 3696 Grade 1 purified water.

5.1 Nitric acid solution, c (HNO₃) = 0.9 mol/L.

NOTE Refer to 11.4 for other electrolyte options.

- **5.2** Amidosulphuric acid solution, c (NH₂HSO₃) = 1.5 mol/L.
- **5.3 Sulphuric acid solution,** $c(H_2SO_4) = 3 \text{ mol/L}.$

NOTE Molarity is not a critical parameter for sulphuric acid used to fume plutonium test samples, provided the concentration of the reagent is well above the level where colloidal plutonium complexes form.

- **5.4 Pure argon or nitrogen,** $(O_2 \text{ content lower than } 10 \text{ ppm}).$
- **5.5 Pure air,** free of organic contaminants.

6 Apparatus

Usual laboratory equipment found in a medium-activity radiochemical laboratory suitable for work with plutonium shall be used.

6.1 Analytical balance, installed in radiological containment unit and must be capable of weighing 1 g mass, with an uncertainty of ± 0.1 mg (coverage factor, K = 1). This represents a relative uncertainty of 0.01 %.

- Weighing less than 1 g will increase the relative uncertainty to >0,01 %, in an inversely proportional manner.
- If the uncertainty of the balance, as installed, does not meet the ±0,01 mg criterion, then correspondingly larger test samples are required.
- **6.2 Weighing burette,** glass or plastic, the material selection is not critical provided it maintains a stable mass (tare weight) and static charge is controlled as described in <u>7.1.1</u>.
- **6.3 Equipment for test sample evaporation in the coulometric cell,** comprising of an overhead radiant heater or hot-plate with controls to adjust temperature. Design requirements and optional features for effective evaporation and fuming include:
- providing settings that allow both rapid and well-controlled rate of initial evaporation, followed by fuming the remaining sulphuric acid solution to dryness at a higher temperature;
- preventing mechanical loss of the test sample solution from boiling and/or spattering;
- preventing contamination by extraneous chemicals, such as those which may be used to neutralize acid vapours;
- heating of the coulometer cell wall to optimize fuming and minimize refluxing of sulphuric acid by placing the cell inside an optional aluminium tube with an inner diameter that is 1 mm to 3 mm larger than the outer diameter of the cell and a height that is 1 mm to 5 mm shorter than the cell may be placed around the cell during the fuming step to heat the walls of the cell;
 - NOTE An aluminium block with holes bored to a similar specification for inserting the cell may be used instead of the aluminium tubes.
- addition of an optional air supply with the delivery tube directed towards the surface of the liquid to optimize the evaporation rate and disperse the acid fumes;
- addition of an optional vapour capture and local neutralization to control acid fumes, depending upon facility design and ventilation system requirements.

See Figure 1.

Dimensions in centimetres

Figure 1 — Sample evaporation system

6.4 Controlled-potential coulometer. and ards. iteh.ai)

See Figure 2.

SIST EN ISO 12183:2019

6.4.1 Coulometer cell assembly, comprising the following:

a stirrer motor with a rotation frequency of at least 1 000 min⁻¹;

NOTE 1 Adjustable-speed motors allow optimizing rotation rates for individual cell designs. Stirrer motors powered by isolated DC power supplies are desirable to prevent electrical noise from being superimposed on the blank and test sample electrolysis current signals sent to the integrator.

- a cylindrical or tapered glass coulometric cell of capacity 50 mL, or less, with an O-ring seal and a tight-fitting lid with openings to insert the following internal equipment:
 - an inlet tube for humidified, inert gas to displace dissolved and atmospheric oxygen from the solution and the electrolysis cell, respectively;
 - a stirrer with blade and shaft made from chemically inert materials [e.g. polytetrafluoroethylene (PTFE)], and designed to prevent splashing; the shaft of the stirrer is typically located in the centre of the cell and connected directly to the stirrer motor;
 - a working electrode made of gold (e.g. 99,99 %) and consisting of a gold wire welded or machined to a cylindrical gold wire frame, nominally 15 mm high and 20 mm in diameter, around which is welded or machined a very fine gold mesh, which is typically several layers (e.g. four layers);


NOTE 2 Refer to 11.4 for other working electrode options.

- a glass tube plugged at the bottom end with a sintered-glass disc (typical dimensions of 2,5-mm thick and pore size $<0.01 \mu m$), the tube filled with nitric acid (5.1) and the tip of the sintered-glass end positioned within the ring of the working electrode;
- a reference electrode, saturated calomel electrode (SCE), or other reference electrodes as described in 11.3, is inserted into the glass tube;

- another glass tube, similar to the first one, also filled with nitric acid (5.1), and the tip of the sintered-glass end positioned within the ring of the working electrode;
- an auxiliary electrode consisting of a platinum wire, 0,5 mm to 3,0 mm in diameter, is inserted into the second glass tube;
 - NOTE 3 The platinum wire may be coiled to increase the surface area submerged in the supporting electrolyte, as illustrated in Figure 2.
- a gas washer bottle, filled with reagent water as described in <u>Clause 5</u>, to humidify the inert gas before it is introduced into the coulometer cell assembly.

The diameter of the glass tube and sintered-glass disc containing the auxiliary electrode may be larger than that of the glass tube and sintered-glass disc containing the reference electrode. The flow rate of the solution through both glass discs shall be less than 0,05 mL/h.

- a) A thermocouple or resistance thermometer installed in the coulometer cell assembly for measuring the temperature of the test sample solution during the measurement process is an optional feature. The solution temperature should be measured either during the oxidation of the test sample or immediately following the analysis. An uncertainty goal for the temperature measurement is ± 0.2 °C (K = 1).
 - If it is not possible to insert a temperature sensor into the electrolysis cell or not desirable to measure the temperature of the test sample solution immediately after the electrolysis is completed, then estimate the solution temperature from the ambient air temperature or the reagent temperature. Note that the purge gas is cooled by expansion causing the solution temperature to decrease relative to the ambient temperature; the extent of this decrease is a function of the inert-gas flow rate and the cell design. The measured air or reagent temperature value must be corrected for this cooling effect. A higher uncertainty of ± 1 °C, K = 1, is expected in the calculated solution temperature.
- b) For optimum potential control, position the sintered-glass discs of the reference and auxiliary electrodes glass tubes to meet the following requirements: 10-4188-454d-921c-
 - the closest distance from the reference electrode sintered-glass disc to the working electrode is 2 mm or less;
 - the distance between the two sintered-glass discs containing the auxiliary and reference electrodes is less than the distance between the auxiliary electrode disc and the nearest point on the working electrode.
- c) The hole through which the stirrer shaft is inserted serves as the primary escape vent for the inert gas. Except for this hole, all other insertions are tight fitting. The inert-gas flow rate must be sufficiently high to quickly remove oxygen from the supporting electrolyte and the test sample solution. Furthermore, it must prevent leakage of air into the cell assembly during the electrolysis. A practical guide for adjusting the flow rate is to direct all or part of the inert gas supply toward the solution, such that a 2 mm to 4 mm dimple is formed on the surface without causing the solution to splash.
 - Cell assemblies with an optimized design, an adequate inert-gas flow rate, and a tight fit, will remove oxygen in 5 min or less. The time required to remove oxygen from the solution should be established by users based on testing of their cell assembly under routine conditions.

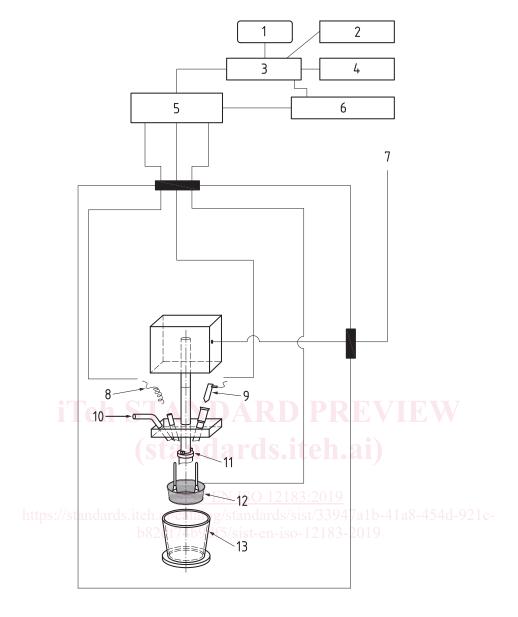

Key

- 1 video
- 2 printer (optional)
- 3 control computer
- 4 keyboard
- 5 potentiostat and integrator
- 6 digital voltmeter (DVM)
- 7 AC/DC power for stirring motor

- 8 auxiliary (or counter) electrode in bridge tube filled with supporting electrolyte
- 9 reference electrode in bridge tube filled with supporting electrolyte
- 10 inert gas
- 11 stirrer
- 12 working electrode
- 13 cell

Figure 2 — Coulometric cell assembly connections

6.4.2 Instrumentation, comprising the following[3][4]:

- a) Potentiostat with the desired range of electrolysis potentials for plutonium measurement and the following capabilities:
 - a power amplifier with a current output capability of 250 mA, or greater;