
**Implants for surgery — Wear of total
knee prostheses —**

**Part 5:
Durability performance of the
patellofemoral joint**

Implants chirurgicaux — Usure des prothèses totales du genou —

*Partie 5: Performance de durabilité de l'articulation fémoro-
patellaire*

ITeH Standards
(<https://standards.iteh.ai>)
Document Preview

[ISO 14243-5:2019](https://standards.iteh.ai/catalog/standards/iso/4bc824ad-14c4-41ec-b4e0-3cf8b6119947/iso-14243-5-2019)

<https://standards.iteh.ai/catalog/standards/iso/4bc824ad-14c4-41ec-b4e0-3cf8b6119947/iso-14243-5-2019>



iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

[ISO 14243-5:2019](https://standards.iteh.ai/catalog/standards/iso/4bc824ad-14c4-41ec-b4e0-3cf8b6119947/iso-14243-5-2019)

<https://standards.iteh.ai/catalog/standards/iso/4bc824ad-14c4-41ec-b4e0-3cf8b6119947/iso-14243-5-2019>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2019

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Fax: +41 22 749 09 47
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword.....	iv
Introduction.....	v
1 Scope.....	1
2 Normative references.....	1
3 Terms and definitions.....	1
4 Principle.....	4
5 Reagents and materials.....	5
6 Test specimen and number of samples.....	5
7 Apparatus.....	5
8 Procedure.....	11
9 Test report.....	15
10 Disposal of test specimen.....	15
Bibliography.....	16

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

[ISO 14243-5:2019](https://standards.iteh.ai/catalog/standards/iso/4bc824ad-14c4-41ec-b4e0-3cf8b6119947/iso-14243-5-2019)

<https://standards.iteh.ai/catalog/standards/iso/4bc824ad-14c4-41ec-b4e0-3cf8b6119947/iso-14243-5-2019>

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 150, *Implants for surgery*, Subcommittee SC 4, *Bone and joint replacements*.

A list of all parts in the ISO 14243 series can be found on the ISO website.

The main changes compared to the previous edition are as follows:

- In Clause 4, Principle: Total number of cycles has been changed from 220 000 to 50 000;
- [3.14](#), [3.15](#) and [3.16](#) have been changed;
- Figures have been renumbered;
- Failure and damage pattern ([8.14](#)) has been updated;
- a Typo in [Formula \(2\)](#) has been corrected.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

This document is applied for the qualitative visual assessment of durability of an ultra-high molecular weight polyethylene patella when articulating against a femoral component by observing the occurrence of delamination, cracking, or other damage characteristics that occur as a result of the specified displacement and loading inputs.

This standard test method is comprehensive, but it needs to be noted that it is complex to implement - maybe the most complex in its particular field. The reader/user needs to note that:

- 1) The main compressive force waveforms are to be calculated to suit the individual implant (size).
- 2) The waveforms for the kinematics on two testing actuators are calculated to suit the particular geometry of the implant tested involving sophisticated CAD measurements, and in each case thorough care is needed when using degrees or radians for the angle computations in setting up the test.
- 3) Intricate friction sensitive medial-lateral force imposing fixtures are involved, with measurement needed of such force to be provided on the testing machines.

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

[ISO 14243-5:2019](https://standards.iteh.ai/catalog/standards/iso/4bc824ad-14c4-41ec-b4e0-3cf8b6119947/iso-14243-5-2019)

<https://standards.iteh.ai/catalog/standards/iso/4bc824ad-14c4-41ec-b4e0-3cf8b6119947/iso-14243-5-2019>

Implants for surgery — Wear of total knee prostheses —

Part 5: Durability performance of the patellofemoral joint

1 Scope

This document specifies the relative angular movement between articulating patellofemoral joint components, the pattern of the applied force, speed and duration of testing, sample configuration and test environment to be used for the durability testing of total knee-joint prostheses in wear-testing machines with load control and displacement.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 5833, *Implants for surgery — Acrylic resin cements*

ISO 7207-1, *Implants for surgery — Components for partial and total knee joint prostheses — Part 1: Classification, definitions and designation of dimensions*

ISO 14243-1, *Implants for surgery — Wear of total knee-joint prostheses — Part 1: Loading and displacement parameters for wear-testing machines with load control and corresponding environmental conditions for test*

ISO 14243-2, *Implants for surgery — Wear of total knee-joint prostheses — Part 2: Methods of measurement*

ISO 14243-3, *Implants for surgery — Wear of total knee-joint prostheses — Part 3: Loading and displacement parameters for wear-testing machines with displacement control and corresponding environmental conditions for test*

ASTM F2003, *Standard Practice for Accelerated Aging of Ultra-High Molecular Weight Polyethylene after Gamma Irradiation in Air*


3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 7207-1 and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

Applied nomenclature is illustrated in [Figure 1](#).

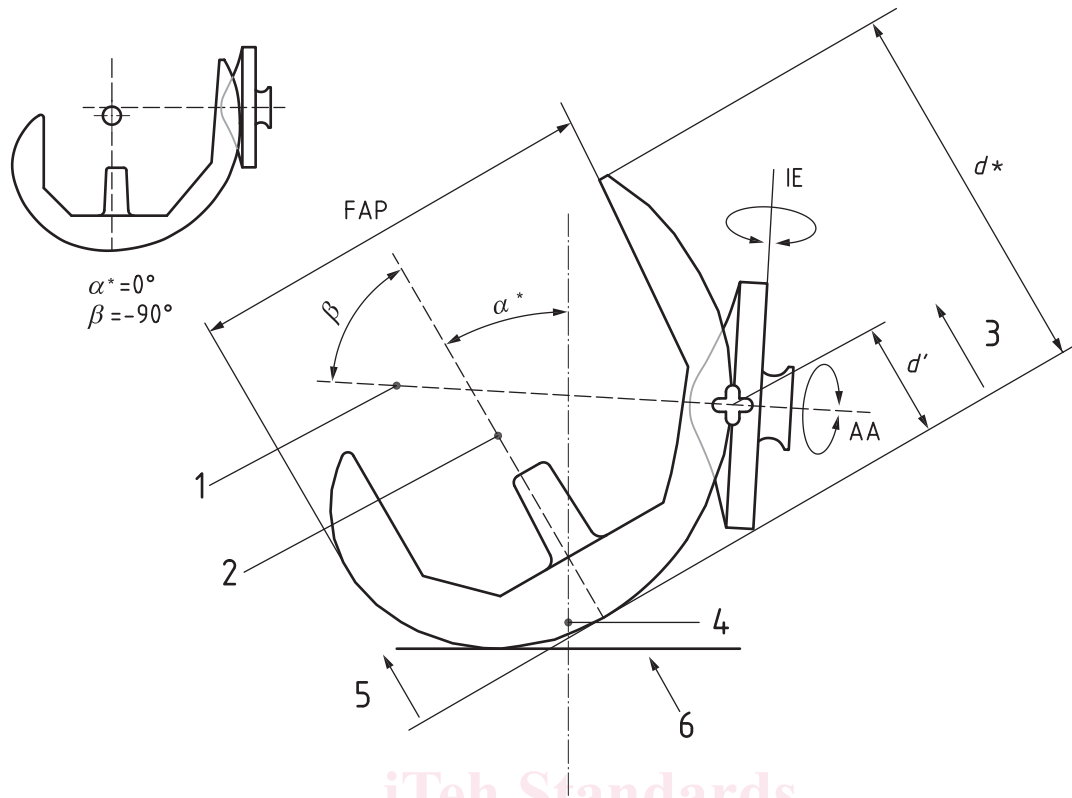

Key	
1	patellar axis
2	femoral axis
3	positive values for d'
4	tibial axis
5	negative values for d'
6	tibial plane
α^*	tibiofemoral flexion angle
β	patellofemoral angle
d^*	femoral height
d'	patellar location
IE	internal/external rotation
AA	abduction/adduction
FAP	functional A-P

Figure 1 — Nomenclature

3.1

femoral axis

imaginary line that is orthogonal to the tibial plane and bisects the midpoint of the line that connects the deepest (most distal) points of both condyles at 0° tibiofemoral flexion

3.2

patellar axis

imaginary line, orthogonal to the patellar component backface plane, passing through the peak of the articulation surface of the patellar component

3.3

tibial axis

nominal longitudinal axis of the tibia, corresponding to the central axis of the medullary cavity of the proximal tibia

Note 1 to entry: At 0° tibiofemoral flexion, the tibial axis is parallel with the femoral axis

3.4

tibial plane

imaginary plane orthogonal to the tibial axis

3.5 tibiofemoral flexion angle

α^*

angle in the sagittal plane between the tibial axis and the femoral axis

Note 1 to entry: This value is considered to be positive in the direction of tibiofemoral flexion and negative in the direction of tibiofemoral hyperextension.

Note 2 to entry: The unit of measure for the tibiofemoral flexion angle is degrees.

3.6 patellofemoral angle

β

angle in the sagittal plane between the patellar axis and the femoral axis

Note 1 to entry: The machine flexion-extension waveform is based on the patellofemoral angle.

Note 2 to entry: The coordinate system that describes this parameter is non-intuitive, since the *in vivo* rotation centre is not static. For simplicity when being applied as the machine flexion-extension angle the patellofemoral angle is defined mathematically in [Formula \(1\)](#), and its unit of measure is degrees.

$$\beta = 0,7\alpha^* - 90 \quad (1)$$

3.7 femoral height

d^*

overall height of the femoral component

Note 1 to entry: It is the distance between the most proximal point of the anterior flange and the most distal condylar point. For a bi compartmental knee, the femoral height is the sum of parameters d and g , according to ISO 7207-1.

Note 2 to entry: The unit of measure for the overall height of the femoral component is millimetres.

3.8 patellar location

d'

distance to translate the patella fixture on the test simulator to complement the femoral component rotation to achieve effective wrapping of the patella around the femoral component during knee flexion

Note 1 to entry: d' is an offset distance between the perceived intersection of the femoral component articulating surface and the patellar axis in the sagittal plane when the patella is contacting the femoral component either in the trochlear groove or between the condyles.

Note 2 to entry: d' changes in sign when the patella and femoral axis line up, such that positive values of d' occur when the patella is located anteriorly to the femoral axis; while negative values of d' occur posteriorly to the femoral axis.

Note 3 to entry: The unit of measure for the patellar location is millimetres.

3.9 functional A-P

FAP

distance in the anterior-posterior direction orthogonal to the femoral axis of the femoral component, between the most proximal, interior point of the anterior flange and the most posterior point along the condyle

Note 1 to entry: The unit of measure for the FAP dimension is millimetres.

3.10

patellar internal/external rotation

rotation about an axis that is orthogonal to the patellar axis and is parallel to the tibial and femoral axes at 0° tibiofemoral flexion

3.11

patellar abduction/adduction rotation

rotation around the patella axis

Note 1 to entry: Rotation is positive (abduction) for a left knee when the patella rotates clockwise when viewed from anterior. It is positive (abduction) for a right knee when the patella rotates counter clockwise when viewed from anterior.

3.12

cycle limit

number of cycles at which the test is terminated if no functional failure has occurred

3.13

mediolateral force

force acting parallel to the femoral flexion-extension axis

3.14

patellar translation

Y

measure between the patellar axis and the flexion extension axis measured orthogonally to the patellar axis (see 8.7)

Note 1 to entry: The unit of measure for Y is millimetres.

3.15

femoral flexion/extension axis

nominal axis of rotation of the femoral component

3.16

similar device

device that is defined as a legally marketed device with significant human clinical experience and for which there is evidence showing it has performed well in clinical use (absence of product-related recalls and/or statistically-significant number of failures) and that has the same intended use, similar materials, and similar design (for example, fixation, modularity, features, key dimensions, surface treatment, etc.)

Note 1 to entry: Identification of a similar device is at the discretions of the manufacturer in accordance with the regulatory requirements in the jurisdictions where the device is marketed.

4 Principle

This document describes a durability testing method which uses cyclic waveforms that simulate the patellofemoral kinetics and kinematics by combining a squatting sub-cycle with two low flexion sub-cycles based on individual knee design characteristics. Loading and displacement waveforms are performed until delamination, cracking, or another identified failure mode occurs. If the implants do not demonstrate any failure modes (8.14) by 50 000 cycles, the test can be stopped. The value of 50 000 is based on laboratory experience gained by comparing the results of delaminated components with retrieved components. The squatting sub-cycle simulates up to 120° of tibiofemoral flexion at a rate of 1/3 Hz with a compressive load range from 0,5 to 3 times body weight. The low flexion (walking) sub-cycles simulate 0° to 58° of tibiofemoral flexion at a rate of 1,1 Hz ± 0,1 Hz and ranges from 0,3 to 0,5 times body weight. The resulting cycle time is 4,82 s. The low flexion sub-cycles challenge the dome of the patella whereas the squat sub-cycle challenges the periphery of the patella.