
**Brown coals and lignites —
Determination of the volatile matter
in the analysis sample: one furnace
method**

*Charbons bruns et lignites — Détermination des matières volatiles
dans l'échantillon pour analyse : méthode avec utilisation d'un four*

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[ISO 20360:2020](https://standards.iteh.ai/catalog/standards/sist/9341e2c9-3860-4df4-b586-9b7162693305/iso-20360-2020)

<https://standards.iteh.ai/catalog/standards/sist/9341e2c9-3860-4df4-b586-9b7162693305/iso-20360-2020>



iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 20360:2020

<https://standards.iteh.ai/catalog/standards/sist/9341e2c9-3860-4df4-b586-9b7162693305/iso-20360-2020>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2020

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword.....	iv
Introduction.....	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	1
5 Reagent and materials	2
6 Apparatus	2
7 Preparation of test sample	8
7.1 Preparation of the general analysis test sample.....	8
7.2 Preparation of the sample pellets.....	8
8 Procedure	8
8.1 Furnace temperature check.....	8
8.2 Crucible and lid process.....	9
8.3 Volatile matter determination.....	9
9 Expression of results	9
10 Precision	10
10.1 Repeatability limit.....	10
10.2 Reproducibility limit.....	10
11 Test report	10
Bibliography	12

iTech STANDARD PREVIEW
(standards.iteh.ai)

[ISO 20360:2020](https://standards.iteh.ai/catalog/standards/sist/9341e2c9-3860-4df4-b586-9b7162693305/iso-20360-2020)

<https://standards.iteh.ai/catalog/standards/sist/9341e2c9-3860-4df4-b586-9b7162693305/iso-20360-2020>

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 27, *Coal and coke*, Subcommittee SC 5, *Methods of analysis*.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

The volatile matter is determined as the loss in mass, corrected for moisture, when an analysis sample of brown coals or lignites is heated out of contact with air under specified conditions. Due to the nature of brown coals and lignites, the sample being pressed and cut into small pellets is necessary to minimize the possibility of ejection of sample from the test crucible when the sample is heated at 900 °C, which has been demonstrated for its good precision and accuracy, and applied in GB/T 212 for many years. Results obtained by this method agree with measurements of volatile matter content by ISO 5071-1.

The test of volatile matter is empirical and, in order to obtain reproducible results, it is essential that the rate of heating, the final temperature and the overall duration of the test are carefully controlled. It is also essential to exclude air from the coal during heating to prevent oxidation. The fit of the crucible lid is, therefore, critical. The moisture content of the sample is determined at the same time as the volatile matter so that the appropriate correction can be made.

To arrive at a valid comparison of volatile matter results conducted in different laboratories, it is essential that the moisture condition of the test samples in the two laboratories is within the expected variance of the moisture test. If a sample is re-equilibrated with the laboratory atmosphere or partially dried in one laboratory and not the other then oxidation can and will most definitely occur for brown coals and lignites. Oxidation will alter the, as-determined, volatile matter of a test sample.

The dry basis precision for volatile matter includes a variance contribution from the moisture determination and potentially a covariance component, both of which can influence the precision statistics for volatile matter on a dry basis.

Mineral matter associated with the sample may also lose mass under the conditions of the test, the magnitude of the loss being dependent on both the nature and the quantity of the minerals present.

ISO 20360:2020
<https://standards.iteh.ai/catalog/standards/sist/9341e2c9-3860-4df4-b586-9b7162693305/iso-20360-2020>

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 20360:2020

<https://standards.iteh.ai/catalog/standards/sist/9341e2c9-3860-4df4-b586-9b7162693305/iso-20360-2020>

Brown coals and lignites — Determination of the volatile matter in the analysis sample: one furnace method

1 Scope

This document specifies a method of determining the volatile matter of brown coals and lignites by the one furnace method.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1170, *Coal and coke — Calculation of analyses to different bases*

ISO 1213-2, *Solid mineral fuels — Vocabulary — Part 2: Terms relating to sampling, testing and analysis*

ISO 5068-2, *Brown coals and lignites — Determination of moisture content — Part 2: Indirect gravimetric method for moisture in the analysis sample*

ISO 13909-4, *Hard coal and coke — Mechanical sampling — Part 4: Coal — Preparation of test samples*

ISO 18283, *Hard coal and coke — Manual sampling*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 1213-2 and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

— ISO Online browsing platform: available at <https://www.iso.org/obp>

— IEC Electropedia: available at <http://www.electropedia.org/>

3.1

total volatile matter

$w_{V,T}$

fractional loss in mass, without correction for moisture, when a solid mineral fuel is heated out of contact with air under specified conditions

3.2

volatile matter

loss in mass, corrected for moisture, when a solid mineral fuel is heated out of contact with air under specified conditions

[SOURCE: ISO 1213-2:2016, 3.239]

4 Principle

A portion of the general analysis sample which is pressed and cut into pellets with the side length of about 3 mm is heated out of contact with air at 900 °C for 7 min. The percentage mass fraction of volatile matter is calculated from the loss in mass of the test portion after deducting the loss in mass due to moisture.

5 Reagent and materials

5.1 Desiccant, fresh or freshly regenerated and preferably self-indicating. Suitable desiccants are magnesium perchlorate and silica gel.

WARNING — Magnesium perchlorate is a strong oxidizing agent. Do not attempt to regenerate the absorbent. Do not permit contact with organic materials or a reducing agent.

6 Apparatus

6.1 Furnace, heated by electricity, in which a zone of uniform temperature of $900\text{ °C} \pm 5\text{ °C}$ can be maintained (see [Figure 1](#), which is the same as the one given in ISO 562:2010, Figure 1).

It may be of the stop-ended type or fitted at the back with a flue approximately 25 mm in diameter and 150 mm in length.

It is important for furnaces with flues that the furnace door seals well. The flue should not reach far out of the oven and should be fitted with a butterfly valve to restrict airflow through the furnace.

The heat capacity of the furnace should be such that, with an initial temperature of 900 °C , the temperature of $900\text{ °C} \pm 10\text{ °C}$ is regained within 3 min after insertion of a cold stand and its crucibles. The temperature shall be measured with a thermocouple as described in [6.2](#). The initial temperature of 900 °C may be adjusted to a temperature determined by calibration that will guarantee the furnace temperature of $900\text{ °C} \pm 10\text{ °C}$ is regained within 3 min after insertion of the cold stand and its crucible(s).

The furnace is designed specifically either for multiple determinations using a number of crucibles in one stand or for receiving one crucible and its stand. In the first case, the zone of uniform temperature shall be at least $160\text{ mm} \times 100\text{ mm}$; in the latter case, a zone with a diameter of 40 mm is sufficient.

A position for the crucible stand shall be chosen within the zone of uniform temperature and this position shall be used for all determinations.

6.2 Thermocouple, unsheathed.

The thermo-junction shall be inserted midway between the base of the crucibles in its stand and the floor of the furnace from which there is 20 mm to 30 mm distance. If the stand holds more than one crucible, the temperature under each crucible shall be checked in the same manner.

If desired, a sheathed thermocouple may be permanently installed in the furnace with the thermo-junction as close as possible to the centre of the zone of uniform temperature; in this case its temperature readings shall be correlated at frequent intervals with those of the unsheathed thermocouple, which is thus inserted only when necessary.

NOTE The thermal/electromotive force relationship of a thermo-junction maintained at elevated temperatures gradually changes with time.

6.3 Crucible and lid, cylindrical, with a well-fitting lid, both made of glazed porcelain. Crucibles of fused silica and other refractory materials can be used, provided that they give the results which agree with the recommended porcelain crucible, within the stated precision of the method (see [Clause 10](#)).

The glazed porcelain crucible and lid shall have a mass between 15 g and 20 g, and dimensions approximate to those shown in [Figure 2 a\)](#), and the fused silica crucible and lid shall have a mass between 10 g and 14 g, and dimensions approximate to those shown in [Figure 2 b\)](#).

The fit of the lid on the crucible is critical for the determination; a lid shall be selected to match the crucible so that the horizontal clearance between them is not greater than 0,5 mm. After selection, the crucible and lid shall be ground together to give a smooth surface, and they will then be given a common distinguishing mark.

6.4 Crucible stand, made of nichrome wire or other heat-resistant metal, on which the crucible is placed in the furnace, so that the appropriate specified rate of heating can be achieved (see [Figure 3](#)).

For example, it may consist of the following:

- a) for single determinations, a ring of heat-resistant steel wire as shown in [Figure 3 a\)](#) with ceramic discs, 25 mm in diameter and 2 mm in thickness, resting on the inner projection of its legs, or
- b) for multiple determinations, a tray of nichrome wire or heat-resistant steel wire as shown in [Figure 3 b\)](#) of approximate size, with nichrome wire mesh or ceramic plates 2 mm in thickness supporting the crucibles.

6.5 Crucible stand tong (see [Figure 4](#)).

6.6 Analytical balance, with a resolution of at least 0,1 mg.


6.7 Pellet presser, screw or level type (see [Figure 5](#)), mechanical or automatic, capable of making a sample cake with the thickness of 1,0 cm to 1,5 cm and about 1,0 cm in diameter under the force created by a mass of over 100 kg (980 N). If the pellets presser can display the force (displayed as mass, in kg) automatically, it can be set between a mass of 200 kg (1 960 N) and a mass of 300 kg (2 940 N), for example a mass of 280 kg (2 740 N).

6.8 Desiccator, with fresh desiccant ([5.1](#)) to assure that the air in it is dry.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[ISO 20360:2020](#)

<https://standards.iteh.ai/catalog/standards/sist/9341e2c9-3860-4df4-b586-9b7162693305/iso-20360-2020>

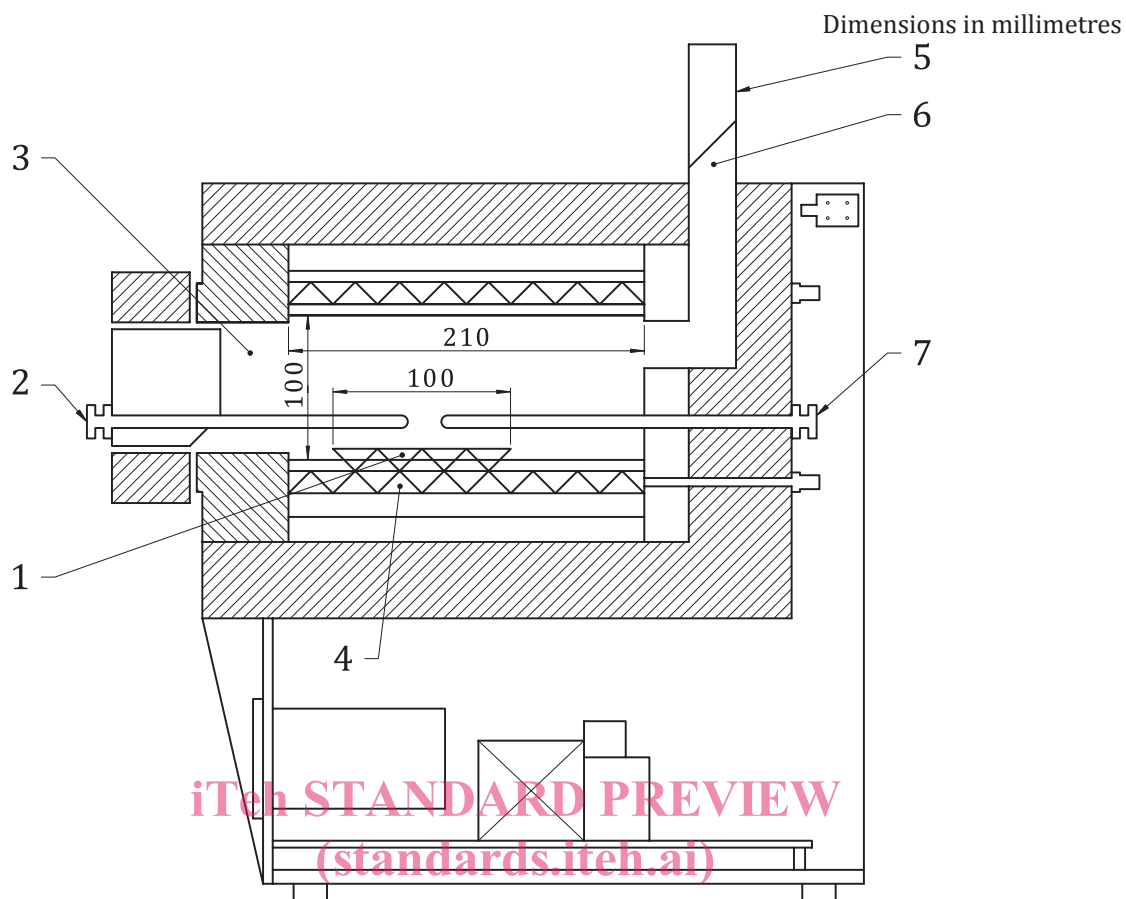

Key

- 1 zone of uniform temperature
- 2 check thermocouple
- 3 chamber (width 200 mm)
- 4 heating system


ISO 20360:2020

<https://standards.iteh.ai/catalog/standards/sist/9341e2c9-3860-4df4-b586-9b7162693305/iso-20360-2020>


- 5 flue
- 6 valve
- 7 thermocouple

Figure 1 — Example of a suitable furnace

Dimensions in millimetres

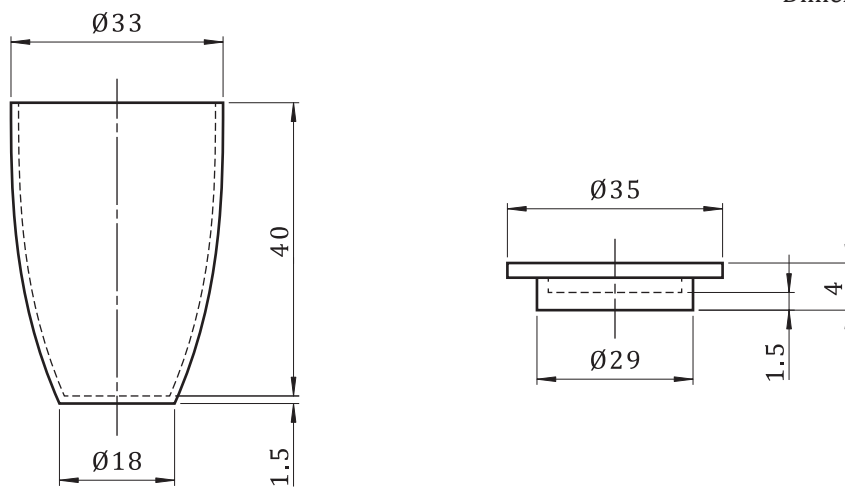

a) Glazed porcelain crucible and lid

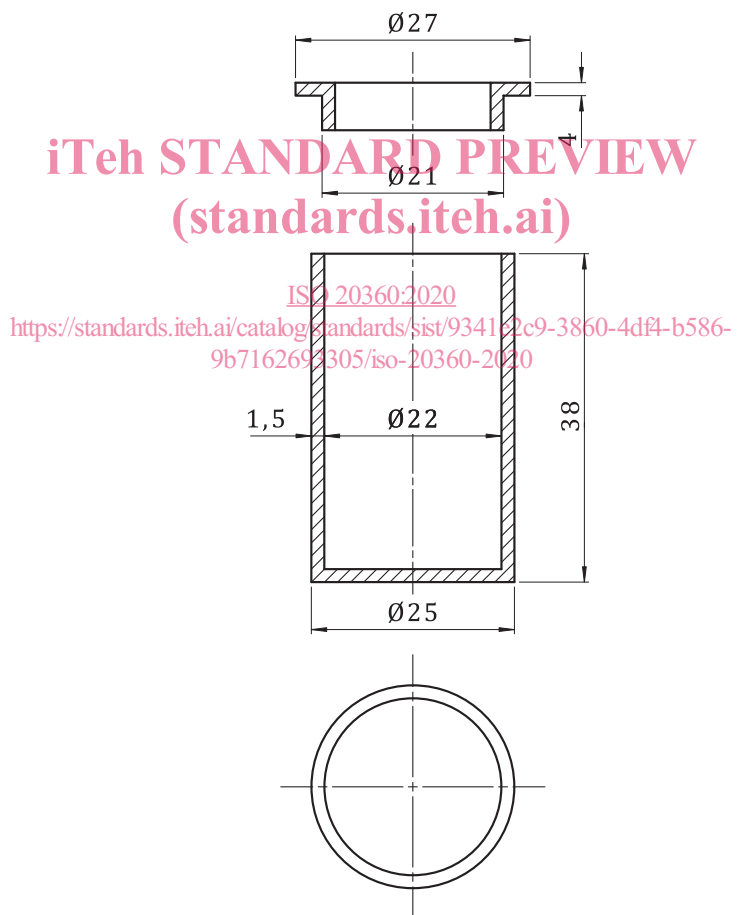

b) Fused silica crucible and lid

Figure 2 — Crucible and lid