

**SLOVENSKI STANDARD**  
**oSIST prEN ISO 13468-1:2019**  
**01-maj-2019**

---

**Polimerni materiali - Določevanje celotne prepustnosti svetlobe prozornih materialov - 1. del: Instrument z enim žarkom (ISO/FDIS 13468-1:2019)**

Plastics - Determination of the total luminous transmittance of transparent materials - Part 1: Single-beam instrument (ISO/FDIS 13468-1:2019)

Kunststoffe - Bestimmung des totalen Lichttransmissionsgrades von transparenten Materialien - Teil 1: Einstrahlinstrument (ISO/FDIS 13468-1:2019)

Plastiques - Détermination du facteur de transmission du flux lumineux total des matériaux transparents - Partie 1: Instrument à faisceau unique (ISO/FDIS 13468-1:2019)

**Ta slovenski standard je istoveten z: prEN ISO 13468-1**

---

**ICS:**

83.080.01	Polimerni materiali na splošno	Plastics in general
-----------	--------------------------------	---------------------

**oSIST prEN ISO 13468-1:2019**

**en,fr,de**



FINAL  
DRAFT

INTERNATIONAL  
STANDARD

ISO/FDIS  
13468-1

ISO/TC 61/SC 5

Secretariat: DIN

Voting begins on:  
2019-02-22

Voting terminates on:  
2019-05-17

## Plastics — Determination of the total luminous transmittance of transparent materials —

### Part 1: Single-beam instrument

*Plastiques — Détermination du facteur de transmission du flux  
lumineux total des matériaux transparents —  
Partie 1: Instrument à faisceau unique*

SIST EN ISO 13468-1:2019

<https://standards.iteh.ai/catalog/standards/sist/296616a0-5842-4172-93a7-50a8059933cc/sist-en-iso-13468-1-2019>

RECIPIENTS OF THIS DRAFT ARE INVITED TO SUBMIT, WITH THEIR COMMENTS, NOTIFICATION OF ANY RELEVANT PATENT RIGHTS OF WHICH THEY ARE AWARE AND TO PROVIDE SUPPORTING DOCUMENTATION.

IN ADDITION TO THEIR EVALUATION AS BEING ACCEPTABLE FOR INDUSTRIAL, TECHNOLOGICAL, COMMERCIAL AND USER PURPOSES, DRAFT INTERNATIONAL STANDARDS MAY ON OCCASION HAVE TO BE CONSIDERED IN THE LIGHT OF THEIR POTENTIAL TO BECOME STANDARDS TO WHICH REFERENCE MAY BE MADE IN NATIONAL REGULATIONS.

ISO/CEN PARALLEL PROCESSING



Reference number  
ISO/FDIS 13468-1:2019(E)

© ISO 2019

# iTeh STANDARD PREVIEW (standards.iteh.ai)

SIST EN ISO 13468-1:2019

<https://standards.iteh.ai/catalog/standards/sist/296616a0-5842-4172-93a7-50a8059933cc/sist-en-iso-13468-1-2019>



## **COPYRIGHT PROTECTED DOCUMENT**

© ISO 2019

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva  
Phone: +41 22 749 01 11  
Fax: +41 22 749 09 47  
Email: [copyright@iso.org](mailto:copyright@iso.org)  
Website: [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

Page

<b>Foreword</b> .....	<b>iv</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>2</b>
<b>4 Apparatus</b> .....	<b>2</b>
<b>5 Test specimens</b> .....	<b>4</b>
<b>6 Conditioning</b> .....	<b>4</b>
<b>7 Procedure</b> .....	<b>4</b>
<b>8 Expression of results</b> .....	<b>4</b>
<b>9 Precision</b> .....	<b>5</b>
<b>10 Test report</b> .....	<b>5</b>
<b>Annex A (informative) Use of a compensation port to increase the efficiency of an integrating sphere</b> .....	<b>7</b>
<b>Bibliography</b> .....	<b>9</b>

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

SIST EN ISO 13468-1:2019

<https://standards.iteh.ai/catalog/standards/sist/296616a0-5842-4172-93a7-50a8059933cc/sist-en-iso-13468-1-2019>

## ISO/FDIS 13468-1:2019(E)

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 61, *Plastics*, Subcommittee SC 5, *Physical-chemical properties*.

SIST EN ISO 13468-1:2019

This second edition cancels and replaces the first edition (ISO 13468-1:1996), of which it constitutes a minor revision. The changes compared to the previous edition are as follows:

- the format of figures has been revised;
- the normative references have been revised;
- editorial changes have been applied.

A list of all parts in the ISO 13468 series can be found on the ISO website.

# Plastics — Determination of the total luminous transmittance of transparent materials —

## Part 1: Single-beam instrument

### 1 Scope

This document covers the determination of the total luminous transmittance, in the visible region of the spectrum, of planar transparent and substantially colourless plastics, using a single-beam photometer with a specified CIE Standard light source and photodetector. This document cannot be used for plastics which contain fluorescent materials.

This document is applicable to transparent moulding materials, films and sheets not exceeding 10 mm in thickness.

NOTE 1 Total luminous transmittance can also be determined by a double-beam spectrophotometer as in ISO 13468-2. This document, however, provides a simple but precise, practical and quick determination. This method is suitable for use not only for analytical purposes but also for quality control.

NOTE 2 Substantially colourless plastics include those which are faintly tinted.

NOTE 3 Specimens more than 10 mm thick can be measured provided the instrument can accommodate them, but the results might not be comparable with those obtained using specimens less than 10 mm thick.

### 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 291, *Plastics — Standard atmospheres for conditioning and testing*

ISO 5725-1, *Accuracy (trueness and precision) of measurement methods and results — Part 1: General principles and definitions*

ISO 5725-2, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*

ISO 5725-3, *Accuracy (trueness and precision) of measurement methods and results — Part 3: Intermediate measures of the precision of a standard measurement method*

ISO 11664-1, *Colorimetry — Part 1: CIE standard colorimetric observers*

ISO 11664-2, *Colorimetry — Part 2: CIE standard illuminants*

CIE Publication No. 15, *Colorimetry*

CIE Publication No. 17, *CIE International lighting vocabulary*<sup>1)</sup>

1) Also published as IEC 60050-845.

## ISO/FDIS 13468-1:2019(E)

### 3 Terms and definitions

For the purposes of this document, the terms and definitions given in CIE Publication No. 17 and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

#### 3.1 transparent plastics

plastics in which the transmission of light is essentially regular and which have a high transmittance in the visible region of the spectrum


Note 1 to entry: Provided their geometrical shape is suitable, objects will be seen distinctly through plastic which is transparent in the visible region.

#### 3.2 total luminous transmittance

ratio of the transmitted luminous flux to the incident luminous flux when a parallel beam of light passes through a specimen

### 4 Apparatus

**4.1** The apparatus shall consist of a stabilized light source, an associated optical system, an integrating sphere fitted with ports, and a photometer. Ingress of external light into the integrating sphere shall be prevented. A schematic arrangement of the apparatus is shown in [Figure 1](#).

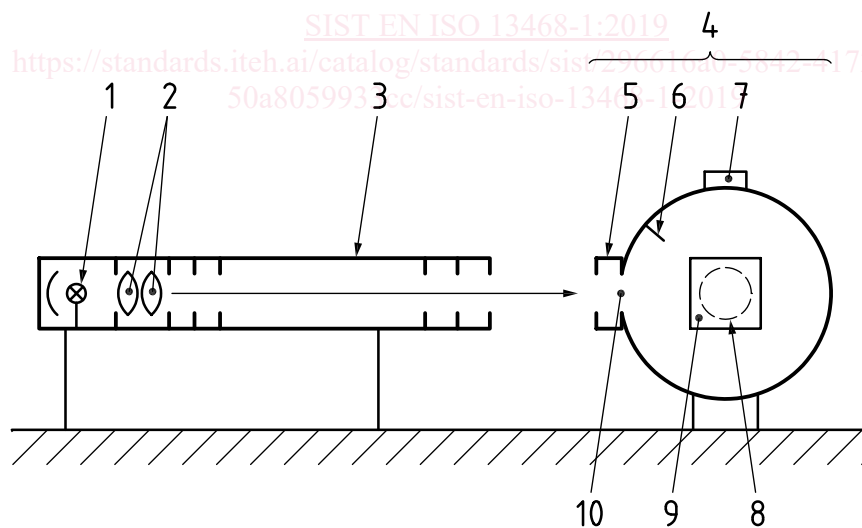

#### Key

- |                      |                     |
|----------------------|---------------------|
| 1 lamp               | 6 baffle            |
| 2 condensing lens    | 7 photodetector     |
| 3 collimator tube    | 8 compensation port |
| 4 integrating sphere | 9 light trap        |
| 5 specimen holder    | 10 entrance port    |

**Figure 1 — Schematic arrangement of the apparatus**



**4.2** The light source and/or photodetector shall be fitted with filters so that the output of the combined system corresponds to the CIE standard colorimetric observer as specified in ISO 11664-1 and CIE standard illuminant D<sub>65</sub> as specified in ISO 11664-2. The output of the photodetector shall be proportional, to within 1 %, to the incident flux over the flux range used. The spectrophotometric characteristics of the light source and the photodetector shall be kept constant during measurements on specimens. The measurement conditions shall be such that the specimen temperature does not increase while measurements are made.

**4.3** The light source shall be combined with an optical system to produce a parallel beam of light; the angle which any ray of this beam makes with the axis of the beam shall not exceed 0,087 rad (5°). The beam shall not be vignetted at either port of the sphere.

The diameter of the beam shall be 0,5 to 0,8 times the diameter of the entrance port of the integrating sphere.

**4.4** Using this instrument, the repeatability standard deviation shall be 0,2 % or less. The within-laboratory reproducibility over long time intervals shall not exceed the repeatability by a factor of more than 3.

**4.5** The design of the instrument shall be such that it reads zero when the incident flux is zero.

**4.6** The integrating sphere used to collect the transmitted flux may be of any diameter as long as the total port area does not exceed 3,0 % of the internal area of the sphere.

It is recommended that the diameter of the integrating sphere is not less than 150 mm so that specimens of a reasonable size can be used.

**NOTE** When the diameter of the integrating sphere is 150 mm and the diameters of the entrance, compensation and photodetector ports are 30 mm, the ratio of the total port area to the internal area of the sphere is 3,0 %.

**4.7** The entrance and compensation ports of the integrating sphere shall be circular and of the same size. The entrance port, compensation port and photodetector port shall not lie on a great circle of the sphere.

**4.8** The photodetector shall be fitted with baffles to prevent light falling on it directly from the specimen.

**4.9** The surfaces of the interior of the integrating sphere and the baffles shall be of substantially equal luminous reflectance which, determined in accordance with CIE Publication No. 15, shall be 90 % or more and shall not vary by more than  $\pm 3$  %. When direct measurement of the reflectance of the internal surface of an integrating sphere is difficult, the measurement may be carried out instead on a surface prepared from the same material in the same way as the internal surface.

**4.10** The light trap shall absorb 95 % or more of the light incident on it.

**4.11** The specimen holder shall be such as to hold the specimen rigidly in a plane normal  $\pm 2^\circ$  to the light beam and as closely as possible to the integrating sphere to ensure that all the light which passes through the specimen, including scattered light, is collected.

The holder shall be designed so that it keeps flexible specimens, such as film, flat.

It is recommended that thin, flexible film is clamped around the edge in a double-ring-type holder or that a double-sided adhesive tape is used to stick it to the edge of the holder. The latter method is used for thicker specimens, which cannot be mounted in the double-ring-type holder.

## ISO/FDIS 13468-1:2019(E)

### 5 Test specimens

5.1 Specimens shall be cut from film, sheet or injection-moulded or compression-moulded mouldings.

5.2 Specimens shall be free of defects, dust, grease, adhesive from protecting materials, scratches and blemishes, and shall be free from visibly distinct internal voids and particles.

5.3 Specimens shall be large enough to cover the entrance port and the compensation port of the integrating sphere.

For a 150 mm diameter sphere, a disc of 50 mm or 60 mm in diameter or a square with a side of the same length is recommended.

5.4 Three specimens shall be taken from each sample of a given material unless otherwise specified.

### 6 Conditioning

6.1 Prior to the test, condition the specimens in accordance with ISO 291, at  $23\text{ °C} \pm 2\text{ °C}$  and  $(50 \pm 5)\%$  relative humidity, for a length of time dependent on the specimen thickness and material such that the specimens reach thermal equilibrium.

16 h is usually sufficient for specimens less than 0,025 mm thick. For thicker material, more than 40 h is recommended.

6.2 Set up the test apparatus in an atmosphere maintained at  $23\text{ °C} \pm 2\text{ °C}$  and  $(50 \pm 5)\%$  relative humidity.

### 7 Procedure

7.1 Allow the apparatus sufficient time to reach thermal equilibrium before making any measurements.

7.2 Make the two readings described in [Table 1](#). The specimen shall be mounted directly on the integrating sphere. The compensation port shall be covered with a light trap.

Adjust the photometer so that the reading  $\tau_1$  is 100.

7.3 Repeat the readings  $\tau_1$  and  $\tau_2$ , making additional readings with the specimen in positions selected to determine uniformity.

7.4 Measure the thickness of the specimen in three places to an accuracy of 0,02 mm for sheet and 1  $\mu\text{m}$  for film.

7.5 Carry out the procedure on each of the three specimens in turn.

### 8 Expression of results

Calculate the total luminous transmittance  $\tau_t$ , in percent, using [Formula \(1\)](#):

$$\tau_t = \frac{\tau_2}{\tau_1} \times 100 \quad (1)$$

NOTE [Annex A](#) discusses in mathematical terms the effect of the compensation port on the efficiency of the integration sphere.