

DRAFT INTERNATIONAL STANDARD

ISO/DIS 8655-2

ISO/TC 48

Secretariat: DIN

Voting begins on:
2020-07-29

Voting terminates on:
2020-10-21

Piston-operated volumetric apparatus —

Part 2: Pipettes

Appareils volumétriques à piston —

Partie 2: Pipettes

ICS: 17.060

iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO/DIS 8655-2](#)

<https://standards.iteh.ai/catalog/standards/sist/1caeacdc-015d-4906-ae77-3f201411b26e/iso-dis-8655-2>

THIS DOCUMENT IS A DRAFT CIRCULATED FOR COMMENT AND APPROVAL. IT IS THEREFORE SUBJECT TO CHANGE AND MAY NOT BE REFERRED TO AS AN INTERNATIONAL STANDARD UNTIL PUBLISHED AS SUCH.

IN ADDITION TO THEIR EVALUATION AS BEING ACCEPTABLE FOR INDUSTRIAL, TECHNOLOGICAL, COMMERCIAL AND USER PURPOSES, DRAFT INTERNATIONAL STANDARDS MAY ON OCCASION HAVE TO BE CONSIDERED IN THE LIGHT OF THEIR POTENTIAL TO BECOME STANDARDS TO WHICH REFERENCE MAY BE MADE IN NATIONAL REGULATIONS.

RECIPIENTS OF THIS DRAFT ARE INVITED TO SUBMIT, WITH THEIR COMMENTS, NOTIFICATION OF ANY RELEVANT PATENT RIGHTS OF WHICH THEY ARE AWARE AND TO PROVIDE SUPPORTING DOCUMENTATION.

This document is circulated as received from the committee secretariat.

ISO/CEN PARALLEL PROCESSING



Reference number
ISO/DIS 8655-2:2020(E)

© ISO 2020

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO/DIS 8655-2

<https://standards.iteh.ai/catalog/standards/sist/1caeacdc-015d-4906-ae77-3f201411b26e/iso-dis-8655-2>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2020

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle of operation	2
5 Adjustment	2
5.1 Basis of adjustment.....	2
5.2 Initial adjustment.....	2
5.3 Subsequent adjustment.....	2
5.4 Adjustment for other liquid properties.....	2
6 Design	3
6.1 Types of pipette.....	3
6.2 Transfer of hand warmth.....	4
7 Pipette tips	4
7.1.....	4
7.1.1 General.....	4
7.1.2 Air-displacement pipette tips.....	4
7.1.3 Positive-displacement pipette tips.....	4
8 Type, designation	5
9 Metrological performance requirements	5
9.1 General.....	5
9.1.1 Reference test.....	5
9.1.2 Routine testing.....	5
9.2 Fixed-volume pipettes of types A and D1.....	5
9.3 Fixed-volume pipettes of type D2.....	6
9.4 Variable-volume pipettes of types A, D1 and D2.....	6
9.5 Multi-channel pipettes.....	6
9.6 Calculation of maximum permissible errors for volumes not listed in Tables 1, 2 and 3	6
9.7 Pipette tips.....	9
10 Marking	9
10.1 Pipettes.....	9
10.2 Pipette tips.....	9
Annex A (normative) Information to be provided with pipettes and tips	10
Annex B (informative) Possible sources of error for air displacement pipettes	11
Annex C (informative) Electronic motorized air displacement pipettes and method for testing in multi-dispensing mode	13
Bibliography	15

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html. (standards.iteh.ai)

This document was prepared by Technical Committee ISO/TC 48, *Laboratory Equipment*, Working Group WG 4, *Piston-operated instruments*. [ISO/DIS 8655-2](https://standards.iteh.ai/catalog/standards/sist/1caecdc-015d-4906-ae77-89f461e2d105/iso-dis-8655-2)

This second edition cancels and replaces the first edition (ISO 8655-2:2002 and ISO 8655-2:2002/Cor 1:2008), which has been technically revised.

The main changes compared to the previous edition are as follows:

- ISO 8655-7, ISO 8655-8 and ISO 8655-9 have been added as normative references;
- Metrological Performance requirements for pipette tips have been further specified;
- [Tables 1](#) and [2](#) have been revised;
- A new [Table 3](#) has been introduced;
- A new informative [Annex C](#) for motorized pipettes has been introduced;
- [Annex A](#) has been revised.

A list of all parts in the ISO 8655 series can be found on the ISO website.

[Annex A](#) forms a normative part of this part of ISO 8655. [Annex B](#) and [Annex C](#) are for information only.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

ISO 8655 addresses the needs of:

- manufacturers, as a basis for quality control including, where appropriate, the issuance of manufacturers' declarations;
- calibration laboratories, test houses, users of the equipment and other bodies as a basis for independent calibration, verification and routine checking.

The tests specified in the ISO 8655 series are intended to be carried out by trained personnel.

iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO/DIS 8655-2

<https://standards.iteh.ai/catalog/standards/sist/1caeacdc-015d-4906-ae77-3f201411b26e/iso-dis-8655-2>

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO/DIS 8655-2

<https://standards.iteh.ai/catalog/standards/sist/1caeacdc-015d-4906-ae77-3f201411b26e/iso-dis-8655-2>

Piston-operated volumetric apparatus —

Part 2: Pipettes

1 Scope

This part of ISO 8655 specifies

- metrological requirements,
- maximum permissible errors,
- requirements for marking and
- information to be provided for users,

for air-displacement (type A) and positive displacement (type D) single-channel and multi-channel pipettes, complete with their selected tip(s) and any other essential, consumable parts, designed to deliver the selected volume (Ex).

NOTE General requirements and definitions of terms for piston-operated volumetric apparatus are given in ISO 8655-1. The gravimetric reference measurement procedure for the determination of volume is given in ISO 8655-6. The photometric reference measurement procedure for the determination of volume is given in ISO 8655-8. Alternative methods for the determination of volume are described in ISO 8655-7. For safety requirements of electrically powered pipettes, see regional or national safety standards.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3696:1991, *Water for analytical laboratory use — Specification and test methods*

ISO/DIS 8655-1:2020, *Piston-operated volumetric apparatus — Part 1: Terminology, general requirements and user recommendations*

ISO/DIS 8655-6:2020, *Piston-operated volumetric apparatus — Part 6: Gravimetric reference measurement procedure for the determination of volume*

ISO/DIS 8655-7:2020, *Piston operated volumetric apparatus — Part 7: Alternative test methods for the determination of volume*

ISO/DIS 8655-8:2020, *Piston-operated volumetric apparatus — Part 8: Photometric reference measurement procedure for the determination of volume*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO/DIS 8655-1:2020 apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>

— IEC Electropedia: available at <http://www.electropedia.org/>

4 Principle of operation

Pipettes are used to accurately handle preselected volumes. The tip is attached to the pipette. Pipettes are typically operated using forward pipetting. Using forward pipetting, with the piston positioned at the lower aspiration limit, the tip is dipped into the liquid to be dispensed. When moved to the upper aspiration limit, the piston aspirates the liquid. The liquid volume to be dispensed is then expelled by depressing or sliding the piston between the volume-defining limits. Some air-displacement pipettes (see 6.1, Type A) have an extra air volume which can be used to expel the last drop of liquid.

See also [Figure 1](#).

Manufacturers' instruction manuals should contain detailed and specific information about the proper operation of pipettes.

5 Adjustment

5.1 Basis of adjustment

A pipette shall be adjusted for the delivery (Ex) of its nominal volume (or selected volume, in the case of a variable-volume model).

For countries that have adopted the standard reference temperature of 20 °C, the adjustment shall be for the temperature 20 °C, a relative air humidity of 50 % and a barometric pressure of 101,3 kPa, when handling grade 3 water as specified in ISO 3696.

For those countries that have adopted a standard reference temperature of 27 °C, the adjustment shall be for the temperature 27 °C, a relative air humidity of 50 % and a barometric pressure of 101,3 kPa, when handling grade 3 water as specified in ISO 3696.

5.2 Initial adjustment

A pipette shall be provided with an initial adjustment.

5.3 Subsequent adjustment

Some pipettes have provision for adjustment when, for example, it is found in a routine check that the volume delivered is not within specification. Such adjustment shall be made according to the manufacturer's instructions and by reference to a measurement procedure according to ISO 8655-6, ISO 8655-7 or ISO 8655-8.

Any pipette so adjusted shall have clear, visible evidence that the initial adjustment has been modified. This information shall also be recorded.

5.4 Adjustment for other liquid properties

Some pipettes are designed to have their factory pre-set adjustment altered by the user so that they will dispense their specified volume when used with liquids with physical properties differing from those of water (see [Annex B](#) for details). In such cases, the design shall prevent unintentional readjustment. Such adjustment shall be made according to the manufacturer's instructions or by reference to the selected test procedure from ISO 8655-7 and the modifications made.

If the pipette is readjusted, it shall be clearly and unequivocally indicated on the outside of the pipette that readjustment has been affected. The outside of the pipette shall be marked with the name of the liquid and the adjusted volume range. This information shall be documented appropriately.

6 Design

6.1 Types of pipette

A pipette may be designed as follows:

- fixed volume, designed by the manufacturer to dispense only its nominal volume, e.g. 100 μl ;
- variable volume, designed by the manufacturer to dispense volumes selectable by the user within its specified useable volume range, e.g. between 10 μl and 100 μl .

The piston may

- either have a body of air contained between the piston and the surface of the liquid (air displacement – Type A); or
- be in direct contact with the surface of the liquid (positive or direct displacement – Type D).

In the case of the type D pipette, either the plunger or the capillary, or both may be reusable (Type D1) or disposable (Type D2). See [Figure 1](#) for details.

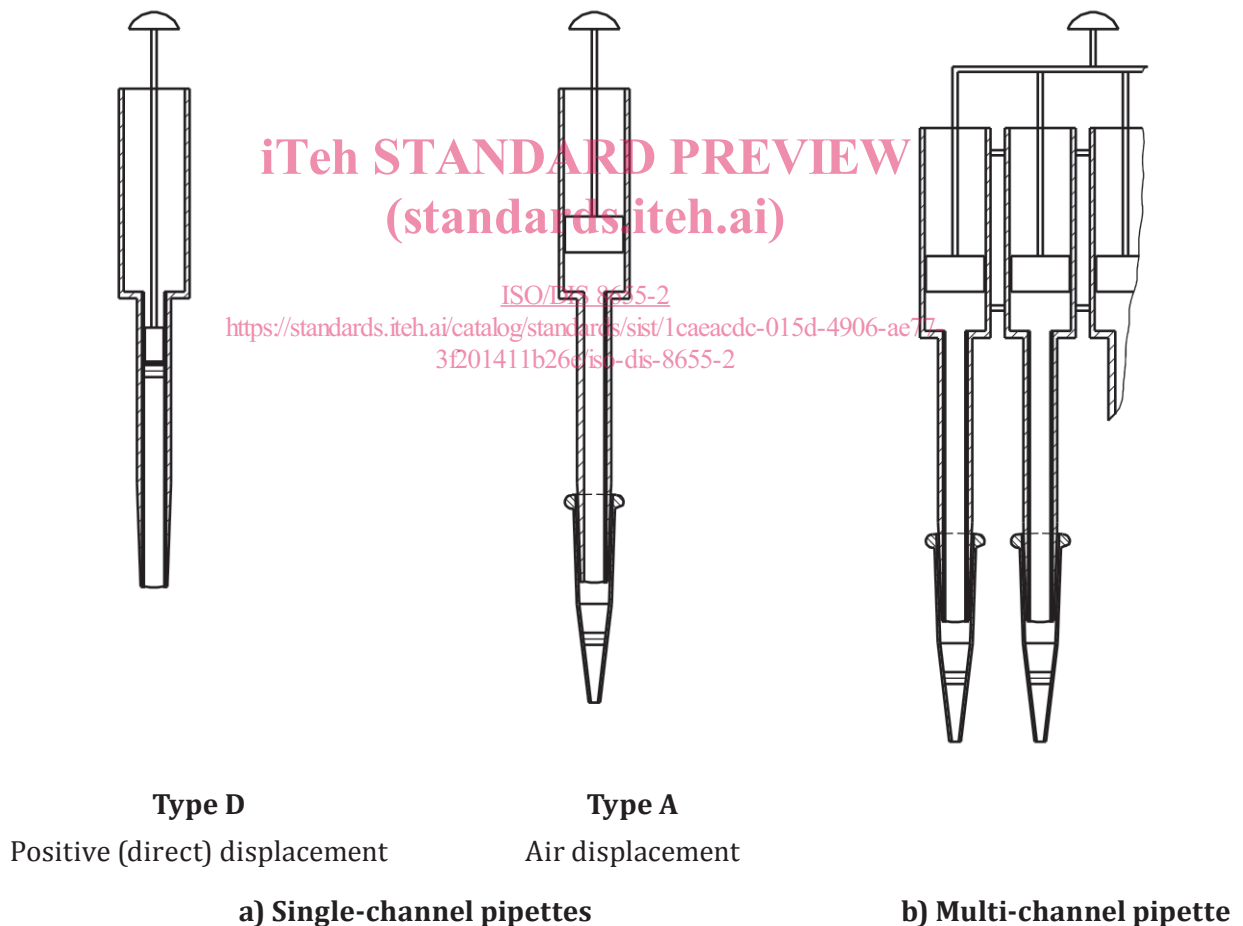


Figure 1 — Pipettes

6.2 Transfer of hand warmth

The construction of pipettes and the materials used for their manufacture shall be chosen in such a way that any heat transmitted from the user's hand to the apparatus during periods of use is minimized.

NOTE Transfer of hand warmth will appear as a systematic drift of results (the delivered volume decreases over time) during a series of deliveries.

7 Pipette tips

7.1

7.1.1 General

7.1.1.1 The dispensing orifice of the tip shall be shaped in such a way that consistent dispensing of the liquid to be measured is achieved. When the tip is touched against the wall of a vessel in successive operations, any amount of liquid remaining in or around the dispensing orifice of the tip shall be consistent.

7.1.1.2 In the case of sterilisable pipette tips the sterilisation procedures indicated as appropriate by the manufacturer in user information or on packaging (see [Annex A](#)) shall not negatively affect the metrological characteristics of the tips such as shape, seal and wettability.

NOTE This requirement can be assessed by comparing errors of measurement using tips which have and have not been sterilised.

STANDARD PREVIEW
(standards.iteh.ai)

7.1.2 Air-displacement pipette tips

ISO/DIS 8655-2

7.1.2.1 Air-displacement pipette tips shall be disposable parts, usually made of plastic, which fit on the tip cone of the pipette and prevent the instrument from contact with the aspirated liquid.

7.1.2.2 Tips for air-displacement shall be fitted in accordance with the pipette supplier's instructions to form a good seal between the tip and the tip cone of the pipette.

NOTE Variability of amount of externally retained liquid or an incomplete seal will contribute to poor precision.

Pipette tips made of plastic for pipettes with air interface are designed for single use. They shall not be cleaned for reuse as their metrological characteristics will no longer be reliable. Single use of a pipette tip means mounting the tip to the pipette only once, and then discarding it after use. While the tip is mounted to the pipette, it may be used to handle several replicate aspiration and delivery cycles.

7.1.2.3 The form of the pipette tips to be used with a multi-channel pipette shall be such that all tips fitted are positioned with parallel axes in the same plane in order to allow for even liquid dispensing in the target vessels, e.g. the adjacent wells of a microplate. The bottoms of properly fitted tips shall not vary in spacing from their nominal axes, nor from their common plane by more than $\pm 0,5$ mm for less than 100 μl , $\pm 1,0$ mm for 100 μl up to 350 μl and $\pm 1,5$ mm for nominal volumes exceeding 350 μl (nominal volumes).

7.1.3 Positive-displacement pipette tips

7.1.3.1 Positive-displacement pipette tips shall consist of a plunger and a capillary which fit on the tip holder of the pipette. Various materials may be used for the plunger, such as metal or plastic, and the capillary, such as plastic or glass. These pipette tips may be reusable (D1) or disposable (D2).

7.1.3.2 The shape and material of the plunger and capillary shall confer a good seal of the tip, as well as a smooth action between the plunger and the capillary, to ensure consistent dispensing of the liquid.

7.1.3.3 Sterilisability shall be in accordance with [7.1.1.2](#).

8 Type, designation

Designation of a Type D1 single-channel pipette (positive displacement with reusable plunger) with a nominal volume of 100 μl :

Pipette ISO 8655 - D1-100

Designation of a Type D2 variable-volume single-channel pipette (positive displacement with disposable plunger/capillary), volume range variable from 20 μl to 200 μl :

Pipette ISO 8655 - D2 - 20-200

Designation of a Type A variable-volume single-channel pipette with air interface, volume range variable from 10 μl to 100 μl :

Pipette ISO 8655 - A - 10-100

Designation of an 8-channel pipette with air interface (A) and with a nominal volume of 200 μl :

Pipette ISO 8655 - A - 200 \times 8

Designation of a 12-channel pipette with air interface (A), volume range variable from 20 μl to 200 μl :

Pipette ISO 8655 - A - 20-200 \times 12

9 Metrological performance requirements

9.1 General

The metrological performance of pipettes (especially pipettes of type A) can be affected in many ways. [Annex B](#) lists parameters which influence the metrological performance of pipettes and recommendations for their handling.

9.1.1 Reference test

In order to state the metrological trueness and precision of the pipette and thus determine its systematic and random errors, a reference measurement procedure as specified in ISO 8655-6 and ISO 8655-8 or a measurement procedure according ISO 8655-7 shall be used. The maximum permissible errors of [Tables 1, 2](#) and [3](#) shall apply.

9.1.2 Routine testing

Users shall establish a routine testing of pipettes in accordance with ISO 8655-1.

9.2 Fixed-volume pipettes of types A and D1

For air-displacement pipettes (Type A) with fixed volume and for positive-displacement pipettes with reusable plunger and capillary (Type D1) and with fixed volume, the maximum permissible errors of [Table 1](#) apply.