



Standard Test Method for Determination of the Impact Value (IV) of a Soil¹

This standard is issued under the fixed designation D 5874; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method covers the determination of the Impact Value (IV) of a soil either in the field or a test mold.

1.2 The standard test method, using a 4.5 kg (10 lbm) hammer, is suitable for, but not limited to, evaluating the strength of an unsaturated compacted fill, in particular pavement materials, soils, and soil-aggregates having maximum particle sizes less than 37.5 mm (1.5 in.).

1.3 By using a lighter 0.5 kg (1.1 lbm) hammer, this test method is applicable for evaluating lower strength soils such as fine grained cohesionless, highly organic, saturated, or highly plastic soils having a maximum particle size less than 9.5 mm (0.375 in.).

1.4 By performing laboratory test correlations for a particular soil using the 4.5 kg (10 lbm) hammer, IV may be correlated with an unsoaked California Bearing Ratio (CBR) or may be used to infer percentage compaction.

1.5 The values stated SI are to be regarded as the standard. The values stated in parentheses are given for information only.

1.6 *This standard may involve hazardous materials, operations, and equipment. This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

NOTE 1—The equipment and procedures contained in this test method are similar to those developed by B. Clegg in the 1970s at the University of Western Australia, Nedlands, Australia. Impact Value is also commonly known as Clegg Impact Value (CIV).

2. Referenced Documents

2.1 ASTM Standards:

- D 653 Terminology Relating to Soil, Rock, and Contained Fluids²
- D 698 Test Method for Laboratory Compaction Characteristics of Soils Using Standard Effort (12 400 ft lbf/ft³(600 kNm/m³))²
- D 1556 Test Method for Density of Soil in Place by the Sand-Cone Method²

¹ This test method is under the jurisdiction of ASTM Committee D-18 on Soil and Rock and is the direct responsibility of Subcommittee D18.08 on Special and Control Tests.

Current edition approved Dec. 10, 1995. Published May 1996.

² Annual Book of ASTM Standards, Vol 04.08.

D 1557 Test Method for Laboratory Compaction Characteristics of Soils Using Modified Effort (56 000 ft lbf/ft³(2700 kNm/m³))²

D 1883 Test Method for CBR (California Bearing Ratio) of Laboratory Compacted Soils²

D 2167 Test Method for Density of Soil in Place by the Rubber-Balloon Method²

D 2216 Method for Laboratory Determination of Water (Moisture) Content of Soil, Rock, and Soil-Aggregate Mixtures²

D 2922 Test Methods for Density of Soil and Soil-Aggregates in Place by Nuclear Methods (Shallow Depth)²

D 2937 Test Method for Density of Soil in Place by the Drive-Cylinder Method²

D 3017 Test Method for Water Content of Soil and Rock in Place by Nuclear Methods (Shallow Depth)²

D 3740 Practice for Minimum Requirements for Agencies Engaged in the Testing and/or Inspection of Soil and Rock as Used in Engineering Design and Construction²

3. Terminology

3.1 *Definitions*—Except as listed below, all definitions are in accordance with Terminology D 653.

3.1.1 *impact value (IV), n*—the value expressed in units of tens of gravities (g) derived from the peak deceleration of a 4.5 kg (10 lbm) instrumented compaction hammer 50 mm (1.97 in.) in diameter free falling 450 mm (18 in.).

3.1.2 *light impact value (IV/L), n*—the IV derived from using a 0.5 kg (1.1 lbm) mass hammer 50 mm (1.97 in.) in diameter free falling 300 mm (12 in.).

3.1.3 *impact soil tester, n*—testing apparatus used to obtain an IV of a soil.

3.1.4 *target iv, n*—the desired strength, in terms of IV, to be achieved in the field for a particular material and construction process. This may also be referred to as *target strength*.

4. Summary of Test Method

4.1 The test apparatus is placed on the material to be tested either in a mold or on naturally occurring or compacted soil in the field. The hammer is raised to a set height and allowed to free fall. The instrumentation of the test apparatus displays a value in tens of gravities (g) of the peak deceleration of the hammer's impact as recorded by an accelerometer fitted to the top of the hammer body. A total of four blows of the hammer

are applied on the same spot to determine the IV for each test performed.

4.2 A light hammer of 0.5 kg (1.1 lbm) may be used for softer conditions or fragile materials instead of the 4.5 kg (10 lbm) standard hammer to determine the IV. When used the resulting value is termed the Light Impact Value (IV/L).

5. Significance and Use

5.1 Impact Value, as determined using the standard 4.5 kg (10 lbm) hammer, has direct application to design and construction of pavements and a general application to earthworks compaction control and evaluation of strength characteristics of a wide range of materials, such as soils, soil aggregates, stabilized soil and recreational turf. Impact Value is one of the properties used to evaluate the strength of a layer of soil up to about 150 mm (6 in.) in thickness and by inference to indicate the compaction condition of this layer. Impact Value reflects and responds to changes in physical characteristics that influence strength. It is a dynamic force penetration property and may be used to set a strength parameter.

5.2 This test method provides immediate results in terms of IV and may be used for the process control of pavement or earthfill activities where the avoidance of delays is important and where there is a need to determine variability when statistically based quality assurance procedures are being used.

5.3 This test method does not provide results directly as a percentage of compaction but rather as a strength index value from which compaction may be inferred for the particular moisture conditions. From observations, strength either remains constant along the dry side of the compaction curve or else reaches a peak and declines rapidly with increase in water content slightly dry of optimum water content. This is generally between 95 and 98 % maximum dry density (see Fig. 1 and Fig. 2). A field target strength in terms of IV may be designated from laboratory testing or field trials for a desired density and water content. If testing is performed after compaction when conditions are such that the water content has changed from the critical value, determination of the actual water content by laboratory testing enables the field density to be inferred from regression equations using IV, density and water content.

NOTE 2—Impact Value may be used as a means to improve the compaction process by giving instant feedback on roller efficiency, uniformity, confirming the achievement of the target strength, and by inference the achieved density. When inferring density from IV, however, it should be considered as only indicative of density. Where strict acceptance on a density ratio basis is required, test methods that measure density directly shall be used.

5.4 This test method may be used to monitor strength changes during a compaction process or over time due to seasonal, environmental or traffic changes.

NOTE 3—For in-place soil strength evaluation where there may be a dry and hard surface layer (crust), testing both the crust and the underlying layer may be required.

5.5 The standard instrument is based on a 4.54 kg (10 lbm) compaction hammer using a 457.2 mm (18 in.) drop height. The hammer has been equipped with an accelerometer and instrumented using a peak hold electronic circuit to read the peak deceleration on impact. The circuitry is filtered electronically to remove unwanted frequencies and the peak deceleration

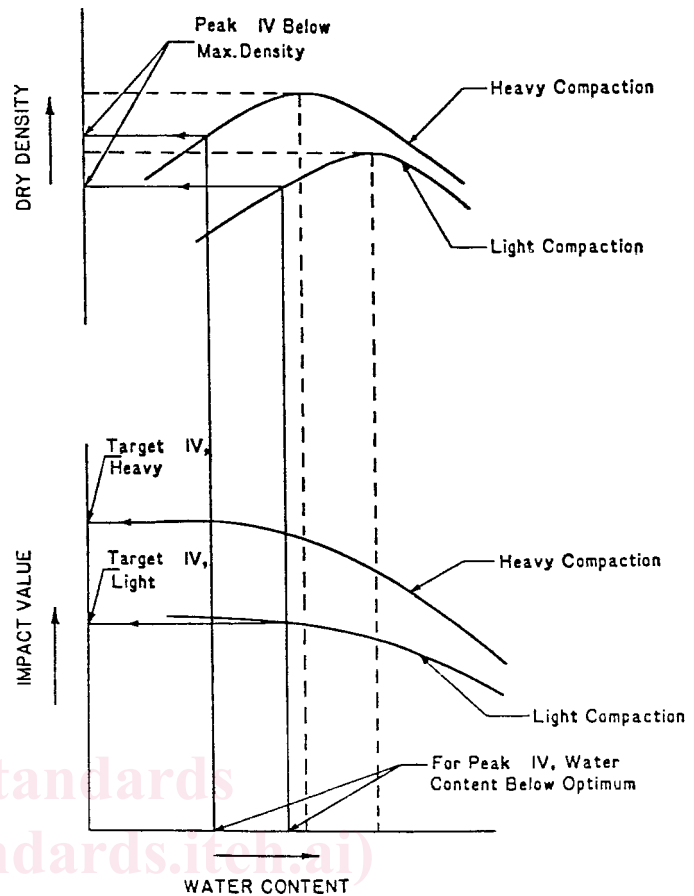


FIG. 1 Illustration of Target IV for Material With No Peak but Drop

tion is displayed in units of ten gravities (g) with the output below units of ten gravities truncated.

5.6 The peak deceleration on which IV is derived represents the area under the deceleration versus time curve which for most soils may be assumed as half a sinusoid. Applying double integration provides first the time velocity relationship and second, the time penetration relationship. As force is also directly related to deceleration, the IV therefore, represents both stress and penetration and may be taken as a direct measurement of stiffness or strength (see Fig. 3).

5.7 Impact Value may be correlated with an unsoaked CBR.

5.8 Impact Value may be expressed as a hammer modulus, analogous with elastic modulus or deformation modulus.

5.9 The light hammer uses the same accelerometer and instrumentation as the standard hammer. The smaller mass of 0.5 kg (1.1 lbm) results in more sensitivity for lower strength materials compared to the standard mass; that is, the zero to 100 IV scale is expanded with this lighter hammer mass and provides more definition on softer materials. To avoid confusion, the IV of the light hammer is notated as IV/L.

5.10 Light Impact Value has applications for recreation turf hardness evaluation, where the condition of the surface affects ball bounce characteristics, the performance or injury potential to participants, and where more sensitivity compared to the standard hammer is required or an imprint left by the 4.5 kg (10 lbm) hammer or other test methods is undesirable, such as on a golf putting green.

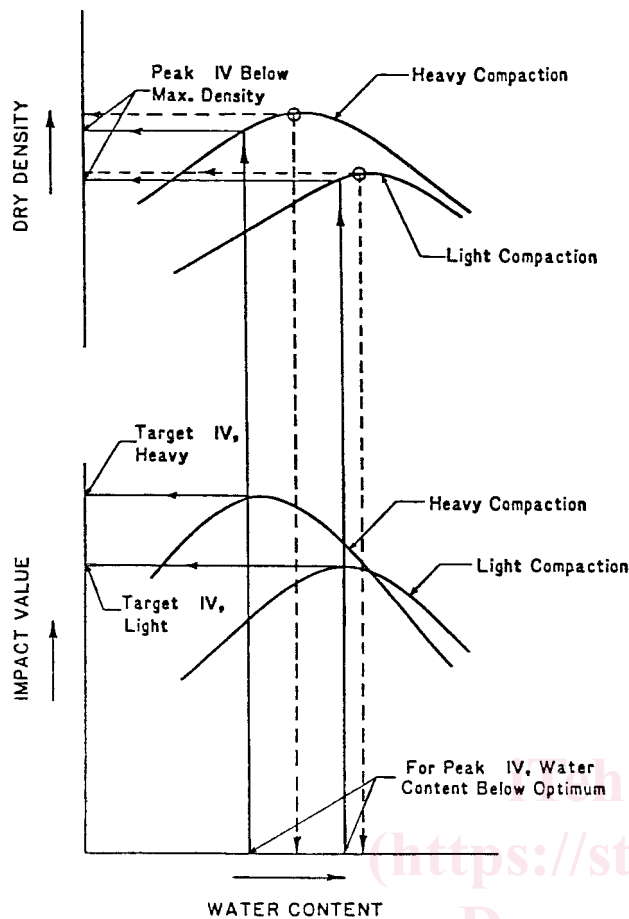


FIG. 2 Illustration of Target IV for Material With Pronounced Peak

NOTE 4—The agency performing this test method can be evaluated in accordance with Practice D 3740. Notwithstanding oil precision and bias contained in this test method, the precision of this test method is dependent on the competence of the personnel performing it and the suitability of the equipment and facilities used. Agencies that meet the criteria of Practice D 3740 are generally considered capable of competent and objective testing. Users of this test method are cautioned that compliance with Practice D 3740 does not assure reliable testing. Reliable testing depends on many factors, and Practice D 3740 provides a means of evaluating some of those factors.

6. Apparatus

6.1 *Impact Soil Tester*—A test apparatus consisting of a hammer, guide tube, and electronic instrumentation. Detailed information on the apparatus is contained in Annex A1. A typical configuration is shown in Fig. 4.

6.2 *Mold*—A 152.4 mm (6 in.) diameter mold conforming to the requirements of Test Methods D 698 Procedure C, D 1557 Procedure C, or D 1883 with a spacer disc.

6.2.1 Molds of other, typically larger, dimensions may be used but must be reported accordingly in the report.

NOTE 5—For a particular material, the smaller 101.6 mm (4 in.) mold may be used if it has been proven by a laboratory test comparison with the 152.4 mm (6 in.) mold that there is no significant difference in the IV results.

7. Procedure

7.1 *Operational Verification Checks*—Perform operational verification checks at the commencement of any testing pro-

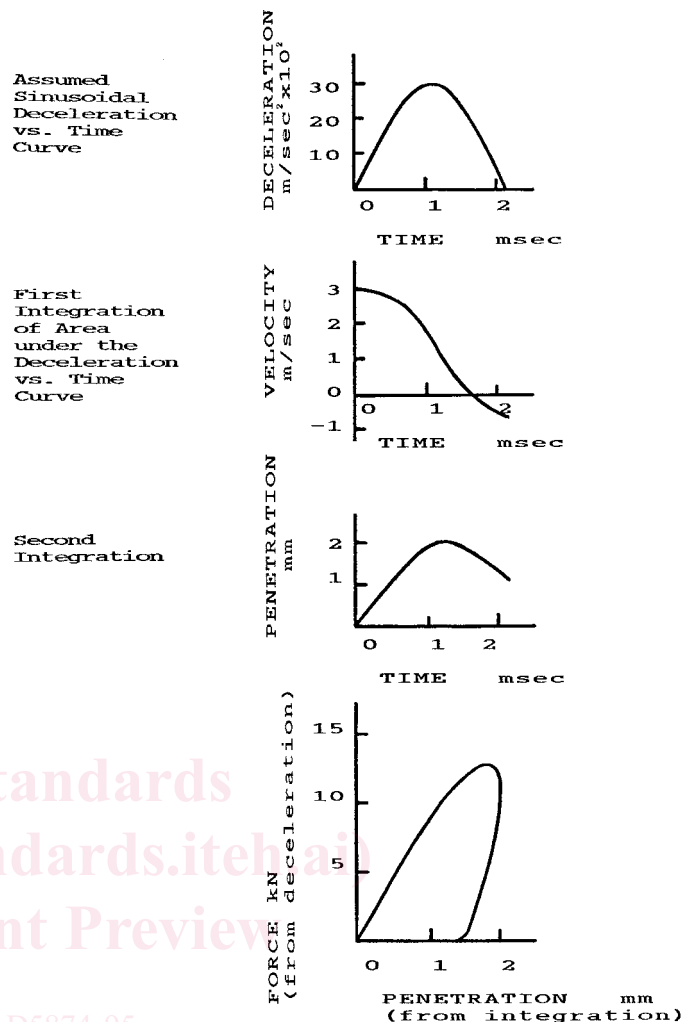


FIG. 3 Development of Force-Penetration from Deceleration Versus Time

gram, after repair, or when the instrument is suspect using the operational check ring as follows.

7.1.1 Place the ring on a dry, grease free smooth hard surface of a solid massive object, such as a concrete floor over ground. Place the guide tube centrally over the ring and drop the hammer five times from the set height mark as described in A2.1.3 for the standard 4.5 kg hammer or A2.1.4 for the light 0.5 kg hammer. Operate the instrumentation so as to obtain five separate readings. If this operational check procedure gives significantly different values than shown on the ring, examine the dryness, cleanliness, smoothness and firmness of the support for the ring and the ring itself and review the operational check procedure and rerun the check at the same or another location. If the ring value is not satisfactorily achievable, an electronic check may be carried out according to the manufacturer's calibration instruction for the accelerometer.

NOTE 6—To avoid the possibility of damage to the electronics or the hammer, the impact soil tester should not be used directly on hard surfaces such as concrete or otherwise in such a way on materials that it would give results of more than 100 IV (1000 g).

NOTE 7—The impact energy provided by the 4.5 kg hammer can cause undesired damage to surfaces and materials such as brick or concrete paving slabs or smoothly prepared turf surfaces.

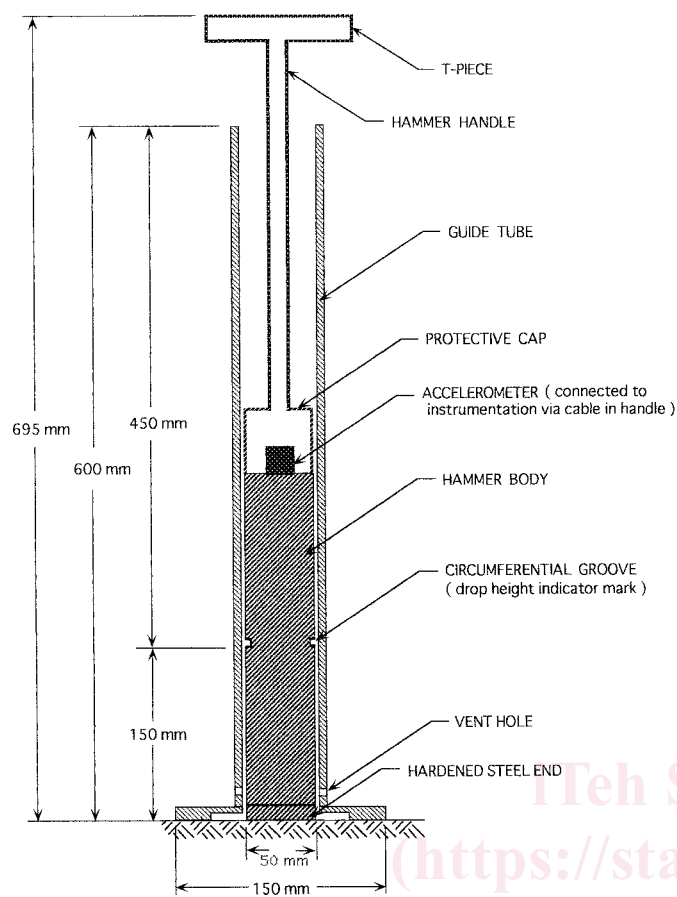


FIG. 4 Illustration (Cross Section) of a 4.5 kg Impact Soil Tester with Hammer at Rest in the Guide Tube

7.2 Determine an IV as follows.

7.2.1 The peak deceleration that is the highest of the four successive blows is taken as the IV. The maximum of the first four blows has been found through experiment and practice to be the simplest means by which to obtain consistent results. Analysis of the blow count has shown that the first blow or two may be considered as seating procedure as they create a compacted wedge or hemisphere of soil that is subsequently forced into the body of the soil causing an increase in deceleration, that is, an increase in IV, as successive blows are applied. In general, deceleration remains practically unchanged after the third or fourth blow with additional blows continuing to produce a constant amount of penetration. If lower values occur with subsequent blows, this is due apparently to the hammer striking the sides of the indentation or by loose material falling onto the strike surface causing a bias in this direction.

7.2.2 Impact Values obtained from other blow counts, or an average thereof, shall be reported accordingly in the report.

7.3 *Field Procedure A*—If necessary, prepare the surface of the compacted or natural soil to be tested by lightly scuffing with the foot to remove loose surface material. Before beginning a test, ensure that the hammer strike face is clean of any soil build-up and that the guide tube is reasonably clean so as not to restrict a free fall. Place the impact soil tester in position with the guide tube base set on the ground. Steady the guide tube to hold vertical in place, activate the instrumentation, and

apply four free falling blows in succession from the set height of drop. Take and record the highest value of the four blows as the IV.

NOTE 8—A method of securing the guide tube in a vertical position is for the operator to place a foot on the guide tube base and steady the guide tube with the lower leg or knee, or both. Raising of the hammer is done by the hand on the same side of the body as the foot securing the guide tube.

NOTE 9—For sloping sites, a level test surface may need to be prepared so that the guide tube base rests on the surface with the guide tube as near to vertical as possible.

7.4 *Field Procedure B*—Follow *Field Procedure A* but determine the water content of the material at a location 100 mm (4 in.) to 150 mm (6 in.) from the edge of the guide tube flange content. Determine the water content according to the applicable test methods listed in 2.1.

7.5 *Field Procedure C*—Follow *Field Procedure B* but determine also the density of the material at a location 100 mm (4 in.) to 150 mm (6 in.) from the edge of the guide tube flange. Determine the density according to the applicable test methods listed in 2.1.

7.6 *Mold Procedure*—Obtain a soil sample representative of that to be tested in the field and prepare a test specimen according to the requirements of either Test Method D 698 or D 1557. Prepare the test specimen at a water content and density at which it is desired to determine the IV. Compact the test specimen in a mold as given in 6.2. Perform the impact test on the compacted specimen in the mold with the base plate left attached to the mold. Before beginning a test, ensure that the hammer strike face is clean of any soil build-up and that the guide tube is reasonably clean so as not to restrict a free fall. To aid in centering and steadying the guide tube, replace the mold collar after trimming the surface of the compacted soil and brushing off loose material if necessary. Place the mold with the specimen on a firm, smooth base such that it cannot be rocked. Place the impact soil tester on the trimmed surface in a vertical position with the guide tube base set inside the mold collar or centered on the soil. Activate the instrumentation, and without moving the guide tube, apply four free falling blows in succession from the standard height of drop. Take and record the highest value of the four blows as the IV.

8. Correlation of IV With Other Soil Properties and Determination of a Target IV

8.1 *A Target Strength*, for a particular soil, may be chosen from the following IV correlations. All procedures given below for determination of a Target IV are performed with a compaction curve according to either Test Method D 698 or D 1557. Each of the following three procedures apply to density or CBR correlations. Where CBR correlations are requested, a duplicate specimen is required for each of the following procedures, that is, an IV test is performed on one specimen and an unsoaked CBR test is carried out on the duplicate specimen.

8.1.1 *Target IV at Optimum Water Content Only*—After determining the optimum water content of the sample in accordance with either Test Method D 698 or D 1557, compact a specimen in a mold as described in 6.2 to the desired optimum water content and maximum dry unit weight or