



~~Designation: A 263-03~~ Designation: A263 – 09

## Standard Specification for Stainless Chromium Steel-Clad Plate<sup>1</sup>

This standard is issued under the fixed designation A263; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reappraisal.

*This standard has been approved for use by agencies of the Department of Defense.*

### 1. Scope\*

1.1 This specification<sup>2</sup> covers plate of a carbon steel or low-alloy steel base to which is integrally and continuously bonded on one or both sides a layer of stainless chromium steel. The material is generally intended for pressure vessel use.

~~1.2 The values stated in inch-pound units are to be regarded as the standard.~~

1.2 The values stated in inch-pound units are to be regarded as standard. The values given in parentheses are mathematical conversions to SI units that are provided for information only and are not considered standard.

### 2. Referenced Documents

#### 2.1 ASTM Standards:<sup>3</sup>

A6/A6M Specification for General Requirements for Rolled Structural Steel Bars, Plates, Shapes, and Sheet Piling

A20/A20M Specification for General Requirements for Steel Plates for Pressure Vessels

A240/A240M Specification for Chromium and Chromium-Nickel Stainless Steel Plate, Sheet, and Strip for Pressure Vessels and for General Applications

A370 Test Methods and Definitions for Mechanical Testing of Steel Products

A480/A480M Specification for General Requirements for Flat-Rolled Stainless and Heat-Resisting Steel Plate, Sheet, and Strip

A578/A578M Specification for Straight-Beam Ultrasonic Examination of ~~Plain and Clad~~ Rolled Steel Plates for Special Applications

A751 Test Methods, Practices, and Terminology for Chemical Analysis of Steel Products

Document Preview

ASTMA263-09

<https://standards.iteh.ai/catalog/standards/sist/0d9b758b-3b11-4543-a582-0cdd63b5ec5e/astm-a263-09>

<sup>1</sup> This specification is under the jurisdiction of ASTM Committee A01 on Steel, Stainless Steel and Related Alloys and is the direct responsibility of Subcommittee A01.11 for Steel Plates for Boilers and Pressure Vessels.

~~Current edition approved Feb. 2, 2006. Published April 2003. Originally approved in 1943. Last previous edition approved in 1999 as A 263-94a (1999).~~

~~Current edition approved May 1, 2009. Published June 2009. Originally approved in 1943. Last previous edition approved in 2003 as A263 – 03. DOI: 10.1520/A0263-09.~~

<sup>2</sup> For ASME Boiler and Pressure Vessel Code applications see related Specification SA-263 in Section II of that Code.

<sup>3</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

\*A Summary of Changes section appears at the end of this standard.

## 2.2 *ASME Code:*

Boiler and Pressure Vessel Code, Section IX, Welding Qualifications ~~Other Standards:~~  
 ASME Code Boiler and Pressure Vessel Code, Section IX, Welding Qualifications<sup>4</sup>

## 3. Terminology

### 3.1 *Definitions of Terms Specific to This Standard:*

3.1.1 This material is considered as single-clad or double-clad stainless chromium-steel plate, depending on whether one or both sides are covered.

3.1.2 ~~base metal (backing steel)~~—component to which the alloy cladding is applied, usually the greater percentage of the composite plate.

~~3.1.3 alloy cladding~~—the stainless chromium steel component of the composite plate.

3.1.3 ~~base metal (backing steel)~~—component to which the alloy cladding is applied, usually the greater percentage of the composite plate.

3.1.4 *integrally and continuously bonded*—a condition in which the alloy cladding and base metal are brought together to form a metallurgical bond at essentially the entire interface of the two metals by means other than those processes that do not produce a homogeneous composite plate.

## 4. Ordering Information

4.1 It is the responsibility of the purchaser to specify all requirements that are necessary for material ordered under this specification. Such requirements may include, but are not limited to, the following:

4.1.1 Quantity (weight or number of pieces).

4.1.2 Cladding alloy specification (UNS or ASTM Specification ~~A 240/A 240M~~A240/A240M) and whether cladding is for corrosion allowance only.

4.1.3 Base metal specification.

4.1.4 Bond integrity Class (1, 3, or 5; see Section 13).

4.1.5 Dimensions including the minimum or nominal thicknesses of the cladding alloy and the backing steel, or of the total composite and if more or less restrictive thickness tolerances apply.

4.1.6 Product analysis, if required (see Section 10). Specify whether applicable to the cladding alloy, backing steel, or both.

4.1.7 Mechanical properties including shear test if required (see Sections 7, 8, and 9).

4.1.8 Finish (see Section 12).

4.1.9 Restrictions, if required, on repair by welding (see Section 14).

4.1.10 Additions to the specification or special requirements.

4.2 In addition to the basic requirements of this specification and the backing steel specification, certain supplementary requirements are available when necessary to meet end use requirements. These include:

4.2.1 Nondestructive examination,

4.2.2 Impact testing, and

4.2.3 Simulated Post-Weld Heat Treatment of Mechanical Test Coupons (SPWHT).

4.3 The purchaser is referred to the listed supplementary requirements in this specification and to the detailed requirements in Specification ~~A 20/A 20M~~A20/A20M.

4.4 If the requirements of this specification are in conflict with the requirements of Specification ~~A 20/A 20M~~A20/A20M, the requirements of this specification shall prevail.

## 5. Materials and Manufacture

### 5.1 *Process:*

5.1.1 The steel shall be made by the open-hearth, electric-furnace, or basic-oxygen processes, or by secondary processes whereby steel made from these primary processes is remelted using, but not limited to electroslag remelting or vacuum-arc remelting processes.

5.1.2 The alloy-cladding metal may be metallurgically bonded to the base metal by any method that will produce a clad steel that will conform to the requirements of this specification.

5.2 *Heat Treatment*—Unless otherwise specified or agreed upon between the purchaser and the manufacturer, all plates shall be furnished in the normalized, tempered, normalized and tempered, or quenched and tempered condition as permitted by the backing steel specification. Stress relieving of the composite plate by heating subcritically is permitted, provided the temperature is 75°F [40°C] (40°C) or more below the minimum tempering temperature (when tempered).

## 6. Chemical Composition

6.1 The composite plate shall conform to any desired combination of alloy-cladding metal and base metal as described in 6.2

<sup>4</sup> Annual Book of ASTM Standards, Vol 01.03.

<sup>4</sup> Available from American Society of Mechanical Engineers (ASME), ASME International Headquarters, Three Park Ave., New York, NY 10016-5990, <http://www.asme.org>.

and 6.3 and as agreed upon between the purchaser and the manufacturer.

6.2 *Alloy Cladding Metal*—The alloy-cladding metal specified shall conform to the requirements as to chemical composition prescribed for the respective chromium steel in Specification A-240/A240M/A-240M.

6.3 *Base Metal*—The base metal shall be carbon steel or low-alloy steel conforming to the ASTM specifications for steels for pressure vessels or other as agreed by the purchaser and the manufacturer. The base metal shall conform to the chemical requirements of the specification to which it is ordered.

**7. Mechanical Properties**

7.1 *Tensile Requirements:*

7.1.1 The tensile properties shall be determined by a tension test of the composite plate for clad plates that meet all of the following conditions.

(a)(1) The nominal composite gage is less than or equal to 1 1/2 in.-in. (38 mm).

(b)(2) The specified minimum tensile strength of the base steel is less than or equal to 70 000 psi [485 MPa]-(485 MPa).

(c)(3) The specified minimum yield strength of the base steel is less than or equal to 40 000 psi [275 MPa]-(275 MPa).

The tensile properties thus determined shall be not less than the minimum and not more than 5000 psi [35 MPa](35 MPa) over the maximum prescribed in the specification for the base steel used. All other tensile test requirements of the specification for the base steel shall be met.

7.1.2 The tensile properties shall be determined by a tension test of the base steel only for clad plates that meet one of the following conditions. The properties thus determined shall meet all of the tensile test requirements for the base steel.

(a)(1) The composite gage is greater than 1 1/2 in.-in. (38 mm).

(b)(2) The specified minimum tensile strength of the base steel is greater than 70 000 psi [485 MPa]-(485 MPa).


(c)(3) The specified minimum yield strength of the base steel is greater than 40 000 psi [275 MPa]-(275 MPa).

7.1.3 If the cladding is for corrosion allowance only, the cladding need not be included in the tensile test. The tensile properties thus determined shall meet the base steel requirements.

7.2 Tests for strength of the bond, when required, must be specified by the purchaser and shall consist of one of the following.

7.2.1 *Shear Strength*—When required by the purchaser, the minimum shear strength of the alloy cladding and base metals shall be 20 000 psi [140 MPa]-(140 MPa). The shear test, when specified, shall be made in the manner indicated in Fig. 1. The minimum cladding thickness for shear testing shall be 0.075 in. [1.9 mm] exclusive as ordered. The minimum cladding thickness for shear testing shall be 0.075 in. (1.9 mm) exclusive as ordered. Testing for shear strength for clad plates with minimum cladding thickness of 0.075 in. (1.9 mm) or less shall be permitted upon agreement between the purchaser and the manufacturer.

7.2.2 *Bond Strength*—As an alternative to the shear strength test provided in 7.2.1, or when agreed upon by the purchaser and the manufacturer, or both, three bend tests shall be made with the alloy cladding in compression to determine the quality of the bond. These bend tests shall be made in the manner of the tension tests indicated in Fig. 2 and shall be bent through an angle of 180° to the bend diameters provided for in either Specification A-6/A-6MA6/A6M or Specification A-20/A-20MA20/A20M,

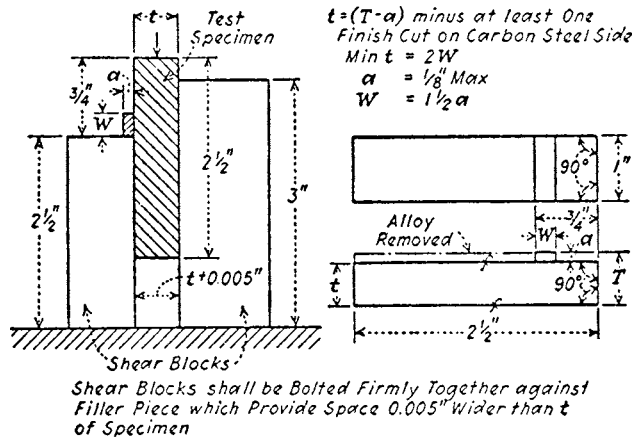

Shear Blocks shall be Bolted Firmly Together against Filler Piece which Provide Space 0.005" Wider than t of Specimen

Metric Equivalents

in.	mm	in.	mm
0.005	0.127	1	25.4
1/8	3.18	2 1/2	64.5
3/4	19.1	3	76.2

FIG. 1 Test Specimen and Method of Making Shear Test of Clad Plate