



SLOVENSKI STANDARD
oSIST prEN 17721:2023

01-maj-2023

Rastlinski biostimulanti - Določanje pH-vrednosti za tekoče mikrobne biostimulante/mikrobne proizvode - Določanje pH-vrednosti

Plant biostimulants - Determination of the pH for liquid microbial plant biostimulants/pH in microbial products - Determination of pH

Pflanzen-Biostimulanzien - Bestimmung des pH Wertes für flüssige mikrobielle Pflanzen-Biostimulanzien/pH Wert in mikrobiellen Produkten - Bestimmung des pH Wertes

Biostimulants des végétaux - Détermination du pH des biostimulants microbiens liquides des végétaux/pH dans les produits microbiens - Détermination du pH

Ta slovenski standard je istoveten z: prEN 17721

ICS:

65.080 Gnojila Fertilizers

oSIST prEN 17721:2023 **en,fr,de**

EUROPEAN STANDARD
NORME EUROPÉENNE
EUROPÄISCHE NORM

DRAFT
prEN 17721

April 2023

ICS 65.080

Will supersede CEN/TS 17721:2022

English Version

Plant biostimulants - Determination of the pH for liquid microbial plant biostimulants/pH in microbial products - Determination of pH

Biostimulants des végétaux - Détermination du pH des biostimulants microbiens liquides des végétaux/pH dans les produits microbiens - Détermination du pH

Pflanzen-Biostimulanzien - Bestimmung des pH Wertes für flüssige mikrobielle Pflanzen-Biostimulanzien/pH Wert in mikrobiellen Produkten - Bestimmung des pH Wertes

This draft European Standard is submitted to CEN members for enquiry. It has been drawn up by the Technical Committee CEN/TC 455.

If this draft becomes a European Standard, CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration.

This draft European Standard was established by CEN in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN-CENELEC Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Republic of North Macedonia, Romania, Serbia, Slovakia, Slovenia, Spain, Sweden, Switzerland, Türkiye and United Kingdom.

Recipients of this draft are invited to submit, with their comments, notification of any relevant patent rights of which they are aware and to provide supporting documentation.

Warning : This document is not a European Standard. It is distributed for review and comments. It is subject to change without notice and shall not be referred to as a European Standard.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

CEN-CENELEC Management Centre: Rue de la Science 23, B-1040 Brussels

Contents	Page
European foreword.....	3
Introduction	4
1 Scope	5
2 Normative references.....	5
3 Terms and definitions	5
4 Principle	9
5 Apparatus and materials	9
5.1 General.....	9
5.2 pH measuring apparatus	9
5.3 Water	10
5.4 pH meter.....	10
5.5 pH electrode.....	11
5.6 Standard buffer solutions	11
5.7 Storage solution for the pH electrodes.....	11
6 Sampling.....	11
7 Procedure.....	12
7.1 General.....	12
7.2 Test conditions.....	12
7.3 Calibration.....	12
7.4 Number of determinations	12
7.5 Measuring the pH value	12
8 Evaluation	13
9 Precision.....	13
10 Test report.....	13
Annex A (informative) Repeatability and Reproducibility data	14
A.1 Materials used in the interlaboratory study	14
A.2 Samples.....	14
A.3 Procedure.....	14
A.4 Replicate determination.....	14
A.5 Results.....	14
Annex ZA (informative) Relationship of this European Standard and the essential requirements of Regulation (EU) 2019/1009 making available on the market of EU fertilising products aimed to be covered.....	17
Bibliography.....	18

European foreword

This document (prEN 17721:2023) has been prepared by Technical Committee CEN/TC 455 “Plant Biostimulants”, the secretariat of which is held by AFNOR.

This document is currently submitted to the CEN enquiry.

This document will supersede CEN/TS 17721:2022.

This document has been prepared under a Standardization Request given to CEN by the European Commission and the European Free Trade Association, and supports essential requirements of EU Directive(s) / Regulation(s).

For relationship with EU Directive(s) / Regulation(s), see informative Annex ZA, which is an integral part of this document.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[oSIST prEN 17721:2023](https://standards.iteh.ai/catalog/standards/sist/4da5976e-4269-4212-917c-22fe2cd6f105/osist-pren-17721-2023)

<https://standards.iteh.ai/catalog/standards/sist/4da5976e-4269-4212-917c-22fe2cd6f105/osist-pren-17721-2023>

Introduction

The new Fertilising Products Regulation (Reg. (EU) 2019/1009) introduces new requirements related to quality, safety, and labelling of fertilizing products and extends the scope to organic fertilizers, organo-mineral fertilizers, growing media, biostimulants and others. The Regulation harmonizes EU rules for products derived from waste organic materials and by products, and provides rules to recover nutrients into secondary raw materials – largely boosting the EU Circular Economy.

CEN/TC 455 “Plant Biostimulants” is one of the three Technical Committees in charge of developing deliverables to ensure full harmonization of fertilizing products on the European Single Market under the Fertilizing Products Regulation, standardizing terminology, specifications, testing methods for safety and environmental criteria of the fertilizing products.

This document was prepared by the experts of CEN/TC 455 “Plant Biostimulants”. The European Committee for Standardization (CEN) was requested by the European Commission (EC) to draft European standards or European standardization deliverables to support the implementation of Regulation (EU) 2019/1009 of 5 June 2019 laying down rules on the making available on the market of EU fertilising products (“FPR” or “Fertilising Products Regulation”). This standardization request, presented as SR M/564, also contributes to the Communication on “Innovating for Sustainable Growth: A Bio economy for Europe”. Working Group 5 “Labelling and denominations”, was created to develop a work program as part of this standardization request.

Technical committee CEN/TC 455 “Plant Biostimulants” was established to carry out the work program that will prepare a series of standards. The interest in biostimulants has increased significantly in Europe as a valuable tool to use in agriculture. Standardization was identified as having an important role in order to promote the use of biostimulants. The work of CEN/TC 455 seeks to improve the reliability of the supply chain, thereby improving the confidence of farmers, industry, and consumers in biostimulants, and will promote and support commercialisation of the European biostimulant industry.

Liquid microbial plant biostimulants have a pH optimal for contained microorganisms and for plants [1].

WARNING — Persons using this document should be familiar with normal laboratory practice. This document does not purport to address all of the safety problems, if any, associated with its use. It is the responsibility of the user to establish appropriate safety and health practices and to ensure compliance with any national regulatory conditions.

IMPORTANT — It is absolutely essential that tests conducted in accordance with this document be carried out by suitably trained staff.

1 Scope

This document specifies a method for laboratory measurement of the pH value in liquid microbial plant biostimulants, using pH electrodes with a glass membrane.

Plant biostimulants other than microbial plant biostimulants are excluded from the scope of this document because there is no essential requirement in the Regulation [1] for measuring the pH of non-microbial plant biostimulants.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

EN 17702-1:—¹, *Plant biostimulants — Sampling and sample preparation — Part 1: Sampling*

EN 17702-2:—², *Plant biostimulants — Sampling and sample preparation — Part 2: Sample preparation*

EN 17724:—³, *Plant biostimulants — Terminology*

EN ISO 3696:1995, *Water for analytical laboratory use — Specification and test methods (ISO 3696:1987)*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in EN 17724:—³ and the following apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

3.1

pH

measure for the acidic or basic reaction of an aqueous solution or dispersion

Note 1 to entry: Notation of pH: the p and the H are vertically on one line.

Note 2 to entry: The acidic reaction is determined by the activity of the existing hydrogen ions. The basic reaction is determined by the activity of the existing hydroxide ions. The direct relationship between the activities of the hydrogen ions and the hydroxide ions is described by the ionic product of the water.

¹ Under preparation

² Under preparation

³ Under preparation

prEN 17721:2023 (E)**3.2****pH value**

decadal logarithm of the hydrogen ion activity multiplied with (-1)

$$pH = pa_{H^+} = -\lg\left(\frac{a_{H^+}}{m_0}\right) = -\lg\left(\frac{m_{H^+} \cdot \gamma_{m, H^+}}{m_0}\right)$$

with

$$a_{H^+} = m_{H^+} \cdot \gamma_{m, H^+}$$

where

a_{H^+} is the activity of the hydrogen ion, expressed in mole per kilogram (mol/kg);

m_0 is the standard molality expressed in mole per kilogram (mol/kg);

γ_{m, H^+} is the activity coefficient of the hydrogen ion;

m_{H^+} is the molality of the hydrogen ion, expressed in mole per kilogram (mol/kg).

Note 1 to entry: The pH value is not measurable as a measure of a single ion activity. Therefore, pH(PS) values of solutions of primary reference material (PS, en: Primary Standard) are determined, which are approximated to it and can be attributed to it. This is based on a worldwide agreement; see EN ISO 80000-9:2019, Annex C [3].

3.3**potentiometric measuring chain**

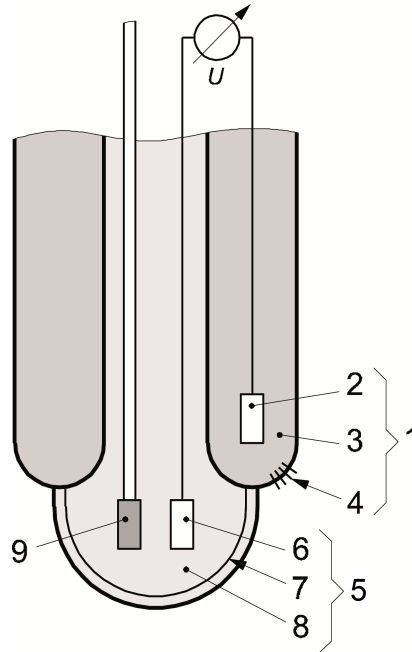
combination of electrochemical half cells

3.4**pH (combination) electrode****pH (single-rod) measuring chain**

potentiometric measuring chain (3.3) providing a voltage which depends on the *pH value* (3.2) of the measuring solution

Note 1 to entry: One of the two electrochemical half cells is the pH measuring electrode, the second is a *reference electrode* (3.5) (see Figure 1).

Note 2 to entry: An integrated temperature sensor is recommended (see Figure 1).

**Key**

- 1 reference electrode, consisting in 2, 3 and 4
 2 reference element
 3 reference electrolyte
 4 diaphragm
 5 pH measuring electrode, consisting of 6, 7 and 8
 6 reference element
 7 glass membrane
 8 internal buffer
 9 temperature sensor
 U pH proportional voltage

Figure 1 — Design of a pH electrode with glass membrane and temperature sensor (schematic illustration)

Note 3 to entry: This document refers to pH electrodes with glass membranes. The electrode shaft should be made of material resistant to chemicals and solvents.

3.5 reference electrode

electrode providing a constant potential which is independent from the *pH value* (3.2) of the measuring medium

Note 1 to entry: At present, the most commonly used type is the silver/silver chloride reference electrode, whose potential is stabilized by a constant concentration of potassium chloride (KCl) in the *reference electrolyte* (3.7).

3.6 reference element

galvanic cell which dips into the *reference electrolyte* (3.7) and transmits the reference potential to the pH meter

Note 1 to entry: The reference elements of the pH measuring electrode and of the reference electrode should be aligned so that identical temperature characteristics are given.

prEN 17721:2023 (E)

3.7
reference electrolyte
aqueous salt solution (generally potassium chloride solution), whose chloride ion activity determines the potential of the *reference electrode* (3.5)

Note 1 to entry: At the *diaphragm* (3.8), the reference electrolyte has contact with the measuring solution. Potassium chloride solution is used as reference electrolyte, because K⁺ ions and Cl⁻ ions have almost the same ion mobility and, therefore, only slight diffusion potential result.

Note 2 to entry: The reference electrolyte should flow out of the diaphragm in order to ensure a constant reference potential. Therefore, it shall be refilled occasionally. For *reference electrodes* (3.5) or *pH electrodes* (3.4) with thickened/gel or solidified electrolyte, refilling of the electrolyte can be omitted. Such reference electrodes or pH electrodes are called low-maintenance.

3.8
diaphragm
permeable material in the sides of the casing of *reference electrodes* (3.5), which enables the electrolytic contact between *reference electrolyte* (3.7) and measuring solution and simultaneously impedes the exchange of electrolyte

3.9
measuring electrode with glass membrane
electrode providing a potential which is a function of the *pH value* (3.2)

3.10
pH glass membrane
membrane made of special glass, on whose interface to the solution an electrical potential (electrode function) results, which is proportional to the *pH* (3.1) of the solution

3.11
temperature compensation
compensation of the temperature-dependent measuring signal only of the *buffer solutions* (3.15) with known temperature dependency

Note 1 to entry: By this, the temperature dependency of the *pH value* (3.2) of the measuring medium cannot be compensated. Therefore, the temperature is always recorded together with the pH value.

3.12
theoretical slope
k
change of the voltage of the *pH electrode* (3.4) with temperature

$$k = -\frac{R \cdot T}{F} \ln 10 = -2,303 \cdot \frac{R \cdot T}{F}$$

where

- T* is the thermodynamic temperature, in Kelvin (measuring temperature, in °C + 273,15 °C);
- R* is the gas constant 8,314 Jmol⁻¹K⁻¹;
- F* is the Faraday constant 96 485 Cmol⁻¹.

Note 1 to entry: At 23°C, *k* = -58,77 mV.

3.13**practical slope** k'

slope of a *pH electrode* (3.4), which is obtained by measuring the pH proportional voltages of the pH electrode in at least two reference *buffer solutions* (3.15)

$$k' = \frac{\Delta U}{\Delta pH}$$

Note 1 to entry: The slope obtained during calibration is a characteristic for the quality of the pH electrode.

3.14**zero point**

pH value (3.2), pH_0 , of a *pH electrode* (3.4), for which the pH proportional voltage of the pH electrode is $U = 0$ mV at a given temperature

Note 1 to entry: The zero point can also be indicated in terms of a voltage (offset voltage).

Note 2 to entry: The zero point obtained during calibration is a characteristic for the quality of the pH electrode.

3.15**buffer solution**

solution with a *pH value* (3.2) of known measurement uncertainty

Note 1 to entry: The buffer solution is used for calibration and adjustment of pH meters. Buffer solutions have a pH value that is largely non-sensitive to dilution and acid or alkali addition.

3.16**stability of measured value**

change of the measurement signal over time (dU/dt) under unchanged measurement conditions

Note 1 to entry: The stability of measured value is specified in accordance with the reproducibility requirement of the measurement.

4 Principle

This document comprises the description of suitable pH electrodes and their calibration and cleaning, as well as the procedure of pH measurement. The specified methods and measuring conditions are based on the results of an interlaboratory test.

5 Apparatus and materials**5.1 General**

Ordinary laboratory glass apparatus.

5.2 pH measuring apparatus

A pH measuring apparatus (see Figure 2) for pH measurement of solutions or dispersions consists of a pH meter, a pH electrode, at least two buffer solutions, containers for the buffer solutions and the material to be measured. For cleaning, the electrode, a spray bottle with deionized water (5.3) or a suitable cleaning solution is recommended. In addition, it can be helpful to use a stand, a stirring tool, thermostats, as well as data recording and analysis systems.