
**Rubber, vulcanized — Determination
of temperature rise and resistance to
fatigue in flexometer testing —**

Part 3:

**Compression flexometer (constant-
strain type)**

iTech Standards

*Caoutchouc vulcanisé — Détermination de l'élévation de température
et de la résistance à la fatigue dans les essais aux flexomètres —*

Partie 3: Flexomètre à compression (type à déformation constante)

[ISO 4666-3:2016](#)

<https://standards.iteh.ai/catalog/standards/iso/7198aa66-e71c-4012-a979-1c5e21b6b3d8/iso-4666-3-2016>



Reference number
ISO 4666-3:2016(E)

iTeh Standards

(<https://standards.iteh.ai>)

Document Preview

[ISO 4666-3:2016](#)

<https://standards.iteh.ai/catalog/standards/iso/7198aa66-e71c-4012-a979-1c5e21b6b3d8/iso-4666-3-2016>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2016, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	2
5 Apparatus	2
5.1 Flexometer	2
5.1.1 General description	2
5.1.2 Detailed description	2
5.2 Measuring gauge	4
5.3 Timer	4
6 Calibration	4
7 Test piece	4
8 Test conditions	5
9 Procedure	6
9.1 Preparation of flexometer	6
9.2 Test procedure	6
9.2.1 General	6
9.2.2 Determination of temperature rise and of compression set	7
9.2.3 Determination of fatigue resistance	7
9.2.4 Determination of creep	7
10 Expression of results	8
10.1 Temperature rise	8
10.2 Creep	8
10.3 Compression set	9
10.4 Fatigue life	9
11 Test report	9
Annex A (informative) Precision	11
Annex B (informative) Guidance for using precision results	13
Annex C (normative) Calibration schedule	14
Bibliography	17

<https://standards.iso.org/iso/7198aa06-e/1c-4012-a979-1c5e21b0b5d8/iso-4666-3-2016>

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html.

The committee responsible for this document is ISO/TC 45, *Rubber and rubber products*, Subcommittee SC 2, *Testing and analysis*.

Document Preview

This third edition cancels and replaces the second edition (ISO 4666-3:2010), [5.1.2](#) of which has been technically revised.

A list of all parts in the ISO 4666 series can be found on the ISO website.

<https://standards.iec.ch/catalog/standards/iso/7198aa06-e/1c-4012-a979-1c5e21b6b3d8/iso-4666-3-2016>

Introduction

One major consequence of the internal heat generation of rubber under a flexing compression is the development of an elevated temperature in the rubber. This document provides for the measurement of the temperature rise.

Under particularly severe heat generation and temperature rise conditions, internal rupture of the test piece can occur with fatigue failure. Provision is also made for the measurement of resistance to this type of fatigue.

The test is conducted under conditions of a selected static pre-stress or compression and a selected cyclic strain of constant maximum amplitude imposed upon the pre-stressed test piece.

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

[ISO 4666-3:2016](#)

<https://standards.iteh.ai/catalog/standards/iso/7198aa66-e71c-4012-a979-1c5e21b6b3d8/iso-4666-3-2016>

Rubber, vulcanized — Determination of temperature rise and resistance to fatigue in flexometer testing —

Part 3: Compression flexometer (constant-strain type)

WARNING 1 — Persons using this document should be familiar with normal laboratory practice. This document does not purport to address all of the safety problems, if any, associated with its use. It is the responsibility of the user to establish appropriate safety and health practices and to ensure compliance with any national regulatory conditions.

WARNING 2 — Certain procedures specified in this document might involve the use or generation of substances, or the generation of waste, that could constitute a local environmental hazard. Reference should be made to appropriate documentation on safe handling and disposal after use.

1 Scope

This document specifies the flexometer test with constant-strain amplitude for the determination of the temperature rise and resistance to fatigue of vulcanized rubber. The flexometer specified is known as the Goodrich flexometer, but any other apparatus giving equivalent performance can be used.

This document gives directions for carrying out measurements which make possible predictions regarding the durability of rubbers in finished articles subject to dynamic flexing in service, such as tyres, bearings, supports, V-belts, and cable-pulley insert rings. However, owing to the wide variations in service conditions, no simple correlation between the accelerated tests described in the various parts of this document and service performance can be assumed.

The method is not recommended for rubber having a hardness greater than 85 IRHD.

<https://standards.iec.ch/catalog/standards/iso/198aa06-e/1c-4012-a979-1c5e2166b3d8/iso-4666-3-2016>

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 48, *Rubber, vulcanized or thermoplastic — Determination of hardness (hardness between 10 IRHD and 100 IRHD)*

ISO 23529, *Rubber — General procedures for preparing and conditioning test pieces for physical test methods*

ISO 18899:2013, *Rubber — Guide to the calibration of test equipment*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 4666-1 apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- IEC Electropedia: available at <http://www.electropedia.org/>
- ISO Online browsing platform: available at <http://www.iso.org/obp>

4 Principle

A specified compressive load is applied to a test piece through a lever system having high inertia, while imposing on the test piece an additional high-frequency cyclic compression of specified amplitude. Measurements are made of the increase in temperature at the base of the test piece with a thermocouple which provides a relative indication of the heat generated in flexing the test piece and of the number of cycles which produces fatigue breakdown.

With the test piece subject to a constant applied load or to a constant initial compression during the test, continuous measurement is made of the change in height of the test piece. The compression set of the test piece is measured after testing.

5 Apparatus

5.1 Flexometer

5.1.1 General description

The essential parts of the apparatus are shown in [Figure 1](#).

The test piece is placed between anvils faced with a thermal insulating material. The top anvil is connected to an adjustable eccentric usually driven at an oscillation rate of $30\text{ Hz} \pm 0,2\text{ Hz}$.

An anvil is sometimes called a "plate". However, do not confuse "anvil" with the plate described in [Clause 7](#).

The load is applied by means of a lever resting on a knife edge. The moment of inertia of the lever system is increased and its natural frequency reduced by suspending masses of 24 kg at each end of the lever system. The lower anvil can be raised or lowered relative to the lever by means of a calibrated micrometer device. This device permits the lever system to be maintained in a horizontal position during the test as determined by a pointer and a reference mark on the end of the bar.

The increase in temperature at the base of the test piece is determined by means of a thermocouple placed at the centre of the bottom anvil.

5.1.2 Detailed description

The apparatus (see [Figure 1](#)) consists of a balance beam (6) which can be locked in its horizontal position by means of a steel pin. The beam is provided with masses of 24 kg (8) at both ends. The distance between the knife edge supporting the beam and the edges supporting the masses is $288\text{ mm} \pm 0,5\text{ mm}$. An equivalent inertial system can be used.

The test piece (2) is placed upon an anvil (3) on one arm of the balance beam. The distance of the test piece support (10) from the fulcrum is $127\text{ mm} \pm 0,5\text{ mm}$. On the other side of the balance beam, additional masses (7) are placed in order to apply a load to the test piece. The desired weights are 11 kg or 22 kg which correspond to a pre-stress of $1,0\text{ MPa} \pm 0,03\text{ MPa}$ or $2,0\text{ MPa} \pm 0,06\text{ MPa}$, respectively.

The test piece (2) is placed between the anvils (1 and 3), which are made of a thermal insulating material having a thermal conductivity of not more than $0,28\text{ W/(m}\cdot\text{K)}$ or, equivalently, $0,24\text{ kcal/(h}\cdot\text{m}\text{ }^\circ\text{C)}$. Phenolic hardpaper can be used for this purpose. In the centre of the lower anvil, a thermocouple, for example, iron-constantan, is attached for temperature measurement. The sensing point of the thermocouple shall be in contact with the test piece. The sensitivity of the thermocouple shall be $\pm 0,5\text{ }^\circ\text{C}$.

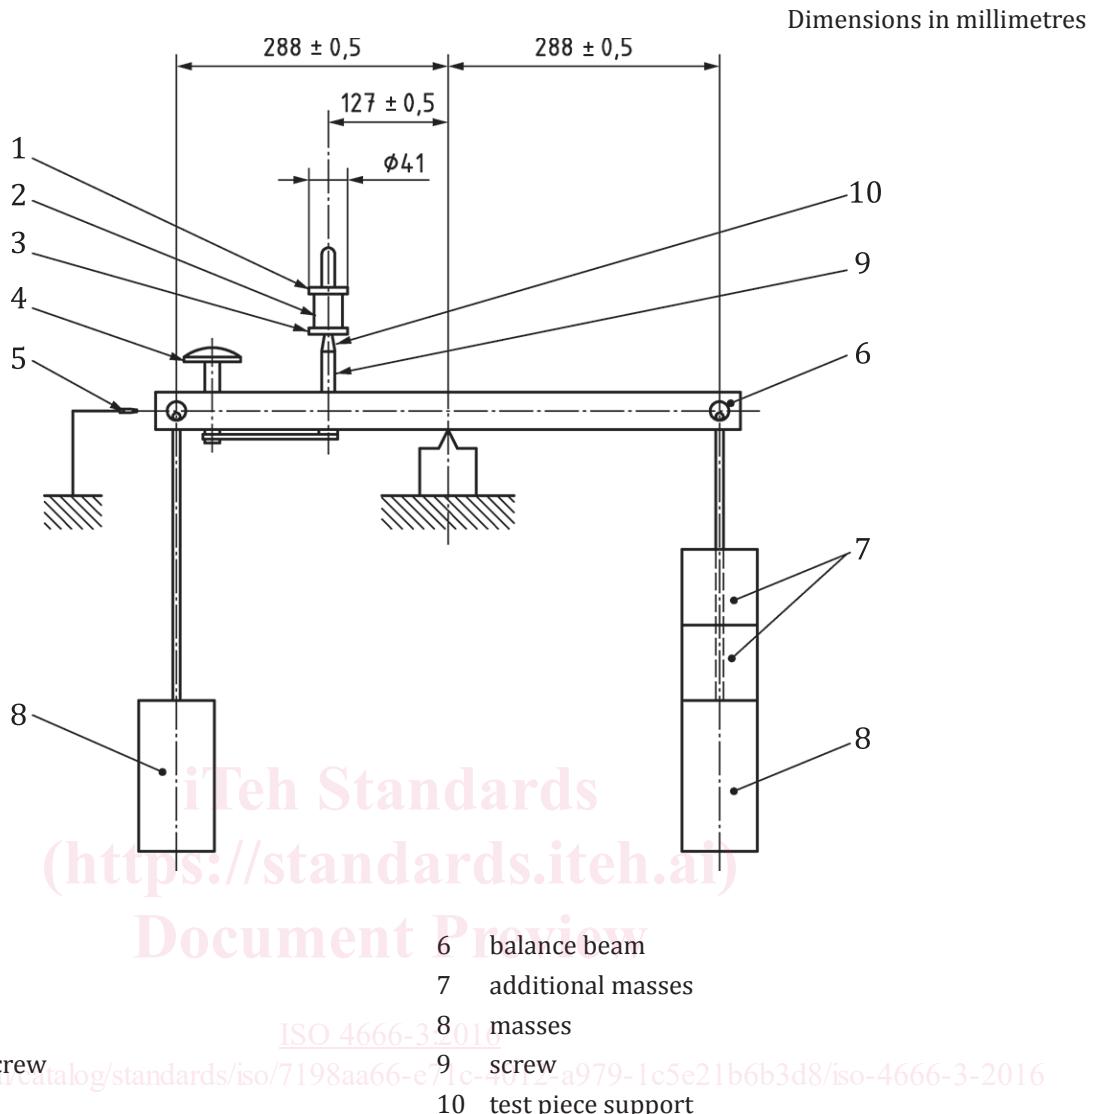


Figure 1 — Compression flexometer (constant-strain type) — General arrangement

Means shall be provided for measuring the decrease in height of the test piece, as the test proceeds, with an accuracy of 0,1 mm. For this purpose, the distance between the lower and upper anvils can be varied by means of a calibrated micrometer device until it returns to the horizontal position, which can be recognized by a mark on the balance beam and a pointer (5) on the casing. The adjustment device consists of a micrometer screw (4) which, by means of a chain and sprocket-wheel drive, moves the screw (9) up or down without rotating the lower anvil (3). The degree of adjustment is read from the micrometer screw (4). The centre point of the upper anvil (1) remains in the same position. The upper anvil (1) is connected through a guide bearing to an eccentric which can be set to the desired stroke in a range from 4,45 mm to 6,35 mm and is driven by a motor at $30 \text{ Hz} \pm 0,2 \text{ Hz}$.


[Figure 2](#) shows a heating chamber. The test piece (7) with the supporting anvils is located in the chamber, the temperature of which can be maintained to within $\pm 1 \text{ }^{\circ}\text{C}$ of a test temperature generally in the range $40 \text{ }^{\circ}\text{C}$ to $100 \text{ }^{\circ}\text{C}$. The chamber shall have the following dimensions:

- width 100 mm to 220 mm;
- depth 130 mm to 250 mm;
- height approximately 230 mm.

The bottom of the chamber shall be situated $25 \text{ mm} \pm 2 \text{ mm}$ above the balance beam (9).

A thermocouple of the same type as that used in the lower anvil (8) shall be used for measurement of the temperature in the chamber. The thermocouple shall be positioned at a distance of 6 mm to 9 mm towards the right-hand side behind the rear edge of the anvil and at a height midway between the anvils. A length of at least 100 mm of the thermocouple wire shall be within the chamber.

The air circulation within the chamber is provided by a radial fan (4) of 75 mm diameter, operating at a rotational frequency of 25 Hz to 28 Hz. The air intake shall have a diameter of 60 mm. The air outlet (5) shall measure 40 mm \times 45 mm. The grid shelf for supporting the test piece during conditioning (2) shall be fitted 10 mm \pm 2 mm above the bottom of the chamber.

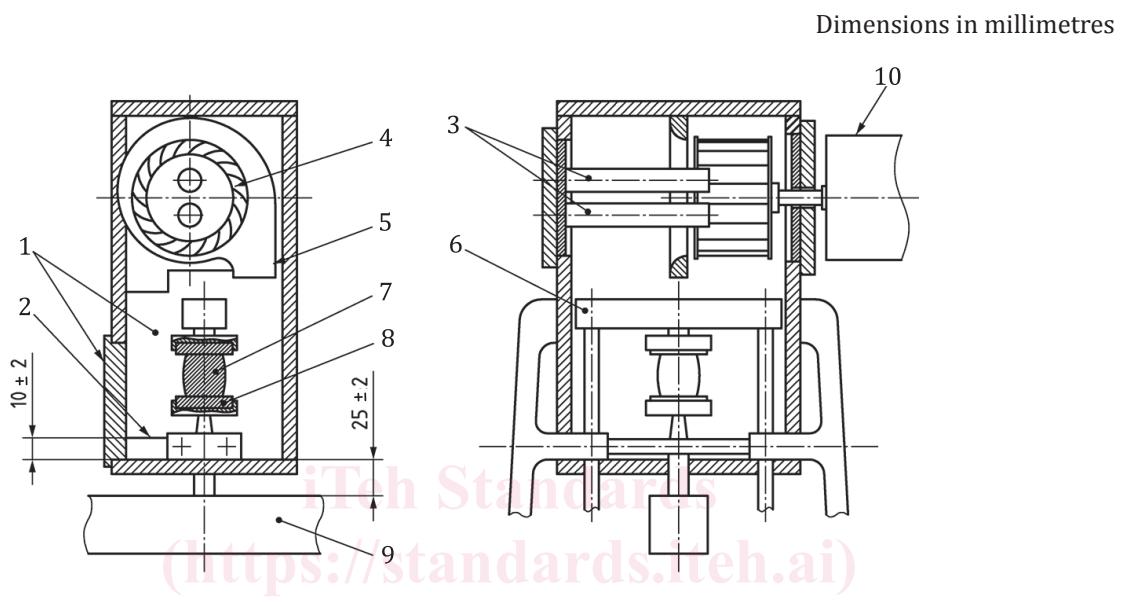

Key

1	heating chamber with door	6	crossbar with lifting rods and upper anvil
2	grid shelf for supporting test pieces during conditioning	7	test piece
3	heating elements	8	lower anvil with thermocouple
4	radial fan	9	balance beam
5	air outlet	10	motor of radial fan

Document Preview

<https://standards.iteh.ai/catalog/standards/iso/7198aa69-1c5e21b6b3d8/iso-4666-3-2016>

Figure 2 — Example of a heating chamber

5.2 Measuring gauge

The gauge for measuring the height and diameter of test pieces shall conform to the requirements of ISO 23529.

5.3 Timer

A stopwatch or other similar device shall be used.

6 Calibration

The test apparatus shall be calibrated in accordance with the schedule given in [Annex C](#).

7 Test piece

The test piece shall be cylindrical in shape, having a diameter of 17,8 mm \pm 0,15 mm and a height of 25 mm \pm 0,25 mm.