



Designation: D4922 – 09

Standard Test Method for Determination of Radioactive Iron in Water¹

This standard is issued under the fixed designation D4922; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reappraisal.

1. Scope

1.1 This test method covers the determination of ^{55}Fe in the presence of ^{59}Fe by liquid scintillation counting. The *a-priori* minimum detectable concentration for this test method is 7.4 Bq/L.²

1.2 This test method was developed principally for the quantitative determination of ^{55}Fe . However, after proper calibration of the liquid scintillation counter with reference standards of each nuclide, ^{59}Fe may also be quantified.

1.3 This test method was used successfully with Type III reagent water conforming to Specification D1193. It is the responsibility of the user to ensure the validity of this test method for waters of untested matrices.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.* For a specific hazard statement, see Section 9.

2. Referenced Documents

2.1 *ASTM Standards:*³

D1068 Test Methods for Iron in Water

D1129 Terminology Relating to Water

D1193 Specification for Reagent Water

D2777 Practice for Determination of Precision and Bias of Applicable Test Methods of Committee D19 on Water

D3370 Practices for Sampling Water from Closed Conduits

D5847 Practice for Writing Quality Control Specifications for Standard Test Methods for Water Analysis

D7282 Practice for Set-up, Calibration, and Quality Control of Instruments Used for Radioactivity Measurements

¹ This test method is under the jurisdiction of ASTM Committee D19 on Water and is the direct responsibility of Subcommittee D19.04 on Methods of Radiochemical Analysis.

Current edition approved July 15, 2009. Published August 2009. Originally approved in 1989. Last previous edition approved in 2001 as D4922 – 01. DOI: 10.1520/D4922-09.

² Currie, L., "Limits for Qualitative Detection and Quantitative Determination," *Analytical Chemistry*, Vol. 40, 1968, pp. 586–593.

³ For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

3. Terminology

3.1 *Definitions*—For definitions of terms used in this test method, refer to Terminology D1129. For terms not defined in this test method or in Terminology D1129, refer to other published glossaries.⁴

4. Summary of Test Method

4.1 This test method describes the effective separation of iron from the interfering cations of manganese, cobalt, zirconium, niobium, and cesium by anion exchange using acid washes of various molarities. Subsequent elution of the iron is followed by phosphate precipitation to remove any residual zinc. The iron phosphate precipitate is dissolved in phosphoric acid and water and mixed with liquid scintillation cocktail. The chemical yield is determined by the recovery of iron carrier using atomic absorption spectrophotometry. Alternatively, any procedure described in Test Method D1068 may be used, but this will need to be validated by the user prior to reporting sample results.

5. Significance and Use

5.1 Radioactive iron is produced by neutron activation of stable iron. Its concentration in reactor coolant is used to monitor the corrosion of reactor parts such as reactor fuel-cladding material and reactor structural components.

5.2 This technique effectively removes other activation and fission products such as isotopes of iodine, zinc, manganese, cobalt, and cesium by the addition of hold-back carriers and an anion exchange technique. The fission products (zirconium-95 and niobium-95) are selectively eluted with hydrochloric-hydrofluoric acid washes. The iron is finally separated from Zn^{+2} by precipitation of FePO_4 at a pH of 3.0.

6. Interferences

6.1 Samples of reactor origin will also contain ^{59}Fe after other radioactive contaminants have been removed by anion exchange (see Fig. 1). ^{59}Fe is also an activation product which decays by β - γ emission and will be a source of interference in the quantitative determination of ^{55}Fe . The large difference in

⁴ "American National Standard Glossary of Terms," *Nuclear Science and Technology (ANSI N1.1)*, American National Standards Institute, 1430 Broadway, New York, NY 10018.

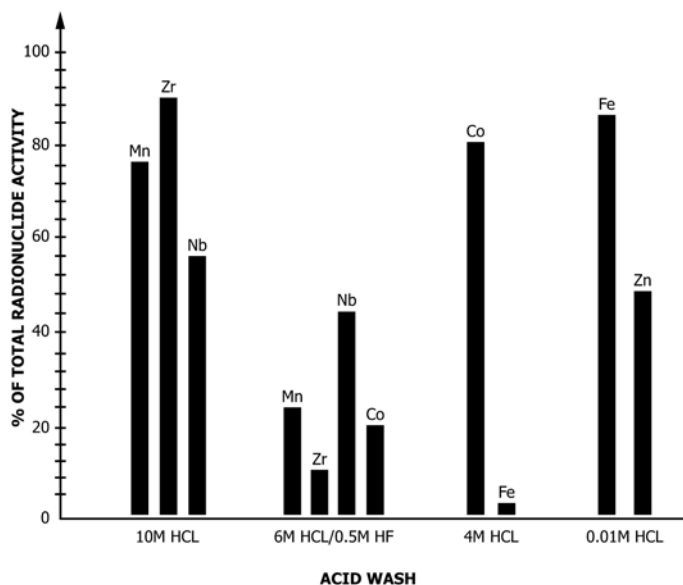


FIG. 1 Percent of Total Radionuclide Activity Removed Per Acid Wash

the energies of their characteristic decay emissions makes it possible to determine appropriate factors to correct for the ^{59}Fe spectral cross-talk in the ^{55}Fe region.

6.2 Quenching, which may be caused by a number of factors, results in a reduction in light output from the sample. The subsequent decrease in the spectral pulse height will cause variations in the counting efficiency with varying degrees of quench. For this reason, it is necessary to monitor both the changes in the ^{55}Fe efficiency and the ^{59}Fe cross-talk in the ^{55}Fe region as a function of quench. This technique recommends the use of the automatic external standard ratio supplied by most liquid scintillation counters to monitor the amount of quench in a sample.

6.3 The final heating of the sample solution will drive off all excess hydrochloric acid, ammonia, and water. These substances are, therefore, effectively removed as possible quenching agents.

6.4 Scintillation stock or sample solutions which have been exposed to light must be dark adapted to avoid erratic results due to light activation of the scintillator.

NOTE 1—It is the responsibility of the user to determine the required dark adaptation period for the specific cocktail used.

6.5 The stable iron content in a sample will interfere in the determination of the chemical recovery. Since the amount of stable iron in a sample will depend on its sources, a correction for the iron in the sample must be made.

7. Apparatus

7.1 *Liquid Scintillation Counter*, with an automatic external standard and multiple energy region of interest (ROI) capabilities.

7.2 *Glass Scintillation Vials*, 20-mL vials exhibiting suitable optical reproducibility so as not to cause erratic results among samples.

7.3 *Atomic Absorption Spectrophotometer*.

7.4 *Variable Speed Peristaltic Pump*, with controller. Pump speed should be between 5 and 8 mL/min.

7.5 *Centrifuge*, using 100 mL centrifuge tubes.

7.6 *Volumetric Flasks*.

7.7 *Anion Exchange Columns*:

7.7.1 *Columns*—Commercially available plastic drying tubes and ends (40 mL volume, 1.5 cm diameter, 15 cm long).

7.7.2 *Tubing*—Pump inlet tubing, approximately 45.7 cm (18 in.) in length, and pump outlet tubing, approximately 76.2 cm (30 in.) in length.

7.7.3 *Polyethylene Porous Disc*—35- μm pore size and 3.2 mm thick.

8. Reagents and Materials

8.1 *Purity of Reagents*—Reagent grade chemicals shall be used for all tests. Unless otherwise indicated, it is intended that all reagents shall conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society, where such specifications are available.⁵ Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination.

8.2 *Purity of Water*—Unless otherwise indicated, references to water shall be understood to mean reagent water conforming to Specification D1193, Type III.

8.3 *Resin*—AG1-X8, AG1-X10, 200–400 mesh; 25 mL previously equilibrated with 125 mL concentrated hydrochloric acid.

8.4 *Scintillation Cocktail*—Commercially prepared Insta-Gel scintillator or equivalent non-ionic detergent scintillator of the *octyl-phenyl polyglycol ether* type.⁶

NOTE 2—To obtain a clear aqueous final sample, the sample volume must be kept below 1.8 mL with the addition of 15 mL Insta-Gel. It is the responsibility of the user to determine the optimum sample volume to cocktail volume to obtain a clear homogeneous solution for any other liquid scintillation cocktail used.

8.5 *Ammonium Hydroxide* (NH_4OH)—Concentrated (approximately 15M) (sp gr 0.90).

8.6 *Ammonium Phosphate* (0.5 M)—Dissolve 66 g of ammonium monohydrogen phosphate [$(\text{NH}_4)_2\text{HPO}_4$] in water and dilute to 1000 mL with water in a volumetric flask.

⁵ *Reagent Chemicals, American Chemical Society Specifications*, American Chemical Society, Washington, DC. For Suggestions on the testing of reagents not listed by the American Chemical Society, see *Annual Standards for Laboratory Chemicals*, BDH Ltd., Poole, Dorset, U.K., and the *United States Pharmacopeia and National Formulary*, U.S. Pharmacopeial Convention, Inc. (USPC), Rockville, MD.

⁶ The sole source of supply of the apparatus known to the committee at this time is Insta-Gel scintillator, available from PerkinElmer Life and Analytical Sciences, 940 Winter Street, Waltham, MA 02451. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee,¹ which you may attend.

8.7 *Cesium Carrier Solution* (1 mg/1 mL)—Cesium as cesium chloride (CsCl) in dilute hydrochloric acid.⁷

8.8 *Cobalt Carrier Solution* (1 mg/1 mL)—Cobalt as cobalt chloride (CoCl₂) in dilute hydrochloric acid.⁷

8.9 *Hydrochloric Acid* (sp gr 1.187)—Concentrated HCl.

8.10 *Hydrochloric Acid 10 M*—Dilute 833 mL of concentrated hydrochloric acid in 100 mL water and dilute to 1000 mL with water in a volumetric flask.

8.11 *Hydrochloric Acid 6 M*—Dilute 500 mL of concentrated hydrochloric acid in 400 mL of water, dilute to 1000 mL with water in a volumetric flask.

8.12 *Hydrochloric Acid 4 M*—Dilute 333 mL of concentrated hydrochloric acid in 600 mL of water, dilute to 1000 mL with water in a volumetric flask.

8.13 *Hydrochloric Acid 0.5 M*—Dilute 42 mL of concentrated hydrochloric acid in 900 mL of water, dilute to 1000 mL with water in a volumetric flask.

8.14 *Hydrochloric Acid 0.01 M*—Dilute 20 mL of 0.5 M HCl in 900 mL of water, dilute to 1000 mL with water in a volumetric flask.

8.15 *Hydrochloric—(6 M)—Hydrofluoric Acid (0.5 M)*—Dilute 500 mL of concentrated hydrochloric acid (HCl) (sp gr 1.187) and 20 mL of 49 % concentrated hydrofluoric acid (HF) in 400 mL of water, dilute to 1000 mL with water in a plastic or TFE-fluorocarbon volumetric flask.

8.16 *Iron Carrier Solution* (Fe⁺³ as ferric chloride)⁷—Dissolve 5.00 g of metallic iron in 300 mL of 6 M HCl, filter, dilute to 1 L, and calibrate using an atomic absorption spectrophotometer (Test Methods [D1068](#)).

8.17 *Manganese Carrier Solution* (1 mg/1 mL)—Mn⁺² in dilute nitric acid (HNO₃).⁷

8.18 *Niobium Carrier Solution* (1 mg/1 mL)—Nb⁺⁵ in 5 % hydrofluoric acid (1 + 9 M).⁷

8.19 *Nitric Acid* (sp gr 1.42)—Concentrated (HNO₃).

8.20 *Phosphoric Acid* (sp gr 1.834)—Concentrated (H₃PO₄).

8.21 *Sodium Hydroxide (6 M)*—Dissolve 24 g sodium hydroxide (NaOH) in 90 mL water, allow to cool, and dilute to 100 mL with water and store in plastic bottles; a commercially prepared solution may also be used.

8.22 *Zinc Carrier Solution* (1 mg/mL)—Zn⁺² in dilute hydrochloric acid.⁷

8.23 *Zirconium Carrier Solution* (1 mg/mL)—Zr⁺⁴ in dilute hydrochloric acid.⁷

8.24 *⁵⁵Fe Standard Solution*—Traceable to a national standards laboratory such as National Institute of Standards and Technology (NIST) or UK National Physical Laboratory (NPL).

8.25 *⁵⁹Fe Standard Solution*—Traceable to a national standards laboratory such as NIST or NPL.

9. Hazards

9.1 HF is extremely hazardous and should be used in a well-ventilated hood. Wear rubber gloves, safety glasses or goggles, and a laboratory coat. Avoid breathing any HF fumes. Clean all spills and wash thoroughly after using HF. Also, do not add HF to any glassware for it is a significant hazard and can affect analytical accuracy.

10. Sampling

10.1 Collect samples in accordance with procedures presented in Practices [D3370](#), as applicable.

10.2 If the sample is not acidified at the time of collection, 20 mL of concentrated HCl or HNO₃ should be added per 1000 mL of sample. After acidification of the sample, the sample should be allowed to sit overnight prior to analysis.

11. Calibration

11.1 The reference standard for both iron isotopes will contain 5 mg iron carrier. Add 6 drops of concentrated phosphoric acid to the carrier solution and heat on a hot plate until it clears. This will drive off any excess hydrochloric acid and water (to less than 0.5 mL but do not allow to bake dry). Add 1 mL of water and swirl in the glass vial. This final carrier solution should be colorless. Cool the vial to room temperature. Spike with the appropriate isotope and add 15 mL of scintillation cocktail. Cap and shake until the mixture is clear; this step ensures that the proper sample volume to scintillation cocktail volume ratio is obtained for a clear, homogeneous solution. The volume of the reference standard should be such that its addition to the sample does not cause additional quench.

11.2 Prepare a series of quenched ⁵⁵Fe standards and a series of quenched ⁵⁹Fe standards using various weights of iron carrier or concentration or volumes, or both, of acid. Use the least quenched standards in each set to optimize the liquid scintillation counter (LSC) discriminator settings and amplifier gain. Ensure that the ⁵⁵Fe spectrum does not spill over into the ⁵⁹Fe ROI. If your instrument does not allow for multiple nuclides to be optimized follow Practice [D7282](#) for instrument optimization.

11.3 Count each set of standards with the LSC automatic external standard ratio selected on to obtain approximately 1 % counting statistics (approximately 10 000 counts) in the ROI.

11.4 Prepare a curve of the ⁵⁵Fe efficiency versus the external standard ratio.

11.5 Prepare a crosstalk (XT) curve of the ratio of ⁵⁹Fe counts in the ⁵⁵Fe ROI to the ⁵⁹Fe counts in the ⁵⁹Fe ROI versus the external standard ratio.

11.6 Additional guidance on the set-up, calibration and calibration verification of the instrument can be found in Practice [D7282](#).

12. Procedure

12.1 Measure an acidified and filtered aliquant of the sample (approximately 0.05 L) into a 100 mL centrifuge tube.

⁷ Commercially available atomic absorption reference standards in 1 mg = 1 mL concentrations may be used as carriers.