
**Rubber — Measurement of
vulcanization characteristics using
curemeters —**

**Part 1:
Introduction**

iTeh STANDARD PREVIEW
*Caoutchouc — Mesure des caractéristiques de vulcanisation à l'aide
de rhéomètres —*
(standards.iteh.ai)
Partie 1: Introduction

[ISO 6502-1:2018](https://standards.iteh.ai/catalog/standards/sist/0cd2ae3b-a30e-4e4f-b8ae-d041592ebaf3/iso-6502-1-2018)

[https://standards.iteh.ai/catalog/standards/sist/0cd2ae3b-a30e-4e4f-b8ae-
d041592ebaf3/iso-6502-1-2018](https://standards.iteh.ai/catalog/standards/sist/0cd2ae3b-a30e-4e4f-b8ae-d041592ebaf3/iso-6502-1-2018)



iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 6502-1:2018

<https://standards.iteh.ai/catalog/standards/sist/0cd2ae3b-a30e-4e4f-b8ae-d041592ebaf3/iso-6502-1-2018>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2018

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Fax: +41 22 749 09 47
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword.....	iv
Introduction.....	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Basic principles	2
5 Types of curemeter	5
6 Apparatus	6
6.1 General.....	6
6.2 Dies.....	7
6.3 Die closure.....	8
6.4 Moving member.....	8
6.5 Movement.....	8
6.6 Stiffness measurement.....	9
6.7 Heating and temperature control.....	9
6.8 Calibration.....	9
7 Test piece	9
8 Vulcanization temperature	9
9 Conditioning	10
10 Procedure	10
10.1 Preparation for test.....	10
10.2 Loading the curemeter.....	10
11 Expression of results	10
Annex A (informative) Effect of thermal parameters on measured cure properties	11
Bibliography	14

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html. (standards.iteh.ai)

This document was prepared by Technical Committee ISO/TC 45, *Rubber and rubber products*, Subcommittee SC 2, *Testing and analysis*. ISO 6502-1:2018

This first edition of ISO 6502-1 cancels and replaces the fourth edition of ISO 6502:2016, which has been technically revised to keep consistency within the ISO 6502 series.

A list of all parts in the ISO 6502 series can be found on the ISO website.

Introduction

An International Standard specifying requirements for the use of oscillating disc curemeters was established in 1977 as ISO 3417, *Rubber — Measurement of vulcanization characteristics with the oscillating disc curemeter*. Later, when various rotorless curemeters were developed and became popular, an International standard for these instruments was produced as ISO 6502, *Rubber — Measurement of cure characteristics with rotorless curemeters*. However, because of the variety of available instruments that differed in geometry and construction, ISO 6502 was not able to specify such requirements in detail. In 1999, it became clear that a number of different rotorless curemeters were available and that significant developments had taken place and were continuing. Hence, it was concluded that, rather than specify individual rotorless instruments, possibly restricting future developments, a more general document was required. Accordingly, it was decided to provide guidance and assistance in the design and use of curemeters generally, and the title of ISO 6502 was changed to *Rubber — Guide to the use of curemeters*. As the use of rotorless curemeters has become more mature, it has now been decided to revise the Guide as *Rubber — Measurement of vulcanization characteristics using curemeters — Part 1: Introduction*, with subsequent parts for oscillating disc curemeters and rotorless curemeters.

iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO 6502-1:2018](https://standards.iteh.ai/catalog/standards/sist/0cd2ae3b-a30e-4e4f-b8ae-d041592ebaf3/iso-6502-1-2018)

<https://standards.iteh.ai/catalog/standards/sist/0cd2ae3b-a30e-4e4f-b8ae-d041592ebaf3/iso-6502-1-2018>

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 6502-1:2018

<https://standards.iteh.ai/catalog/standards/sist/0cd2ae3b-a30e-4e4f-b8ae-d041592ebaf3/iso-6502-1-2018>

Rubber — Measurement of vulcanization characteristics using curemeters —

Part 1: Introduction

WARNING 1 — Persons using this document should be familiar with normal laboratory practice. This document does not purport to address all of the safety problems, if any, associated with its use. It is the responsibility of the user to establish appropriate safety and health practices and to determine the applicability of any other restrictions.

WARNING 2 — Certain procedures specified in this document might involve the use or generation of substances, or the generation of waste, that could constitute a local environmental hazard. Reference should be made to appropriate documentation on safe handling and disposal after use.

1 Scope

This document provides an introduction to the determination of vulcanization characteristics of rubber compounds by means of curemeters.

2 Normative references (standards.iteh.ai)

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1382, *Rubber — Vocabulary*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 1382 and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

3.1 oscillating-disc curemeter

ODC

curemeter consisting of a biconical disc oscillated within a temperature-controlled die cavity containing the test piece

Note 1 to entry: An oscillating-disc curemeter is also known as an oscillating disc rheometer (ODR).

3.2 rotorless curemeter

RCM

curemeter consisting of two dies forming a temperature-controlled cavity, one of which is moved relative to the other to apply a stress or strain to the test piece

Note 1 to entry: A rotorless curemeter is also known as a moving die rheometer (MDR).

**3.3
marching-modulus cure**

type of vulcanization during which the modulus does not reach a maximum value but, after a rapid rise, continues to rise slowly at the vulcanization temperature

**3.4
vulcanization characteristics**
characteristics which can be taken from a vulcanization curve

Note 1 to entry: See [Figure 1](#).

Note 2 to entry: More explanations are given in [Clause 4](#).

**3.5
stiffness**
measure of the resistance offered by rubber to deformation

Note 1 to entry: Force and torque have not been defined since they have a generally accepted scientific meaning.

4 Basic principles

The properties of a rubber compound change during the course of vulcanization, and the vulcanization characteristics can be determined by measuring properties as a function of time and temperature. Vulcanization characteristics are most commonly determined using instruments known as curemeters in which a cyclic stress or strain is applied to a test piece and the associated strain or force is measured. Normally, the test is carried out at a predetermined constant temperature and the measure of stiffness recorded continuously as a function of time.

The stiffness of the rubber increases as vulcanization proceeds. Vulcanization is complete when the recorded stiffness rises to a plateau value or to a maximum and then declines (see [Figure 1](#)). In the latter case, the decrease in stiffness is caused by reversion. In cases where the recorded stiffness continues to rise (marching-modulus cure), vulcanization is deemed to be complete after a specified time. The time required to obtain a vulcanization curve is a function of the test temperature and the characteristics of the rubber compound. Curves analogous to [Figure 1](#) are obtained for a curemeter in which strain is measured.

Direct proportionality between torque and stiffness cannot be expected under all conditions and all instruments because, particularly at in high torque ranges, elastic deformation of the disc shaft and driving device has to be taken into account, Moreover, in cases of small amplitudes of deformation, the strain can be expected to have a considerable elastic component. However, for routine control purposes, corrections are not necessary.

The following vulcanization characteristics can be taken from the measure of stiffness against time curve (see [Figure 1](#)).

Minimum force or torque	F_L or M_L
Force or torque at a specified time t	F_t or M_t
Scorch time (time to incipient cure)	t_{sx}
Time to a percentage y of full cure from minimum force or torque	$t'_c(y)$
Plateau force or torque	F_{HF} or M_{HF}
Maximum force or torque (reverting cure)	F_{HR} or M_{HR}
Force or torque value attained after a specified time (marching-modulus cure)	F_H or M_H

The minimum force or torque F_L or M_L characterizes the stiffness of the unvulcanized compound at the curing temperature.

The scorch time (time to incipient cure) t_{sx} is a measure of the processing safety of the compound.

The time $t'_c(y)$ and the corresponding forces or torques give information on the progress of cure. The optimum cure is often taken as $t'_c(90)$.

The highest force or torque is a measure of the stiffness of the vulcanized rubber at the curing temperature.

NOTE The term F denotes force and the term M denotes torque.

The scorch time t_{sx} is the time required for the force or torque to increase by x units from F_L . It might be convenient to define the scorch as a given percentage, e.g. 2 % or 5 %, of the total cure.

The time to a percentage of full cure from minimum force, $t'_c(y)$, is the time taken for the force (or torque) to reach:

$$F_L + 0,01y(F_{HF} - F_L) \quad (1)$$

or

$$M_L + 0,01y(M_{HF} - M_L) \quad (2)$$


— $t'_c(10)$ is a measure of the early stages of cure.

— $t'_c(50)$ can be determined accurately providing the slope of the curve is greatest at this point.

— $t'_c(90)$ is often used as an indicator of optimum press cure.

The cure rate index is the average slope of the rising curve and is given by:

$$100 / [t'_c(y) - t_{sx}] \quad (3)$$

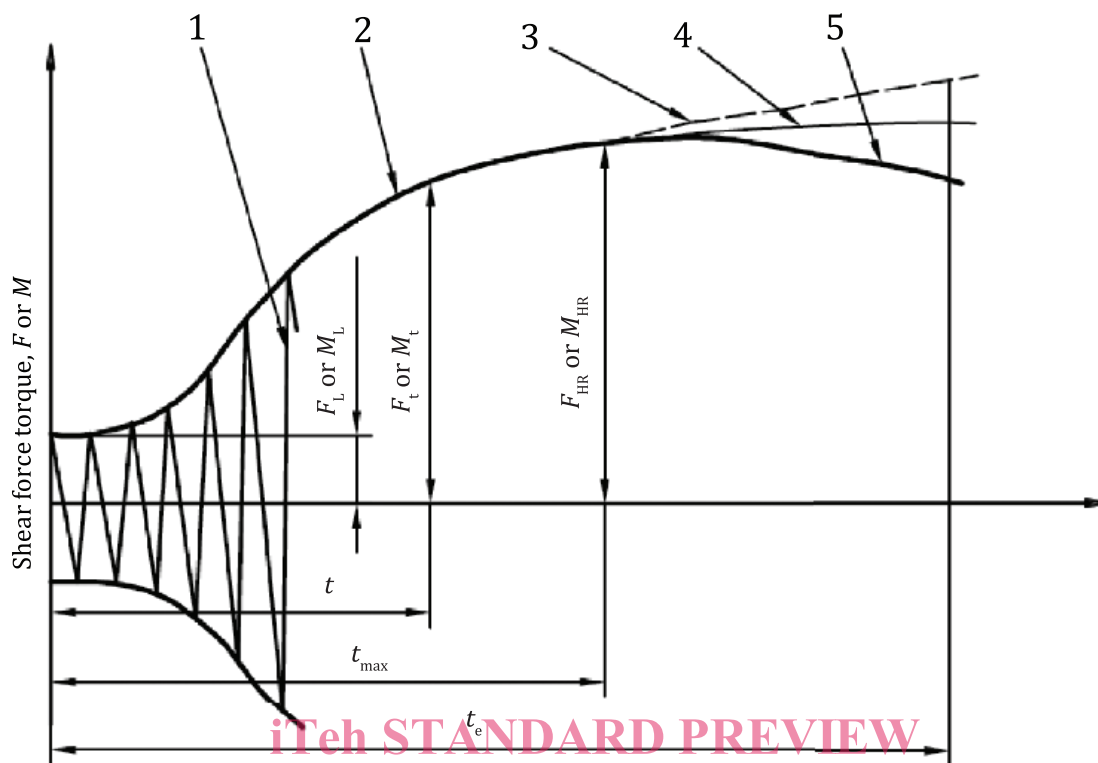


iTeh STANDARD PREVIEW

(standards.iteh.ai)

a) Vulcanization curve F or $M = f(t)$

ISO 6502-1:2018

<https://standards.iteh.ai/catalog/standards/sist/0cd2ae3b-a30e-4e4f-b8ae-d041592ebaf3/iso-6502-1-2018>

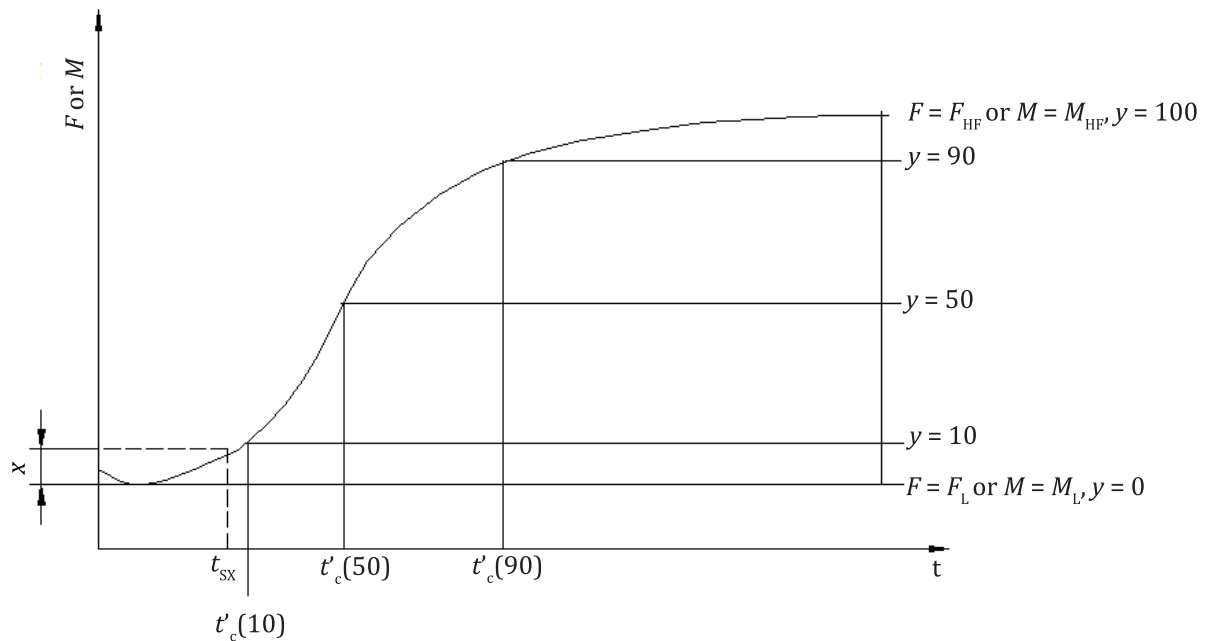

b) Method of evaluation

Key

- 1 sinusoidal curve
- 2 envelope curve
- 3 vulcanization curve with steady increase to F_H or M_H at time t_e at end of test (marching-modulus cure)
- 4 vulcanization curve with plateau at F_{HF} or M_{HF} (plateau cure)
- 5 vulcanization curve with maximum F_{HR} or M_{HR} at time t_{max} (reverting cure)

Figure 1 — Typical vulcanization curve and method of evaluation

5 Types of curemeter

Three types of curemeters have found widespread use:

- oscillating-disc;
- reciprocating-paddle;
- rotorless.

Other geometries are possible, for example with a vibrating probe or needle.

The reciprocating-paddle type was popular, but is now more or less obsolete and is not considered further in this document.

The oscillating-disc curemeter consists of a biconical disc that oscillates in a closed cavity. It was for many years the most widely used type of instrument.

In rotorless curemeters, one half of a die enclosing the test piece, rather than a disc within the test piece, oscillates or reciprocates. The rotorless type of curemeter has increased greatly in popularity, largely because of its advantages of the specified temperature being reached in a shorter time after insertion of the test piece into the die cavity and better temperature distribution in the test piece (see [Annex A](#)).