
**Methods for the calibration of
vibration and shock transducers —
Part 34:
Testing of sensitivity at fixed
temperatures**

iTeh STANDARD PREVIEW
*Méthodes pour l'étalonnage des transducteurs de vibrations et de
chocs —
(standards.iteh.ai)
Partie 34: Essai de sensibilité à des températures fixes*

[ISO 16063-34:2019](https://standards.iteh.ai/catalog/standards/sist/7B49882-347d-446c-9ba0-a484b91842a9/iso-16063-34-2019)

<https://standards.iteh.ai/catalog/standards/sist/7B49882-347d-446c-9ba0-a484b91842a9/iso-16063-34-2019>



iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 16063-34:2019

<https://standards.iteh.ai/catalog/standards/sist/7B49882-347d-446c-9ba0-a484b91842a9/iso-16063-34-2019>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2019

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Fax: +41 22 749 09 47
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword.....	iv
Introduction.....	v
1 Scope.....	1
2 Normative references.....	1
3 Terms and definitions.....	1
4 Uncertainty of measurement.....	2
5 Ambient conditions.....	3
6 Apparatus.....	3
7 Method 1: Determination of complex sensitivity using a laser interferometer.....	4
7.1 General.....	4
7.2 Method.....	5
7.2.1 Test procedure.....	5
7.2.2 Expression of results.....	5
8 Method 2: Determination of complex sensitivity using a reference transducer inside a temperature chamber.....	6
8.1 General.....	6
8.2 Method.....	6
8.2.1 Test procedure.....	6
8.2.2 Expression of results.....	7
9 Method 3: Determination of complex sensitivity using a reference transducer outside the temperature chamber.....	7
9.1 General.....	7
9.2 Method.....	8
9.2.1 Test procedure.....	8
9.2.2 Expression of results.....	9
10 Preferred amplitudes, frequencies and temperatures.....	9
11 Test report.....	10
Annex A (informative) Determination of the achieving time of setpoint temperature for a device under test.....	12
Annex B (informative) Evaluating uncertainty caused by temperature tolerance.....	14
Bibliography.....	16

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 108, *Mechanical vibration, shock and condition monitoring*.

This first edition of ISO 16063-34 cancels and replaces ISO 5347-17:1993, which has been technically revised. The main changes are as follows:

- a method for the determination of complex sensitivity using a laser interferometer has been added;
- a method for the determination of complex sensitivity using a reference transducer inside the temperature chamber has been added;
- a procedure for testing phase changes has been added;
- [Annex A](#) for the determination of the achievement time of the setpoint temperature for the device under test has been added;
- [Annex B](#) for the evaluating uncertainty caused by temperature tolerance has been added.

A list of all parts in the ISO 16063 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

The purpose of this document is to establish the procedures for testing the complex sensitivity of vibration transducers at fixed temperatures in the temperature range from -190 °C to 800 °C and frequency range from 10 Hz to 3 kHz.

The three methods described in this document allow the determination of the complex sensitivity or temperature response of complex sensitivity of a transducer to sinusoidal vibration in the temperature chamber.

Principles, procedures, and uncertainties of calibrations such as a comparison to a reference transducer or an absolute measurement by laser interferometer are given in this document. Calibrations are carried out using one of the three methods, depending on the different principles to be used and the temperature and frequency range limitations.

iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO 16063-34:2019](https://standards.iteh.ai/catalog/standards/sist/7B49882-347d-446c-9ba0-a484b91842a9/iso-16063-34-2019)

<https://standards.iteh.ai/catalog/standards/sist/7B49882-347d-446c-9ba0-a484b91842a9/iso-16063-34-2019>

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO 16063-34:2019

<https://standards.iteh.ai/catalog/standards/sist/7B49882-347d-446c-9ba0-a484b91842a9/iso-16063-34-2019>

Methods for the calibration of vibration and shock transducers —

Part 34: Testing of sensitivity at fixed temperatures

1 Scope

This document details specifications for the instrumentation and methods to be used for testing fixed temperature sensitivity of vibration transducers. It applies to rectilinear velocity and acceleration transducers.

The methods specified use both a comparison to a reference transducer and an absolute measurement by laser interferometer.

This document is applicable for a frequency range from 10 Hz to 3 kHz (method-dependent), a dynamic range from 1 m/s² to 100 m/s² (frequency-dependent) and a temperature range from -190 °C to 800 °C (method-dependent). Although it is possible to achieve these ranges among all the described systems, generally each has limitations within them.

Method 1 (using a laser interferometer) is applicable to magnitude of sensitivity and phase calibration in the frequency range 10 Hz to 3 kHz at fixed temperatures (see [Clause 7](#)). Method 2 (using a reference transducer inside a chamber whose temperature limit is -70 °C to 500 °C) can be used for magnitude of sensitivity and phase calibration in the frequency range 10 Hz to 1 kHz at fixed temperatures (see [Clause 8](#)). Method 3 (using a reference transducer outside the chamber) can only be used for the determination of the temperature response of complex sensitivity over a certain temperature range (see [Clause 9](#)).

NOTE Method 1 and Method 2 can provide the deviation of complex sensitivity over a certain temperature range if the calibration is also done at the reference temperature (room temperature 23 °C ± 5 °C).

To ensure the consistency of the use and test condition, the transducer, its cable and the conditioning amplifier are intended to be considered as a single unit and tested together.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 2041, *Mechanical vibration, shock and condition monitoring — Vocabulary*

ISO 16063-11:1999, *Methods for the calibration of vibration and shock transducers — Part 11: Primary vibration calibration by laser interferometry*

ISO 16063-21:2003, *Methods for the calibration of vibration and shock transducers — Part 21: Vibration calibration by comparison to a reference transducer*

3 Terms and definitions

For the purpose of this document, the terms and definitions given in ISO 2041 and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp/>
- IEC Electropedia: available at <http://www.electropedia.org/>

3.1

temperature response

sensitivity of the transducer at a given frequency as a function of its steady-state temperature

Note 1 to entry: Temperature response is measured at specified frequencies within the rated frequency range of the transducer.

Note 2 to entry: In general, the sensitivity is a complex-valued function quantity and can be expressed in terms of its magnitude and phase.

4 Uncertainty of measurement

The limits of the uncertainty of measurement in terms of expanded uncertainty applicable to this document are as follows.

- a) For the magnitude of sensitivity:
- when using a laser interferometer (Method 1): 0,5 % of the measured value at reference conditions; 1 % of the measured value outside reference conditions,
 - when using a reference transducer (Method 2): 1 % of the measured value at reference conditions; 2 % of the measured value outside reference conditions,
 - when using a reference transducer (Method 3): 2 % of the measured value at reference conditions; 3 % of the measured value outside reference conditions.
- b) For the phase shift of sensitivity:
- when using a laser interferometer (Method 1): 0,5° at reference conditions; 1° outside reference conditions,
 - when using a reference transducer (Method 2): 1° at reference conditions; 2,5° outside reference conditions,
 - when using a reference transducer (Method 3): 2° at reference conditions; 3° outside reference conditions.
- c) Recommended reference conditions are as follows:
- frequency $f = 160, 80, 40$ or 16 Hz (or angular frequency $\omega = 1\ 000$ rad/s, 500 rad/s, 250 rad/s or 100 rad/s),
 - acceleration (acceleration amplitude or RMS value): 50 m/s^2 , 20 m/s^2 , 10 m/s^2 or 5 m/s^2 .

NOTE In practice, these limits can be exceeded depending on the vibratory characteristics of the fixture on the exciter; higher uncertainty values are accepted at some frequencies according to use requirements.

To undertake measurements over the proposed temperature range in supporting uncertainty budgets for transverse, bending, rocking accelerations, hum and noise, and relative motion issues, those measurements should be done at room temperature because the selected ceramic rod shall be rigid throughout the proposed temperature range.

The uncertainty of measurement shall be assessed and reported according to ISO 16063-11:1999, Annex A, and ISO 16063-21:2003, Annex A, to document the level of uncertainty expressed as expanded uncertainties for a coverage factor of 2 or a confidence probability of 95 %. It is the responsibility of the laboratory or end user to make sure that the reported values of expanded uncertainty are credible.

5 Ambient conditions

Calibration shall be carried out under the following ambient conditions:

- a) room temperature, (23 ± 5) °C;
- b) relative humidity, 75 % max.

6 Apparatus

The usual laboratory apparatus and, in particular, the following.

6.1 Vibration exciter.

Orientated vertically or horizontally, the vibrator exciter shall be used to cover the requested frequency and dynamic ranges.

6.2 Fixture.

Made of machinable ceramics, the fixture shall have low thermal conductivity and high stiffness. By mounting the tested transducer on the top of a ceramic rod, the rod protrudes into the temperature chamber from a vibration exciter on which it is placed. To reflect the laser, the surface of the mounting transducer should be optically polished, covered by a mirror, or be plated with chrome, or as adequate.

6.3 Temperature chamber.

The chamber should have a temperature range from -190 °C to 800 °C and should be specially designed so that the air temperature in the working space (the part of the chamber in which the device under test [DUT] can be maintained within the specified temperature tolerances) evenly achieves temperature uniformity within ± 2 °C at fixed temperatures. At the top of the chamber, a hole should be sealed with glass, so that the laser passes through. An additional aperture on the side of the chamber is required to enable cables to be fed from the transducer under test to the external conditioning amplifier. A suitable sealing arrangement needs to be provided to maintain the chamber temperature. The design of the equipment shall also take into consideration the clamping of the transducer cables to reduce cable strain and flap. The indicated temperature range and temperature uniformity within ± 2 °C are not mandatory. The chamber shall cover the required temperature range. Temperature uniformity within ± 2 °C is recommended in some cases.

6.4 Temperature sensor.

The air temperature in the chamber is measured and controlled by a temperature sensor located close to the transducer under test. The location of the temperature sensor has no influence on the mounting and vibration of the transducer. Beside the control sensor, a second measurement sensor for temperature should be introduced; at least thermal stability of the air in the temperature chamber should be monitored separately.

6.5 Interferometer.

Refer to ISO 16063-11:1999, 3.6.

6.6 Reference transducer.


Together with the conditioning amplifier, the reference transducer should be calibrated according to [Clause 7](#) with documented uncertainty (for Method 2) and calibrated by primary or comparison means with documented uncertainty (for Method 3). For Method 3, the temperature influence on the reference transducer shall be less than $\pm 0,5$ % of the reading.

Other apparatuses (e.g. data acquisition instrumentation) shall be as specified in ISO 16063-11:1999, Clause 3 for Method 1 and in ISO 16063-21:2003, Clause 4 for Methods 2 and 3.

7 Method 1: Determination of complex sensitivity using a laser interferometer

7.1 General

This test system primarily contains a vibration exciter equipped with a specially designed fixture for mounting a transducer, a temperature chamber and a laser interferometer; see [Figure 1](#).

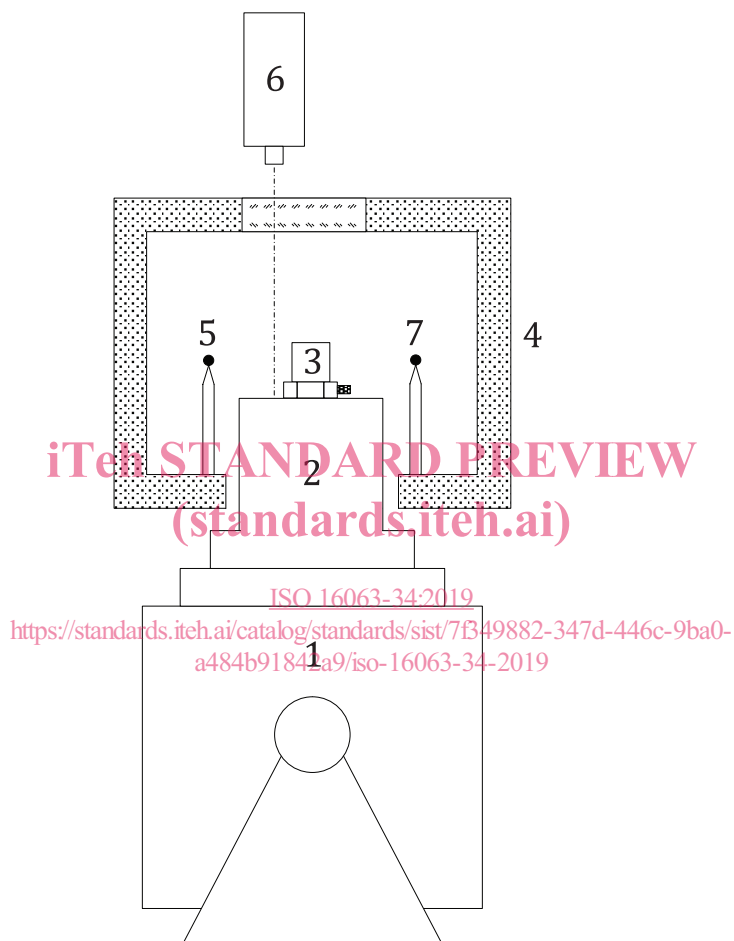

Key

- | | | | |
|---|--|---|----------------------------|
| 1 | vibration exciter (vertical or horizontal) | 5 | control temperature sensor |
| 2 | fixture (ceramic rod) | 6 | interferometer |
| 3 | transducer under test | 7 | measure temperature sensor |
| 4 | temperature chamber | | |

Figure 1 — Test system with a laser interferometer

When testing by laser interferometer, the fixture transfer function error may be ignored, and the frequency response of the tested transducer's complex sensitivity for a certain frequency range at a fixed temperature can be determined. The laser interferometer can be positioned to measure the amplitude of the top of the ceramic rod close to the transducer under test. To reduce bending, tipping and transverse motion errors, several measurements can be taken around the base of the transducer under test and the average measurement can be used in the acceleration calculation.

The fringe-counting method and sine-approximation method are used to determine the complex sensitivity in the case of a fixed temperature. The fringe-counting method is applicable to sensitivity magnitude testing in the frequency range from 10 Hz to 800 Hz; this method may also be applied to higher frequencies if the quantization error is suppressed by special means. The sine-approximation method is applicable to sensitivity magnitude and phase shift testing in the frequency range from 10 Hz to 3 kHz. For more details, see ISO 16063-11.

7.2 Method

7.2.1 Test procedure

Install the equipment as per [Figure 1](#).

The transducer under test is mounted by using the recommended torque from the manufacture's manual under ambient conditions. Tests in this condition permit the comparison of the complex sensitivity of the transducer at other temperatures.

Set the temperature of the chamber to the specified value. Once the temperature measured by the temperature sensor has reached the set value, maintain this temperature until the transducer under test has achieved temperature stability (see [Annex A](#)). Stability is recommended within ± 2 °C. Then set the test frequency and adjust the vibrator amplitude to a certain level and measure the complex sensitivity using a laser interferometer. Several test frequencies are needed to determine the frequency response of complex sensitivity. Change the temperature and repeat the procedure above. The temperature response of the tested transducer can then be obtained.

NOTE The temperature stability within ± 2 °C is not mandatory. However, in some cases where the transducer sensitivity is changed greatly around a temperature, especially at extreme temperatures, bigger tolerances can result in higher uncertainty (see [Annex B](#)).

The design of the system should also ensure that there is no condensation/icing on the glass window and the reflective surface on the ceramic rod occurs which would prejudice the laser interferometer amplitude measurement. For temperature ranges containing positive and negative temperatures, it is better to perform the positive temperature test first and then to dry the chamber and perform the negative temperature test to avoid ice and frost.

7.2.2 Expression of results

If the fringe-counting method is used, calculate the sensitivity magnitude S_t according to ISO 16063-11:1999, 7.3. The magnitude S_t of the transducer at the selected frequency or frequency response can be obtained at a fixed temperature.

If the sine-approximation method is used, calculate the sensitivity magnitude S_t and phase shift $\Delta\phi_t$ according to ISO 16063-11:1999, 9.4. The magnitude S_t and phase shift $\Delta\phi_t$ of the transducer at the selected frequency or frequency response can be obtained at a fixed temperature.

If the test data under room temperature are available, calculate the change of the complex sensitivity with respect to the temperature. The results can be expressed as a curve of temperature response for the transducer.

NOTE 1 The testing frequency range can be from 10 Hz to 3 kHz or even higher, depending on the working range of the vibration exciter, on the mass of the fixtures and the tested transducer, etc.

NOTE 2 Instead of an interferometer, a laser vibrometer can be used as the reference standard.