



SLOVENSKI STANDARD
oSIST prEN 16479:2022

01-januar-2022

Kakovost vode - Zahteve za zmogljivost in postopki preskušanja skladnosti opreme za monitoring vode - Avtomatski vzorčevalniki za vodo in odpadno vodo

Water quality - Performance requirements and conformity test procedures for water monitoring equipment - Automated sampling devices (samplers) for water and waste water

Wasserbeschaffenheit - Leistungsanforderungen und Konformitätsprüfungen für Geräte zum Wassermonitoring - Automatische Probenahmegeräte für Wasser und Abwasser

(standards.iteh.ai)

Qualité de l'eau - Exigences de performance et modes opératoires d'essai de conformité pour les équipements de surveillance de l'eau - Dispositifs d'échantillonnage automatiques (échantillonneurs) pour l'eau et les eaux usées

Ta slovenski standard je istoveten z: prEN 16479

ICS:

13.060.45 Preiskava vode na splošno Examination of water in general

oSIST prEN 16479:2022

en,fr,de

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[oSIST prEN 16479:2022](#)

<https://standards.iteh.ai/catalog/standards/sist/acb8f028-a492-44a8-bae0-43288f2cd140/osist-pren-16479-2022>

EUROPEAN STANDARD
NORME EUROPÉENNE
EUROPÄISCHE NORM

DRAFT
prEN 16479

December 2021

ICS 13.060.45

Will supersede EN 16479:2014

English Version

Water quality - Performance requirements and conformity test procedures for water monitoring equipment - Automated sampling devices (samplers) for water and waste water

Qualité de l'eau - Exigences de performance et modes opératoires d'essai de conformité pour les équipements de surveillance de l'eau - Dispositifs d'échantillonnage automatiques (échantillonneurs) pour l'eau et les eaux usées

Wasserbeschaffenheit - Leistungsanforderungen und Konformitätsprüfungen für Geräte zum Wassermonitoring - Automatische Probenahmegeräte für Wasser und Abwasser

This draft European Standard is submitted to CEN members for enquiry. It has been drawn up by the Technical Committee CEN/TC 230.

If this draft becomes a European Standard, CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration.

This draft European Standard was established by CEN in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN-CENELEC Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Republic of North Macedonia, Romania, Serbia, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and United Kingdom.

Recipients of this draft are invited to submit, with their comments, notification of any relevant patent rights of which they are aware and to provide supporting documentation.

Warning : This document is not a European Standard. It is distributed for review and comments. It is subject to change without notice and shall not be referred to as a European Standard.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

CEN-CENELEC Management Centre: Rue de la Science 23, B-1040 Brussels

Contents	Page
European foreword.....	3
Introduction	4
1 Scope	5
2 Normative references	5
3 Terms and definitions	5
4 General requirements for samplers	8
5 Performance requirements	11
5.1 Sample volume	11
5.2 Sampling principles.....	11
5.3 Sample line velocity.....	11
5.4 Power supply	11
5.5 Sample integrity	11
5.6 Sample timing error	12
5.7 Effect of ambient air temperature	12
5.7.1 Samplers not incorporating sample temperature control.....	12
5.7.2 Samplers incorporating sample temperature control	12
6 Conformity testing	13
6.1 General requirements	13
6.2 Test conditions.....	13
6.3 Verification by inspection.....	14
6.4 Performance tests.....	14
6.4.1 Collected sample volume.....	14
6.4.2 Testing of sampling principles	16
6.4.3 Sample line velocity.....	17
6.4.4 Power supply test.....	18
6.4.5 Sample integrity	19
6.4.6 Sampler timing error	20
6.4.7 Ambient air temperature effects	20
Annex A (normative) Evaluation of conformity test data	23
Annex B (informative) Example calculations	28
Annex C (informative) Example procedure for demonstrating sample integrity for samplers to be used for Urban Waste Water Treatment Directive (UWWTD) sampling	41
Annex D (informative) Example format for the report	43
Bibliography	46

European foreword

This document (prEN 16479:2021) has been prepared by Technical Committee CEN/TC 230 “Water analysis”, the secretariat of which is held by DIN.

This document is currently submitted to the CEN Enquiry.

This document will supersede EN 16479:2014.

iTeh STANDARD PREVIEW (standards.iteh.ai)

[oSIST prEN 16479:2022](https://standards.iteh.ai/catalog/standards/sist/acb8f028-a492-44a8-bae0-43288f2cd140/osist-pren-16479-2022)

<https://standards.iteh.ai/catalog/standards/sist/acb8f028-a492-44a8-bae0-43288f2cd140/osist-pren-16479-2022>

prEN 16479:2021 (E)**Introduction**

This document is a product standard for automatic sampling devices (samplers) for water and waste water. It defines general requirements, performance requirements, and procedures for the conformity testing of samplers.

The general requirements include functional facilities that samplers need to meet users' applications and information that needs to be included in associated documents. Conformity with these requirements is verified by inspection. The performance requirements define the capability of a sampler to collect samples of water reliably. Conformity with these requirements is determined by testing carried out in a laboratory under controlled conditions. Statistical procedures are defined for evaluation of the conformity test data and some example calculations are provided.

These requirements and statistical procedures take into account those specified in ISO 5667-10:2020^[1] for automatic samplers. Samplers that are shown, by means of the tests, to conform to the requirements specified in this document are considered to be fit for purpose. However, this document does not cover the installation and on-going use of samplers.

This document is associated with EN 17075^[2] which covers measuring devices for water and waste water.

Automatic sampling devices are widely used for compliance monitoring purposes under national and European regulations. This document supports the requirements of the following EU Directives:

- Industrial Emissions Directive (2010/75/EU) [3].
- Urban Waste Water Treatment Directive (UWWTD) (91/271/EEC and 98/15/EEC) [4].
- Water Framework Directive (2000/60/EC) [5].
- Marine Strategy Framework Directive (2008/56/EC) [6].

The use of an automatic sampling device, for example in a hazardous environment, can also be subject to national, European and international rules and legislation governing the safety of products.

1 Scope

This document defines general requirements, performance requirements and conformity test procedures for automatic sampling devices (samplers) for water and waste water that:

- sample water and waste water from non-pressurized (i.e. open to atmosphere) channels or vessels;
- sample over extended periods to collect discrete or composite samples based on time, event or flow proportional sampling.

It does not include sampling systems built into online and in-line analysers.

The general requirements include functional facilities that samplers need to meet users' applications and information that needs to be included in associated documents.

The test procedures specify uniform methods to be used when determining key performance characteristics of samplers. All of the test procedures are expected to be carried out under laboratory conditions. It is recognized that for some samplers certain test procedures are not applicable.

Statistical procedures are defined for evaluation of the test data. Some example calculations are provided.

Specific sample integrity requirements are defined for samplers to be used for the collection of samples of final effluent or influent for the purpose of monitoring the performance of waste water treatment works, as required under the EU's Urban Waste Water Treatment Directive (UWWTD). Samplers to be used for other industrial applications do not need to be assessed against these specific sample integrity requirements.

This document does not cover the installation and on-going use of samplers.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

EN ISO/IEC 17025, *General requirements for the competence of testing and calibration laboratories (ISO/IEC 17025)*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

3.1

automatic sampling device for water and waste water

automatic sampler

equipment for collecting and storing samples of water or waste water for subsequent laboratory analysis

prEN 16479:2021 (E)**3.2****bias**

estimate of a systematic measurement error

Note 1 to entry: The systematic measurement error is a component of measurement error that in replicate measurements remains constant or varies in a predictable manner.

[SOURCE: ISO/IEC Guide 99:2007, 2.18, modified — Note 1 to entry has been added.]

3.3**composite sample**

two or more samples or sub-samples, mixed together in appropriate known proportions (either discretely or continuously), from which the average value of a desired characteristic may be obtained

Note 1 to entry: The proportions are usually based on time or flow measurements.

[SOURCE: ISO 6107:2021, 3.126]

3.4**constant volume variable time sampling****C.V.V.T.**

flow proportional sampling based on collecting equal volumes of sample at frequencies proportional to flow

3.5**constant time variable volume sampling****C.T.V.V.**

flow proportional sampling based on collecting samples at fixed time intervals but where the volume of sample is varied in proportion to the flow

3.6**constant time constant volume sampling****C.T.C.V.**

equal volumes of sample or sub-sample collected at equal increments of time

3.7**determinand**

property/substance that is required to be measured and to be reflected by/present in a calibration solution

[SOURCE: EN ISO 15839:2006, 3.13]

3.8**discrete sample**

single sample taken from a body of water

[SOURCE: ISO 6107:2021, 3.183, modified — “process, whereby” deleted]

iTeh STANDARD PREVIEW

(standards.iteh.ai)

oSIST prEN 16479:2022
<https://standards.iteh.ai/catalog/standards/sist/acb8f028-a492-44a8-bac0-43288f2cd140/osist-pren-16479-2022>

3.9**measurement error
error of measurement
error**

measured quantity value minus a reference quantity value

Note 1 to entry: The concept of "measurement error" can be used both:

- a) when there is a single reference quantity value to refer to, which occurs if a calibration is made by means of a measurement standard with a measured quantity value having a negligible measurement uncertainty or if a conventional quantity value is given, in which case the measurement error is known, and
- b) if a measurand is supposed to be represented by a unique true quantity value or a set of true quantity values of negligible range, in which case the measurement error is not known.

Note 2 to entry: "Measurement error" is not to be confused with production error or mistake.

[SOURCE: ISO/IEC Guide 99:2007, 2.16]

3.10**rated operating conditions**

minimum to maximum values of any environmental, fluid or electrical parameter within which the sampler is designed to operate without adjustment and with errors within performance limits

3.11**lift height**

vertical distance between the surface of the water being sampled and the highest point to which the sample is lifted

iTeh STANDARD PREVIEW
(standards.iteh.ai)

Note 1 to entry: Sometimes called "sampling head" or "suction height".
<https://standards.iteh.ai/catalog/standards/sist/acb8f028-492-44a8-bac0-43288f2cd140/osist-pren-16479-2022>

Note 2 to entry: The maximum lift height for samplers using vacuum pumps (e.g. pneumatic samplers and peristaltic samplers) is set to an atmospheric pressure of 1 000 mbar. At low atmospheric pressure the maximum lift height will be consequentially lower.

3.12**measurement repeatability
repeatability**

measurement precision under a set of repeatability conditions of measurement

[SOURCE: ISO/IEC Guide 99:2007, 2.21]

prEN 16479:2021 (E)**3.13****repeatability condition of measurement****repeatability condition**

condition of measurement, out of a set of conditions that includes the same measurement procedure, same operators, same measuring system, same operating conditions and same location, and replicate measurements on the same or similar objects over a short period of time

Note 1 to entry: A condition of measurement is a repeatability condition only with respect to a specified set of repeatability conditions.

Note 2 to entry: In chemistry, the term “intra-serial precision condition of measurement” is sometimes used to designate this concept.

[SOURCE: ISO/IEC Guide 99:2007, 2.20]

3.14**precision**

closeness of agreement between indications or measured quantity values obtained by replicate measurements on the same or similar objects under specified conditions

Note 1 to entry: Measurement precision is usually expressed numerically by measures of imprecision, such as standard deviation, variance, or coefficient of variation under specified conditions of measurement.

Note 2 to entry: The “specified conditions” can be, for example, repeatability conditions of measurement, intermediate precision conditions of measurement, or reproducibility conditions of measurement (see ISO 5725-3:1994).

Note 3 to entry: Measurement precision is used to define measurement repeatability, intermediate measurement precision, and measurement reproducibility.

<https://standards.iteh.ai/catalog/standards/sist/acb8f028-a492-44a8-bae0->

Note 4 to entry: Sometimes “measurement precision” is erroneously used to mean measurement accuracy.

[SOURCE: ISO/IEC Guide 99:2007, 2.15]

3.15**sampling interval**

time between successive sampling events

3.16**sampling line**

conduit from intake point to inlet of dosing system

[SOURCE: ISO 6107:2021, 3.494, modified — “sampling probe” was replaced by “intake point” and delivery point was replaced by “inlet of dosing system”]

4 General requirements for samplers

See 6.3 for details on verification by inspection.

A sampler shall:

- a) have an unique designation that unambiguously identifies it (e.g. model, serial number);
- b) be designed (including its operating methodology) and constructed to ensure that the composition of the sample is, as far as is practicable, not altered by the sampling procedure.

It can be impracticable to prevent the loss of volatile substances during sampling with vacuum and peristaltic samplers.

- c) have a rated maximum lift height at which all of the performance requirements of this standard are fulfilled. The rated maximum lift height shall be inscribed on the sampler or declared in the operating manual published by the manufacturer;

Conformity testing of the sampler shall be based on a range of lift heights up to and including the sampler's rated maximum lift height.

- d) have provision for the user to set the volume of a discrete sample;
- e) have rated minimum and maximum sample volumes of a discrete sample inscribed on the sampler or declared in the operating manual published by the manufacturer;
- f) have the stated capacities, for any integrated sample storage, both by number(s) and volume(s) of individual bottles and of a composite container, inscribed on the sampler or declared in the operating manual published by the manufacturer;
- g) be capable of collecting a series of samples, on a timed, event and/or a flow proportional basis. Samples can be collected and stored in individual bottles or a single composite sample bottle;
- h) have its possible sampling intervals inscribed on the sampler or declared in the operating manual published by the manufacturer;
- i) have provision for the user to set the sample interval as a minimum in the range 5 min to 1 h with increments of 1 min, for time proportional samplers;
- j) have provision for the sample interval (in the case of C.V.V.T. sampling) or the sample volume (in the case of C.T.V.V. sampling) to be set on the basis of a flow signal (e.g. pulse or analogue) from a flow meter. For pulse inputs, the relationship between pulse input and sample interval or volume should be adjustable as a minimum over the range 1 pulse to 999 pulses in increments of 1 pulse;
- k) have a control unit capable of recording sample collection failures;
- l) have a control unit capable of recording any low battery alarm during sample collection;
- m) be designed to minimize the possibility of clogging of the sample line by suspended solids in waste water. The nominal internal diameter of the sample line shall be not less than 9 mm and the average sample line velocity shall not be less than 0,5 m/s. The sampler shall be capable of achieving this average sample line velocity at all lift heights up to and including its maximum rated lift height at all rated operating voltages.

The requirement on sample line diameter excludes pipe restriction caused by the normal operation of pinch valves and peristaltic pumps.

National legal requirements can specify different minimum values for internal sample line diameter and average sample line velocity. These may need to be taken into account.


- n) be capable of purging the contents of the sampling line between each sampling event;
- o) have stated ingress protection (IP) rating inscribed on the sampler or stated in the operating manual.

Requirements for ingress protection are detailed in EN 60529:1991^[7]

prEN 16479:2021 (E)

- p) have a rated sample water and/or waste water temperature range of at least +1 °C to +25 °C" at which all of the performance requirements of this standard are met. The rated temperature range shall be inscribed on the sampler or declared in the operating manual published by the manufacturer.
- q) have rated minimum and maximum voltages at which all of the performance requirements of this standard that are relevant to the sampler are met. The rated minimum and maximum operating voltages shall be inscribed on the sampler or declared in the operating manual published by the manufacturer.

The possible sampling options are illustrated in Figure 1.

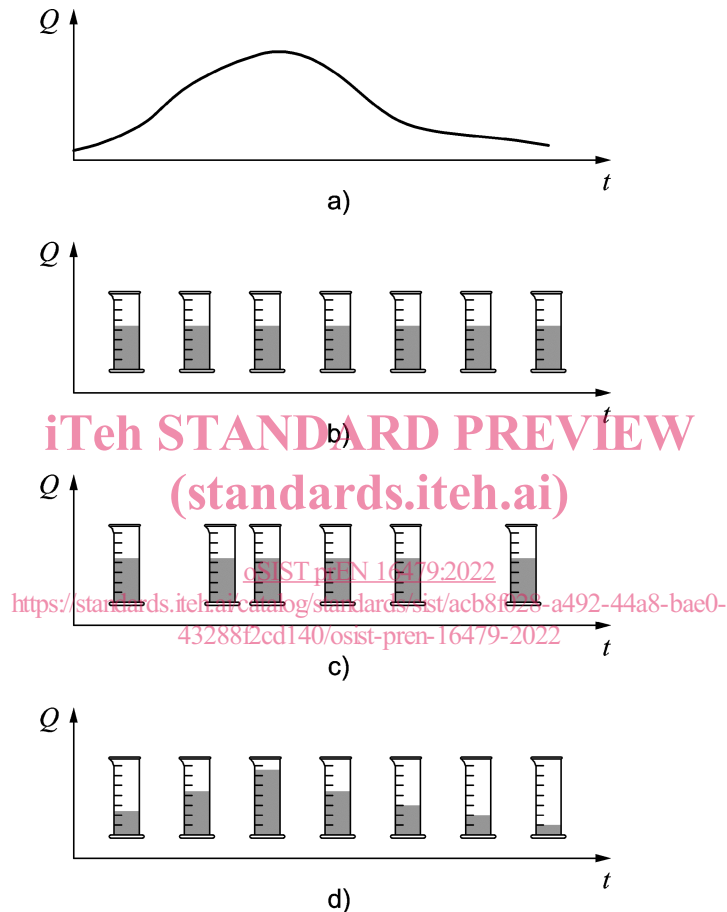

Key

- Q discharge
 t time
 a) flow rate curve
 b) C.T.C.V. time proportional sampling
 c) C.V.V.T. flow proportional sampling
 d) C.T.V.V. flow proportional sampling

Figure 1 — Sampling options

5 Performance requirements

5.1 Sample volume

The bias of the collected sample volume shall not be greater than 5 % of the set volume over the tested range for lift height.

The repeatability of the collected sample volume shall not be greater than 5 %, expressed as the repeatability variation coefficient at the 95 % confidence limit, for the set volume over the tested range for lift height.

The set volume for the conformity tests is 250 ml (or the stated maximum sample volume if less than 250 ml). However, these performance requirements also apply to additional set volumes between 50 ml and 250 ml selected for test 6.4.1.1 and the set volumes selected for test 6.4.1.2.

NOTE Details of how to calculate bias and repeatability are given in Annex A. Example calculations are detailed in Annex B.

5.2 Sampling principles

See conformity tests 6.4.2.2, 6.4.2.3, 6.4.2.4 and 6.4.2.5.

The performance of the sampling principle shall be tested and the results reported. The timing error for each operating principle shall not be greater than 1 %.

Event triggered timing error

The sampler shall start sample extraction, unless it is already doing so, within 10 s of a trigger signal being received from an external input.

5.3 Sample line velocity

See conformity test 6.4.3.

The mean velocity of the sample water as it passes through the sample line during the sampling event shall not be less than 0,5 m/s at each tested lift height and at the rated voltage for the power supply.

NOTE 1 An example calculation of sample line velocity is given in Annex B.

NOTE 2 National legal requirements can specify different minimum values for internal sample line diameter and mean sample line velocity and these possibly need to be taken into account.

5.4 Power supply

See conformity test 6.4.4.

The mean velocity of the sample water as it passes through the sample line during the sampling event shall not be less than 0,5 m/s between the minimum and maximum rated voltages for the power supply.

NOTE An example calculation of sample line velocity is given in Annex B.

5.5 Sample integrity

See conformity test 6.4.5 and the example procedure at Annex C.

Analyses for BOD (biochemical oxygen demand), COD (chemical oxygen demand), total nitrogen, and total phosphorus in samples taken by the sampler and in samples taken manually from a test water representative of a waste water from an urban waste water treatment plant in accordance with the conformity test detailed in 6.4.5 shall show no significant statistical difference based on an analysis of variance.