
Polimerni materiali - Ugotavljanje celotne prepustnosti svetlobe prozornih materialov - 2. del: Instrument z dvojnimi žarkom (ISO/FDIS 13468-2:2021)

Plastics - Determination of the total luminous transmittance of transparent materials - Part 2: Double-beam instrument (ISO/FDIS 13468-2:2021)

Kunststoffe - Bestimmung des totalen Lichttransmissionsgrades von transparenten Materialien - Teil 2: Zweistrahlinstrument (ISO/FDIS 13468-2:2021)

Plastiques - Détermination du facteur de transmission du flux lumineux total des matériaux transparents - Partie 2: Instrument à double faisceau (ISO/FDIS 13468-2:2021)

<https://standards.iteh.ai/catalog/standards/sist/5b84d726-b62a-401a-8454-a06ca8cbcd43/osist-pren-iso-13468-2-2021>

Ta slovenski standard je istoveten z: prEN ISO 13468-2

ICS:

83.080.01	Polimerni materiali na splošno	Plastics in general
-----------	--------------------------------	---------------------

oSIST prEN ISO 13468-2:2021	en,fr,de
------------------------------------	-----------------

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[oSIST prEN ISO 13468-2:2021](https://standards.iteh.ai/catalog/standards/sist/5b84d726-b62a-401a-8454-a06ca8cbed43/osist-pren-iso-13468-2-2021)

<https://standards.iteh.ai/catalog/standards/sist/5b84d726-b62a-401a-8454-a06ca8cbed43/osist-pren-iso-13468-2-2021>

FINAL
DRAFTINTERNATIONAL
STANDARDISO/FDIS
13468-2

ISO/TC 61/SC 5

Secretariat: DIN

Voting begins on:
2020-12-22Voting terminates on:
2021-03-16

**Plastics — Determination of the
total luminous transmittance of
transparent materials —****Part 2:
Double-beam instrument**

iTeh STANDARD PREVIEW
(standards.iteh.ai)
*Plastiques — Détermination du facteur de transmission du flux
lumineux total des matériaux transparents —
Partie 2: Instrument à double faisceau*

[oSIST prEN ISO 13468-2:2021](https://standards.iteh.ai/catalog/standards/sist/5b84d726-b62a-401a-8454-a06ca8cbcd43/osist-pren-iso-13468-2-2021)<https://standards.iteh.ai/catalog/standards/sist/5b84d726-b62a-401a-8454-a06ca8cbcd43/osist-pren-iso-13468-2-2021>**ISO/CEN PARALLEL PROCESSING**

RECIPIENTS OF THIS DRAFT ARE INVITED TO SUBMIT, WITH THEIR COMMENTS, NOTIFICATION OF ANY RELEVANT PATENT RIGHTS OF WHICH THEY ARE AWARE AND TO PROVIDE SUPPORTING DOCUMENTATION.

IN ADDITION TO THEIR EVALUATION AS BEING ACCEPTABLE FOR INDUSTRIAL, TECHNOLOGICAL, COMMERCIAL AND USER PURPOSES, DRAFT INTERNATIONAL STANDARDS MAY ON OCCASION HAVE TO BE CONSIDERED IN THE LIGHT OF THEIR POTENTIAL TO BECOME STANDARDS TO WHICH REFERENCE MAY BE MADE IN NATIONAL REGULATIONS.

Reference number
ISO/FDIS 13468-2:2020(E)

© ISO 2020

iTeh STANDARD PREVIEW (standards.iteh.ai)

<https://standards.iteh.ai/catalog/standards/sist/5b84d726-b62a-401a-8454-a06ca8cbcd43/osist-pren-iso-13468-2-2021>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2020

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Apparatus	2
5 Test specimens	4
6 Conditioning	5
7 Procedure	5
8 Expression of results	6
9 Precision	6
10 Test report	6
Bibliography	7

iTeh STANDARD PREVIEW (standards.iteh.ai)

[oSIST prEN ISO 13468-2:2021](https://standards.iteh.ai/catalog/standards/sist/5b84d726-b62a-401a-8454-a06ca8cbed43/osist-pren-iso-13468-2-2021)

<https://standards.iteh.ai/catalog/standards/sist/5b84d726-b62a-401a-8454-a06ca8cbed43/osist-pren-iso-13468-2-2021>

ISO/FDIS 13468-2:2020(E)

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 61, *Plastics*, Subcommittee SC 5, *Physical-chemical properties*, in collaboration with the European Committee for Standardization (CEN) Technical Committee CEN/TC 249, *Plastics*, in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

This second edition cancels and replaces the first edition (ISO 13468-2:1999), of which it constitutes a minor revision.

The changes compared to the previous edition are as follows:

- the normative references have been updated.

A list of all parts in the ISO 13468 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Plastics — Determination of the total luminous transmittance of transparent materials —

Part 2: Double-beam instrument

1 Scope

This document covers the determination of the total luminous transmittance, in the visible region of the spectrum, of planar transparent plastics and substantially colourless plastics, using a double-beam scanning spectrophotometer. This document cannot be used for plastics which contain fluorescent materials.

This document is applicable to transparent moulding materials, films and sheets not exceeding 10 mm in thickness.

NOTE 1 Total luminous transmittance can also be determined by a single-beam instrument as in ISO 13468-1.

NOTE 2 Substantially colourless plastics include those which are faintly tinted.

NOTE 3 Specimens more than 10 mm thick can be measured provided the instrument can accommodate them, but the results cannot be comparable with those obtained using specimens less than 10 mm thick.

2 Normative references

oSIST prEN ISO 13468-2:2021
<https://standards.iteh.ai/catalog/standards/sist/5b84d726-b62a-401a-8454-a06ca8cbe143/osist-pr-en-iso-13468-2-2021>

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 291, *Plastics — Standard atmospheres for conditioning and testing*

CIE PUBLICATION NO 15, *Colorimetry*

CIE PUBLICATION NO ¹⁾ 17.4, *International lighting vocabulary*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in CIE Publication No. 17.4 and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

1) Also published as IEC 50(845):1987, International electrotechnical vocabulary — Chapter 845: Lighting.

ISO/FDIS 13468-2:2020(E)

3.1 transparent plastic
 plastics in which the transmission of light is essentially regular and which have a high transmittance in the visible region of the spectrum

Note 1 to entry: Provided their geometrical shape is suitable, objects will be seen distinctly through plastic which is transparent in the visible region.

3.2 total spectral transmittance
 ratio of the transmitted radiant flux (regular and diffuse) to the incident radiant flux when a parallel beam of monochromatic radiation of a given wavelength passes through a specimen

3.3 total luminous transmittance
 ratio of the transmitted luminous flux to the incident luminous flux when a parallel beam of light passes through a specimen

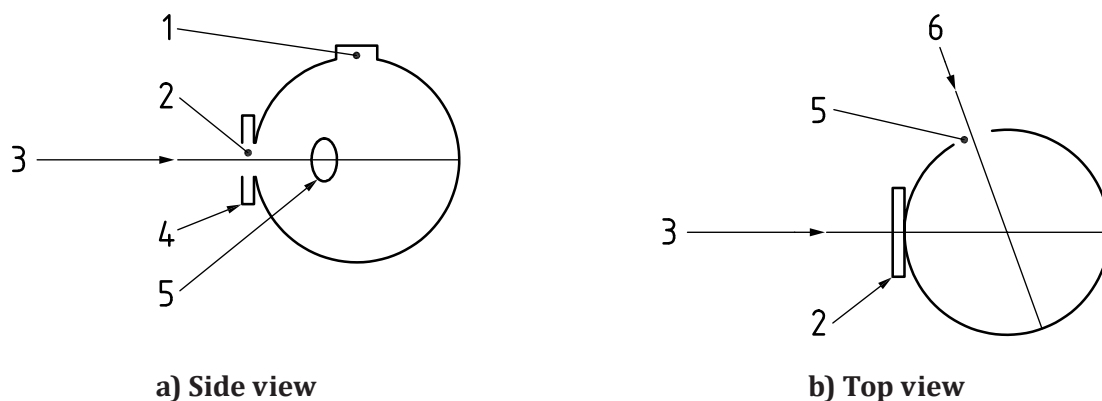
4 Apparatus

4.1 The apparatus shall consist of the following elements:

- a stabilized light source;
- a monochromator;
- an optical system that forms two parallel beams of monochromatic radiation of equal wavelength λ and approximately equal radiant flux from the output of the monochromator (called the sample and the reference beam);
- and an integrating sphere fitted with ports and a photodetector.

The sample beam enters the sphere through the entrance port. The reference beam enters the sphere through the reference port. The photodetector is mounted on the photodetector port in a manner that allows it to view with equal efficiency all parts of the sphere. Ingress of external light into the integrating sphere shall be prevented. A schematic arrangement of the integrating sphere is shown in [Figure 1](#).

4.2 The value of the total luminous transmittance determined by the instrument shall be accurate to $\pm 1,0$ %. To fulfil this requirement, the response of the photodetector shall be sufficiently linear in the visible region of the spectrum and the spectral bandwidth at half power of the monochromator shall be sufficiently small. The measurement conditions shall be such that the specimen temperature does not increase while measurements are made.

**Key**

1	photodetector	4	specimen holder
2	entrance port	5	reference port
3	sample beam	6	reference beam

Figure 1 — Schematic arrangement of the integrating sphere (baffles not shown)

4.3 The optical system shall produce two parallel beams; the angle which any ray of either of these beams makes with the axis of the beam shall not exceed 0,087 rad (5°). The beams shall not be vignetted at either port of the sphere. (standards.iteh.ai)

The diameter of each beam shall be 0,5 times to 0,8 times the diameter of its respective port.

4.4 Using this instrument, the repeatability standard deviation shall be 0,2 % or less. The within-laboratory reproducibility over long time intervals shall not exceed the repeatability by a factor of more than 3.

4.5 The design of the instrument shall be such that the total spectral transmittance is zero when the radiant flux incident on the specimen is zero.

4.6 The integrating sphere may be of any diameter as long as the total port area does not exceed 3,0 % of the internal area of the sphere.

NOTE 1 The diameter of the integrating sphere is not less than 150 mm so that specimens of a reasonable size can be used.

NOTE 2 When the diameter of the integrating sphere is 150 mm and the diameters of the entrance, reference and photodetector ports are 30 mm, the ratio of the total port area to the internal area of the sphere is 3,0 %.

4.7 The entrance and reference ports of the integrating sphere shall be circular and of the same size. The angle between the straight line defined by the centre of the entrance port and the centre of the sphere and the straight line defined by the centre of the reference port and the centre of the sphere shall be less than or equal to 90°. The angle between each of these straight lines and the straight line defined by the centre of the photodetector port and the centre of the sphere shall be 90°.

NOTE The entrance and reference ports have other shapes provided they give the same total luminous transmittance values.

4.8 The photodetector shall be fitted with baffles to prevent light falling on it directly from the specimen. It shall also be shielded from light reflected from the internal surface of the sphere.

ISO/FDIS 13468-2:2020(E)

4.9 The surfaces of the interior of the integrating sphere and the baffles shall be of substantially equal luminous reflectance which, determined in accordance to CIE Publication No. 15, shall be 90 % or more and shall not vary by more than ± 3 %. When direct measurement of the reflectance of the internal surface of an integrating sphere is difficult, the measurement may be carried out instead on a surface prepared from the same material in the same way as the internal surface.

4.10 The apparatus shall be contained in a light-tight box. No radiant flux other than the sample and reference beams may enter the sphere.

4.11 The specimen holder shall be such as to hold the specimen rigidly in a plane normal $\pm 2^\circ$ to the sample beam and as close as possible to the entrance port of the integrating sphere to ensure that all light which passes through the specimen, including scattered light, is collected.

The holder shall be designed so that it keeps flexible specimens, such as film, flat.

NOTE Thin, flexible film is clamped round the edge in a double-ring-type holder or double-sided adhesive tape is used to stick it to the edge of the holder. The latter method is used for thicker specimens, which cannot be mounted in the double-ring-type holder.

4.12 Errors caused by inter-reflections between the optics and the sample shall be minimized by tilting sensitive components or by applying an anti-reflection coating to them.

4.13 The apparatus shall allow the wavelength λ to be varied over the range $380 \text{ nm} \leq \lambda \leq 780 \text{ nm}$ in intervals of 5 nm.

NOTE In most cases, a bandwidth of 5 nm will be sufficiently small to fulfil the requirements of 4.2.

4.14 By blocking each of the beams in turn, the radiant flux of each beam can be made equal to zero. The apparatus includes provision for recording the ratio

$$\xi(\lambda) = I_{\text{sam}}(\lambda)/I_{\text{ref}}(\lambda)$$

of two photodetector signals $I_{\text{sam}}(\lambda)$ and $I_{\text{ref}}(\lambda)$ as a function of wavelength λ . $I_{\text{sam}}(\lambda)$ is measured with the reference beam blocked, $I_{\text{ref}}(\lambda)$ with the sample beam blocked.

5 Test specimens

5.1 Specimens shall be cut from film, sheet or injection-moulded or compression-moulded mouldings.

5.2 Specimens shall be free of defects, dust, grease, adhesive from protecting materials, scratches and blemishes, and shall be free from visibly distinct internal voids and particles.

5.3 Specimens shall be large enough to cover the entrance port of the integrating sphere.

For a 150 mm diameter sphere, a disc of 50 mm or 60 mm in diameter or a square with a side of the same length is recommended.

NOTE Concerning specimen thickness, see NOTE 3 to [Clause 1](#).

5.4 Three specimens shall be taken from each sample of a given material unless otherwise specified.