



Designation: E 499 – 95 (Reapproved 2000)

## Standard Test Methods for Leaks Using the Mass Spectrometer Leak Detector in the Detector Probe Mode<sup>1,2</sup>

This standard is issued under the fixed designation E 499; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

*This specification has been approved for use by agencies of the Department of Defense.*

### 1. Scope

1.1 These test methods cover procedures for testing and locating the sources of gas leaking at the rate of  $4.5 \times 10^{-13}$  mol/s ( $1 \times 10^{-8}$  Std cm<sup>3</sup>/s)<sup>3</sup> or greater. The test may be conducted on any device or component across which a pressure differential of helium or other suitable tracer gas may be created, and on which the effluent side of the leak to be tested is accessible for probing with the mass spectrometer sampling probe.

1.2 Two test methods are described:

1.2.1 *Test Method A*—Direct probing, and

1.2.2 *Test Method B*—Accumulation.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

### 2. Referenced Documents

2.1 *ASTM Standards:*

E 1316 Terminology for Nondestructive Examinations<sup>4</sup>

2.2 *Other Documents:*

SNT-TC-1A Recommended Practice for Personnel Qualification and Certification in Nondestructive Testing<sup>5</sup>

ANSI/ASNT CP-189 ASNT Standard for Qualification and Certification of Nondestructive Testing Personnel<sup>5</sup>

### 3. Terminology

3.1 *Definitions*—For definitions of terms used in this standard, see Terminology E 1316, Section E.

<sup>1</sup> These test methods are under the jurisdiction of ASTM Committee E07 on Nondestructive Testing and are the direct responsibility of Subcommittee E07.08 on Leak Testing.

Current edition approved Sept. 10, 1995. Published November 1995. Originally published as E 499 – 73. Last previous edition E 499 – 94.

<sup>2</sup> (Atmospheric pressure external, pressure above atmospheric internal). This document covers the Detector Probe Mode described in Guide E 432.

<sup>3</sup> The gas temperature is referenced to 0°C. To convert to another gas reference temperature,  $T_{ref}$ , multiply the leak rate by  $(T_{ref} + 273)/273$ .

<sup>4</sup> *Annual Book of ASTM Standards*, Vol 03.03.

<sup>5</sup> Available from American Society for Nondestructive Testing, 1711 Arlington Plaza, P.O. Box 28518, Columbus, OH 43228-0518.

### 4. Summary of Test Methods

4.1 Section 1.8 of the Leakage Testing Handbook<sup>6</sup> will be of value to some users in determining which leak test method to use.

4.2 These test methods require a leak detector with a full-scale readout of at least  $4.5 \times 10^{-12}$  mol/s ( $1 \times 10^{-7}$  Std cm<sup>3</sup>/s)<sup>3</sup> on the most sensitive range, a maximum 1-min drift of zero and sensitivity of  $\pm 5\%$  of full scale on this range, and  $\pm 2\%$  or less on others (see 7.1). The above sensitivities are those obtained by probing an actual standard leak in atmosphere with the detector, or sampling, probe, and *not* the sensitivity of the detector to a standard leak attached directly to the vacuum system.

4.3 *Test Method A, Direct Probing* (see Fig. 1), is the simplest test, and may be used in parts of any size, requiring only that a tracer gas pressure be created across the area to be tested, and the searching of the atmospheric side of the area be with the detector probe. This test method detects leakage and its source or sources. Experience has shown that leak testing down to  $4.5 \times 10^{-11}$  mol/s ( $1 \times 10^{-6}$  Std cm<sup>3</sup>/s)<sup>3</sup> in factory environments will usually be satisfactory if reasonable precautions against releasing gas like the tracer gas in the test area are observed, and the effects of other interferences (Section 6) are considered.

4.4 *Test Method B, Accumulation Testing* (see Fig. 2), provides for the testing of parts up to several cubic metres in volume as in Fig. 2(a) or in portions of larger devices as in Fig. 2(b). This is accomplished by allowing the leakage to accumulate in the chamber for a fixed period, while keeping it well mixed with a fan, and then testing the internal atmosphere for an increase in tracer gas content with the detector probe. The practical sensitivity attainable with this method depends primarily on two things: first, on the volume between the chamber and the object; and second, on the amount of outgassing of tracer gas produced by the object. Thus, a part having considerable exposed rubber, plastic, blind cavities or threads cannot be tested with the sensitivity of a smooth metallic part. The

<sup>6</sup> Marr, J. William, "Leakage Testing Handbook," prepared for Liquid Propulsion Section, Jet Propulsion Laboratory, National Aeronautics and Space Administration, Pasadena, CA, Contract NAS 7-396, June 1961.

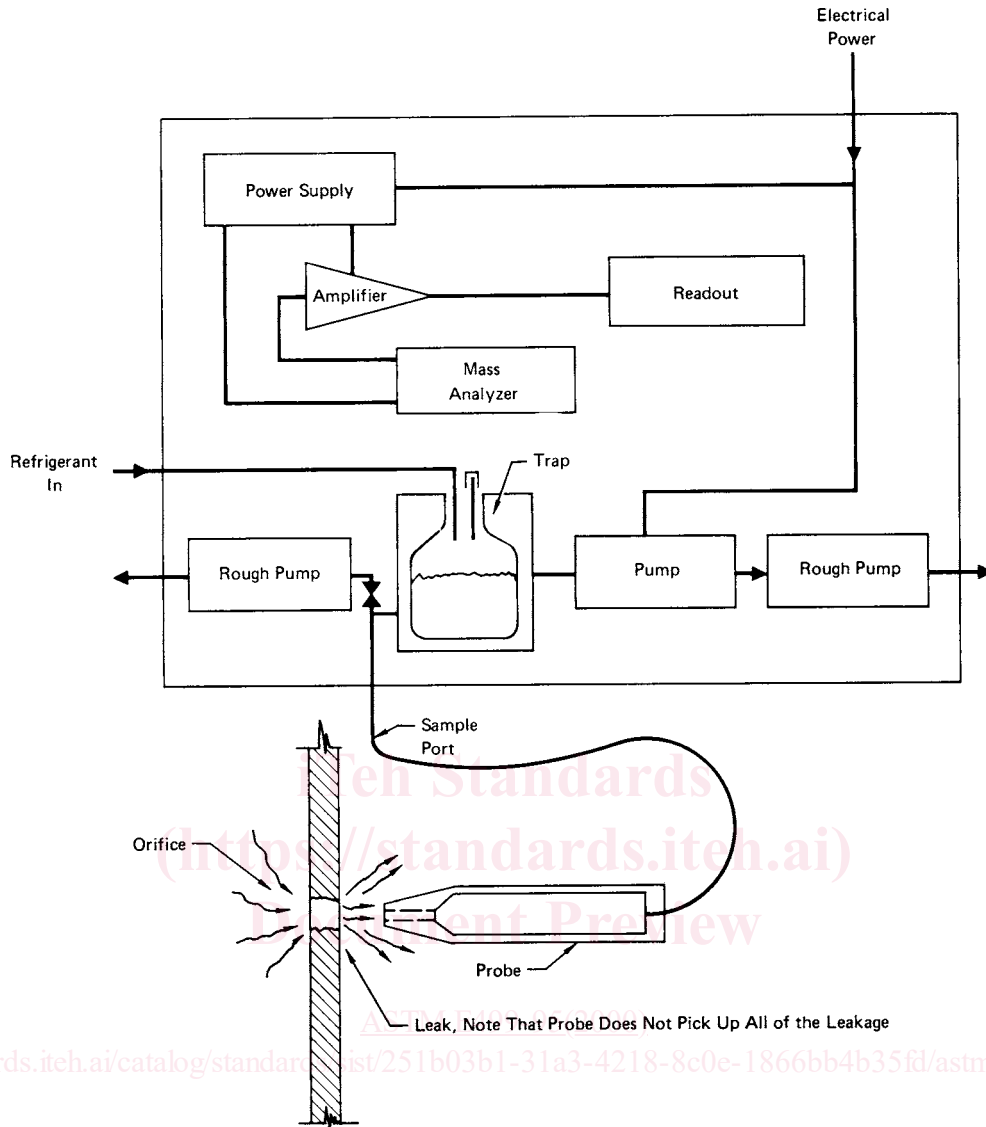


FIG. 1 Method A

time in which a leak can be detected is directly proportional to the leak rate and inversely proportional to the volume between the chamber and the part. In theory, extremely small leaks can be detected by this test method; however, the time required and the effects of other interferences limit the practical sensitivity of this test method to about  $4.5 \times 10^{-13}$  mol/s ( $1 \times 10^{-8}$  Std  $\text{cm}^3/\text{s}$ )<sup>3</sup> for small parts.

### 5. Personnel Qualification

5.1 It is recommended that personnel performing leak testing attend a dedicated training course on the subject and pass a written examination. The training course should be appropriate for NDT level II qualification according to Recommended Practice No. SNT-TC-1A of the American Society for Nondestructive Testing or ANSI/ASNT Standard CP-189.

### 6. Significance and Use


6.1 Test Method A is frequently used to test large systems and complex piping installations that can be filled with a trace

gas. Helium is normally used. The test method is used to locate leaks but cannot be used to quantify except for approximation. Care must be taken to provide sufficient ventilation to prevent increasing the helium background at the test site. Results are limited by the helium background and the percentage of the leaking trace gas captured by the probe.


6.2 Test Method B is used to increase the concentration of trace gas coming through the leak by capturing it within an enclosure until the signal above the helium background can be detected. By introducing a calibrated leak into the same volume for a recorded time interval, leak rates can be measured.

### 7. Interferences

7.1 *Atmospheric Helium*—The atmosphere contains about five parts per million (ppm) of helium, which is being continuously drawn in by the detector probe. This background must be “zeroed out” before leak testing using helium can proceed. Successful leak testing is contingent on the ability of

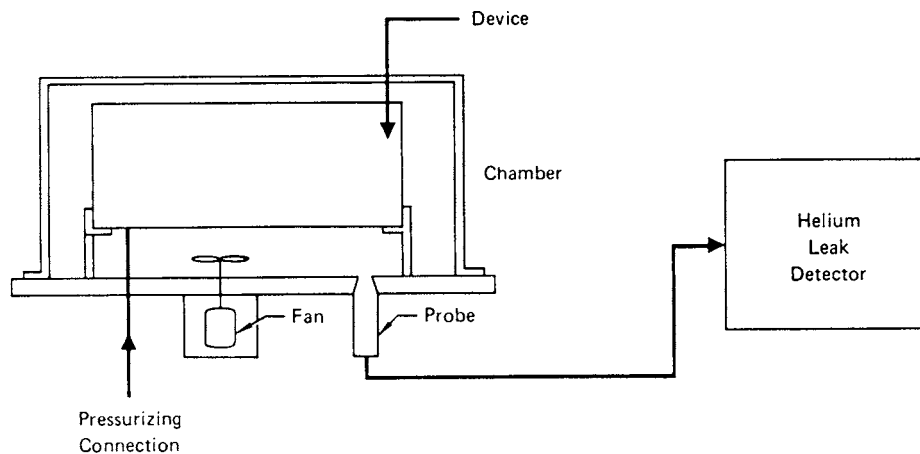

a) Accumulation Leak Test, Complete Device in Chamber

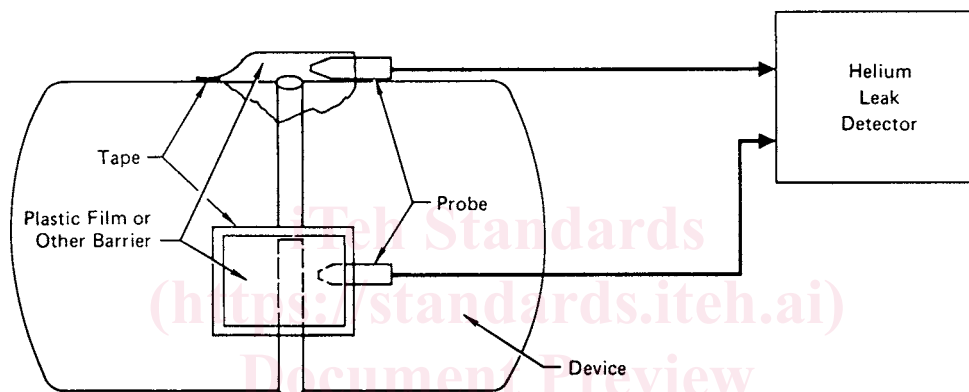

b) Accumulation Leak Test, Flexible Shroud over a Small Portion of Device

FIG. 2 Method B

the detector to discriminate between normal atmospheric helium, which is very constant, and an increase in helium due to a leak. If the normally stable atmospheric helium level is increased by release of helium in the test area, the reference level becomes unstable, and leak testing more difficult.

7.2 *Helium Outgassed from Absorbent Materials*—Helium absorbed in various nonmetallic materials (such as rubber or plastics) may be released during the test. If the rate and magnitude of the amount released approaches the amount released from the leak, the reliability of the test is decreased. The amount of such materials or their exposure to helium must then be reduced to obtain a meaningful test.

7.3 *Pressurizing with Test Gas*—In order to evaluate leakage accurately, the test gas in all parts of the device must contain substantially the same amount of tracer gas. When the device contains air prior to the introduction of test gas, or when an inert gas and a tracer gas are added separately, this may not be true. Devices in which the effective diameter and length are not greatly different (such as tanks) may be tested satisfactorily by simply adding tracer gas. However, when long or restricted systems are to be tested, more uniform tracer distribution will be obtained by first evacuating to less than 100 Pa (a few torr), and then filling with the test gas. The latter must be premixed if not 100 % tracer.

7.4 *Dirt and Liquids*—As the orifice in the detector probe is very small, the parts being tested should be clean and dry to avoid plugging. Reference should be frequently made to a standard leak to ascertain that this has not happened.

## 8. Apparatus

8.1 *Helium Leak Detector*, equipped with atmospheric detector probe. To perform tests as specified in this standard, the detector should be adjusted for testing with helium and should have the following minimum features:

8.1.1 *Sensor Mass Analyzer*.

8.1.2 *Readout*, analog or digital.

8.1.3 *Range (linear)*—A signal equivalent to  $4.5 \times 10^{-11}$  mol/s ( $1 \times 10^{-6}$  Std cm<sup>3</sup>/s)<sup>3</sup> or larger must be detectable.

8.1.4 *Response time*, 3 s or less.

8.1.5 *Stability of Zero and Sensitivity*— A maximum variation of  $\pm 5\%$  of full scale on the most sensitive range while the probe is active; a maximum variation of  $\pm 2\%$  of full scale on other ranges for a period of 1 min.

NOTE 1—Variations may be a function of environmental interferences rather than equipment limitations.

8.1.6 *Controls*:

8.1.6.1 *Range*, preferable in scale steps of  $3\times$  and  $10\times$ .