
**Optics and photonics — Optical
materials and components — Test
method for climate resistance of
optical glass**

*Optique et photonique — Matériaux et composants optiques —
Méthode d'essai pour la résistance climatique du verre optique*

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

ISO 22531:2020

<https://standards.iteh.ai/catalog/standards/iso/81505e34-41b5-4dfd-9875-c4e87cedeec7/iso-22531-2020>



iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

ISO 22531:2020

<https://standards.iteh.ai/catalog/standards/iso/81505e34-41b5-4dfd-9875-c4e87cedeec7/iso-22531-2020>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2020

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Fax: +41 22 749 09 47
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	1
5 Test apparatus	1
5.1 Configuration.....	1
5.2 Thermostatic chamber.....	3
5.3 Glass water tank and lid.....	3
5.4 Water.....	3
5.5 Stirring unit.....	4
5.6 Seal.....	4
5.7 Specimen holder.....	4
5.8 Specimen holder stand.....	4
5.9 Water tank stand.....	4
6 Specimens	5
6.1 Shape and size of specimens.....	5
6.2 Number of specimens.....	5
6.3 Surface treatment of specimens before test.....	5
7 Test method	6
7.1 Procedure of the test.....	6
7.2 Calculation.....	7
8 Classification and designation	8
9 Test report	8
Annex A (normative) Test conditions for the thermostatic chamber	10
Annex B (normative) Procedure for polishing and cleaning the specimens	12
Bibliography	14

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 172, *Optics and Photonics*, Subcommittee SC 3, *Optical materials and components*.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

<https://standards.iteh.ai/catalog/standards/iso/81505e34-41b5-4dfd-9875-c4e87cedeec7/iso-22531-2020>

Optics and photonics — Optical materials and components — Test method for climate resistance of optical glass

1 Scope

This document specifies the test method for climate resistance of optical glass and the classification of the optical glass according to the test results.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3585, *Borosilicate glass 3.3 — Properties*

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 14782, *Plastics — Determination of haze for transparent materials*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

— ISO Online browsing platform: available at <https://www.iso.org/obp>

— IEC Electropedia: available at <http://www.electropedia.org/>

3.1

haze

percentage of transmitted light, passing through a specimen, which deviates from the incident light by no more than 0,044 rad (2,5°) by forward scattering

[SOURCE: ISO 14782:1999, 3.1]


4 Principle

To evaluate the climate resistance of optical glass in its operating environment, the hazes of polished glass surfaces before and after testing are measured with the haze meter specified in ISO 14782, and the climate resistance is determined by the change in the amount of haze.

5 Test apparatus

5.1 Configuration

The test apparatus consists of the components shown in [Figure 1](#). The size and arrangement of the components in the glass water tank are shown in [Figure 2](#).

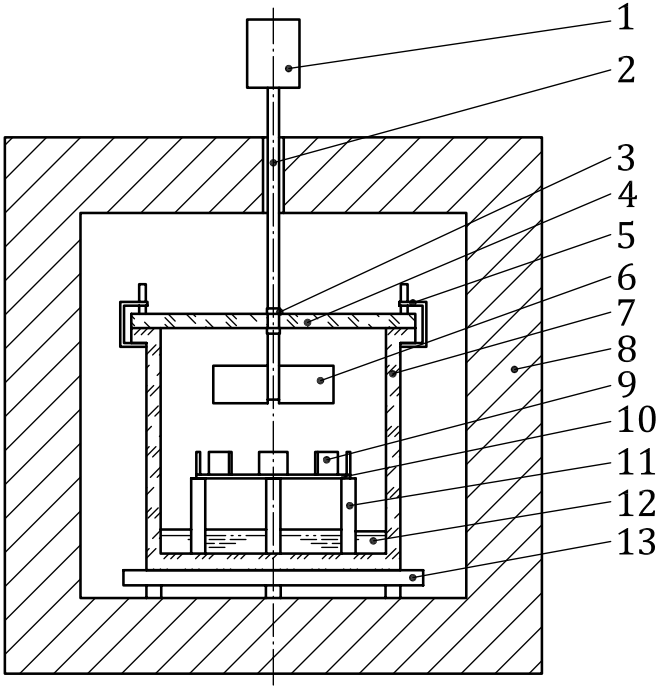


Key

- | | | | |
|---|------------------|----|-------------------------|
| 1 | stirring motor | 8 | thermostatic chamber |
| 2 | stirring rod | 9 | specimens |
| 3 | seal | 10 | specimen holder |
| 4 | lid | 11 | specimen holder stand |
| 5 | clamp | 12 | distilled water (1,8 l) |
| 6 | stirring fan | 13 | water tank stand |
| 7 | glass water tank | | |

Figure 1 — Test apparatus

Dimensions in millimetres

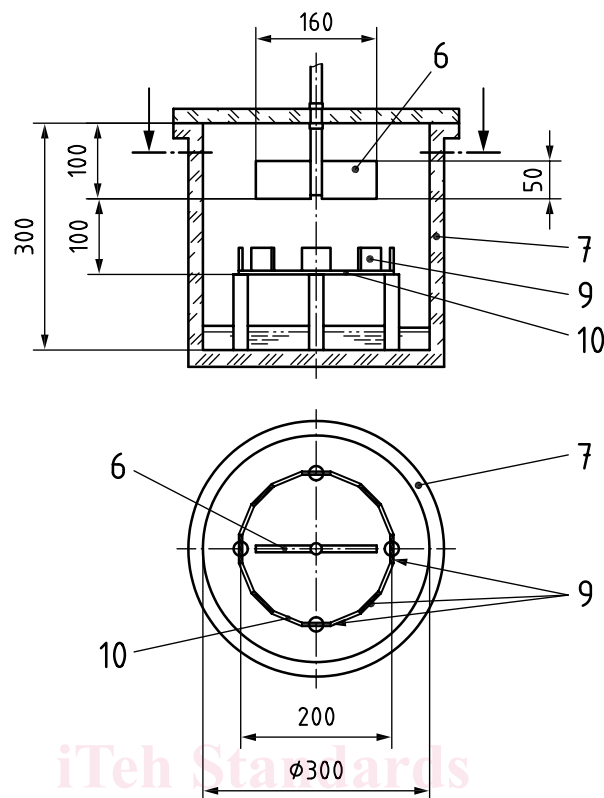**Key**

- 6 stirring fan
- 7 glass water tank
- 9 specimens
- 10 specimen holder (stainless steel)

iTeh Standards
(<https://standards.itih.ai>)
Document Preview

ISO 22531:2020

<https://standards.itih.ai/catalog/standards/iso/81505e34-41b5-4dfd-9875-c4e87cedec7/iso-22531-2020>

Figure 2 — Arrangement of specimens and units in the glass water tank

5.2 Thermostatic chamber

The chamber shall have an automatic temperature adjustment capability.

The ceiling of chamber shall have a through-hole for the stirring rod which is rotated by the stirring motor as shown in [Figure 1](#).

5.3 Glass water tank and lid

The water tank and the lid shall be made of either borosilicate glass 3.3 in accordance with ISO 3585 or quartz glass, the thickness of which shall be between 5 mm and 20 mm. They shall be placed in the thermostatic chamber as shown in [Figure 1](#).

Eliminate the gap of the contacting part between the lid and the rim of the tank by lapping. A hole shall be provided at the centre of the lid so that the stirring rod passes through it.

5.4 Water

The purity of the water used shall be in accordance with the grade 2 of ISO 3696. The amount of water contained by the water tank shall be 1,8 l.

5.5 Stirring unit

The stirring unit consists of a stirring motor, a stirring rod and a stirring fan as shown in [Figure 1](#). The stirring rod shall be straight, not bent or warped. The dimension of the stirring fan is shown in [Figure 2](#).

NOTE If the stirring rod is bent or warped, the stirring rod will be decentered during rotation and the stirring fan will be shifted from the correct position.

5.6 Seal

An elastic seal, such as an O-ring, shall be provided at the gap between the stirring rod and the lid to keep humidity in the tank constant during the test. Confirm the condition of the elastic seal before the test and exchange the seal if it deteriorates.

5.7 Specimen holder

[Figure 3](#) shows an example configuration of a hexadecagonal specimen holder at the position of 100 mm under the stirring fan above the water level, which keeps the specimen's surface vertical. This holder shall be fabricated in a shape that allows up to eight specimens to be placed at equal intervals from the central axis of the stirring rod as shown in [Figure 1](#).

The specimen holder shall be placed in the centre of the water tank, as shown in [Figure 2](#).

Dimensions in millimetres

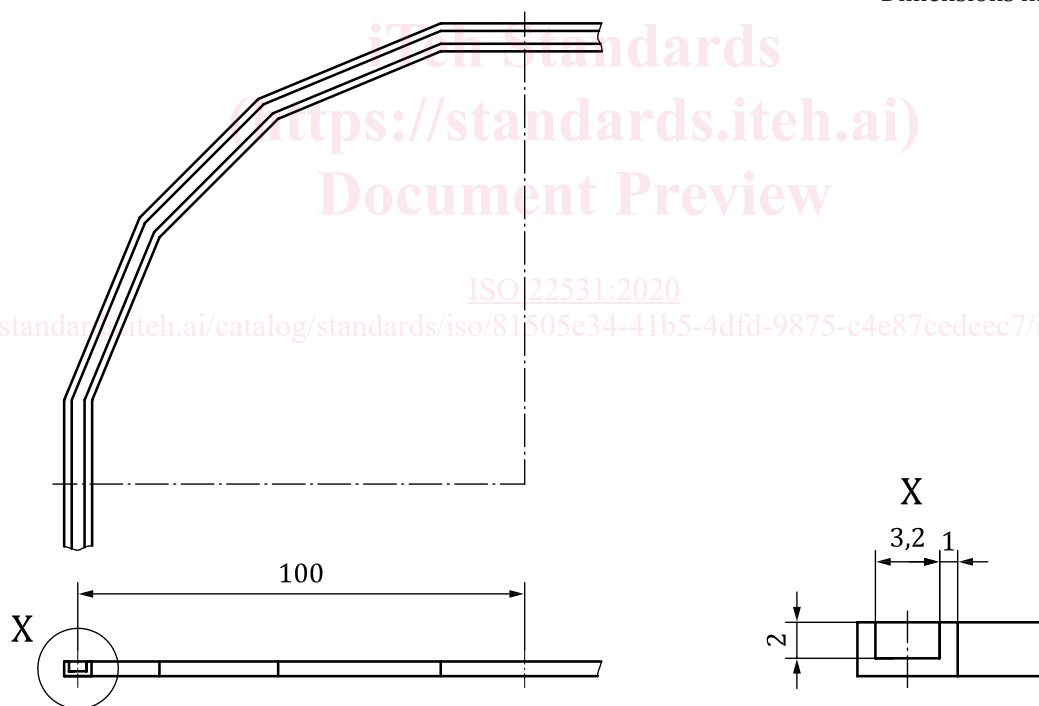


Figure 3 — Configuration example of the specimen holder

5.8 Specimen holder stand

The specimen holder stand shall hold the specimens 100 mm from the inner bottom of the water tank.

5.9 Water tank stand

Place a stand under the water tank to ensure a pathway of airflow.

6 Specimens

6.1 Shape and size of specimens

The shape of the specimen shall be a square-formed plate, and its size shall be 30 mm × 30 mm × 3 mm.

6.2 Number of specimens

The number of specimens per test shall be 5 to 8.


6.3 Surface treatment of specimens before test

Both sides of surfaces of each specimen shall be polished with cerium oxide slurry, then contamination shall be removed from the polished surfaces with an organic solvent. After that, the polished specimens are cleaned with detergent, distilled water and alcohols such as IPA (isopropyl alcohol). The detailed cleaning method shall be described in [Annex B](#). The cleaning shall be started within 24 h after the polished surface has been exposed to the atmosphere, and after that, the test shall be started immediately.

If the cleaning procedure of the specimens is started more than 24 h after polishing, the protective materials, i.e. the films or resins for the glass lens polishing process shall be applied to the polished surfaces immediately after polishing in order to avoid exposing the glass surface to the atmosphere. Dissolve the protective film with organic solvent or remove it before the cleaning of the specimens.

Even with the presence of protective materials, keeping moisture away from the glass perfectly is difficult, so the storage period of the specimens should not exceed 100 h. Further, if the glass surface changes with a protective material, cleaning and testing process shall be started promptly after polishing without using the protective material.

NOTE The duration to prepare for cleaning, i.e. T_p , changes depending on the time period from polishing to cleaning procedure, as shown in [Figure 4](#). However, the duration that the specimens are exposed to the atmosphere, T_E , is within 24 h in each condition.

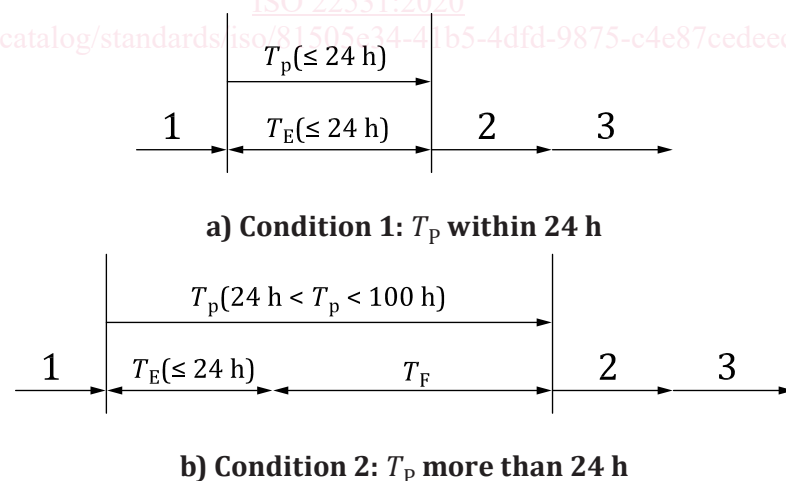

Key

- T_p the duration to prepare for cleaning
- T_E the duration that the specimens are exposed to the atmosphere
- T_F the duration that the protective films on the specimens are applied
- 1 polishing
- 2 cleaning
- 3 testing

Figure 4 — Schematic figure of time durations regarding the exposure time T_E of the specimen

7 Test method


7.1 Procedure of the test

The test shall be conducted in the following sequence.

- Measure the haze of the pre-testing specimens using the haze meter specified in ISO 14782. Haze shall be measured more than 5 mm inside from the edge of the specimen.
- With the stirring fan rotating at 100 r/min, set the temperature T_1 of the thermostatic chamber and keep for t_H , holding time, minutes or longer in order to achieve and maintain the air temperature within the water tank at 57,5 °C. The temperature T_1 and the holding time t_H , are determined in [Annex A](#). Temperature tolerance should be $\pm 0,5$ °C.
- Place the specimens into the holder so that the distance between specimens is at least 30 mm.
- Put the lid on the tank and clamp them together.
- Rotate the stirring fan at 100 r/min during the test.
- Maintain the air temperature in the water tank at 57,5 °C for 50 min.
- Apply the temperature profile of the thermostatic chamber as shown in [Figure 5](#) so that the actual air temperature in the water tank has a cycle in which the minimum temperature is 57,5 °C and the maximum temperature is 64,0 °C, as shown in [Figure 6](#). To achieve such a temperature profile, use the set temperatures T_1 and T_2 determined in [Annex A](#).

NOTE As shown in [Figure 6](#), the actual air temperature change in the water tank is more moderate than the temperature cycle shown in [Figure 5](#).

- Apply the temperature cycle for 48 h, then remove the specimens and transfer them to a desiccator. Cool the specimens to room temperature and dry them.
- Measure the haze of the post-testing specimens using the haze meter. Haze shall be measured more than 5 mm inside from the edge of the specimen.

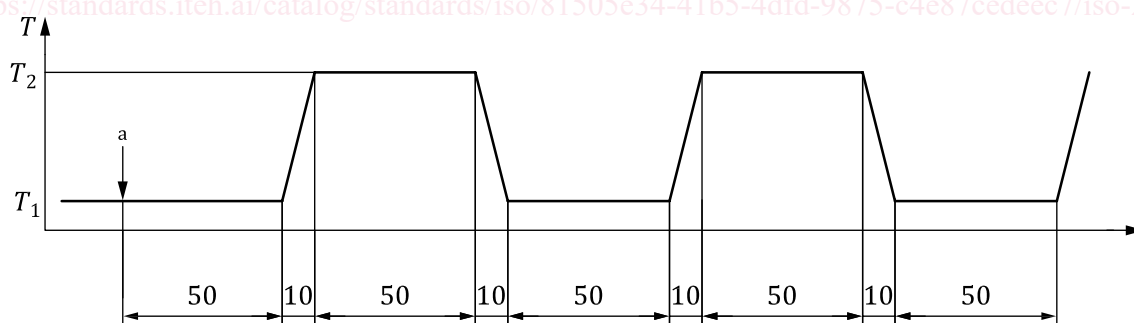

Key

- T temperature (°C)
 T_1 lower set temperature
 T_2 upper set temperature
 t time (min)
 a Specimen set time.

Figure 5 — Temperature profile of thermostatic chamber