

ISO/TC 150/SC 6

Secretariat: ANSI

Voting begins on:
2021-11-15

Voting terminates on:
2022-01-10

Implants for surgery — Active implantable medical devices —

Part 4: Implantable infusion pump systems

Implants chirurgicaux — Dispositifs médicaux implantables actifs —

Partie 4: Systèmes de pompe à perfusion implantables

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO/FDIS 14708-4

<https://standards.iteh.ai/catalog/standards/sist/fbf05d1d-4bd2-44a1-97ed-52c330967b79/iso-fdis-14708-4>

ISO/CEN PARALLEL PROCESSING

RECIPIENTS OF THIS DRAFT ARE INVITED TO SUBMIT, WITH THEIR COMMENTS, NOTIFICATION OF ANY RELEVANT PATENT RIGHTS OF WHICH THEY ARE AWARE AND TO PROVIDE SUPPORTING DOCUMENTATION.

IN ADDITION TO THEIR EVALUATION AS BEING ACCEPTABLE FOR INDUSTRIAL, TECHNOLOGICAL, COMMERCIAL AND USER PURPOSES, DRAFT INTERNATIONAL STANDARDS MAY ON OCCASION HAVE TO BE CONSIDERED IN THE LIGHT OF THEIR POTENTIAL TO BECOME STANDARDS TO WHICH REFERENCE MAY BE MADE IN NATIONAL REGULATIONS.



Reference number
ISO/FDIS 14708-4:2021(E)

© ISO 2021

iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO/FDIS 14708-4

<https://standards.iteh.ai/catalog/standards/sist/fbf05d1d-4bd2-44a1-97ed-52c330967b79/iso-fdis-14708-4>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2021

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword.....	v
Introduction.....	vii
1 Scope.....	1
2 Normative references.....	1
3 Terms and definitions.....	1
4 Symbols and abbreviated terms.....	3
5 General requirements for active implantable medical devices.....	3
5.1 General requirements for non-implantable parts.....	3
5.2 General requirements for software.....	3
5.3 Usability of non-implantable parts.....	3
5.4 Data security and protection from harm caused by unauthorized information tampering.....	3
5.5 General requirements for risk management.....	3
5.6 Misconnection of parts of the active implantable medical device.....	3
6 Requirements for particular active implantable medical devices.....	3
6.1 Implantable infusion pump system specifications.....	3
6.2 Septum puncture test.....	4
7 General arrangement of the packaging.....	5
8 General markings for active implantable medical devices.....	5
9 Markings on the sales packaging.....	6
10 Construction of the sales packaging.....	6
11 Markings on the sterile pack.....	7
12 Construction of the non-reusable pack.....	7
13 Markings on the active implantable medical device.....	7
14 Protection from unintentional biological effects caused by the active implantable medical device.....	7
15 Protection from harm to the patient or user caused by external physical features of the active implantable medical device.....	8
16 Protection from harm to the patient caused by electricity.....	8
17 Protection from harm to the patient caused by heat.....	8
18 Protection from ionizing radiation released or emitted from the active implantable medical device.....	9
19 Protection from unintended effects caused by the active implantable medical device.....	9
20 Protection of the active implantable medical device from damage caused by external defibrillators.....	10
21 Protection of the active implantable medical device from changes caused by high- power electrical fields applied directly to the patient.....	10
22 Protection of the active implantable medical device from changes caused by miscellaneous medical treatments.....	10
22.1 Diagnostic ultrasound.....	10
22.2 Magnetic resonance imaging.....	10
23 Protection of the active implantable medical device from mechanical forces.....	11
24 Protection of the active implantable medical device from damage caused by electrostatic discharge.....	12

25	Protection of the active implantable medical device from damage caused by atmospheric pressure changes.....	12
26	Protection of the active implantable medical device from damage caused by temperature changes.....	12
27	Protection of the active implantable medical device from electromagnetic non-ionizing radiation.....	12
27.1	General.....	12
27.2	Test conditions.....	13
27.2.1	Acceptance criteria.....	13
27.2.2	Test configuration.....	13
27.2.3	Operating functions, modes, and settings.....	13
27.3	Documentation.....	13
27.4	Protection from static magnetic fields of flux density up to 50 mT.....	14
27.5	Protection from magnetic fields over the frequency range 16 Hz to 26 MHz.....	15
27.6	Protection from EM disturbances over the frequency range 80 MHz to 2,7 GHz.....	16
27.7	Protection from proximity fields due to RF wireless communications equipment.....	17
27.8	Optional characterization testing.....	18
28	Accompanying documentation.....	18
Annex A (informative)	Relationship between the fundamental principles in ISO/TR 14283 and the clauses of this document.....	21
Annex B (informative)	Rationale.....	42
Annex C (informative)	Guidance on the allocation of requirements to non-implantable parts connected to a power source.....	51
Bibliography	58

[ISO/FDIS 14708-4](https://standards.iteh.ai/catalog/standards/sist/f05d1d-4bd2-44a1-97ed-52c330967b79/iso-fdis-14708-4)
<https://standards.iteh.ai/catalog/standards/sist/f05d1d-4bd2-44a1-97ed-52c330967b79/iso-fdis-14708-4>

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 150, *Implants for surgery*, SC 6, *Active implants*, in collaboration with the European Committee for Standardization (CEN) Technical Committee CEN/JTC 16, *Active Implantable Medical Devices*, in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

This second edition cancels and replaces the first edition (ISO 14708-4:2008), which has been technically revised.

The main changes compared to the previous edition are as follows:

- the title of this document has been modified;
- 9.4 additions have been deleted;
- 11.101 has been deleted;
- 14.2 replacement has been deleted;
- 14.101 has been deleted;
- 14.5 has been added;
- Clause 17 has been revised;
- 19.2 replacement has been deleted;
- 19.3 replacement has been deleted;
- 19.101 has been deleted;
- 19.7 has been added;

- [23.2](#) amendment has been deleted;
- [Clause 27](#) has been revised;
- [28.8](#) additions has been deleted;
- [28.10](#) additions has been deleted;
- [28.12](#) addition has been deleted;
- 28.101 through 28.103 has been deleted;
- [28.31](#) and [28.32](#) has been added.

A list of all parts in the ISO 14708 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO/FDIS 14708-4
https://standards.iteh.ai/catalog/standards/sist/f05d1d-4bd2-44a1-97ed-52c330967b79/iso-fdis-14708-4](https://standards.iteh.ai/catalog/standards/sist/f05d1d-4bd2-44a1-97ed-52c330967b79/iso-fdis-14708-4)

Introduction

An *implantable infusion pump system* is a device that delivers either a constant infusion rate or a variable infusion rate from which a medicinal substance is delivered via an implanted catheter to site-specific locations within the human body. An external programmer might be used to adjust device parameters.

Requirements for physiologic sensing functions of *implantable infusion pump systems* are not included in this edition of this document but might be considered in future editions.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO/FDIS 14708-4

<https://standards.iteh.ai/catalog/standards/sist/f05d1d-4bd2-44a1-97ed-52c330967b79/iso-fdis-14708-4>

iTeh STANDARD PREVIEW **(standards.iteh.ai)**

ISO/FDIS 14708-4

<https://standards.iteh.ai/catalog/standards/sist/f05d1d-4bd2-44a1-97ed-52c330967b79/iso-fdis-14708-4>

Implants for surgery — Active implantable medical devices —

Part 4: Implantable infusion pump systems

1 Scope

This document specifies particular requirements for active implantable medical devices intended to deliver a medicinal substance to site-specific locations within the human body, to provide basic assurance of safety for both patients and users. It amends and supplements ISO 14708-1:2014. The requirements of this document take priority over those of ISO 14708-1.

This document is applicable to active implantable medical devices intended to deliver medicinal substances to site-specific locations within the human body.

This document is also applicable to some non-implantable parts and accessories of the devices defined in [Clause 3](#).

The tests that are specified in this document are type tests intended to be carried out on a sample of a device to show compliance and are not intended to be used for the routine testing of manufactured products.

NOTE This document is not intended to apply to non-implantable infusion systems.

<https://standards.iteh.ai/catalog/standards/sist/fbf05d1d-4bd2-44a1-97ed-52c330967b79/iso-fdis-14708-4>

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 14708-1, *Implants for surgery — Active implantable medical devices — Part 1: General requirements for safety, marking and for information to be provided by the manufacturer*

ISO/TS 10974, *Assessment of the safety of magnetic resonance imaging for patients with an active implantable medical device*

IEC 60601-1, *Medical electrical equipment — Part 1: General requirements for basic safety and essential performance*

IEC 60601-1-2, *Medical electrical equipment — Part 1-2: General requirements for basic safety and essential performance — Collateral standard: Electromagnetic compatibility — Requirements and tests*

IEC 61000-4-3, *Electromagnetic compatibility (EMC) — Part 4-3: Testing and measurement techniques — Radiated, radio-frequency, electromagnetic field immunity test*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 14708-1 and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

— IEC Electropedia: available at <http://www.electropedia.org/>

— ISO Online browsing platform: available at <http://www.iso.org/obp>

3.1

bolus

specific amount of fluid (dose or volume) delivered once for a prescribed length of time (duration)

3.2

catheter access port

port allowing access to the delivery catheter

3.3

fluid pathway

internal surfaces of the *implantable infusion pump system* (3.4) which are in direct contact with a medicinal substance

Note 1 to entry: This also includes catheters and refill kits.

3.4

implantable infusion pump system

active implantable medical device intended for delivery of a medicinal substance to a specific location within the human body

Note 1 to entry: For purposes of this document, an *implantable infusion pump system* can be a single article, or a set of components and accessories. Not all of these components or accessories might be required to be partially or totally implanted, e.g. programmers.

3.5

infusion rate accuracy

closeness of the true (actual) infusion rate to the programmed rate

3.6

maximum infusion rate

highest rate selectable by the user

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO/FDIS 14708-4
<https://standards.iteh.ai/catalog/standards/sist/f05d1d-4bd2-44a1-97ed-52c330967b79/iso-fdis-14708-4>

3.7

minimum infusion rate

lowest rate selectable by the user

3.8

magnetic resonance conditional

MR conditional

item with demonstrated safety in the MR environment within defined conditions including conditions for the static magnetic field, the time-varying gradient magnetic fields and the radiofrequency fields

[SOURCE: ASTM F2503-20, 3.1.11]

3.9

pump

implantable part of an *implantable infusion pump system* (3.4) containing the *reservoir* (3.12), energy source and, in some cases, control electronics

3.10

refill access port

port allowing access to the *reservoir* (3.12)

3.11

repeatability

ability to consistently deliver the same results over time, under the same conditions

Note 1 to entry: A method for calculating *repeatability* is given in Annex B of ISO 11631:1998.

3.12**reservoir**

space designed to hold fluid

3.13**reservoir volume**

fluid volume of the *reservoir* (3.12) that can be discharged

3.14**service life**

period after implantation when the *implantable infusion pump system* (3.4) remains within stated specifications and characteristics

4 Symbols and abbreviated terms

The text in Clause 4 of ISO 14708-1:2014 applies with the following addition:

DUT device under test

5 General requirements for active implantable medical devices**5.1 General requirements for non-implantable parts**

The text in 5.1 of ISO 14708-1:2014 applies.

5.2 General requirements for software

The text in 5.2 of ISO 14708-1:2014 applies. <https://standards.iteh.ai/catalog/standards/sist/fbf05d1d-4bd2-44a1-97ed-52c330967b79/iso-fdis-14708-4>

5.3 Usability of non-implantable parts

The text in 5.3 of ISO 14708-1:2014 applies.

5.4 Data security and protection from harm caused by unauthorized information tampering

The text in 5.4 of ISO 14708-1:2014 applies.

5.5 General requirements for risk management

The text in 5.5 of ISO 14708-1:2014 applies.

5.6 Misconnection of parts of the active implantable medical device

The text in 5.6 of ISO 14708-1:2014 applies.

6 Requirements for particular active implantable medical devices**6.1 Implantable infusion pump system specifications**

The specifications (e.g. *infusion rate accuracy* and *repeatability*) stated by the manufacturer in the accompanying documentation (see 28.8) shall be maintained over the *service life* and over the range of environmental conditions and characteristics (e.g. *reservoir volume*) stated by the manufacturer.

NOTE Minimum environmental conditions for atmospheric pressure are specified in [Clause 25](#).

Infusion rate accuracy shall be stated for all selectable rates (including *bolus* rates).

The manufacturer shall provide a plot of *infusion rate accuracy* versus environmental conditions and characteristics (e.g. *reservoir volume*) that affect *infusion rate accuracy*. For variable rate *implantable infusion pump systems*, the plot shall contain curves for *minimum infusion rate*, *maximum infusion rate*, and at least one rate in between the *minimum infusion rate* and *maximum infusion rate*.

The method of computing and determining the *infusion rate accuracy* shall be clearly stated in the accompanying documentation. Environmental test conditions used to establish *infusion rate accuracy* shall also be stated. Environmental conditions and characteristics that affect *infusion rate accuracy* shall be clearly stated in the accompanying documentation.

For all selectable infusion rates, the *repeatability* of the actual rate shall also be stated. The method of computing and determining the stated *repeatability* shall be clearly described in the accompanying documentation.

Compliance is checked by inspection of accompanying documentation and test procedures and reports, supported by the manufacturer's calculations, as appropriate.

6.2 Septum puncture test

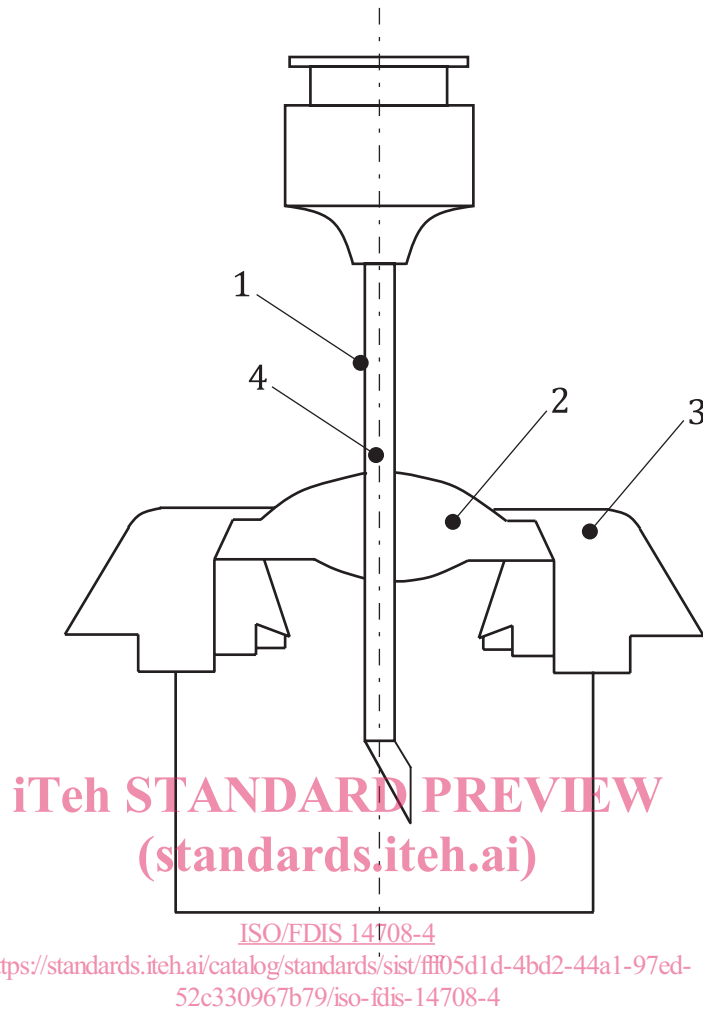
A septum that allows entry to an access port (e.g. *refill access port* or *catheter access port*), shall be able to withstand repeated insertions of a hypodermic needle while maintaining the integrity of the *reservoir* throughout the *service life*.

Test: The DUT shall be conditioned at $37\text{ °C} \pm 1\text{ °C}$ for not less than 12 h to achieve thermal equilibration. Each *pump* septum shall be punctured randomly using the needle specified by the manufacturer for septum puncture and in accordance with the manufacturer's instructions. The needle used for septum puncture shall be replaced if damage to the needle or the needle's tip is noted by the operator. The needle shall completely penetrate the septum and care should be taken not to damage the needle's tip during the test. Puncturing shall be done using a straight-line motion parallel to the septum's axial centre-line as shown in [Figure 1](#).

Septum leakage shall be determined by immersing the test unit in a water bath at $37\text{ °C} \pm 1\text{ °C}$ and allowing the temperature of the assembly to stabilize for a minimum of 30 min. Leakage shall be determined by air pressure applied slowly to a pressure of twice the *pump's* maximum operating pressure or a minimum of 276 kPa. The septum's exposed surfaces shall be examined for air bubble leakage for 1 min.

The minimum number of punctures for which the septum maintains integrity shall be stated (see [28.8](#)).

Compliance is checked by inspection of accompanying documentation and test reports.

**Key**

- 1 needle
- 2 septum
- 3 body
- 4 centre-line

Figure 1 — Septum puncture test**7 General arrangement of the packaging**

7.1 The text in 7.1 of ISO 14708-1:2014 applies.

7.2 The text in 7.2 of ISO 14708-1:2014 applies.

8 General markings for active implantable medical devices

8.1 The text in 8.1 of ISO 14708-1:2014 applies.

8.2 The text in 8.2 of ISO 14708-1:2014 applies.

8.3 If special handling measures have to be taken during transport, the shipping packaging shall be marked accordingly.

Compliance is checked by inspection.

8.4 The permissible environmental conditions for transport shall be marked on the outside of the shipping packaging (see ISO 15223-1).

Compliance is checked by inspection.

9 Markings on the sales packaging

9.1 The text in 9.1 of ISO 14708-1:2014 applies.

9.2 The text in 9.2 of ISO 14708-1:2014 applies.

9.3 The text in 9.3 of ISO 14708-1:2014 applies.

9.4 The text in 9.4 of ISO 14708-1:2014 applies.

9.5 The text in 9.5 of ISO 14708-1:2014 applies.

9.6 The text in 9.6 of ISO 14708-1:2014 applies.

9.7 The text in 9.7 of ISO 14708-1:2014 applies.

9.8 The text in 9.8 of ISO 14708-1:2014 applies.

9.9 The text in 9.9 of ISO 14708-1:2014 applies.

9.10 The text in 9.10 of ISO 14708-1:2014 applies.

9.11 The text in 9.11 of ISO 14708-1:2014 applies.

9.12 The text in 9.12 of ISO 14708-1:2014 applies.

9.13 The text in 9.13 of ISO 14708-1:2014 applies.

9.14 The text in 9.14 of ISO 14708-1:2014 applies.

10 Construction of the sales packaging

10.1 The text in 10.1 of ISO 14708-1:2014 applies.

10.2 The text in 10.2 of ISO 14708-1:2014 applies.

10.3 The text in 10.3 of ISO 14708-1:2014 applies.

10.4 The text in 10.4 of ISO 14708-1:2014 applies.

11 Markings on the sterile pack

11.1 The text in 11.1 of ISO 14708-1:2014 applies.

11.2 The text in 11.2 of ISO 14708-1:2014 applies.

11.3 The text in 11.3 of ISO 14708-1:2014 applies.

11.4 The text in 11.4 of ISO 14708-1:2014 applies.

11.5 The text in 11.5 of ISO 14708-1:2014 applies.

11.6 The text in 11.6 of ISO 14708-1:2014 applies.

11.7 The text in 11.7 of ISO 14708-1:2014 applies.

11.8 The text in 11.8 of ISO 14708-1:2014 applies.

11.9 The text in 11.9 of ISO 14708-1:2014 applies.

12 Construction of the non-reusable pack

12.1 The text in 12.1 of ISO 14708-1:2014 applies.

12.2 The text in 12.2 of ISO 14708-1:2014 applies.

12.3 The text in 12.3 of ISO 14708-1:2014 applies.

13 Markings on the active implantable medical device

13.1 The text in 13.1 of ISO 14708-1:2014 applies.

13.2 The text in 13.2 of ISO 14708-1:2014 applies.

13.3 The text in 13.3 of ISO 14708-1:2014 applies.

13.4 The text in 13.4 of ISO 14708-1:2014 applies.

14 Protection from unintentional biological effects caused by the active implantable medical device

14.1 The text in 14.1 of ISO 14708-1:2014 applies.

14.2 The text in 14.2 of ISO 14708-1:2014 applies.

An appropriate test method shall be established to test the *fluid pathway* in addition to external surfaces.