
**Laboratory glass and plastic ware —
Volumetric instruments — Methods
for testing of capacity and for use**

*Verrerie et matériel en plastique de laboratoire — Instruments
volumétriques — Méthodes d'essai de la capacité et d'utilisation*

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[ISO 4787:2021](https://standards.iteh.ai/catalog/standards/sist/d201436a-78c3-48e8-90a5-8c65b1303885/iso-4787-2021)

[https://standards.iteh.ai/catalog/standards/sist/d201436a-78c3-48e8-90a5-
8c65b1303885/iso-4787-2021](https://standards.iteh.ai/catalog/standards/sist/d201436a-78c3-48e8-90a5-8c65b1303885/iso-4787-2021)



iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO 4787:2021

<https://standards.iteh.ai/catalog/standards/sist/d201436a-78c3-48e8-90a5-8c65b1303885/iso-4787-2021>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2021

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

| Contents | | Page |
|-------------------|--|-----------|
| Foreword..... | | v |
| Introduction..... | | vi |
| 1 | Scope | 1 |
| 2 | Normative references | 1 |
| 3 | Terms and definitions | 2 |
| 4 | Principle | 2 |
| 5 | Volume and reference temperature | 2 |
| | 5.1 Unit of volume..... | 2 |
| | 5.2 Reference temperature..... | 2 |
| 6 | Apparatus and calibration liquid | 2 |
| | 6.1 Balance..... | 2 |
| | 6.2 Measurement devices..... | 2 |
| | 6.3 Calibration liquid..... | 3 |
| | 6.4 Receiving vessel..... | 3 |
| 7 | Factors affecting the accuracy of volumetric instruments | 3 |
| | 7.1 General..... | 3 |
| | 7.2 Temperature..... | 3 |
| | 7.2.1 Temperature of the volumetric instrument..... | 3 |
| | 7.2.2 Temperature of calibration liquid..... | 3 |
| | 7.3 Cleanliness of surface..... | 4 |
| | 7.4 Conditions of used volumetric instruments..... | 4 |
| | 7.5 Delivery time and waiting time..... | 4 |
| 8 | Setting the meniscus | 5 |
| | 8.1 General..... | 5 |
| | 8.2 Setting the meniscus..... | 5 |
| | 8.2.1 Meniscus of transparent liquids..... | 5 |
| | 8.2.2 Meniscus of opaque liquids..... | 7 |
| 9 | Calibration procedure | 7 |
| | 9.1 General..... | 7 |
| | 9.2 Test room..... | 7 |
| | 9.3 Filling and delivery..... | 7 |
| | 9.3.1 Volumetric flasks and measuring cylinders..... | 7 |
| | 9.3.2 Pipettes adjusted to deliver..... | 7 |
| | 9.3.3 Pipettes adjusted to contain..... | 8 |
| | 9.3.4 Burettes adjusted to deliver..... | 8 |
| | 9.3.5 Pycnometers..... | 9 |
| | 9.4 Weighing..... | 9 |
| | 9.5 Volume and uncertainty calculation..... | 9 |
| 10 | Procedure for use | 10 |
| | 10.1 General..... | 10 |
| | 10.2 Volumetric flasks (in accordance with ISO 1042 or ISO 5215)..... | 11 |
| | 10.3 Measuring cylinders (in accordance with ISO 4788 or ISO 6706)..... | 11 |
| | 10.4 Burettes (in accordance with ISO 385)..... | 11 |
| | 10.5 Pipettes..... | 12 |
| | 10.5.1 Pipettes adjusted to deliver (see ISO 648 and ISO 835, or other pipettes, e.g. plastic ones)..... | 12 |
| | 10.5.2 Pipettes adjusted to contain..... | 12 |
| | 10.6 Pycnometers..... | 12 |
| Annex A | (informative) Cleaning of volumetric glassware | 13 |

| | |
|---|-----------|
| Annex B (informative) Cleaning of volumetric plasticware | 14 |
| Annex C (normative) Calculation formulae and tables | 15 |
| Annex D (informative) Coefficient of cubic thermal expansion | 19 |
| Annex E (informative) Uncertainty estimation and repeatability calculation | 20 |
| Bibliography | 21 |

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[ISO 4787:2021](https://standards.iteh.ai/catalog/standards/sist/d201436a-78c3-48e8-90a5-8c65b1303885/iso-4787-2021)

<https://standards.iteh.ai/catalog/standards/sist/d201436a-78c3-48e8-90a5-8c65b1303885/iso-4787-2021>

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html (standards.iteh.ai)

This document was prepared by Technical Committee ISO/TC 48, *Laboratory equipment*, in collaboration with the European Committee for Standardization (CEN) Technical Committee CEN/TC 332, *Laboratory equipment*, in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

This third edition cancels and replaces the second edition (ISO 4787:2010), which has been technically revised.

The main changes compared to the previous edition are as follows:

- a) volumetric plastic ware has been included;
- b) new information on meniscus adjustment of convex meniscus has been added; namely, altered procedure "Upper edge of the graduation line is horizontally tangential to the highest point of meniscus" as compared to older procedure "Upper edge of the graduation line is horizontally tangential to the lowest point of the meniscus";
- c) improved figures for meniscus adjustment have been provided;
- d) [Table 1](#) has been improved;
- e) new [Table 2](#) for minimum requirements for the measurement devices has been added;
- f) new test room ambient conditions have been added;
- g) new information regarding repeatability and uncertainty has been added in [Annex E](#);
- h) [Formula \(C.1\)](#) has been changed to [Formula \(1\)](#).

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

The International Standards for the individual volumetric instruments include clauses on the specification of capacity (volume); these clauses describe the method of manipulation in sufficient detail to determine the capacity without ambiguity. This document contains supplementary information.

iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO 4787:2021](https://standards.iteh.ai/catalog/standards/sist/d201436a-78c3-48e8-90a5-8c65b1303885/iso-4787-2021)

<https://standards.iteh.ai/catalog/standards/sist/d201436a-78c3-48e8-90a5-8c65b1303885/iso-4787-2021>

Laboratory glass and plastic ware — Volumetric instruments — Methods for testing of capacity and for use

1 Scope

This document provides methods for the testing, calibration and use of volumetric instruments made from glass and plastic in order to obtain the best accuracy in use.

NOTE Testing is the process by which the conformity of the individual volumetric instrument with the appropriate standard is determined, resulting in the determination of its error of measurement at one or more points.

This document is applicable to volumetric instruments with nominal capacities in the range of 100 μ l to 10 000 ml. These include single-volume pipettes (see ISO 648), graduated pipettes (see ISO 835), burettes (see ISO 385), volumetric flasks (see ISO 1042 and ISO 5215), and graduated measuring cylinders (see ISO 4788 and ISO 6706).

The methods are not intended for testing of volumetric instruments with capacities below 100 μ l such as micro-glassware.

This document does not deal specifically with pycnometers as specified in ISO 3507. However, the procedures specified for the determination of volume of glassware can, for the most part, also be followed for the determination of a pycnometer volume. For some types of pycnometers, special handling can be necessary.

2 Normative references

[ISO 4787:2021](#)

[.iteh.ai/catalog/standards/sist/d201436a-78c3-48e8-90a5-8c65b1303885/iso-4787-2021](#)

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 385, *Laboratory glassware — Burettes*

ISO 648, *Laboratory glassware — Single-volume pipettes*

ISO 835, *Laboratory glassware — Graduated pipettes*

ISO 1042, *Laboratory glassware — One-mark volumetric flasks*

ISO 1773, *Laboratory glassware — Narrow-necked boiling flasks*

ISO 3507, *Laboratory glassware — Pycnometers*

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 4788, *Laboratory glassware — Graduated measuring cylinders*

ISO 4797, *Laboratory glassware — Boiling flasks with conical ground joints*

ISO 5215¹⁾, *Laboratory plastic ware — Volumetric flasks*

ISO 6706, *Plastics laboratory ware — Graduated measuring cylinders*

ISO 24450, *Laboratory glassware — Wide-necked boiling flasks*

1) Under preparation. Stage at the time of publication: ISO/DIS 5215:2021.

ISO/IEC Guide 99, *International vocabulary of metrology — Basic and general concepts and associated terms (VIM)*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO/IEC Guide 99 apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

4 Principle

The general procedure for testing the capacity (volume) and for use is based upon a determination of volume of water, either contained in or delivered by the volumetric instrument. This volume of water is based upon knowledge of its mass under consideration of buoyancy and its density (gravimetric method).

5 Volume and reference temperature

5.1 Unit of volume

The unit of volume shall be the millilitre (ml), which is equivalent to one cubic centimetre (cm³).

5.2 Reference temperature

The standard reference temperature, i.e. the temperature at which the volumetric instrument is intended to contain or deliver its volume (capacity), shall be 20 °C.

When the volumetric instrument is required for use in a country which has adopted a standard reference temperature of 27 °C (according to ISO 384), this figure shall replace 20 °C in [Formula \(1\)](#).

6 Apparatus and calibration liquid

6.1 Balance

The balance used for testing shall be chosen in accordance with the minimum requirements specified in [Table 1](#), depending on the nominal volume of the volumetric instrument under test.

Table 1 — Minimum requirements for the balance

| Nominal capacity (volume) V | Resolution mg | Repeatability mg | Expanded uncertainty in use $U (k = 2)^a$ mg |
|---|------------------|---------------------|---|
| $100 \mu\text{l} \leq V \leq 10 \text{ ml}$ | 0,1 | 0,2 | 0,4 |
| $10 \text{ ml} < V \leq 1\ 000 \text{ ml}$ | 1 | 2 | 4 |
| $V > 1\ 000 \text{ ml}$ | 10 | 10 | 40 |

^a Expanded uncertainty in use estimated according to Reference [1] (which includes applicable definitions) at the value of the nominal volume. If uncertainty in use is not available, then the uncertainty at calibration should be taken.

6.2 Measurement devices

The minimum requirements for each relevant measurement device are specified in [Table 2](#).

Table 2 — Minimum requirements for the measurement devices

| Device | Resolution | Expanded uncertainty of measurement $U (k = 2)$ |
|--------------------------|-----------------------|--|
| Thermometer for liquids | 0,1 °C | 0,2 °C |
| Thermometer for room air | 0,1 °C | 0,2 °C |
| Hygrometer | 1 % relative humidity | 5 % relative humidity |
| Barometer | 0,1 kPa | 1 kPa |
| Timing device | 1 s | Not applicable |

6.3 Calibration liquid

As calibration liquid during testing, distilled or de-ionized water complying with ISO 3696, Grade 3 or better should be used. The water temperature shall be within $\pm 0,5$ °C of room air temperature.

6.4 Receiving vessel

The receiving vessel shall be a conical flask, manufactured from glass, e.g. in accordance with ISO 1773, ISO 4797, or ISO 24450, if possible, with ground joint. The receiving vessel shall have a capacity adequate to the amount of water delivered by the volumetric instrument.

7 Factors affecting the accuracy of volumetric instruments

7.1 General

The same sources of error are, naturally, inherent to calibration, testing and use. In calibration, every attempt is made to reduce these errors to a minimum; in use, the care needed is dependent upon the degree of accuracy required. When the greatest possible accuracy is desired, the volumetric instrument should be used as closely as possible to the way it has been calibrated.

7.2 Temperature

7.2.1 Temperature of the volumetric instrument

The capacity of the volumetric instruments varies with change of temperature. The particular temperature at which a volumetric instrument is intended to contain or deliver its nominal capacity is the "reference temperature" of the instrument (see 5.2).

When performing calibrations, it is important to refer to the reference temperature in the report. For example, if a volumetric instrument made of borosilicate glass having a coefficient of cubic thermal expansion of $9,9 \times 10^{-6} \text{ °C}^{-1}$ is calibrated at 20 °C but used at a temperature of 27 °C it would show an extra error of 0,007 %. A volumetric instrument made of soda-lime glass having a coefficient of cubic thermal expansion of $27 \times 10^{-6} \text{ °C}^{-1}$ would show an extra error of 0,02 %, for a 7 °C temperature change.

7.2.2 Temperature of calibration liquid

The temperature of the water used for the calibration shall be measured to $\pm 0,1$ °C, with a maximum variation of ± 1 °C during the test. Corrections for differences in temperature, prevailing during testing or use, from the reference temperature shall be applied in accordance with [Formula \(1\)](#) (see 9.5) and [Annex C](#). The liquid temperature should be measured in the vessel where the instruments are filled from or directly inside the instruments, if technically possible.

7.3 Cleanliness of surface

The volume contained in, or delivered by, a volumetric instrument depends on the cleanliness of the internal surface. Lack of cleanliness of glass surface results in errors through a poorly shaped meniscus involving two defects:

- incomplete wetting of the glass surface, i.e. the liquid surface meets the glass at an arbitrary angle instead of forming a curve such that it meets the glass tangentially;
- a generally increased radius of curvature, due to contamination of the liquid surface reducing the surface tension.

Volumetric instruments made of polyolefins, such as polypropylene (PP) and polymethylpentene (PMP), or fluoroplastics, such as perfluoroalkoxy-copolymer (PFA), have water-repellent surfaces which results in a poorly shaped convex or even flat meniscus (see 8.2).

The ascending or descending liquid meniscus shall not change shape (i.e. it shall not crinkle at its edges). To ascertain whether a piece of apparatus is satisfactorily clean, it shall be observed during filling and dispensing. Additionally, an experienced operator can recognize the shape of an uncontaminated meniscus, in relation to its diameter.

Lack of cleanliness causes additional errors with volumetric instruments used for delivery due to the film of liquid on the walls being irregularly distributed or incomplete, e.g. forming drops on the glass surface. Furthermore, chemical residues can introduce an error in the analytical result by contamination. Where volumetric instruments are fitted with ground stoppers, special attention shall be paid to cleaning the ground zone.

NOTE Small residues of acid, for example, can impair the concentration of the alkaline solution with which the volumetric instrument is filled.

Recommended cleaning procedures are included in [Annex A](#) (for glass) and [Annex B](#) (for plastic). Other cleaning procedures can be used as well.

Fluoride containing cleaning agents should be strictly avoided in the case of glassware.

7.4 Conditions of used volumetric instruments

The surface of volumetric instruments shall be free from obvious damage, the graduations and inscriptions shall be clearly readable and especially with instruments adjusted to deliver the jet shall be free from damage and allow an unrestricted outflow of liquid.

Volumetric glassware should not be heated to a temperature considerably above 180 °C. Although the strain point of glasses used for volumetric purposes is in the range of 500 °C, alterations of volume may occur at temperatures considerably below the strain point.

7.5 Delivery time and waiting time

For volumetric instruments used for delivery of a liquid, the volume delivered is always less than the volume contained, due to the film of liquid left on the inner walls of the volumetric instrument. The volume of this film depends on the time taken to deliver the liquid, and the volume delivered decreases with decreasing delivery time. For example, the delivered volume of a pipette or burette decreases if the jet is broken (shorter delivery time) or increases if the jet is not clean and the outflow of liquid is restricted.

In view of the above, delivery times and waiting times have been specified in the International Standards on volumetric instruments; these times shall be used.

8 Setting the meniscus

8.1 General


Most volumetric instruments employ the principle of setting or reading a meniscus (the interface between air and the liquid) against a graduation line or ring mark. Wherever practicable, the meniscus should descend to the position of setting.

The tubing of the volumetric instrument shall be in a vertical position. The eye of the operator shall be in the same horizontal plane as the meniscus or the graduation line (graduation mark).

8.2 Setting the meniscus

8.2.1 Meniscus of transparent liquids

In case of a concave meniscus, the meniscus shall be set so that the plane of the upper edge of the graduation line is horizontally tangential to the lowest point of the meniscus, the line of sight being in the same plane (see [Figure 1](#)).

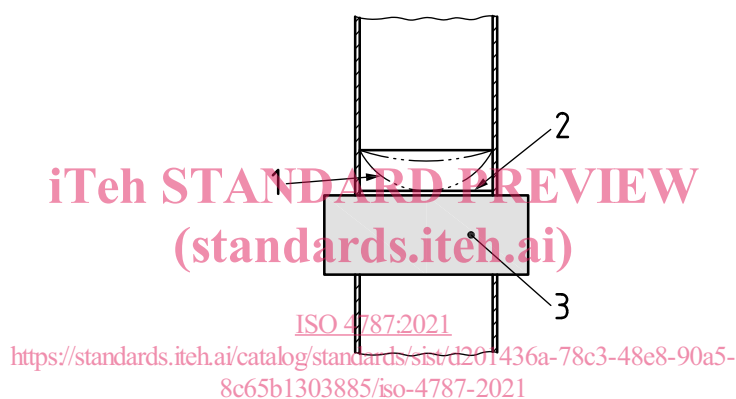

Key

- 1 meniscus
- 2 graduation line
- 3 dark coloured paper

Figure 1 — Setting of concave meniscus

In case of a convex or even flat meniscus, known for water-repellent, non-wetting surfaces of polyolefins, such as PP and PMP, or fluoroplastics, such as PFA, the meniscus shall be set so that the plane of the upper edge of the graduation line is horizontally tangential to the highest point of the meniscus, the line of sight being in the same plane (see [Figure 2](#)).