



# Standard Test Method for Straight Line Movement of Vacuum Cleaners While Cleaning Carpets<sup>1</sup>

This standard is issued under the fixed designation F1409; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 This test method covers the measurement of the relative work required to move the carpet cleaning mechanism of an upright, canister, stick, or combination vacuum cleaner in a straight line with forward and backward stroking on a selection of typical carpeted surfaces.

1.2 This test method can be used in the testing of household and commercial vacuum cleaners.

1.3 This test method measures the relative work needed to move the vacuum cleaner with its motor or motors in operation.

1.4 This test method applies to the vacuum cleaning of carpets only.

1.5 The values stated in inch-pound units are to be regarded as standard. The values given in parentheses are mathematical conversions to SI units that are provided for information only and are not considered standard.

1.6 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

## 2. Referenced Documents

2.1 *ASTM Standards*:<sup>2</sup>

**F608** Test Method for Evaluation of Carpet Embedded Dirt Removal Effectiveness of Household/Commercial Vacuum Cleaners

**F655** Specification for Test Carpets and Pads for Vacuum Cleaner Testing

**F884** Test Method for Motor Life Evaluation of a Built-In

(Central Vacuum) Vacuum Cleaner

**F922** Test Method for Motor Life Evaluation of an Electric Motorized Nozzle

**F1038** Test Method for Motor Life Evaluation of a Canister, Hand-held, Stick, and Utility Type Vacuum Cleaner Without a Driven Agitator

**F1334** Test Method for Determining A-Weighted Sound Power Level of Vacuum Cleaners

2.2 *ASTM Adjunct*:<sup>3</sup>

Mobility fixture book

## 3. Summary of Test Method

3.1 The carpet cleaning mechanism of the vacuum cleaner is moved back and forth on the test carpet in a prescribed manner during the test. A handle clamp assembly with a strain gage is attached to the vacuum cleaner at the location where the user's working hand usually grips the carpet cleaning mechanism. This gage measures the force involved in moving only the carpet cleaning mechanism.

3.2 Simultaneously, by means of a rod pivotally mounted to the test fixture, the distance that the vacuum cleaner moves is monitored. The force and distance signals are then introduced into an X-Y recorder that produces a plot from which relative work is determined. Alternate data acquisition and computing methods are acceptable.

## 4. Significance and Use

4.1 This test method measures the relative work required by the user during the cleaning operation for the movement of a vacuum cleaner in the home or other cleaning location. Relative work is defined as the work measured by the equipment described in this test method.

4.2 This measurement is relative to the work performed by the user of vacuum cleaners and may be used for comparison between vacuum cleaners.

4.3 The relation between actual vacuum cleaner usage and the method of operation is valid only if the vacuum cleaner

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee F11 on Vacuum Cleaners and is the direct responsibility of Subcommittee F11.20 on Performance (Test Methods).

Current edition approved Oct. 1, 2010. Published December 2010. Originally approved in 1992. Last previous edition approved in 2005 as F1409 – 00 (2005). DOI: 10.1520/F1409-00R10.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

<sup>3</sup> A complete set of drawings, photos, vendor information, assembly, calibration and testing instructions for the mobility fixture and associated equipment are available from ASTM International Headquarters. Order Adjunct No. **ADJF1409**. Original adjunct produced in 1992.

user operates the vacuum cleaner properly and in accordance with the manufacturer's instructions.

**5. Apparatus**

5.1 *Mobility Fixture.*<sup>3</sup>

5.2 *Test Platform* (see 5.1 and Fig. 1).

5.3 *Distance Monitor* (see 5.1 and Fig. 1).

5.4 *Uniform Stroke Speed Indicator* (see 5.1 and Fig. 1), or other type of equipment capable of establishing the rate or movement of the carpet cleaning mechanism as specified in Section 9.

5.5 *Force Measuring Device and Auxiliary Equipment*, giving readings accurate to within  $\pm 5\%$ .

5.5.1 *Strain Gage* (see 5.1 and Fig. 1).

5.5.2 *Load Cell Power Supply* (see 5.1 and Fig. 1).

5.5.3 *X-Y Recorder* (see 5.1 and Fig. 1).

NOTE 1—The graph paper plot size should be 4 x 4 in. (10 divisions per in. with the smallest increment equal to 0.1 in.). Increments along X axis equal 2 ft/in. Increments along Y axis equal 10 lb/in.

5.5.4 *Planimeter*—Electronic integrator or suitable method of measurement.

5.5.5 *Calibration Weights*—5, 10, and 20 lb.

5.6 *Test Carpets*, as specified in Specification F655.

NOTE 2—Test carpets should be stored in a vertical position with no weight on the test surface.

NOTE 3—The test carpets for relative work testing should be limited to that use and not used for other tests such as cleanability.

5.7 *Padding*, beneath test carpet, as specified in Specification F655.

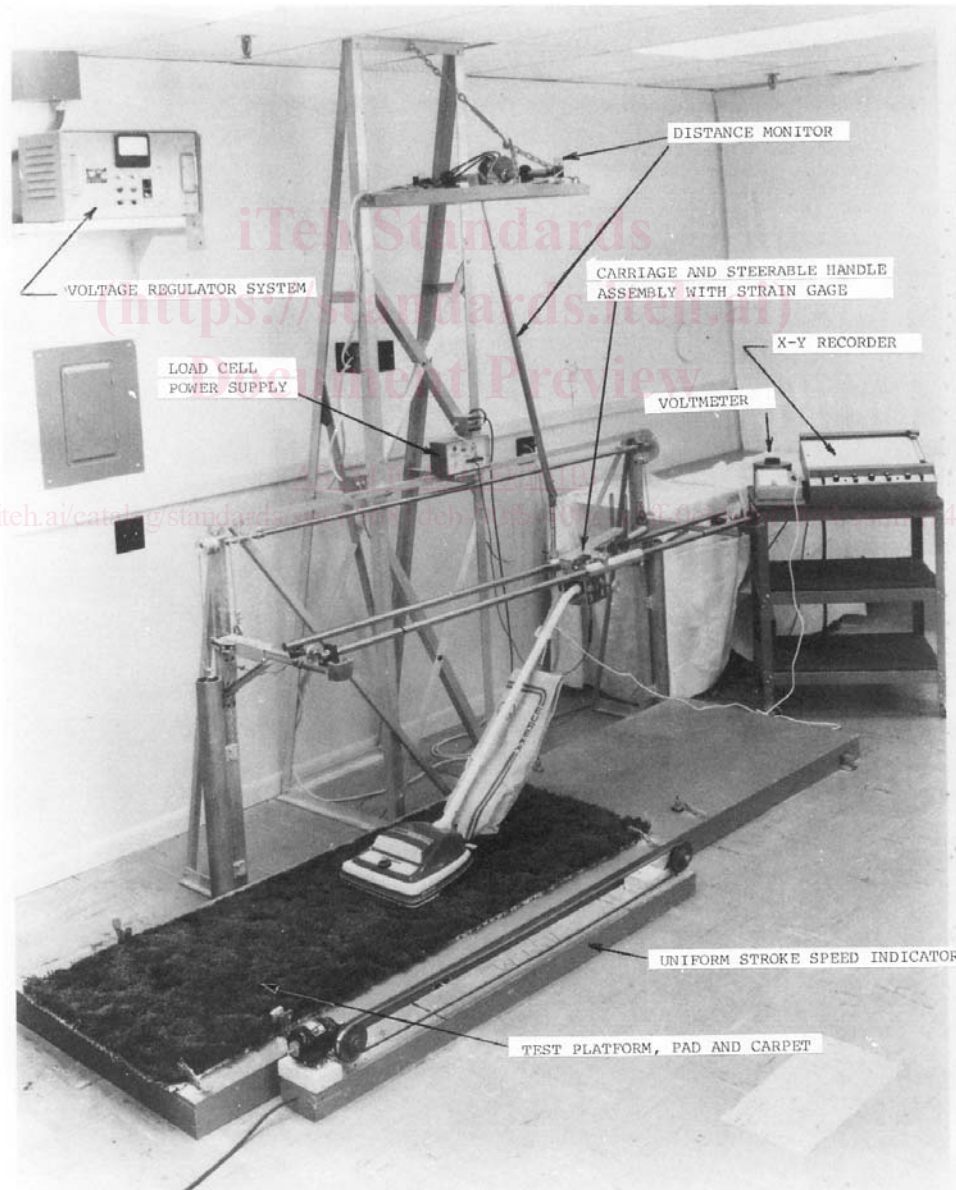


FIG. 1 ASTM Mobility Fixture and Associated Equipment

5.8 *Temperature and Humidity Indicators*, to provide temperature measurements accurate to  $\pm 1^\circ\text{F}$  ( $\pm 0.5^\circ\text{C}$ ) and  $\pm 2\%$  relative humidity.

5.9 *Voltmeter*, to measure input voltage to the vacuum cleaner, capable of providing measurements accurate within  $\pm 1\%$ .

5.10 *Voltage Regulator System*, to control input voltage to the vacuum cleaner. The regulator system shall be capable of maintaining the vacuum cleaner's rated voltage  $< 1\%$  and rated frequency  $< 1\text{ Hz}$  having a wave form that is essentially sinusoidal with  $3\%$  maximum harmonic distortion for the duration of the test.

5.11 *Rotating Agitator Reference Cleaner*, for calibrating test carpets (see 7.1.3).

5.12 *Straight Air Canister Reference Cleaner*, for calibrating test carpets (see 7.1.3).

## 6. Sampling

6.1 A minimum of three units of the same model vacuum cleaner, selected at random in accordance with good statistical practice, shall constitute the population sample.

6.1.1 To determine the best estimate of the total relative work for the population of the vacuum cleaner model being tested, the arithmetic mean of the relative work of the sample from the population shall be established by testing it to a  $90\%$  confidence level within  $\leq \sim 5\%$  of the mean.

6.1.2 **Annex A1** provides a procedural example for determining the  $90\%$  confidence level and when the sample size shall be increased (see **Note 4**).

**NOTE 4**—See **Annex A1** for method of determining  $90\%$  confidence level.

## 7. Preparation of Apparatus and Test Cleaner

### 7.1 *Preconditioning for New Test Carpet Samples:*

7.1.1 Cut a sample of each test carpet to a size of 27 by 72 in. (690 by 1830 mm) minimum. If the warp direction or "lay" of the carpet can be determined, it shall be in the 72 in. direction. Carpets shall be bound on all sides.

7.1.2 Precondition the entire carpet by cleaning with a rotating agitator-type cleaner. Continue the operation until less than 2 g of carpet fibers are picked up in 5 min.

7.1.3 After the preconditioning is completed, run calibration tests on each of the carpets to establish a reference rating for one reference rotating agitator cleaner and one reference straight air canister cleaner to determine when the test carpets need to be replaced. The reference rating, or relative work for each cleaner, is established using the procedure described in 9.1 – 9.4. The relative work thus determined for the rotating agitator cleaner and the straight air canister are the reference ratings for the carpets in new condition.

7.1.4 Repeat the calibration tests after every 50 tests on the carpets, using the same reference cleaners. The performance of these reference cleaners should be maintained through the carpet calibration period. When the total for either reference cleaner varies by more than 5 ft-lbf from the original reference rating, replace the test carpet.

7.2 Prior to each of the basic testing segments, lay the padding (see 5.7) on the platform and place the appropriate carpet on top of the padding, without stretching either one. Position the carpet in such a way that the forward test strokes of the cleaner to be tested are with the lay of the carpet.

**NOTE 5**—The extremes of the stroke can be marked by a tape applied to the test carpet for operator convenience.

### 7.3 *Preconditioning a Test Cleaner:*

7.3.1 Run-in the test cleaner at a rated voltage  $\leq \sim 1\%$  and rated frequency  $\pm 1\text{ Hz}$  with filters in place, to ensure that the motor brushes are properly seated and to precondition the agitator brushes.

7.3.1.1 *Preconditioning a Rotating Agitator-Type Cleaner*—In a stationary position, operate the cleaner for 1 h with the agitator bristles not engaged on any surface.

7.3.1.2 *Preconditioning a Straight Air Canister Cleaner*—Operate for 1 h with wide open inlet (without hose).

### 7.4 *Calibration Check of the Recorder and Measuring Device:*

**NOTE 6**—If equipment does not perform properly after the following check procedure, recalibrate in accordance with Adjunct No. 12-614090-47.

7.4.1 Turn on the X-Y recorder, and the X and Y amplifiers  $\frac{1}{2}$  h before testing to stabilize the components. If the recorder is covered, remove the cover to ensure adequate ventilation.

7.4.2 Loosen the thumb screw holding the pendulum constant length adjustment rod and lower it to its lowest position to avoid damage to the telescoping pendulum.

7.4.3 Place the handle of the carriage in a level position and move the carriage laterally to a position where the pendulum shaft assembly is vertical from side to side. Adjust the pendulum vertical positioning link forward to backward, if required, so that the pendulum is vertical in the front to rear direction.

7.4.4 Set the handle clamp pivot point at  $32\frac{1}{2}$  in. above the carpet test platform (carpet and pad not in place) with the support lifting crank assembly. With the pendulum shaft assembly vertical, align the top of the pendulum outer tube with the black line on the pendulum shaft and tighten the thumb screw holding the pendulum constant length adjustment rod in place.

7.4.5 Remove the calibration spring attached to the calibration screw and attach one end of a cord to the rear calibration cord attaching screw on the carriage. Bring the cord over the pulley at the rear end of the stainless steel shaft and attach it to a 5-lb weight resting on the test platform.

7.4.6 Set the recorder pen on a horizontal line on the recorder chart and push the carriage to lift the weight from the floor.

7.4.7 Hold the carriage in a fixed position after the weight has been lifted from the floor and check the pen position. It should move 5 graph increments to indicate 5 lb. If the pen moved more or less than 5 increments, adjust the Y axis VAR SCALE knob on the recorder in the proper direction to give a movement of 5 increments.

7.4.8 Check the recorder pen movement for linearity in a manner similar to that described in 7.4.7 with the 10- and 20-lb



weights for pen movements of 10 and 20 increments, respectively. There should be little if any *Y* axis VAR SCALE knob adjustment required.

7.4.9 Remove the cord from the rear of the carriage and attach it to the calibration cord attaching screw at the front of the carriage. Place the cord over the pulley at the front end of the stainless steel shaft and attach it to a 5-lb weight resting on the test platform.

7.4.10 Pull the carriage backward to lift the weight from the platform. The pen should move 5 chart increments in the opposite direction from that occurring in 7.4.7. Check the calibration and linearity in a similar manner with the 10 and 20-lb weights. Remove the cord and weights from the test fixture and lift the recorder pen from the chart.

7.4.11 Locate the rear of the carriage at the rear limit line of the stainless steel shaft at the beginning of the forward stroke. Set the pen at the juncture of the two major graph lines at the left side of the graph and lower the recorder pen onto the recorder graph.

7.4.12 Move the carriage through one complete forward stroke to the forward limit line on the stainless steel shaft and back to the rear limit line. Check and adjust the pen VAR SCALE knob on the *X* axis amplifier to give an *X* axis pen displacement of the desired dimension representing 8 ft of carriage travel (let 5 increments equal 1 ft). This completes the calibration.

#### 7.5 Test Cleaner Settings:

7.5.1 If various settings are provided, set the motor speed setting, suction regulator, or nozzle height, or combination thereof, using the manufacturer's specifications as provided in the instruction manual for each type of test carpet. Contact the manufacturer if no instructions are given, or if the instructions are unclear or inadequate.

7.5.1.1 The settings used for this test method (nozzle, motor speed, suction regulator, and so forth) for each specific carpet shall be applied for all embedded dirt cleaning effectiveness (Test Method F608), sound power (Test Method F1334), and motor life evaluation (Specification F655, Test Methods F884, F922, and F1038) tests.

#### 7.6 Apparatus Set-Up For Cleaner Testing:

7.6.1 Turn on the *X-Y* recorder, *X* and *Y* axis amplifier  $\frac{1}{2}$  h before testing to stabilize the components.

7.6.2 The entire test carpet should be vacuumed thoroughly for 2 min with a rotating agitator-type cleaner just prior to the relative work test to remove any residual dirt that may have accumulated.

7.6.3 Place the test carpet and pad on the carpet test platform with the lay of the carpet in the forward direction.

7.6.4 Loosen the thumb screw holding the pendulum constant length adjustment rod and lower it to its lowest position.

7.6.5 The cleaner to be tested should be thoroughly cleaned to remove any residual test dirt or dust that could be drawn into the cleaner's filtration system.

7.6.5.1 For vacuum cleaners using disposable filters as the primary filters, use a new disposable primary filter from the manufacturer for each test.

7.6.5.2 For vacuum cleaners using nondisposable dirt receptacles, empty in accordance with the manufacturer's instructions before each test.

7.6.5.3 For vacuum cleaners using water as the primary filter, empty the receptacle and refill as recommended by the manufacturer before each test.

7.6.6 If the cleaner has a pivoting handle, adjust the angle of the carriage and handle assembly so that the strain gage is parallel to a line extending through the center of the handle grip and the center of the pivot point when the center of the handle grip is 31.5 in. above the carpet surface (see Fig. 2).

NOTE 7—This angle may be mathematically determined prior to testing.

7.6.7 If the cleaner has a nonpivoting handle or wand, adjust the angle of the carriage and handle assembly so that the strain gage is parallel to a line extending through the center of the handle grip and the center of the nozzle at its interface with the carpet surface when the cleaner is set in accordance with 7.5.1 (see Fig. 3).

NOTE 8—This angle may be mathematically determined prior to testing.

7.6.8 Adjust the calibration spring assembly so there is no *Y* axis movement of the recorder pen when the carriage is moved from the "kill switch" area to the "forward stroke" area.

7.6.9 If the cleaner has a pivoting handle or wand, raise or lower the carriage and handle clamp assembly so the handle clamp pivot point is 31.5 in. (0.8 m) from the top of the carpet pile. If the handle or wand does not pivot, adjust for a handle height that will provide maximum suction at the nozzle and a parallel contact between the carpet pile and the bottom surface of the nozzle as determined in 7.5.1.

7.6.10 Set the pendulum constant length adjustment rod by moving the carriage where the pendulum shaft assembly is vertical and raise the adjustment rod and the pendulum outer tube until the top of the tube is level with the line on the pendulum shaft. Tighten the adjustment rod thumb screw.

7.6.11 Mount the cleaner handle to the handle clamping assembly in a manner that securely clamps the handle gripping area so that the center of the clamping assembly is positioned at the center of the handle gripping area.

7.6.12 Move the carriage forward and backward several times and readjust the threaded shafts on the handle clamp, if necessary, to ensure that the cleaning mechanism is straight.

7.6.13 Set the test cleaner settings in accordance with 7.5.1.

7.6.14 Insert a blank sheet of graph paper in the *X-Y* recorder. Position the recorder pen at the desired starting point on the graph.

## 8. Conditioning

8.1 *Test Room*—Maintain the test room in which all conditioning and cleaner testing is done at  $70 \pm 5^\circ\text{F}$  ( $21 \pm 3^\circ\text{C}$ ) and 45 to 55 % relative humidity.

8.2 All components involved in the test must remain and be exposed in the controlled environment for at least 16 h prior to the start of the test.

## 9. Procedure

9.1 Perform this procedure on all test carpets specified in 5.6 with the cleaner motor or motors operating at the cleaners

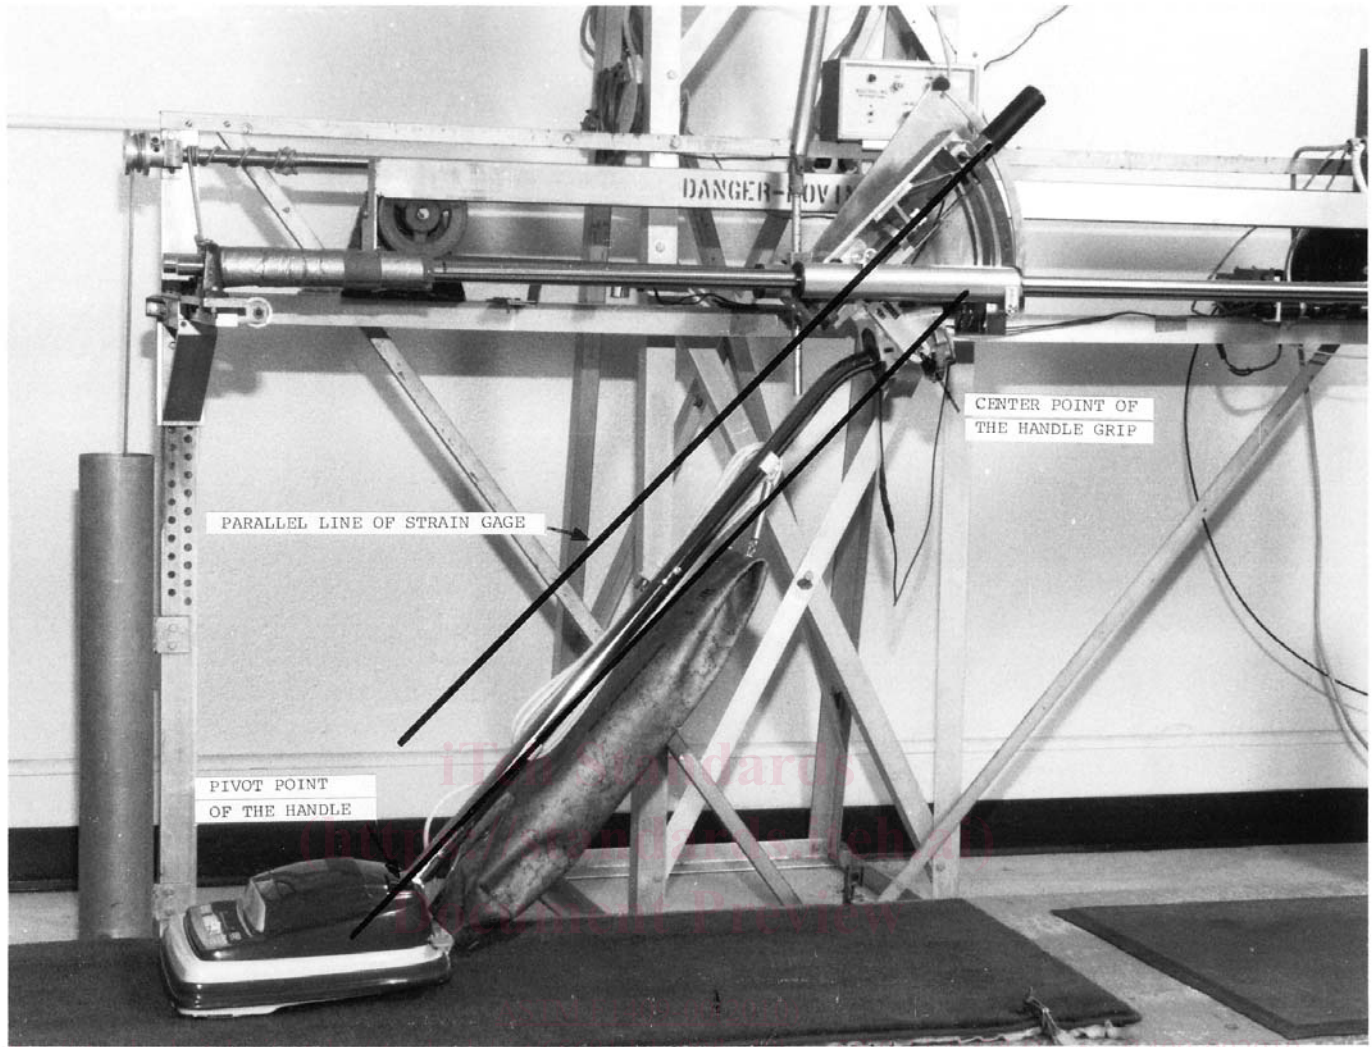


FIG. 2 Adjustment Angle (Pivoting Handle)

nameplate rated voltage  $\pm 1\%$  and frequency  $\pm 1$  Hz. For vacuum cleaners with dual nameplate voltage ratings, conduct testing at the highest voltage.

9.2 Grasping the handle of the carriage, handle, and clamp assembly, apply a force to push the cleaner forward in a straight line for 48 in. (1.22 m) at a rate of 1.8 ft/s (0.55 m/s), paced by the uniform stroke speed indicator. Take care to go up to, but not over, the forward limit line on the stainless steel shaft.

9.3 In similar fashion to 9.2, pull the cleaner backward in a straight line for the same distance at the same rate up to, but not past, the rear limit line on the stainless steel shaft.

9.4 Repeat the operations described in 9.2 and 9.3 for ten uninterrupted cycles recording the force versus distance on the X-Y plotter. The X-Y plotter may be replaced by a data acquisition system or electronic integrator.

9.5 9.1 – 9.4 are considered to be one test run. Repeat 9.1 – 9.4 two additional times, for a total of 3 test runs. The test results of each test run shall be recorded on separate X-Y plots.

## 10. Calculation

10.1 Using a planimeter, electronic integrator, or data acquisition system to measure the area under the forward stroke curve above the zero line only, and under the reverse stroke curve below the zero line only, on the X-Y plot (see Fig. 4) for each test run. Record the values separately for each test run.

10.1.1 If a planimeter is used to measure the area, measure the average path for the ten traces on the plot three separate times for better accuracy.

NOTE 9—The calibration of the planimeter shall be checked carefully and the same planimeter should be used to measure the graph areas obtained throughout the test series with the same flat surfaces under the graph paper.

10.2 Make the necessary calculations to determine if the 90 % confidence level has been met along with the repeatability and reproducibility requirements for precision and bias. See Annex A1.

## 11. Report

11.1 Report the following information:



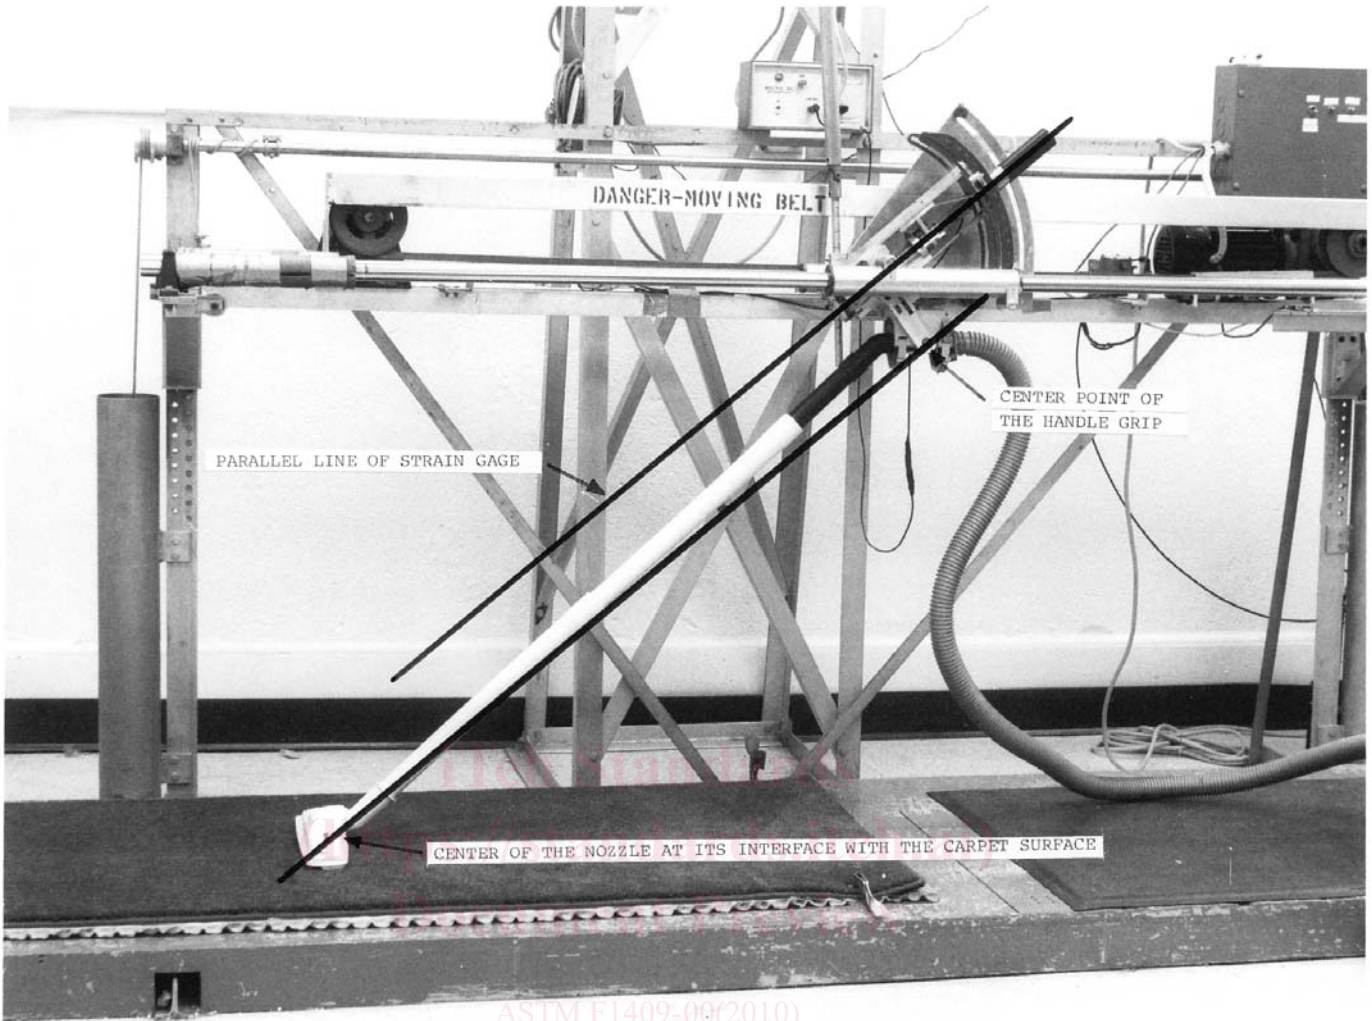


FIG. 3 Adjustment Angle (Nonpivoting Handle)

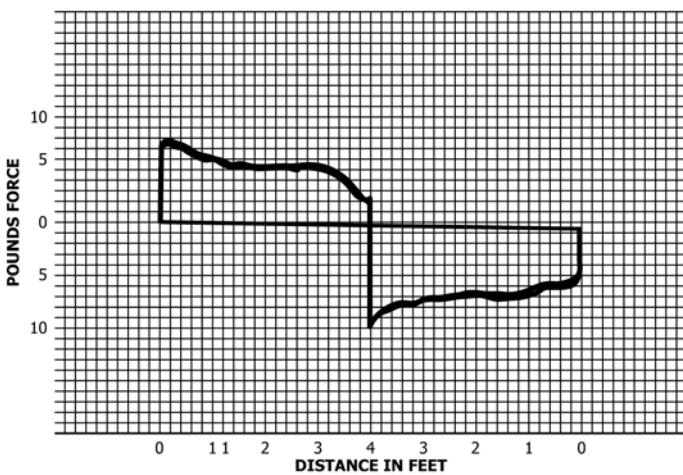


FIG. 4 Typical Forward and Reverse Stroke Curve

11.1.1 The average of the three readings measured in Section 10.1 in foot-pounds force (newton metres or joules) for the forward stroke and the reverse stroke, and the absolute sum

of these two readings as the total relative work for each carpet. The total relative work figures should be used in establishing the confidence level.

11.1.2 The temperature and humidity conditions existing during the test.

11.1.3 Permanently mark or tape the location of the clamp jaws on the cleaning mechanism handle or wand and record the handle height and the angle at which the strain gage and handle clamp assembly was set for future reference and testing of that cleaner.

## 12. Precision and Bias

12.1 Precision statements are based on interlaboratory tests involving five laboratories and four units.

### 12.2 Repeatability (Single-Operator Laboratory):

12.2.1 *Plush Carpet, Upright Cleaner*—The standard deviation within a laboratory divided by the average (coefficient of variation) with the same analyst has been found to be 1.6 % or less. Two values should be considered suspect (at the 95 % confidence level) if they differ by more than 4.5 %.