



Designation: ~~F648-10~~ Designation: **F648 – 10a**

Standard Specification for Ultra-High-Molecular-Weight Polyethylene Powder and Fabricated Form for Surgical Implants¹

This standard is issued under the fixed designation F648; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This specification covers ultra-high molecular weight polyethylene powder (UHMWPE) and fabricated forms intended for use in surgical implants.

1.2 The requirements of this specification apply to UHMWPE in two forms. One is virgin polymer powder (Section 4). The second is any form fabricated from this powder from which a finished product is subsequently produced (Section 5). This specification addresses material characteristics and does not apply to the packaged and sterilized finished implant.

1.3 The requirements of this specification do not apply to UHMWPE virgin powder or fabricated forms intentionally crosslinked or blended with other additives, for example, antioxidants.

1.4 The biological response to polyethylene in soft tissue and bone has been well characterized by a history of clinical use (**1, 2, 3**)² and by laboratory studies (**4, 5, 6**).

1.5 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.6 The following precautionary caveat pertains only to the test method portion, Section 7, of this specification: *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 ASTM Standards:³

D256 Test Methods for Determining the Izod Pendulum Impact Resistance of Plastics

D638 Test Method for Tensile Properties of Plastics

D648 Test Method for Deflection Temperature of Plastics Under Flexural Load in the Edgewise Position

D790 Test Methods for Flexural Properties of Unreinforced and Reinforced Plastics and Electrical Insulating Materials

D792 Test Methods for Density and Specific Gravity (Relative Density) of Plastics by Displacement

D1505 Test Method for Density of Plastics by the Density-Gradient Technique

D1898 Practice for Sampling of Plastics⁴

D4020 Specification for Ultra-High-Molecular-Weight Polyethylene Molding and Extrusion Materials

F619 Practice for Extraction of Medical Plastics

F748 Practice for Selecting Generic Biological Test Methods for Materials and Devices

F749 Practice for Evaluating Material Extracts by Intracutaneous Injection in the Rabbit

F756 Practice for Assessment of Hemolytic Properties of Materials

F763 Practice for Short-Term Screening of Implant Materials

F813 Practice for Direct Contact Cell Culture Evaluation of Materials for Medical Devices

F895 Test Method for Agar Diffusion Cell Culture Screening for Cytotoxicity

F981 Practice for Assessment of Compatibility of Biomaterials for Surgical Implants with Respect to Effect of Materials on Muscle and Bone

2.2 ISO Standards

¹ This specification is under the jurisdiction of ASTM Committee F04 on Medical and Surgical Materials and Devices and is the direct responsibility of Subcommittee F04.11 on Polymeric Materials.

~~Current edition approved Sept. 15, 2010. Published October 2010. Originally approved in 1980. Last previous edition approved in 2007 as F648-07^{ε1}. DOI: 10.1520/F0648-10.~~

Current edition approved Dec. 1, 2010. Published December 2010. Originally approved in 1980. Last previous edition approved in 2010 as F648-10. DOI: 10.1520/F0648-10a.

² The boldface numbers in parentheses refer to the list of references at the end of this specification.

³ For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

⁴ Withdrawn.

ISO 527 Plastics: Determination of Tensile Properties⁵

ISO 3451-1 Plastics—Determination of Ash, Part 1: General Methods⁵

ISO 11542/2; Plastics—Ultra-High Molecular Weight Polyethylene (UHMWPE) Moulding and Extrusion Materials—Part 2: Preparation of Test Specimens and Determination⁵

3. Terminology

3.1 *Definitions of Terms Specific to This Standard:*

3.1.1 *fabricated form, n*—any bulk shape of UHMWPE, fabricated from the virgin polymer powder and used during the process of fabricating surgical implants prior to packaging and sterilization.

3.1.1.1 *Discussion*—This form results from the application of heat and pressure to the virgin polymer powder, and the material characteristics of this form are subject to the applicable requirements of this specification. In present practice, this includes ram-extruded bars or molded blocks from which the final product form is machined, or a molded shape which is subsequently trimmed.

3.1.2 *generic property, n*—that property which is determined solely by the chemical composition and structure of the virgin polymer.

3.1.3 *morphology index (MI), n*—ratio of the total number of Type A and Type B indications (see Annex A2) to the total surface area examined in cm².

3.1.4 *Type A non-fused flake, n*—a Type A non-fused flake (A2.4.1 and Fig. A2.1) is an indication visible under conditions described in A2.5.1 that has an essentially complete circumferential black boundary and a white center.

3.1.5 *Type B non-fused flake, n*—a Type B non-fused flake (A2.4.2 and Fig. A2.2) is an indication visible under conditions described in A2.5.1 that has a partially circumferential black boundary that appears to trace out 50 % to 99 % of a flake's perimeter.

3.1.6 *virgin polymer powder, n*—form of UHMWPE as obtained from the powder manufacturer and prior to fabrication into a bulk shape.

4. Virgin UHMWPE Powder Requirements

4.1 *Generic Properties:*

4.1.1 The virgin polymer shall be a homopolymer of ethylene in accordance with Specification D4020.

4.1.2 The resin type and solution viscosity number requirements are listed in Table 1.

4.2 *Nongeneric Properties:*

4.2.1 When a 300 g sample is prepared and viewed in accordance with 7.1.2, there shall be no more particles of extraneous matter than that specified in Table 1.

4.2.2 To promote uniformity between different lots of polymer powder, concentration limits for trace elements have been established and are listed in Table 1.

4.2.3 When determined as described in ISO 3451-1, the mean ash of duplicate samples shall not exceed the limits established in Table 1.

5. UHMWPE Fabricated Form Requirements

5.1 *Compositional Requirements :*

5.1.1 No stabilizers, antioxidants, or processing aids are to be added to the virgin polymer powder during manufacture of a fabricated form.

5.1.2 No stabilizers, antioxidants, or processing aids are to be added to the fabricated form during manufacture of the final implant.

⁵ Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036, <http://www.ansi.org>.

TABLE 1 Requirements for UHMWPE Powders

| Property | Test Method | Requirement | | |
|--|---------------------|-------------|--------|--------|
| | | Type 1 | Type 2 | Type 3 |
| Resin Type | | | | |
| Viscosity Number, mL/g, | ASTM D4020 (0.02 %) | 2000-3200 | >3200 | >3200 |
| Elongation Stress, (Minimum)† | ASTM D4020 | 0.20 | 0.42 | 0.42 |
| Ash, mg/kg, (Maximum) | ISO 3451-1 | 125 | 125 | 300 |
| Extraneous Matter, No. Particles, (Maximum) | 4.2.1 | 3 | 3 | 25 |
| Titanium, mg/kg, (Maximum) | 7.1.3.1 | 40 | 40 | 150 |
| Aluminum, mg/kg, (Maximum) | 7.1.3.1 | 20 | 20 | 100 |
| Calcium, mg/kg, (Maximum) | 7.1.3.1 | 5 | 5 | 50 |
| Chlorine, mg/kg, (Maximum) | 7.1.3.2 | 30 | 30 | 90 |

† Editorially corrected.

5.2 Physical Requirements:

5.2.1 Foreign Matter Requirements :

5.2.1.1 When 5000 cm² is evaluated according to 7.2.2, there shall be no more than ten particles of extraneous matter visible on the surface when visually inspected by a person with normal or fully corrected vision.

5.2.2 Morphology Requirements:

5.2.2.1 When evaluated according to Annex A2 the calculated morphology index (MI) and total surface area examined shall be reported.

5.3 Mechanical Requirements:

5.3.1 UHMWPE in fabricated form from which implants shall be made shall meet the requirements listed in Table 2.

5.3.2 The following mechanical tests may be conducted based on agreement between the vendor and purchaser:

5.3.2.1 Deflection temperature; Test Method D648 (1.8 MPa), and Flexural modulus; Test Methods D790 (secant, 2 % offset).

6. Sampling

6.1 Where applicable, the requirements of this specification shall be determined for each lot of powder and fabricated form by sampling sizes and procedures according to Practice D1898, or as agreed upon between the purchaser and seller.

7. Test Methods

7.1 UHMWPE Powder:

7.1.1 Determine the solution viscosity number in accordance with the method given in Specification D4020 at a concentration of 0.02 %.

7.1.2 Determine the amount of extraneous matter by the following procedure as agreed upon by the purchaser and seller.

7.1.2.1 A 300 g sample is divided into four 75 g samples. Place a 75 g sample in each of four 1000 mL Erlenmeyer flasks, add 400 mL isopropyl alcohol, shake 5 min, and let settle for 5 min. Count the total number of particles of extraneous matter in the four flasks.

7.1.2.2 Visually examine (20/20 corrected vision if necessary) the four flasks and count the total number of particles of extraneous matter.

7.1.3 Determine the following trace element concentrations by the following methods, or by methods agreed upon by the purchaser and seller.

7.1.3.1 The elements Ti, Al, and Ca may be determined by atomic absorption (AA) or emission spectroscopy (ES); inductively coupled plasma mass spectroscopy (ICP/MS); or inductively coupled plasma spectroscopy (ICP).

7.1.3.2 The element chlorine (Cl) may be determined potentiometrically, titrimetrically, by neutron activation analysis, by inductively coupled plasma mass spectroscopy (ICP/MS), or by the oxygen bomb combustion/UV-Vis spectroscopy method.

7.2 UHMWPE Fabricated Form:

7.2.1 The requirement that there will be no addition of any stabilizer, antioxidant, or processing aid during fabrication of the fabricated form shall be met by certification of the fabricator.

7.2.2 Determine the amount of extraneous matter by the following procedure.

7.2.2.1 Prepare a number of test specimens from the fabricated form as agreed upon by the purchaser and seller.

TABLE 2 Requirements for UHMWPE Fabricated Forms

| Property | Test Method | Requirement | | |
|--|---|-------------|---------|---------|
| | | Type 1 | Type 2 | Type 3 |
| Resin Type | | | | |
| Density, kg/m ³ | ASTM D792 or D1505 | 927-944 | 927-944 | 927-944 |
| Ash, mg/kg, (Maximum) | ISO 3451-1 | 150 | 150 | 300 |
| Ash, mg/kg, (Maximum) | ISO 3451-1 | 125 | 125 | 300 |
| Tensile Strength, 23°C, MPa, (Minimum) ^A | ASTM D638, Type IV, 5.08 cm/min | | | |
| Tensile Strength, 23°C, MPa, (Minimum) ^A | ASTM D638, Type IV, 1.5 mm ± 0.5 mm, 5.08 cm/min | | | |
| Ultimate | | 40 | 40 | 27 |
| Yield | ISO 527, 100 mm/min. | 24 | 19 | 19 |
| Yield | ISO 527, Type IV, 1.5 mm ± 0.5 mm, 100 mm/min | 21 | 19 | 19 |
| Elongation, %, (Minimum) ^A | ASTM D638, Type IV, 5.08 cm/min ISO 527, 100 mm/min. | 380 | 340 | 250 |
| Izod Impact Strength, kJ/m ² , (Minimum) ^B | Annex A1 | 126 | 73 | 25 |
| Charpy Impact Strength, kJ/m ² , (Minimum) ^B | ISO/CD 11542/2.3 | 180 | 90 | 30 |
| Charpy Impact Strength, kJ/m ² , (Minimum) ^B | ISO 11542/2 | 180 | 90 | 30 |

^A Either Test Method D638 or ISO 527 may be used to determine tensile strength and elongation, however the ISO 527 method will be considered the referee method. An extensometer shall be used for measuring strain and calculating percent elongation.

^B Either Charpy or Izod impact strength may be determined, however, the Charpy test will be considered the referee method.

7.2.2.2 Visually examine (20/20 corrected vision if necessary) a total area of 5000 cm² taken from locations within the fabricated form agreed upon by the purchaser and seller.

7.2.3 Determine the density in accordance with Test Methods D792 or D1505.

7.2.4 Determine specific mechanical properties in accordance with the methods listed in Table 2. Mechanical test specimens shall be produced by methods that represent those used to produce the fabricated form.

7.2.5 Unless otherwise specified, the testing described in Table 2 (except for ash) shall be conducted under standard conditions of $23 \pm 2^\circ\text{C}$ after storage of the test specimens for at least 16 h.

8. Biocompatibility

8.1 This material has been shown to produce a well characterized level of biological response following long term clinical use in laboratory animals. The results of these studies and the clinical history indicate an acceptable level of biological response in the applications in which the material has been utilized. When new applications of the material, or modification to the material or physical forms of the materials are being contemplated, the recommendations of Practice F748 should be considered and testing as described in Practices F619, F749, F756, F763, F813, and F981 as well as Test Method F895.

9. Keywords

9.1 fabricated forms; powdered form; ultra-high molecular weight polyethylene

ANNEXES

(Mandatory Information)

A1. IMPACT STRENGTH

A1.1 General Description

A1.1.1 This test method covers the determination of the impact resistance of Ultra-High Molecular Weight Polyethylene (UHMWPE) which is extremely impact resistant. When tested according to Test Method D256, Method A, UHMWPE generally gives a non-break type for failure, rendering the test result invalid. This test method specifies the same type of pendulum impact test machine as given in Test Method D256 but introduces a much higher degree of stress concentration into the specimen by double notching with a razor blade. It is advised that the user be familiar with Test Method D256 before attempting to use this test method.

A1.2 Apparatus

A1.2.1 The Izod type impact machine which conforms to the requirements of Test Method D256, including the calibration and checking methods, shall be used.

A1.3 Test Specimen

A1.3.1 The geometry and dimensions of the specimen are given in Fig. A1.1.

A1.3.2 The specimens shall be made from the fabricated form.

A1.3.3 Each specimen shall be free of twist and shall be bounded by mutually perpendicular pairs of plane parallel surfaces, free from scratches, pits, and sink marks.

A1.4 Notching of Specimens

A1.4.1 Notching shall be done on the sides parallel to the direction of application of molding pressure; if applicable.

A1.4.2 A 4.57 ± 0.076 mm (0.180 ± 0.003 in.) deep notch shall be made with a suitable machine by pressing in a 0.25 mm (0.010 in.) thick single edge razor blade with a 15° included angle at the cutting edge. The notching speed shall be less than 508 mm/min. (20 in./min.). A new blade shall be used after notching 40 specimens.

A1.4.3 The calibration of the notching machine shall be checked by direct measurement of the notch depth, perpendicularity, and offset of the two notches. One of the possible measurement methods is given in A1.8.

A1.5 Conditioning


A1.5.1 *Conditioning*—Condition the notched specimens at $23 \pm 2^\circ\text{C}$ ($73 \pm 4^\circ\text{F}$) for not less than 16 h prior to test.

A1.5.2 *Test Conditions*—Conduct the test in the standard laboratory atmosphere of $23 \pm 2^\circ\text{C}$ ($73 \pm 4^\circ\text{F}$).

A1.6 Procedure

A1.6.1 At least five and preferably ten individual determinations of impact value must be made on each sample to be tested under the conditions prescribed.

A1.6.2 Measure the width of each specimen in the area between notches twice with a micrometer to the nearest 0.025 mm (0.001 in.) and record its average width. Carefully measure the distance between the notch roots on the two sides of the specimen.

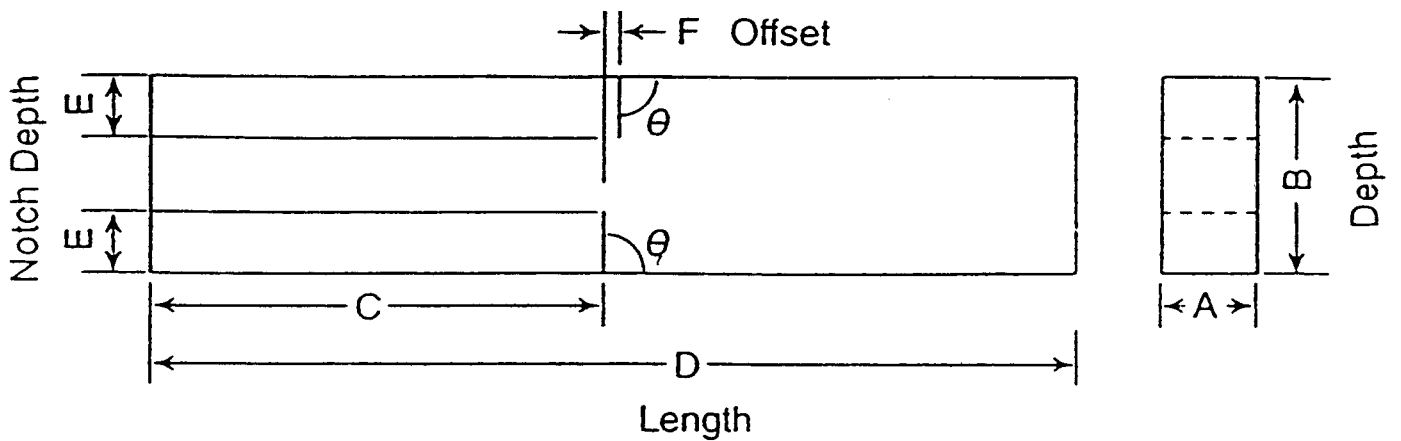

| | mm | | in. |
|---|--------------|---|---------------|
| A | 6.35 ± 0.38 | A | 0.250 ± 0.015 |
| B | 12.70 ± 0.10 | B | 0.500 ± 0.004 |
| C | 31.75 ± 0.25 | C | 1.250 ± 0.010 |
| D | 63.50 ± 0.38 | D | 2.500 ± 0.015 |
| E | 4.57 ± 0.08 | E | 0.180 ± 0.003 |
| F | 0.00 ± 0.13 | F | 0.000 ± 0.005 |
| O | 90° ± 2° | O | 90° ± 2° |

FIG. A1.1 Dimensions of Double Notched Izod Test Specimen

Use of an optical microscope may improve the accuracy of this measurement. Record the average value and multiply this number by the width of the specimen to get the remaining unnotched cross section area, AR. Also record the identifying markings of the specimen.

A1.6.3 Estimate the breaking energy for the specimen and select a pendulum of suitable energy. Start the test with a pendulum of 11 J (8 ft.-lb), if no prior test data is available. Use the lightest standard pendulum that is expected to break each specimen in the group with a loss of not more than 85 % of its energy.

A1.6.4 Before testing the specimens, perform the operations on the machine.

A1.6.4.1 With the excess energy indicating pointer in its normal starting position but without a specimen in the vise, release the pendulum from its normal starting position and note the position the pointer attains after the swing as one reading of Factor A.

A1.6.4.2 Without resetting the pointer, raise the pendulum and release again. The pointer should move up the scale an additional amount. Repeat this procedure until a swing causes no additional movement of the pointer and note the final reading as one reading of Factor B.

A1.6.4.3 Repeat the above two operations several times and calculate and record the average A and B readings.


A1.6.5 Position the specimen precisely and rigidly but not too tightly clamped in the vise. The relationship of the vise, specimen, and striking edge of the pendulum to each other is given in Fig. A1.2. Note that the top plane of the vise shall be 0.13 ± 0.13 mm (0.005 ± 0.005 in.) below the notches.

A1.6.6 Release the pendulum and note and record the excess energy remaining in the pendulum after breaking the specimen.

A1.6.7 From the breaking strength of the specimen and Factors A and B, determine the energy loss of the pendulum due to windage and friction using the correction charts from the commercial testing machine supplier. If these charts are not available, use the method given in Appendix X2 or X3 of Test Method D256. Subtract the correction so calculated from the indicated breaking strength of the specimen. If a pendulum of improper energy was used, discard the result and make additional tests on new specimens with the proper pendulum. If the proper pendulum was used, divide the net value so found by the unnotched area AR of the specimen as measured in A1.6.2 to obtain its double notched Izod impact resistance in kJ/m²(ft.-lb/in.²).

A1.6.8 Record the type of failure for each specimen as one of the three coded categories defined as follows:

A1.6.8.1 *C (Complete Break)*—A break in which the specimen separates into two pieces and the fracture plane contains both lines of the notch roots.

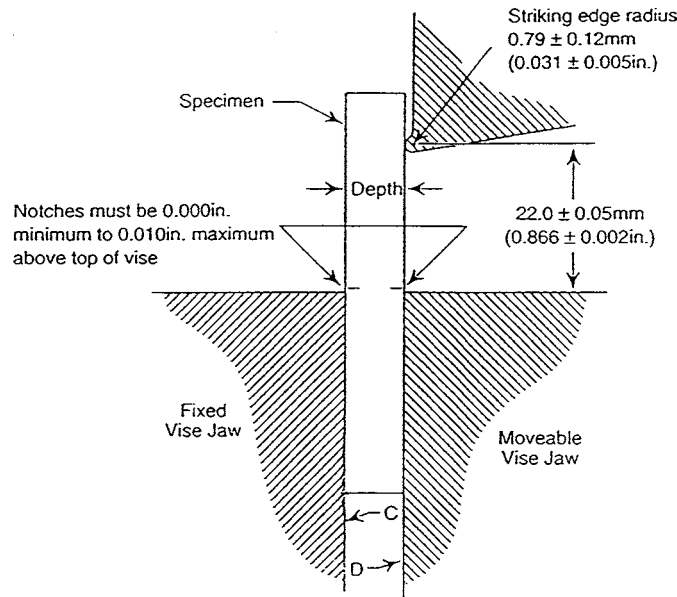

Planes C and D must be parallel to within 0.025mm (0.001in.)
FIG. A1.2 Relationship of Vise, Specimen, and Striking Edge to Each Other

A1.6.8.2 *IB (Irregular Break)*—The specimen separates into two pieces but the fracture plane contains only one of the notch roots.

A1.6.8.3 *NB (Nonbreak)*—A break in which the specimen does not separate into two pieces.

A1.6.9 Calculate the average impact resistance and standard deviation of the group of specimens.

A1.7 Report

A1.7.1 Report the following information:

A1.7.1.1 Complete identification of the material tested, including type, source, and manufacturer's lot number,

A1.7.1.2 Capacity of the pendulum in joules (foot-pounds-force),

A1.7.1.3 Total number of specimens tested,

A1.7.1.4 Average double notched Izod impact resistance in kJ/m^2 (ft-lb/in^2),

A1.7.1.5 Standard deviation, and

A1.7.1.6 Percent of specimens failing in each category suffixed by the corresponding letter code from A1.6.8.

A1.8 Measurement Method of Imperfections in Specimen Notching

A1.8.1 The following is one of the possible test methods to directly measure the imperfections in specimen notching, which can be classified into three kinds: deviation from perpendicularity; incorrect notch depth, and; offset of notches (Fig. A1.3).

A1.8.2 *Apparatus:*

A1.8.2.1 An *Ocular*, 40 to 60 \times , reflective optical microscope with an X-Y stage accurate to 0.0025 mm (0.0001 in.);

A1.8.2.2 An *Eyepiece*, with a crosshair;

A1.8.2.3 *Fiber Optic Illumination*.

A1.8.3 *Procedure:*

A1.8.3.1 Lay the specimen on one of its sides and mount it securely on the X-Y stage.

A1.8.3.2 The beginning and ending points of the notches are labeled from A to D in Fig. A1.3. Select one of the edges of the specimen as the datum line from which the perpendicularity of the notches to the edges is measured (in this case line *AE*). Note that point *E* is approximately 6.35 mm (0.25 in.) from point *A*.

A1.8.3.3 Both the microscope and the base of the X-Y stage should be stationary. Measure the coordinates of points *A* to *E* with respect to an arbitrarily selected coordinate system by moving the X-Y stage and by targeting the points by the crosshair of the eyepiece.

A1.8.4 *Calculation:*

A1.8.4.1 The following equation is used to calculate perpendicularity of the notches:

$$/EAB = \tan^{-1}[(m_2 - m_1)/(1 + m_1 m_2)] \quad (\text{A1.1})$$

where:

m_1 and m_2 are the slopes of line *AE* and *AB* with respect to the coordinate system. m_1 and m_2 are calculated from: