



Designation: D558 – 11

Standard Test Methods for Moisture-Density (Unit Weight) Relations of Soil-Cement Mixtures¹

This standard is issued under the fixed designation D558; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

This standard has been approved for use by agencies of the U.S. Department of Defense.

1. Scope*

1.1 These test methods cover the determination of the relationship between the water content and the density of soil-cement mixtures when compacted before cement hydration as prescribed.

1.2 A $\frac{1}{30}$ -ft³ (944-cm³) mold and a 5.50-lbf (24.5-N or mass of 2.49-kg) rammer dropped from a height of 12.0 in. (30.5 cm) are used and two methods, depending on soil gradation, are covered, as follows:

Test Method A, using soil material passing a No. 4 (4.75-mm) sieve. This method shall be used when 100 % of the soil sample passes the No. 4 (4.75-mm) sieve

Sections

7

Test Method B, using soil material passing a $\frac{3}{4}$ -in. (19.0-mm) sieve. This method shall be used when part of the soil sample is retained on the No. 4 (4.75-mm) sieve. This test method may be used only on materials with 30 % or less retained on the $\frac{3}{4}$ -in. (19.0-mm) sieve

8

1.3 All observed and calculated values shall conform to the guidelines for significant digits and rounding established in Practice D6026.

1.4 The values stated in inch-pound units are to be regarded as standard, except as noted below. The values given in parentheses are mathematical conversions to SI units that are provided for information only and are not considered standard.

1.4.1 The gravitational system of inch-pound units is used when dealing with inch-pound units. In this system, the pound (lbf) represents a unit of force (weight), while the unit for mass is slugs.

1.4.2 The slug unit of mass is almost never used in commercial practice (density, scales, balances, etc.). Therefore, the standard unit for mass in this standard is either kilogram (kg) or gram (g) or both. Also, the equivalent inch-pound unit (slug) is not given.

1.4.3 It is common practice in the engineering/construction profession to concurrently use pounds to represent both a unit

of mass (lbm) and of force (lbf). This implicitly combines two separate systems of units; that is, the absolute system and the gravitational system. It is scientifically undesirable to combine the use of two separate sets of inch-pound units within a single standard. As stated in 1.4.2, this standard includes the gravitational system of inch-pound units and does not use/present the slug unit for mass. However, the use of balances or scales recording pounds of mass (lbm) or recording density in lbm/ft³ shall not be regarded as nonconformance with this standard.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 ASTM Standards:²

- C150 Specification for Portland Cement
- C595 Specification for Blended Hydraulic Cements
- D559 Test Methods for Wetting and Drying Compacted Soil-Cement Mixtures (Withdrawn 2012)³
- D560 Test Methods for Freezing and Thawing Compacted Soil-Cement Mixtures (Withdrawn 2012)³
- D653 Terminology Relating to Soil, Rock, and Contained Fluids
- D698 Test Methods for Laboratory Compaction Characteristics of Soil Using Standard Effort (12 400 ft-lbf/ft³ (600 kN-m/m³))
- D2168 Practices for Calibration of Laboratory Mechanical-Rammer Soil Compactors
- D2216 Test Methods for Laboratory Determination of Water (Moisture) Content of Soil and Rock by Mass
- D3740 Practice for Minimum Requirements for Agencies Engaged in Testing and/or Inspection of Soil and Rock as Used in Engineering Design and Construction

¹ These test methods are under the jurisdiction of ASTM Committee D18 on Soil and Rock and are the direct responsibility of Subcommittee D18.15 on Stabilization With Admixtures.

Current edition approved Jan. 1, 2011. Published February 2011. Originally approved in 1938. Last previous edition approved in 2003 as D558-03. DOI: 10.1520/D0558-11.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ The last approved version of this historical standard is referenced on www.astm.org.

*A Summary of Changes section appears at the end of this standard

D4753 Guide for Evaluating, Selecting, and Specifying Balances and Standard Masses for Use in Soil, Rock, and Construction Materials Testing

D6026 Practice for Using Significant Digits in Geotechnical Data

E11 Specification for Woven Wire Test Sieve Cloth and Test Sieves

E145 Specification for Gravity-Convection and Forced-Ventilation Ovens

3. Terminology

3.1 For common definitions of terms used in this standard, refer to Terminology **D653**.

4. Significance and Use

4.1 These tests determine the optimum water content and maximum density (unit weight) to be used for molding soil-cement specimens in accordance with Test Methods **D559** and **D560**.

NOTE 1—Since these tests are used in conjunction with Test Methods **D559** and **D560** and the criteria referenced therein, the test differs in several aspects from Test Method **D698**. There are three main differences between this standard and Test Method **D698**. Firstly, this standard allows a maximum particle size of $\frac{3}{4}$ -in. (19.0 mm) for a 4-in. (101.6-mm) mold while Test Method **D698** allows a maximum particle size of $\frac{3}{8}$ -in. (9.5-mm) for the same size mold. Secondly, this standard permits the material leftover after the water content specimen has been obtained to be mixed with the rest of the sample and reused for the next determination. Test Method **D698** does not permit the material to be reused. Thirdly, this standard allows the material that is retained on the $\frac{3}{4}$ -in. (19.0-mm) and passing the 3-in. (75-mm) to be discarded (scalping technique) and replaced with an equal mass of material that passes the $\frac{3}{4}$ -in. (19.0-mm) sieve and is retained on the No.4 (4.75-mm) sieve. Test Method **D698** does not permit the scalp and replacement technique.

NOTE 2—The quality of the result produced by this standard is dependent on the competence of the personnel performing it, and the suitability of the equipment and facilities used. Agencies that meet the criteria of Practice **D3740** are generally considered capable of competent and objective testing/sampling/inspection/etc. Users of this standard are cautioned that compliance with Practice **D3740** does not in itself assure reliable results. Reliable results depend on many factors; Practice **D3740** provides a means of evaluating some of those factors.

5. Apparatus

5.1 *Mold*—A cylindrical metal mold having a volume of $\frac{1}{30} \pm 0.00040 \text{ ft}^3$ ($944 \pm 11 \text{ cm}^3$) with an internal diameter of $4.0 \pm 0.016 \text{ in.}$ ($101.60 \pm 0.41 \text{ mm}$) and conforming to **Fig. 1** to permit preparing compacted specimens of soil-cement mixtures of this size. The mold shall be provided with a detachable collar assembly approximately $2\frac{1}{2}$ -in. (63.5 mm) in height. The mold may be of the split type consisting of two half-round sections or section of pipe with one side split perpendicular to the pipe circumference and that can be securely locked in place to form a closed cylinder having the dimensions described above. The mold and collar assembly shall be so constructed that it can be fastened firmly to a detachable base (**Fig. 1**).

5.2 *Rammer*—A rammer, either manually operated as described further in **5.2.1** or mechanically operated as described in **5.2.2**. The rammer shall fall freely through a distance of $12.00 \pm 0.05 \text{ in.}$ ($304.8 \pm 1 \text{ mm}$) from the surface of the specimen. The weight of the rammer shall be $5.50 \pm 0.02 \text{ lbf}$

($24.47 \pm 0.09 \text{ N}$, or mass of $2.495 \pm 0.023 \text{ kg}$), except that the weight of the mechanical rammers may be adjusted as described in Practices **D2168** (See **Note 3**). The striking face of the rammer shall be planar and circular, except as noted in **5.2.2**, with a diameter when new of $2.000 \pm 0.005 \text{ in.}$ ($50.80 \pm 0.13 \text{ mm}$). The rammer shall be replaced if the striking face becomes worn or bellied to the extent that the diameter exceeds $2.000 \pm 0.01 \text{ in.}$ ($50.80 \pm 0.25 \text{ mm}$).

NOTE 3—It is a common and acceptable practice to determine the weight of the rammer using either a kilogram or pound balance and assume 1 lbf is equivalent to 0.4536 kg, 1 lbf is equivalent to 1 lbm, or 1 N is equivalent to 0.2248 lbf or 0.1020 kg.

5.2.1 *Manual Rammer*—The rammer shall be equipped with a guide sleeve that has sufficient clearance that the free fall of the rammer shaft and head is not restricted. The guide sleeve shall have at least four vent holes at each end (eight holes total) located with centers $\frac{3}{4} \pm \frac{1}{16} \text{ in.}$ ($19.0 \pm 2 \text{ mm}$) from each end and spaced 90 degrees apart. The minimum diameter of the vent holes shall be $\frac{3}{8} \text{ in.}$ (9.5 mm). Additional holes or slots may be incorporated in the guide sleeve.

5.2.2 *Mechanical Rammer-Circular Face*—The rammer shall operate mechanically in such a manner as to provide uniform and complete coverage of the specimen surface. There shall be $0.10 \pm 0.03 \text{ in.}$ ($2.5 \pm 0.8 \text{ mm}$) clearance between the rammer and the inside surface of the mold at its smallest diameter. The mechanical rammer shall meet the standardization/calibration requirements of Practices **D2168**. The mechanical rammer shall be equipped with a positive mechanical means to support the rammer when not in operation.

5.2.3 *Mechanical Rammer-Sector Face (See Note 4)*—When used with the 6 in. (152.4 mm) mold, a sector face rammer may be used in place of the circular face rammer. The use of a sector face rammer should be noted in the test report. The specimen contact face shall have the shape of a sector of a circle of radius equal to $2.90 \pm 0.02 \text{ in.}$ ($73.7 \pm 0.5 \text{ mm}$). The rammer shall operate in such a manner that the vertex of the sector is positioned at the center of the specimen.


NOTE 4—The sector face rammer shall not be used to compact test specimens in accordance with Test Methods **D559** and **D560**, unless previous tests on like soils show strength and resistance to wetting-and-drying and freezing-and-thawing of specimens compacted with this rammer are similar to that of specimens compacted with the circular face rammer.

5.3 *Sample Extruder*—A jack, lever frame, or other device adapted for the purpose of extruding compacted specimens from the mold. Not required when a split-type mold is used.

5.4 *Balances*—A balance or scale conforming to the requirements of Class GP5 with a readability of 1g in Specification **D4753**, except that a Class GP2 balance of 0.1g readability is required for water content determination.

5.5 *Drying Oven*—Thermostatically controlled, preferably of the forced-draft type, meeting the requirements of Specification **E145** and capable of maintaining a uniform temperature of $230 \pm 9 \text{ }^\circ\text{F}$ ($110 \pm 5 \text{ }^\circ\text{C}$) throughout the drying chamber.

5.6 *Straightedge*—A stiff steel straightedge of any convenient length but not less than 10-in. (254-mm). The total length

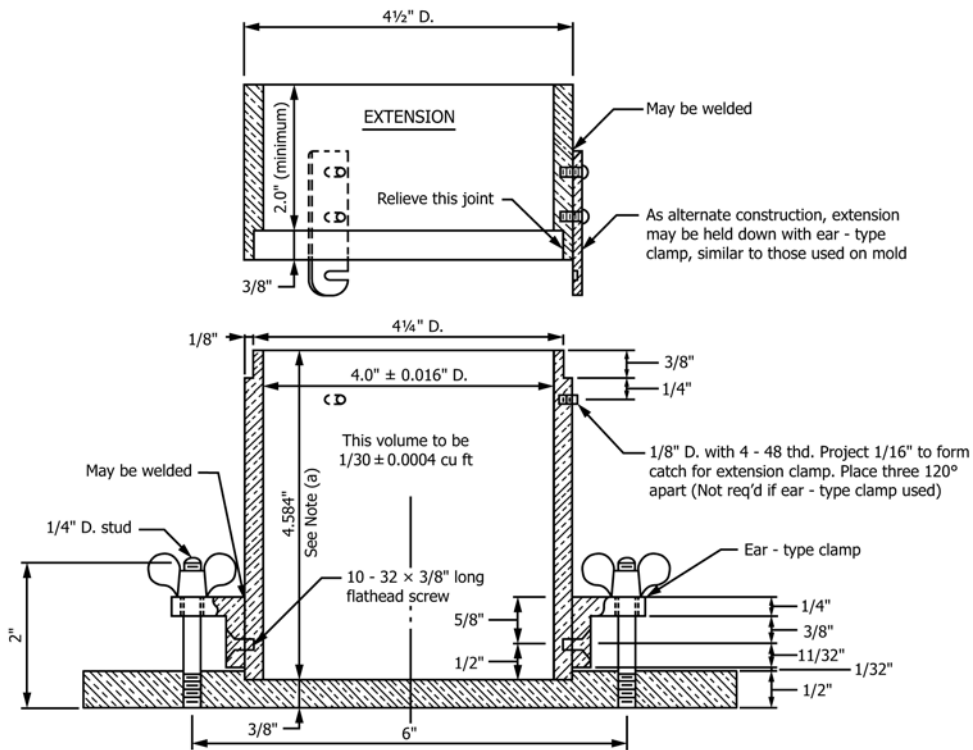

Metric Equivalents

in.	mm
0.016	0.41
0.026	0.66
1/32	0.80
1/16	1.6
1/8	3.2
1/4	6.4
11/32	8.7
3/8	9.5
1/2	12.7
5/8	15.9
2	50.8
2 1/2	63.5
4	101.6
4 1/4	108.0
4 1/2	114.3
4.584	116.43
6	152.4
6 1/2	165.1
8	203.2
ft ³	cm
1/30	944
0.004	11
1/13.333	2124
0.0009	25

NOTE 1—(a)—The tolerance on the height is governed by the allowable volume and diameter tolerances.

NOTE 2—(b)—The methods shown for attaching the extension collar to the mold and the mold to the base plate are recommended. However, other methods are acceptable, providing the attachments are equally as rigid as those shown.

FIG. 1 Cylindrical Mold

of the straightedge shall be machined straight to a tolerance of ± 0.005 -in. (± 0.1 -mm). The scraping edge shall be beveled if it is thicker than 1/8-in. (3-mm).

5.7 Sieves—3-in. (75-mm), 3/4-in. (19.0-mm), and No. 4 (4.75-mm) sieves conforming to the requirements of Specification E11.