

---

---

**Paper and board — Determination  
of roughness/smoothness (air leak  
methods) —**

**Part 4:  
Print-surf method**

**iTeh STANDARD PREVIEW**  
*Papier et carton — Détermination de la rugosité/du lissé (méthodes  
du débit d'air) —  
(standards.iteh.ai)  
Partie 4: Méthode Print-surf*

[ISO 8791-4:2021](https://standards.iteh.ai/catalog/standards/sist/f7b1589b-799e-4012-abcf-fca432457b32/iso-8791-4-2021)

<https://standards.iteh.ai/catalog/standards/sist/f7b1589b-799e-4012-abcf-fca432457b32/iso-8791-4-2021>



## iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO 8791-4:2021](https://standards.iteh.ai/catalog/standards/sist/f7b1589b-799e-4012-abc-fca432457b32/iso-8791-4-2021)

<https://standards.iteh.ai/catalog/standards/sist/f7b1589b-799e-4012-abc-fca432457b32/iso-8791-4-2021>



### **COPYRIGHT PROTECTED DOCUMENT**

© ISO 2021

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva  
Phone: +41 22 749 01 11  
Email: [copyright@iso.org](mailto:copyright@iso.org)  
Website: [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

	Page
Foreword .....	iv
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 Principle</b> .....	<b>1</b>
<b>5 Apparatus</b> .....	<b>2</b>
5.1 Print-surf tester (two types) .....	2
5.2 Principal components of the system .....	3
5.3 Measuring system .....	7
<b>6 Sampling</b> .....	<b>7</b>
<b>7 Condition</b> .....	<b>7</b>
<b>8 Preparation of test pieces</b> .....	<b>7</b>
<b>9 Procedure</b> .....	<b>7</b>
<b>10 Calculation</b> .....	<b>9</b>
<b>11 Precision</b> .....	<b>9</b>
<b>12 Test report</b> .....	<b>9</b>
<b>Annex A Calculation of roughness in micrometres</b> .....	<b>10</b>
<b>Annex B (normative) Maintenance of Print-surf roughness testers</b> .....	<b>12</b>
<b>Annex C (normative) Calibration of variable-area flowmeters</b> .....	<b>14</b>
<b>Annex D (informative) Precision</b> .....	<b>16</b>
<b>Bibliography</b> .....	<b>17</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 6, *Paper, board and pulps*, Subcommittee SC 2, *Test methods and quality specifications for paper and board*.

This third edition cancels and replaces the second edition (ISO 8791-4:2007), which has been technically revised.

The main changes compared to the previous edition are as follows:

- Annex D and Annex E describing the calibration of Print-surf instruments have been removed;
- some minor editorial changes have been made.

A list of all parts in the ISO 8791 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).

# Paper and board — Determination of roughness/ smoothness (air leak methods) —

## Part 4: Print-surf method

### 1 Scope

This document specifies a method for determining the roughness of paper and board using an apparatus which conforms to the Print-surf method, as defined in this document. It is applicable to all printing papers and boards with which it is possible to form a substantially airtight seal against the guard lands of the measuring head.

### 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 186, *Paper and board — Sampling to determine average quality*

ISO 187, *Paper, board and pulps — Standard atmosphere for conditioning and testing and procedure for monitoring the atmosphere and conditioning of samples*

<https://standards.iteh.ai/catalog/standards/sist/f7b1589b-799e-4012-abcf-fca432457b32/iso-8791-4-2021>

### 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

#### 3.1

##### **print-surf roughness**

mean gap between a sheet of paper or board and a flat circular land pressed against it under specified conditions

Note 1 to entry: The mean gap is expressed as the cube root mean cube gap calculated as specified in [Annex A](#). The Print-surf roughness is expressed directly as the average value of roughness, in micrometres.

#### 3.2

##### **print-surf compressibility**

***K***

percentage decrease in surface roughness when measurements are made consecutively at the two standard clamping pressures specified in this document

### 4 Principle

The test piece is placed between a circular flat metal sensing surface and a resilient backing, and inner and outer circular lands form a seal with the test piece. Under the influence of a pressure difference,


air flows across the measuring land between the measuring land and the test piece. The rate of air flow is measured on a variable-area flowmeter, or the pressure difference across the measuring land is compared to the pressure difference across a known impedance. In both cases, the result is expressed as the air gap, in micrometres.

## 5 Apparatus

### 5.1 Print-surf tester (two types)

5.1.1 **Print-surf tester**, which operates according to one of the following principles.

5.1.1.1 **Variable-area flowmeter type**, in which a standard pressure difference is created across the measuring land and the air-flow rate is measured on a variable-area flowmeter. The air-flow rate varies with roughness and the flow rate is converted to roughness, in micrometres. The flow diagram for this type of instrument is shown in [Figure 1](#).

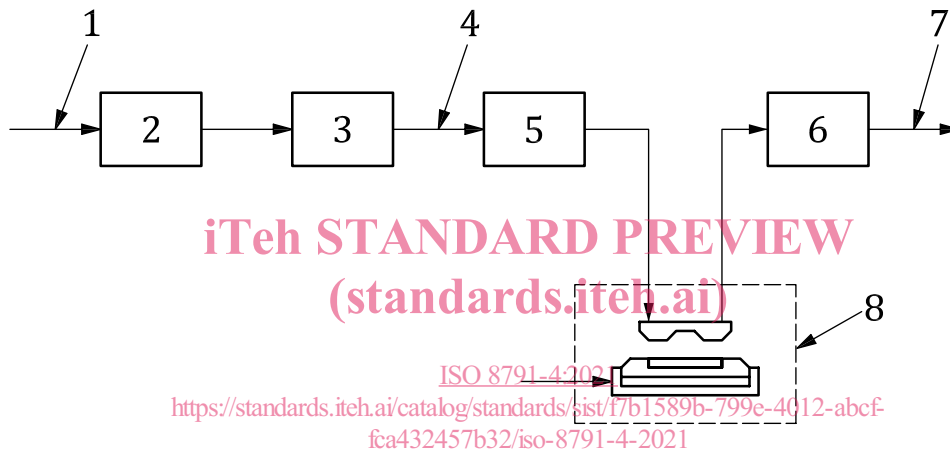


#### Key

- 1 incoming air — 300 kPa to 600 kPa
- 2 filter
- 3 pressure-regulator valve
- 4 6,2 kPa or 19,6 kPa
- 5 on/off valve
- 6 flow indicator tubes
- 7 to atmosphere
- 8 sensing head and clamping device

**Figure 1 — Flow diagram for variable-area flowmeter type**

5.1.1.2 **Impedance type**, in which the air from the controlled pressure source passes first through a fluidic impedance and then through the sensing head, after which it discharges to atmosphere. The pressure differences across the fluidic impedance and across the land are each measured by a

transducer. These pressure differences vary with roughness and the signals are converted to roughness, in micrometres. The flow diagram for this type of instrument is shown in [Figure 2](#).

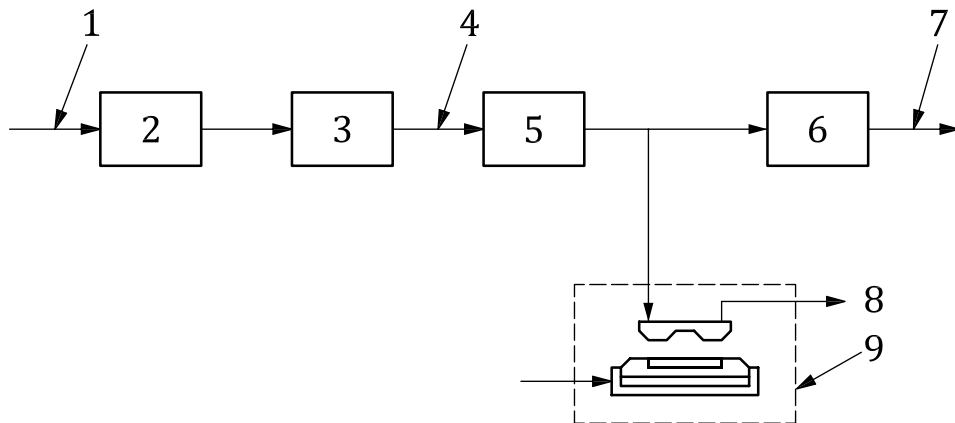

#### Key

- 1 incoming air — 300 kPa to 600 kPa
- 2 filter
- 3 pressure-regulator valve
- 4 19,6 kPa
- 5 fluidic impedance
- 6 pressure transducer
- 7 analogue signal
- 8 to atmosphere
- 9 sensing head and clamping device

**ITeh STANDARD PREVIEW**  
(standards.iteh.ai)  
ISO 8791-4:2021  
<https://standards.iteh.ai/catalog/standards/sist/47b1589b-799e-4012-abcf-1ca432457652/iso-8791-4-2021>  
**Figure 2 — Flow diagram for impedance instrument type**

**5.1.2** The procedures for maintaining these testers in good working order given in [Annex B](#) apply.

## 5.2 Principal components of the system

**5.2.1 Air supply**, in which the air from the controlled pressure source passes first through a fluidic impedance and then through a pressure transducer.


**5.2.2 Sensing-head pressure regulator**, allowing setting of the sensing-head differential pressure to  $19,6 \text{ kPa} \pm 0,1 \text{ kPa}$  or, on variable-area flowmeter instruments only, to either  $6,2 \text{ kPa} \pm 0,1 \text{ kPa}$  or  $19,6 \text{ kPa} \pm 0,1 \text{ kPa}$ .

**5.2.3 Sensing head**, (see [Figures 3](#) and [4](#)), consisting of three concentric, annular lands composed of suitable material which have coplanar, polished surfaces. The centre or measuring land shall be  $51,0 \mu\text{m} \pm 1,5 \mu\text{m}$  wide and have an effective length of  $98,0 \text{ mm} \pm 0,5 \text{ mm}$ . The two guard lands shall each be at least  $1\,000 \mu\text{m}$  wide at any point, and the radial distance between them at any point shall be  $152 \mu\text{m} \pm 10 \mu\text{m}$ . The measuring land shall be centred between them to within  $\pm 10 \mu\text{m}$ .

The lands shall be mounted in an airtight mounting, constructed so that air can be passed into the gap between one guard land and the measuring land, and exhausted from the gap between the measuring land and the other guard land. The back of the mounting shall be flat and form a ground mating surface with the flat surface of a manifold fitted with air inlet and outlet ports.

A spring-loaded protective collar may be fitted outside the guard lands. If such a protective collar is fitted, the force exerted by the loading spring shall be taken into account when setting the clamping pressure.

NOTE In many instruments fitted with the protective collar, the force exerted by the loading spring is 9,8 N.

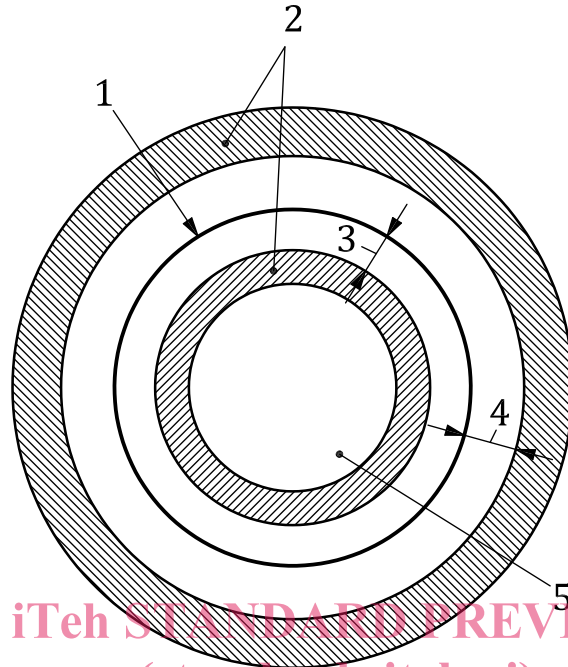


**Key**

- 1 measuring land
- 2 guard lands
- 3 passage air connected to air supply
- 4 passage leading to flowmeters or atmosphere
- 5 fluidic impedance

**Figure 3 — Plan of the measuring and guard lands of the sensing head**

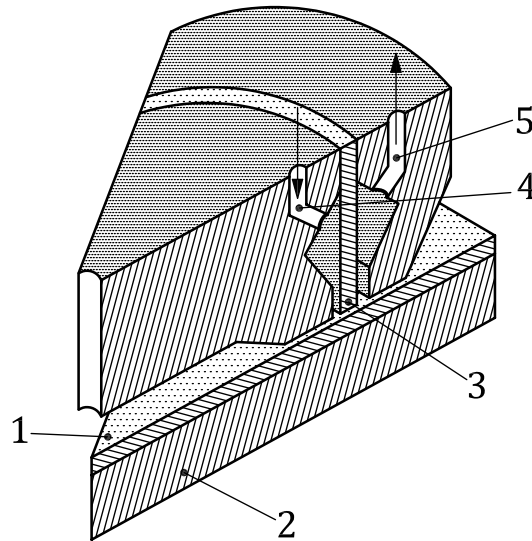

**Key**


- 1 paper
- 2 resilient backing
- 3 measuring land
- 4 regulated low-pressure air
- 5 to flowmeters or atmosphere

ITEN STANDARD PREVIEW

Figure 4 — The sensing head sectioned on two radii

**5.2.4 Backing holders**, consisting of rigid metal discs of known mass, each recessed to accommodate a resilient backing at least 10 mm greater in diameter than the outside diameter of the outer guard land. The mass of both the resilient backing and the holder shall be allowed for in the initial adjustment of the clamping pressure.

It has been observed that high-stiffness papers and boards can interact negatively with the flat metal backing holder and cause erroneously high roughness results. This problem can be solved by using a modified backing holder which relieves those areas of the backing holder not directly below the measuring land, as shown in [Figure 5](#).

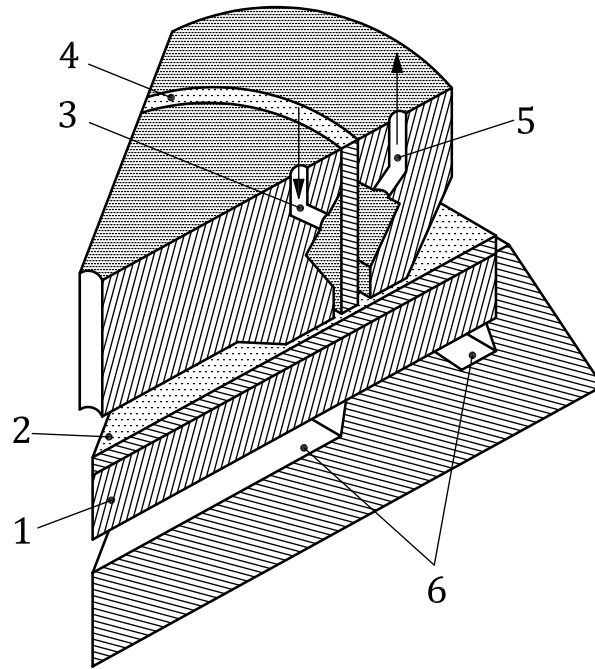

**Key**

- 1 resilient backing
- 2 paper
- 3 regulated low-pressure air
- 4 measuring lands
- 5 to flowmeters or atmosphere
- 6 new modified clamp platen showing machined cut-away

**iTeh STANDARD PREVIEW**  
(standards.iteh.ai)

ISO 8791-4:2021  
<https://standards.iteh.ai/catalog/standards/sist/f7b1589b-799e-4012-abc-fca432457b32/iso-8791-4-2021>

**Figure 5 — The sensing head sectioned on two radii showing cut-away platen**

**5.2.5 Two resilient backings**, of different types, which can be held in the recessed holders by means of double-sided adhesive tape:

**5.2.5.1 Soft backing**, resilient, consisting of an offset printing blanket composed of a layer of synthetic rubber, at least 600 µm thick, bonded to a fabric backing giving an overall thickness of 2 000 µm ± 200 µm. The apparent hardness of the complete backing shall be 83 IRHD ± 6 IRHD (International Rubber Hardness Degrees).

**5.2.5.2 Hard backing**, resilient, usually made from a polyester film bonded at its periphery to cork, offset blanket or similar material. A small exhaust hole shall be provided to prevent air being trapped between the film and the backing. The apparent hardness of the assembly shall be 95 IRHD ± 2 IRHD.

**5.2.6 Clamping mechanism**, allowing clamping of the resilient backing at pressures of either 980 kPa ± 30 kPa or 1960 kPa ± 30 kPa, the pressure being calculated from the total area of the measuring and guard lands.

**NOTE 1** On some earlier instruments, these values can be displayed on the gauge as 10 kgf/cm<sup>2</sup> and 20 kgf/cm<sup>2</sup>.

Note that the spring loading in the protective collar (5.2.3) and the weight of the backing and its holder need to be taken into account. The rate of clamping shall be such that the pressure reaches 90 % of its final value in about 0,4 s, and 99 % of its final value in about 0,8 s.

NOTE 2 A third pressure of 490 kPa (5 kgf/cm<sup>2</sup>) is available on most instruments, but is not acceptable for use with this part document because of a tendency for air to leak under the guard lands.

Variable-area flowmeter measurement systems shall have a pressure gauge fitted to the instrument to indicate the clamping pressure, which shall be adjustable. Impedance measurement systems shall have integrated pneumatic and electronic circuitry which automatically controls the clamping pressure. In each case, the actual pressure achieved shall be verified as specified in B.3.

### 5.3 Measuring system

**5.3.1 The air-flow rate shall be** measured with either a set of variable-area flowmeters or by measuring the pressure drop across an impedance.

**5.3.2 Variable-area flowmeter instruments** shall be fitted with flowmeters which are graduated to show the “cube root mean cube gap” between the paper and the measuring land surface, in micrometres (see Annex A). The flowmeters shall be calibrated by the procedures outlined in Annex C.

**5.3.3 Impedance instruments** measure air leakage by means of fluidic impedance, a pressure transducer and a function generator. They display or print the roughness, in micrometres to the nearest 0,1 µm, based on automatic measurement of pressure difference, over the range 0,6 µm to 6,0 µm. The value displayed shall be the value calculated after 3 s to 5 s.

## 6 Sampling

If the tests are being made to evaluate a lot, the sample should be selected in accordance with ISO 186. If the tests are made on another type of sample, make sure that the test pieces taken are representative of the sample received.

## 7 Condition

The sample shall be conditioned in accordance with ISO 187.

## 8 Preparation of test pieces

Prepare the test pieces in the same atmospheric conditions as those used to condition the sample. Cut at least 10 test pieces for each side to be tested. The size of each test piece shall be 100 mm × 100 mm, and their surfaces shall be identified in some convenient way (for example, side one or side two).

The test area shall be free of all folds, wrinkles, holes or other defects, and should not include watermarks. Do not handle that part of the test piece which will become part of the test area.

## 9 Procedure

**9.1** Carry out the test in the same atmospheric conditions as those used to condition the sample (see Clause 7).

**9.2** Ensure that the instrument is on a rigid horizontal surface free from vibration and that it is level. Before use on any particular day, check the system for leakage as specified in B.1.