



Designation: ~~D4875-05~~ Designation: D4875 - 11

## Standard Test Methods of Polyurethane Raw Materials: Determination of the Polymerized Ethylene Oxide Content of Polyether Polyols<sup>1</sup>

This standard is issued under the fixed designation D4875; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

### 1. Scope\*

1.1 *Test Method A*—Proton Nuclear Magnetic Resonance Spectroscopy ( $^1\text{H}$  NMR) measures polymerized ethylene oxide (EO) in ethylene oxide-propylene oxide polyethers used in flexible urethane foams and nonfoams. It is suitable for diols made from the commonly used initiators and containing EO percentages above five. For triols initiated with glycerin and trimethylol propane, an uncorrected EO value is obtained since both initiators have protons that contribute to the EO measurement.

1.2 *Test Method B*—Carbon-13 Nuclear Magnetic Resonance Spectroscopy ( $^{13}\text{C}$  NMR) measures the polymerized EO content of ethylene oxide-propylene oxide polyethers used in flexible urethane foams and nonfoams. It is suitable for diols and triols made from the commonly used initiators and containing EO percentages above five.  $^{13}\text{C}$  NMR measures the polymerized EO content of ethylene oxide-propylene oxide polyethers used in flexible urethane foams and nonfoams. It is suitable for diols and triols made from the commonly used initiators and containing EO percentages above five.

1.3 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

NOTE 1—There are no equivalent ISO standards.

~~1.3 This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.~~ 1—There is no known ISO equivalent to this standard.

### 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

D883 [Terminology Relating to Plastics](#)

E386 [Practice for Data Presentation Relating to High-Resolution Nuclear Magnetic Resonance \(NMR\) Spectroscopy](#)

E691 [Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method](#)

### 3. Terminology

3.1 *Definitions*—Terminology in these test methods follows the standard terminology defined in Terminology D883 and Practice E386.

3.2 *Definitions of Terms Specific to This Standard:*

3.2.1 *heteric polyol, n*—a polyether polyol in which ethylene oxide and propylene oxide units are randomly arranged.

3.2.2 *initiator, n*—a substance with which ethylene oxide or propylene oxide reacts to form a polyether polyol.

3.2.2.1 *Discussion*—One initiator unit is incorporated into each polymer or oligomer molecule.

3.2.3 *EO capped polyol*—a polyol that contains a terminal block of ethylene oxide units

### 4. Summary of Test Methods

4.1 *Test Method A*—The  $^1\text{H}$  NMR spectra of polyether polyols show two groups of resonance peaks corresponding to the methyl protons of propylene oxide (PO) and to the methylene and methine protons of EO and PO. The EO peak area is obtained by

<sup>1</sup> These test methods are under the jurisdiction of ASTM Committee D20 on Plastics and is the direct responsibility of Subcommittee D20.22 on Cellular Plastics. Current edition approved July 1, 2005. Published August 2005. Originally approved in 1988. Last previous edition approved in 1999 as D4875-99. DOI: 10.1520/D4875-05 on Cellular Materials - Plastics and Elastomers.

Current edition approved April 1, 2011. Published April 2011. Originally approved in 1988. Last previous edition approved in 2005 as D4875-05. DOI: 10.1520/D4875-11.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

\*A Summary of Changes section appears at the end of this standard.

subtracting the area of the PO methyl peaks from the area of the methylene and methine peaks. Initiators other than glycols of EO and PO give systematic errors (see Note 2).

NOTE 2—The initiator error can be estimated by calculating the theoretical contribution of initiator protons to the EO and PO peak areas.

4.2 *Test Method B*—The  $^{13}\text{C}$  NMR spectra of polyether polyols contain multiple resonances arising from initiator, alkoxide, alkoxide-EO, PO, EO/PO, sequencing, and end-group distribution. EO content can be determined relative to PO or relative to PO and triol initiator. In the former, the area of the EO peaks is ratioed to the total area of alkoxide-PO methylene and methine carbons. In the latter, the area of the EO peaks is ratioed to the total area of alkoxide-PO methylene and methine carbons and two initiator carbons. This test method describes the determination of EO relative to PO only.

## 5. Significance and Use

5.1 Measurements of EO content correlate with polyol reactivity (as related to primary hydroxyl content), linearity of foam rise, and the hydrophilicity of the polyol and final product.

5.2 ~~Statistical data suggest that the~~ Statistical data suggest that the  $^{13}\text{C}$  NMR test method is the preferred method for measuring low levels (less than 10 %) of polymerized EO in polyols.

5.3 ~~The~~ The  $^1\text{H}$  and  $^{13}\text{C}$  NMR test methods give different results which are highly correlated. The equation of the linear regression is:

$$\%EO_{\text{proton}} = 1.031 (\%EO_{\text{carbon-13}}) + 0.883 \quad (1)$$

The standard deviation of the regression is 0.49 and the multiple R-square is 0.9990.

## TEST METHOD A—HYDROGEN-1 NMR

## 6. Equipment

6.1 *NMR Continuous Wave (CW) or Fourier Transform (FT) Spectrometer*, with an  $^1\text{H}$  resonance frequency of 60 MHz or higher.

6.2 *NMR Sample Tubes*, having an outside diameter of at least 5 mm.

## 7. Reagents and Materials

7.1 *All* reagents are to be ACS-certified or spectroscopic grade unless otherwise specified.

7.2 *Trifluoroacetic Acid*.

7.3 *Chloroform- $d_1$* , NMR-grade, containing tetramethylsilane as an internal standard.

## 8. Standard

8.1 ~~This~~ This test method does not require standards. To evaluate the test method, standards can be prepared from commercially available poly(propylene oxide) and poly(ethylene oxide).

## 9. Preparation of Sample

9.1 Mix a few drops of polyol with deuterated chloroform to prepare 1 mL of an approximately 10 %<sup>3</sup> polyol solution. Add a drop of trifluoroacetic acid, mix well, and transfer to an NMR tube.

## 10. Instrument Preparation

10.1 ~~The~~ The instrument settings given here are for a Varian EM-390 CW spectrometer, a Varian XL-100 FT spectrometer, and a Bruker AC 300 FT spectrometer. Instrument preparation can vary with the spectrometer. For a description of a particular spectrometer and suitable parameters, refer to the manufacturer's operating manual.

10.2 Typical Varian EM-390 console settings are as follows:

Lock	optional, TMS
Offset	0
Sweep width	5 ppm
Sweep time	2 min
Integration time	2 min
Rf Filter	open
RF power	0.05 mG

10.3 ~~Typical~~ Typical XL-100 console settings are as follows:

10.3 Typical Varian XL-100 console settings are as follows:

Lock	chloroform- $d_1$
------	-------------------

<sup>3</sup> Highfield, FT spectrometers require less concentrated solutions. A 1 % solution is more appropriate for such spectrometers.

Pulse angle	90°
Pulse delay	0
Spectral width	10 ppm
Acquisition time	4 s
Data points	8K
Number of transients	128

10.4 Typical Bruker 300 MHz console settings are as follows:

Lock	chloroform-d-1
Pulse angle	90°
Pulse delay	5 s
Spectral width	10 ppm
Acquisition time	5.3 s
Data points	32K
Number of transients	64

**11. NMR Analysis**

11.1 Place the NMR tube containing the polyol solution into the spectrometer probe and optimize the field homogeneity. For CW NMR, scan the spectrum from 5 to 0 ppm. Integrate the spectrum five times at a power level below that which causes saturation. See Figs. 1 and 2 for examples of polyol spectra with high and low EO concentrations, respectively.

11.2 For FT NMR, acquire the desired number of transients and transform the free induction decay signal to the frequency domain spectrum. Integrate the peaks as shown in Figs. 1 and 2.

11.3 Chemical shifts for the PO methyl proton resonances (area A) range from about 0.6-1.6 ppm and chemical shifts for the EO and PO methylene and methine proton resonances (area B) range from about 2.8-4.0 ppm

**12. Calculation**

12.1 Determine the areas of the PO methyl protons (area A) and the EO and PO methylene and methine protons (area B) from the integrals. Calculate the weight percent EO from the following equation:

$$EO = \frac{33 \times Z}{33 \times Z + 58} \times 100 \tag{2}$$

where:

$$Z = (B/A) - 1$$

33 = g EO/mole after weighting for the number of EO protons vs. PO protons, and

58 = g PO/mole.

**13. Report**

13.1 Report results to the nearest tenth percent EO.

**14. Precision and Bias**

14.1 Table 1 is based on a round robin conducted in 1981 in accordance with Practice E691, involving six polyol samples with EO content ranging from 6 to 45 weight % (see Table 2) tested by eight laboratories. For each polyol, all of the samples were

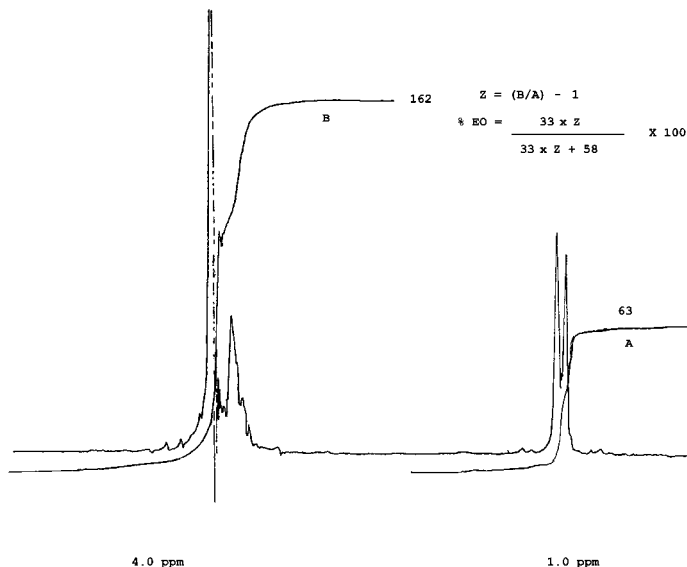


FIG. 1 <sup>1</sup>H NMR Spectrum of a Polyol Containing 45 % EO

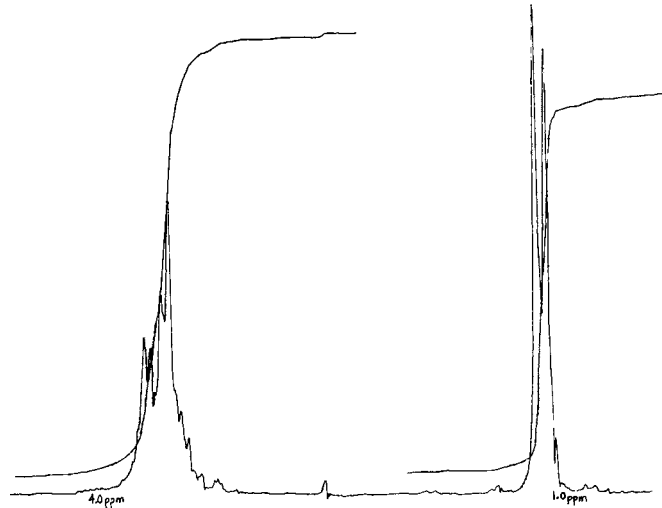


FIG. 2 <sup>1</sup>H NMR Spectrum of a Polyol Containing 8 % EO Uncorrected for Glycerin Initiator

TABLE 1 <sup>1</sup>H Method, % EO Content, for Eight Laboratories, Six Polyols

Sample	Mean	$S_r$	$S_R$	$I_r$	$I_R$
1	10.85	0.3207	1.045	0.898	2.926
2	16.40	0.3951	1.086	1.106	3.041
3	46.05	1.009	1.680	2.825	4.704
4	7.97	0.6809	1.557	1.907	4.360
5	13.61	0.5831	1.225	1.641	3.430
6	24.64	0.4496	0.5573	1.259	1.560

TABLE 2 Description of Samples Analyzed

Sample	Approximate Molecular Weight	Nominal Functionality	Polymerized EO Distribution	Approximate Weight, % EO
1	4000	diol	cap	10
2	2800	diol	cap	15
3	4000	diol	random/cap	45
4	3000	triol	random	6
5	3200	triol	random	10
6	6500	triol	cap	24

prepared at one source, but the individual specimens were prepared at the laboratories that tested them. Each test result was obtained from one individual NMR run. Each lab obtained two test results for each material on two separate days.

14.2 In Table 1, for the polyols indicated and for test results that are derived from testing two specimens of each polyol on each of two separate days:

14.2.1  $S_r$  is the within-laboratory standard deviation of the average;  $I_r = 2.83 S_r$  (see 14.2.3 for application of  $I_r$ ).

14.2.2  $S_R$  is the between-laboratory standard deviation of the average;  $I_R = 2.83 S_R$  (see 14.2.4 for application of  $I_R$ ).

14.2.3 *Repeatability*—In comparing two test results for the same polyol, obtained by the same operator using the same equipment on the same day, those test results are to be judged not equivalent if they differ by more than the  $I_r$  value for that polyol and condition.

14.2.4 *Reproducibility*—In comparing two test results for the same polyol, obtained by different operators using different equipment on different days, those test results are to be judged not equivalent if they differ by more than the  $I_R$  value for that polyol and condition. (This applies between different laboratories or between equipment within the same laboratory.)

14.2.5 Any judgment in accordance with 14.2.3 and 14.2.4 will have an approximate 95 % (0.95) probability of being correct.

14.2.6 Other polyols can give somewhat different results.

14.3 For further information on the methodology used in this section see Practice E691.

14.4 There are no recognized standards on which to base an estimate of bias for this test method.

14.5 Six CW spectrometers (60 and 90 MHz) were used in this study and two FT instruments (100 MHz). The participating companies were Dow, Union Carbide, Mobay, Texaco, Olin, Arco, and Upjohn.