

ISO/TC 229

Secretariat: BSI

Voting begins on:
2023-04-14

Voting terminates on:
2023-06-09

Nanotechnologies — Multiwall carbon nanotubes — Determination of carbon impurity content by thermogravimetric analysis

*Nanotechnologies – Nanotubes de carbone multicouches –
Détermination de la teneur en impureté de carbone par analyse
thermogravimétrique*

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO/DTS 23690

<https://standards.iteh.ai/catalog/standards/sist/03c4a4bc-4234-479b-b65e-153c8cb449af/iso-dts-23690>

RECIPIENTS OF THIS DRAFT ARE INVITED TO SUBMIT, WITH THEIR COMMENTS, NOTIFICATION OF ANY RELEVANT PATENT RIGHTS OF WHICH THEY ARE AWARE AND TO PROVIDE SUPPORTING DOCUMENTATION.

IN ADDITION TO THEIR EVALUATION AS BEING ACCEPTABLE FOR INDUSTRIAL, TECHNOLOGICAL, COMMERCIAL AND USER PURPOSES, DRAFT INTERNATIONAL STANDARDS MAY ON OCCASION HAVE TO BE CONSIDERED IN THE LIGHT OF THEIR POTENTIAL TO BECOME STANDARDS TO WHICH REFERENCE MAY BE MADE IN NATIONAL REGULATIONS.



Reference number
ISO/DTS 23690:2023(E)

iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO/DTS 23690

<https://standards.iteh.ai/catalog/standards/sist/03c4a4bc-4234-479b-b65e-153c8cb449af/iso-dts-23690>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2023

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms, definitions and abbreviated terms	1
3.1 Terms and definitions.....	1
3.2 Symbols.....	2
3.3 Abbreviated terms.....	2
4 Principle	2
5 Sample preparation	3
6 Measurement	3
6.1 Apparatus.....	3
6.1.1 Thermogravimetric analyser.....	3
6.1.2 Drying furnace.....	3
6.1.3 Analytical balance.....	3
6.1.4 Desiccator.....	3
6.2 Reagents.....	3
6.2.1 Inert gas.....	3
6.2.2 Carbon dioxide.....	3
6.3 Measurement procedures.....	3
7 Data analysis and interpretation of results	4
8 Measurement uncertainty	5
8.1 Type A uncertainty.....	5
8.2 Type B uncertainty.....	5
9 Test report	5
Annex A (informative) Repeatability test: Case study	7
Annex B (informative) Reproducibility test: Case study	18
Annex C (informative) Detailed procedures for the analysis of the TG curve	24
Bibliography	26

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO document should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

ISO draws attention to the possibility that the implementation of this document may involve the use of (a) patent(s). ISO takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, ISO had not received notice of (a) patent(s) which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at www.iso.org/patents. ISO shall not be held responsible for identifying any or all such patent rights.

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 229, *Nanotechnologies*.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

Multiwall carbon nanotubes (MWCNTs) are quasi-one-dimensional tubular carbon nanomaterials rolled up or coaxial nested by three or more graphene sheets. The production of carbon nanotubes (CNT) generally contains significant amounts of carbon impurities (carbon material content not in the form of CNT, include amorphous carbon and trace amount of other types of structured carbon), which influence the physical and chemical properties of the nanomaterial. Therefore, the measurement of carbon impurities content in MWCNT samples is highly desired for the determination of its purity.

Several methods have been reported to characterize carbon impurities in MWCNT samples, including transmission electron microscopy (TEM), temperature programmed oxidation (TPO) and thermogravimetric analysis (TGA), etc., among which TGA can provide quantitative results.^{[1][2][3][4][5][6]} This technique takes use of the fact that MWCNTs are more stable than the majority of carbon impurities, so carbon impurities less stable than MWCNTs will react firstly with carbon dioxide in carbon dioxide atmosphere. The oxidation of carbon impurities with carbon dioxide is an endothermal process, which prevents overheating in certain area and restrains the reaction of MWCNTs at the same time. Therefore, the separation of oxidation of carbon impurities and that of MWCNTs are enhanced,^{[7][8][9][10]} allowing the amount of carbon impurities less stable than MWCNTs to be calculated from the mass loss in thermogravimetric analysis.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[ISO/DTS 23690](https://standards.iteh.ai/catalog/standards/sist/03c4a4bc-4234-479b-b65e-153c8cb449af/iso-dts-23690)

<https://standards.iteh.ai/catalog/standards/sist/03c4a4bc-4234-479b-b65e-153c8cb449af/iso-dts-23690>

Nanotechnologies — Multiwall carbon nanotubes — Determination of carbon impurity content by thermogravimetric analysis

1 Scope

This document specifies a mild oxidation method to determine the content of carbon impurities (carbon material content not in the form of CNT, include amorphous carbon and trace amount of other types of structured carbon) less stable than multiwall carbon nanotube (MWCNT) by thermogravimetric analysis (TGA) under carbon dioxide atmosphere.

This document is applicable to the characterization of carbon impurities content in MWCNT samples prepared by chemical vapour deposition (CVD). Measurement of carbon impurities in MWCNT samples prepared by other method can refer to this document. This method is not applicable to functionalized MWCNT samples or MWCNT samples with encapsulant species.

NOTE This method is applicable for the case of TG curve with a single-stage.

2 Normative references

There are no normative references in this document.

3 Terms, definitions and abbreviated terms

3.1 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

3.1.1

multiwall carbon nanotube

MWCNT

multi-walled carbon nanotube

carbon nanotube composed of nested, concentric or near-concentric graphene layers with interlayer distances similar to those of graphite

Note 1 to entry: The structure is normally considered to be many single-walled carbon nanotubes nesting each other and would be cylindrical for small diameters but tends to have a polygonal cross-section as the diameter increases.

[SOURCE: ISO/TS 80004-3:2020, 3.3.6^[11]]

3.1.2

amorphous carbon

carbon material without long-range crystalline order

[SOURCE: IUPAC, Compendium of Chemical Terminology^[12]]

3.2 Symbols

T_0	temperature of the peak on DTG curve (°C)
w_{300}	mass percentage (%) of the sample at 300 °C
w_e	mass percentage (%) of the sample at temperature T_e
ΔH	is the enthalpy change


3.3 Abbreviated terms

CO ₂	carbon dioxide
CVD	chemical vapour deposition
DTG	derivative thermogravimetric
MWCNT	multiwall carbon nanotube
TG	thermogravimetric
TGA	thermogravimetric analysis

4 Principle

Thermogravimetric analysis measures the change in mass of a material as a function of temperature. In order to accomplish this, TGA requires the precise measurements of mass, temperature and temperature change. The change in mass of a material relates to change in composition and structure of the material. Observed mass changes with temperature increases may result from the removal of absorbed moisture, solvent residues, chemically bound moieties and/or the thermal or oxidative decomposition of product.^[13] Experiment carries out in an inert or oxidising atmosphere. The recorded mass change as a function of temperature is a thermogravimetric (TG) curve. Mass change and the extent of this changes of a material in TG curve are indicators of the thermal stability of the material.^[14] Derivative thermogravimetric (DTG) curve is a display of the first derivative of thermogravimetry data with respect to temperature or time^[15].

The method specified in this document based on different reactivity of MWCNTs and carbon impurities under carbon dioxide (CO₂) atmosphere during heating. Carbon dioxide works as mild oxidant to first oxidize carbon impurities less stable than MWCNTs. Moreover, the reaction between carbon impurities and CO₂ absorbs heat from environment,^{[7][8][9]} which prevents local overheating, and thus enhance the separation of carbon impurities and MWCNTs. The amount of carbon impurities in MWCNT samples can be calculated from the mass loss in thermogravimetric analyser. See the reaction formula below.



where

$C_{(s)}$ is the carbon impurities in solid state;

CO_{2(g)} is the carbon dioxide in gaseous state;

CO_(g) is the carbon monoxide in gaseous state;

ΔH is the enthalpy change

5 Sample preparation

MWCNT sample should be of good quality. MWCNT sample is first placed in a thermostatic vacuum drying furnace for 2 h at 150 °C to remove unwanted volatile components.^[16] Then the sample is transferred to a desiccator to cool down to room temperature and it is stored there until used.

6 Measurement

6.1 Apparatus

6.1.1 Thermogravimetric analyser

Thermogravimetric analyser should consist of a furnace, which is capable of heating from room temperature to 1 000 °C or above. Heating rate during experiment should be controlled by temperature programme set in software^[14].

The linear heating rate should be controllable in the range from 1 °C min⁻¹ to 50 °C min⁻¹. The balance sensitivity should be at least 1 µg, and the temperature controller sensitivity less than or equal to 0,01 °C.

A crucible should be used as a sample container. The crucible is generally made of alumina, platinum, quartz or other materials, which does not change or react under the measurement conditions.

6.1.2 Drying furnace

A drying furnace capable of being controlled heating to 150 °C or above is used.

6.1.3 Analytical balance

An analytical balance capable of weighing 0,1 mg or lower is used.

6.1.4 Desiccator

A desiccator containing a desiccant such as dried silica gel impregnated with cobalt chloride is used. The drying agent shall not react with MWCNT samples.

6.2 Reagents

6.2.1 Inert gas

Dry, commercially available inert gas, such as nitrogen gas or argon gas, with minimum volume fraction of 99,999 % should be used in the measurement.

6.2.2 Carbon dioxide

Dry, commercially available carbon dioxide gas with minimum volume fraction of 99,999 % should be used in the measurement.

6.3 Measurement procedures

The thermogravimetric analyser should calibrate according to the manufacturer's protocol to ensure proper temperature and mass measurement.


- a) Turn on the thermogravimetric analyser and wait until equilibrium reaches. Then inert gas and carbon dioxide gas are introduced.

- b) Obtain a baseline correction file using empty crucibles at the same experiment condition. Specifically, set the flow rate of gas to the furnace according to the instrument type. The recommended inert gas flow is 10 ml min⁻¹ to 20 ml min⁻¹ and carbon dioxide gas flow is 20 ml min⁻¹ to 40 ml min⁻¹; set the heating rate as 10 °C min⁻¹ within the temperature range from room temperature to 1 000 °C.
- c) Weigh an appropriate amount of MWCNT sample (3 mg to 5 mg) using an analytical balance and transfer the sample into the crucible.
- d) Before starting the measurement, keep MWCNT sample in a closed thermogravimetric analyser under a gas flow for at least 15 min and wait until the signal (mass, temperature, gas flow) is stable.
- e) Test the sample under the same conditions as in b). Thermogravimetric analyser will automatically record the mass change of MWCNT sample with temperature.

Repeat the measurement at least three times for one MWCNT sample.

7 Data analysis and interpretation of results

TG and DTG curves of one MWCNT sample are shown in [Figure 1](#).

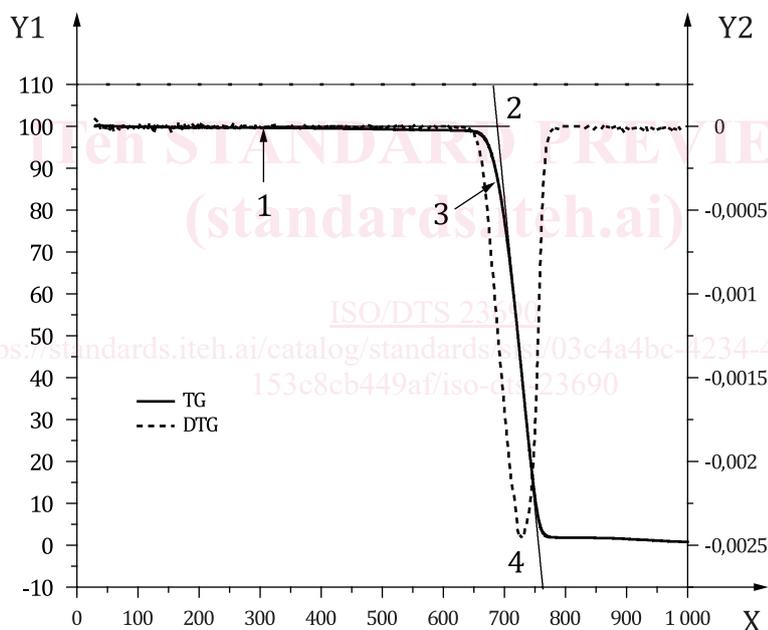

Key

- X temperature (°C)
- Y₁ mass percentage (%)
- Y₂ derivative mass percentage (%/°C)
- 1 mass percentage of the MWCNT sample at 300 °C, w_{300} (%)
- 2 extrapolated initial temperature of MWCNT component oxidation in one MWCNT sample, T_e (°C)
- 3 mass percentage of the sample at T_e , w_e (%)
- 4 temperature of the peak on DTG curve, T_o (°C)

Figure 1 — TG and DTG curves of one MWCNT sample

The mass loss below 300 °C is due to the loss of volatile components^[16].

T_e is the intersection point between the base line and the tangent line at the maximum mass loss rate point, where the maximum mass loss rate point is provided in DTG curve and the tangent line is obtained by ordinary analysis software.

Calculate the content of carbon impurities in MWCNT sample by [Formula \(1\)](#),

$$w = W_{300} - W_e \quad (1)$$

where w is the mass percentage (%) of the carbon impurities.

Conduct three independent TGA measurements for one MWCNT sample. The three measurements results are referred as w_1 , w_2 and w_3 , respectively. Calculate mass percentage of carbon impurities in MWCNT sample according to [Formula \(1\)](#). Calculate the average value of the three measurements by [Formula \(2\)](#):

$$\bar{w} = \frac{w_1 + w_2 + w_3}{3} \quad (2)$$

where \bar{w} is the average mass percentage (%) of the carbon impurities in one MWCNT sample.

[Annex A](#) and [Annex B](#) provides the case studies of repeatability and reproducibility, respectively. [Annex C](#) provides the detail procedures for the analysis of the TG curve.

NOTE This method is applicable for the case of a TG curve with a single-stage.

Sample homogeneity should be considered. The homogeneity of MWCNT samples can be evaluated by the constituency, thermal stability and scatter in the oxidation temperature and the residual material content in several separate TGA runs.^[13] Errors in result calculation can be introduced if the sample is non-homogeneous.

8 Measurement uncertainty

8.1 Type A uncertainty

8.1.1 The uncertainty introduced by measuring method, such as measurement precision, and method bias. It is calculated by measuring repetitive standard deviation of the reference material, which is used for instrument calibration.

8.1.2 The uncertainty introduced by measuring sample, such as the uniformity of samples, weighing, drying and gridding. It is calculated by measuring repetitive standard deviation of the sample.

8.2 Type B uncertainty

The uncertainty is introduced by instrument calibration, such as mass calibration, and temperature calibration^[15].

9 Test report

The test report shall include the following information:

- a) refer to this document (i.e. ISO/TS 23690:XXXX);
- b) sample type and name;
- c) tester and the date;
- d) organization, contact address and telephone number;
- e) type of thermogravimetric analyser and model;
- f) test conditions, including crucible type, atmosphere, gas flow, sample mass, temperature range and heating rate;

- g) test results, including the TG and DTG curves, data and calculated content of carbon impurities in MWCNT sample;
- h) any deviations from the procedure;
- i) any unusual features observed;
- j) the date of the test.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO/DTS 23690

<https://standards.iteh.ai/catalog/standards/sist/03c4a4bc-4234-479b-b65e-153c8cb449af/iso-dts-23690>