
**Fine ceramics (advanced ceramics,
advanced technical ceramics) —
Methods for chemical analysis of
zirconium oxide powders**

*Céramiques techniques — Méthodes pour l'analyse chimique des
poudres d'oxyde de zirconium*

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

[ISO 23739:2021](#)

<https://standards.iteh.ai/catalog/standards/iso/89908206-a6a5-44de-922f-1840cddddcab/iso-23739-2021>



Reference number
ISO 23739:2021(E)

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

[ISO 23739:2021](#)

<https://standards.iteh.ai/catalog/standards/iso/89908206-a6a5-44de-922f-1840cddddcab/iso-23739-2021>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2021

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

Page

Foreword	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Analytes and ranges	1
5 Preparation of the test sample	2
5.1 General	2
5.2 Sampling	2
5.3 Drying	2
5.4 Weighing	2
6 Reporting the analytical values	2
6.1 Number of analyses	2
6.2 Blank test	2
6.3 Evaluation of the analytical values	2
6.4 Expression of analytical values	3
7 Decomposition of the test sample	3
7.1 Classification of the sample decomposition methods	3
7.2 Acid pressure decomposition	3
7.2.1 Reagents	3
7.2.2 Apparatus and instruments	3
7.2.3 Procedure	4
7.2.4 Blank test	4
7.3 Alkali fusion	5
7.3.1 Reagents	5
7.3.2 Apparatus and instruments	5
7.3.3 Procedure	5
7.3.4 Blank test	5
8 Determination of the zirconium content	6
8.1 Precipitation and gravimetric method	6
8.1.1 Principle	6
8.1.2 Reagents	6
8.1.3 Apparatus and instruments	6
8.1.4 Procedure	6
8.1.5 Blank test	7
8.1.6 Calculation	7
8.2 ICP-OES method	7
8.2.1 Principle	7
8.2.2 Reagents	7
8.2.3 Apparatus and instruments	7
8.2.4 Procedure	7
8.2.5 Blank test	8
8.2.6 Drawing of calibration curve	8
8.2.7 Calculation	8
9 Determination of the major elements contents	8
9.1 Precipitation and gravimetric method (for yttrium)	8
9.1.1 Principle	8
9.1.2 Reagents	8
9.1.3 Apparatus and instruments	8
9.1.4 Procedure	9
9.1.5 Blank test	9
9.1.6 Calculation	9

9.2	ICP–OES method (for calcium, hafnium, magnesium and yttrium)	9
9.2.1	Principle	9
9.2.2	Reagents	9
9.2.3	Apparatus and instruments	10
9.2.4	Procedure	10
9.2.5	Blank test	10
9.2.6	Drawing of calibration curve	10
9.2.7	Calculation	11
10	Determination of the trace elements contents	11
10.1	Principle	11
10.2	Reagents	11
10.2.1	Elemental standard solution	11
10.2.2	Mixed standard solution (each element 50 mg/l)	12
10.3	Apparatus and instruments	12
10.4	Procedure	12
10.5	Blank test	13
10.6	Drawing of the calibration curve	13
10.7	Calculation	13
11	Test report	14
Annex A (informative) Analytical results obtained from the interlaboratory test		15
Bibliography		16

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

[ISO 23739:2021](#)

<https://standards.iteh.ai/catalog/standards/iso/89908206-a6a5-44de-922f-1840cddddcab/iso-23739-2021>

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 206, *Fine ceramics*.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

[ISO 23739:2021](http://www.iso.org/iso/23739:2021)

<https://standards.iteh.ai/catalog/standards/iso/89908206-a6a5-44de-922f-1840cddddcab/iso-23739-2021>

Fine ceramics (advanced ceramics, advanced technical ceramics) — Methods for chemical analysis of zirconium oxide powders

1 Scope

This document specifies methods for the chemical analysis of zirconium oxide powders used as the raw material for fine ceramics.

It stipulates the determination methods of the zirconium, aluminium, barium, calcium, cerium, cobalt, gadolinium, hafnium, iron, magnesium, potassium, silicon, sodium, strontium, titanium and yttrium contents in zirconium oxide powders for fine ceramics. The test sample is decomposed by acid pressure decomposition or alkali fusion. Contents of zirconium and yttrium are determined by using either a precipitation and gravimetric method or an inductively coupled plasma-optical emission spectrometry (ICP-OES) method. Contents of aluminium, barium, calcium, cerium, cobalt, gadolinium, hafnium, iron, magnesium, potassium, silicon, sodium, strontium and titanium are determined by using an ICP-OES method.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 835, *Laboratory glassware — Graduated pipettes*

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 8656-1, *Refractory products — Sampling of raw materials and unshaped products — Part 1: Sampling scheme*

3 Terms and definitions

No terms and definitions are listed in this document.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

4 Analytes and ranges

- Zirconium (Zr), range of 60 % to 74 % (mass fraction).
- Aluminium (Al), range of 0,01 % to 0,5 % (mass fraction).
- Barium (Ba), range of 0,01 % to 0,5 % (mass fraction).
- Calcium (Ca), range of 0,01 % to 6 % (mass fraction).
- Cerium (Ce), range of 0,01 % to 0,5 % (mass fraction).
- Cobalt (Co), range of 0,01 % to 0,5 % (mass fraction).

- Gadolinium (Gd), range of 0,01 % to 0,5 % (mass fraction).
- Hafnium (Hf), range of 0,01 % to 2 % (mass fraction).
- Iron (Fe), range of 0,01 % to 0,5 % (mass fraction).
- Magnesium (Mg), range of 0,01 % to 6 % (mass fraction).
- Potassium (K), range of 0,01 % to 0,5 % (mass fraction).
- Sodium (Na), range of 0,01 % to 0,5 % (mass fraction).
- Silicon (Si), range of 0,01 % to 0,5 % (mass fraction).
- Strontium (Sr), range of 0,01 % to 0,5 % (mass fraction).
- Titanium (Ti), range of 0,01 % to 0,5 % (mass fraction).
- Yttrium (Y), range of 0,01 % to 15 % (mass fraction).

5 Preparation of the test sample

5.1 General

The sample preparation method shall be in accordance with ISO 8656-1, unless otherwise mutually agreed upon by the analyser and customer.

5.2 Sampling

(<https://standards.iteh.ai>)

The sample shall be collected in accordance with ISO 8656-1.

5.3 Drying

Place 10 g of the sample into a flat-type weighing bottle (60 mm × 30 mm) and spread it uniformly over the bottom of the bottle. Place the bottle in an air bath at $110\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ for 2 h, uncovered, and cool in a desiccator, covered, for 1 h.

5.4 Weighing

Weigh the test sample to the nearest 0,1 mg of the required quantity using a balance.

6 Reporting the analytical values

6.1 Number of analyses

Analyse the test sample twice on different days.

6.2 Blank test

Upon analysis, perform a blank test to correct the measured values.

6.3 Evaluation of the analytical values

When the difference between the two analytical values does not exceed the tolerance value (Table 1), the average value shall be reported. When the difference between the two analytical values exceeds the tolerance value, perform two additional analyses. When the difference of these further two analyses does not exceed the tolerance value, the average value thereof shall be reported. If the difference also exceeds the tolerance value, the median of four analytical values shall be reported.

Table 1 — Tolerances for the analytical values

Units: % (mass fraction)

Component	Zr	Ca, Hf, Mg, Y	Al, Ba, Ce, Co, Gd, Fe, K, Na, Si, Sr, Ti
Tolerance	0,70	0,01 ^a 0,1 ^b	0,01

^a Applicable to content of less than 0,1 %.
^b Applicable to content of not less than 0,1 %.

6.4 Expression of analytical values

The analytical values shall be given in % (mass fraction) in dryness. The results shall be expressed to two decimal places (see [Annex A](#)).

7 Decomposition of the test sample

7.1 Classification of the sample decomposition methods

- a) Acid pressure decomposition.
- b) Alkali fusion, for the determination of the contents of major elements such as zirconium, calcium, hafnium, magnesium and yttrium, and also for the determination of silicon content.

7.2 Acid pressure decomposition

7.2.1 Reagents

It shall be ascertained that the reagents are of sufficiently high purity to permit their use without compromising the accuracy of the determination.

[ISO 23739:2021](#)

<https://standards.iteh.ai>

7.2.1.1 Water, grade 1 or superior as specified in ISO 3696.


7.2.2 Apparatus and instruments

Use ordinary laboratory apparatus and instruments together with the following:

7.2.2.1 Pressure decomposition vessel. A pressure decomposition vessel is shown in [Figure 1](#). Use the vessel exclusively for this analysis to avoid cross-contamination.

7.2.2.2 Polytetrafluoroethylene (PTFE) bottle, with cap.

7.2.2.3 Air bath, capable of heating at $230\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$.

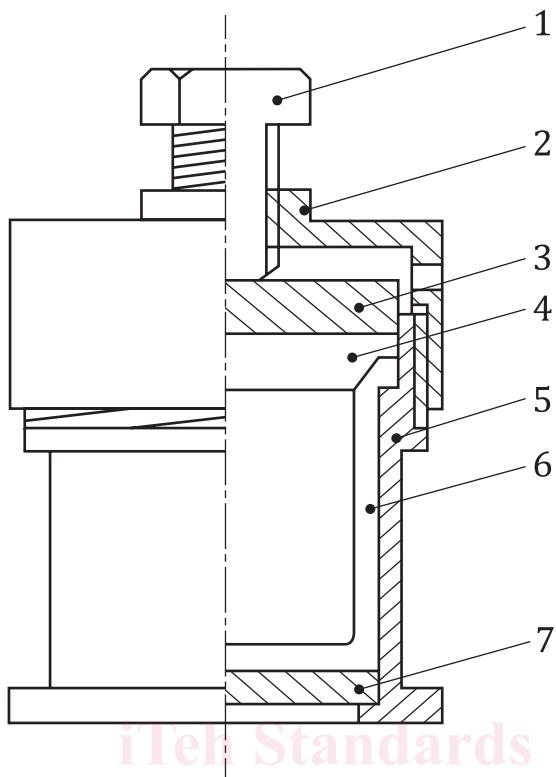

Key	
1	centre screw
2	screw cap
3	top plate
4	PTFE cap
5	cylinder
6	PTFE bottle
7	bottom plate

Figure 1 — Example of a pressure decomposition vessel

7.2.3 Procedure

Weigh 0,2 g of the test sample in a polytetrafluoroethylene bottle (7.2.2.2) and add 10 ml of sulfuric acid (1+1). Put the PTFE bottle into a pressure decomposition vessel (7.2.2.1) and close the vessel according to the manufacturer's instructions. Place the vessel in an air bath and heat it at $230\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ for 16 h.

After cooling, disassemble the vessel and transfer the dissolved solution to a 150-ml beaker. Wash the bottle six times with approximately 10 ml of warm water each time and collect the washings into the beaker. Transfer the solution into a 200-ml volumetric flask, dilute it with water up to the mark and mix well. This solution is designated as the sample solution.

7.2.4 Blank test

Perform the operation described in 7.2.3 without taking a sample to obtain the blank test value. The resulting solution is designated as blank test solution.