

FINAL  
DRAFT

INTERNATIONAL  
STANDARD

ISO/FDIS  
15223-1

ISO/TC 210

Secretariat: ANSI

Voting begins on:  
2021-03-08

Voting terminates on:  
2021-05-03

---

---

## Medical devices — Symbols to be used with information to be supplied by the manufacturer —

### Part 1: General requirements

**iTeh STANDARD PREVIEW**  
*(Partie 1: Exigences générales*  
**(standards.iteh.ai)**

[ISO/FDIS 15223-1](https://standards.iteh.ai/catalog/standards/sist/a058ba19-d5b4-496a-b6ff-82cdf0f04529/iso-fdis-15223-1)

<https://standards.iteh.ai/catalog/standards/sist/a058ba19-d5b4-496a-b6ff-82cdf0f04529/iso-fdis-15223-1>

RECIPIENTS OF THIS DRAFT ARE INVITED TO SUBMIT, WITH THEIR COMMENTS, NOTIFICATION OF ANY RELEVANT PATENT RIGHTS OF WHICH THEY ARE AWARE AND TO PROVIDE SUPPORTING DOCUMENTATION.

IN ADDITION TO THEIR EVALUATION AS BEING ACCEPTABLE FOR INDUSTRIAL, TECHNOLOGICAL, COMMERCIAL AND USER PURPOSES, DRAFT INTERNATIONAL STANDARDS MAY ON OCCASION HAVE TO BE CONSIDERED IN THE LIGHT OF THEIR POTENTIAL TO BECOME STANDARDS TO WHICH REFERENCE MAY BE MADE IN NATIONAL REGULATIONS.

**ISO/CEN PARALLEL PROCESSING**



Reference number  
ISO/FDIS 15223-1:2021(E)

© ISO 2021

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[ISO/FDIS 15223-1](https://standards.iteh.ai/catalog/standards/sist/a058ba19-d5b4-496a-b6ff-82cdf0f04529/iso-fdis-15223-1)

<https://standards.iteh.ai/catalog/standards/sist/a058ba19-d5b4-496a-b6ff-82cdf0f04529/iso-fdis-15223-1>



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2021

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva  
Phone: +41 22 749 01 11  
Email: [copyright@iso.org](mailto:copyright@iso.org)  
Website: [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

	Page
Foreword.....	iv
Introduction.....	v
<b>1 Scope.....</b>	<b>1</b>
<b>2 Normative references.....</b>	<b>1</b>
<b>3 Terms and definitions.....</b>	<b>1</b>
<b>4 General requirements.....</b>	<b>7</b>
4.1 Future <i>symbols</i> .....	7
4.2 Requirements for usage.....	7
4.3 Other <i>symbols</i> .....	7
<b>5 Symbols.....</b>	<b>7</b>
<b>Annex A (informative) Guidance and examples of symbol use, including multiple symbols.....</b>	<b>29</b>
<b>Annex B (informative) Use of general prohibition symbol and negation symbol.....</b>	<b>35</b>
<b>Annex ZA (informative) Relationship between this European standard and the General Safety and Performance Requirements of Regulation (EU) 2017/745 aimed to be covered.....</b>	<b>36</b>
<b>Annex ZB (informative) Relationship between this European standard and the General Safety and Performance Requirements of Regulation (EU) 2017/746 aimed to be covered.....</b>	<b>44</b>
<b>Bibliography.....</b>	<b>52</b>

<https://standards.iteh.ai/catalog/standards/sist/a058ba19-d5b4-496a-b6ff-82cdf0f04529/iso-fdis-15223-1>  
 ISO/FDIS 15223-1

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 210, *Quality management and corresponding general aspects for medical devices*, in collaboration with the European Committee for Standardization (CEN) Technical Committee CEN/CLC/JTC 3, *Quality management and corresponding general aspects for medical devices*, in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

This fourth edition cancels and replaces the third edition (ISO 15223-1:2016), which has been technically revised.

The main changes compared to the previous edition are as follows:

- addition of 20 *symbols* that were validated as per ISO 15223-2;
- addition of 5 *symbols* previously published in ISO 7000, ISO 7001 and IEC 60417;
- deletion of the defined term 'labelling';
- inclusion of defined terms from ISO 20417, ISO 13485 and ISO 14971;
- expansion of the examples given in [Annex A](#);
- information about European regulations has been moved to informative notes throughout.

A list of all parts in the ISO 15223 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).

## Introduction

Medical device *manufacturers* and others in the supply chain must provide specific information on the *medical device* itself, as part of the packaging, or in the *accompanying information*. For simplicity and to avoid translation of text, this information can be provided as *symbols* that have a specific meaning. This document does not specify the information that needs to be provided, but does specify internationally recognized *symbols* for the provision of this specific information.

The *symbols* included in this document have been published in ISO 7000, ISO 7001, IEC 60417 or have been subjected to a formal *symbol* validation process.

This document is intended to be used by *manufacturers of medical devices* who market products in countries where there are specific language requirements. These *symbols* allow for a consistent portrayal of information. It can also be used by consumers or end users of *medical devices* who draw their supplies from a number of sources and can have varied language capabilities.

In this document, the conjunctive “or” is used as an “inclusive or”; so a statement is true if any combination of the conditions is true.

Terms defined in [Clause 3](#) are shown in *italic type* throughout the document.

In this document, the following verbal forms are used:

- “shall” indicates a requirement;
- “should” indicates a recommendation;
- “may” indicates a permission;
- “can” indicates a possibility or a capability;
- “must” indicates an external constraint that is not a requirement of the document.

Information marked as “NOTE” is intended to assist the understanding or use of the document. “Notes to entry” used in [Clause 3](#) provide additional information that supplements the terminological data and can contain provisions relating to the use of a term.

*Symbols* added during the revision of this document were placed at the end of the pertinent section of [Table 1](#) to preserve the numbering of existing *symbols* and facilitate easy referencing of existing *symbols* in other documents.

NOTE Numbers given in square brackets throughout the document refer to the Bibliography.

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[ISO/FDIS 15223-1](#)

<https://standards.iteh.ai/catalog/standards/sist/a058ba19-d5b4-496a-b6ff-82cdf0f04529/iso-fdis-15223-1>

# Medical devices — Symbols to be used with information to be supplied by the manufacturer —

## Part 1: General requirements

### 1 Scope

This document specifies *symbols* used to express information supplied for a *medical device*. This document is applicable to *symbols* used in a broad spectrum of *medical devices*, that are available globally and need to meet different regulatory requirements.

These *symbols* can be used on the *medical device* itself, on its packaging or in the *accompanying information*. The requirements of this document are not intended to apply to *symbols* specified in other standards.

### 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3166-1, *Codes for the representation of names of countries and their subdivisions — Part 1: Country codes*

ISO 8601-1, *Date and time — Representations for information interchange — Part 1: Basic rules*

ISO 8601-2, *Date and time — Representations for information interchange — Part 2: Extensions*

ISO 15223-2, *Medical devices — Symbols to be used with medical device labels, labelling, and information to be supplied — Part 2: Symbol development, selection and validation*

### 3 Terms and definitions

For the purposes of this document the following terms and definitions apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- IEC Electropedia: available at <http://www.electropedia.org/>
- ISO Online browsing platform: available at <https://www.iso.org/obp>

#### 3.1

##### ***accompanying information***

information accompanying or *marked* on a *medical device* or accessory for the user or those accountable for the installation, use, processing, maintenance, decommissioning and disposal of the *medical device* or accessory, particularly regarding safe use

Note 1 to entry: The *accompanying information* shall be regarded as part of the *medical device* or accessory.

Note 2 to entry: The *accompanying information* can consist of the *label*, *marking*, *instructions for use*, technical description, installation manual, quick reference guide, etc.

Note 3 to entry: *Accompanying information* is not necessarily a written or printed document but could involve auditory, visual, or tactile materials and multiple media types (e.g. CD/DVD-ROM, USB stick, website).

# ISO/FDIS 15223-1:2021(E)


Note 4 to entry: See [Figure 1](#).

Note 5 to entry: The *label* can include the information on the packaging of the medical device.

Note 6 to entry: e-documentation can include any or all types of information supplied by the manufacturer partially or entirely.

Note 7 to entry: Marketing information is also known as promotional material.

Note 8 to entry: There is guidance or rationale related to accompanying information in [Annex A](#).

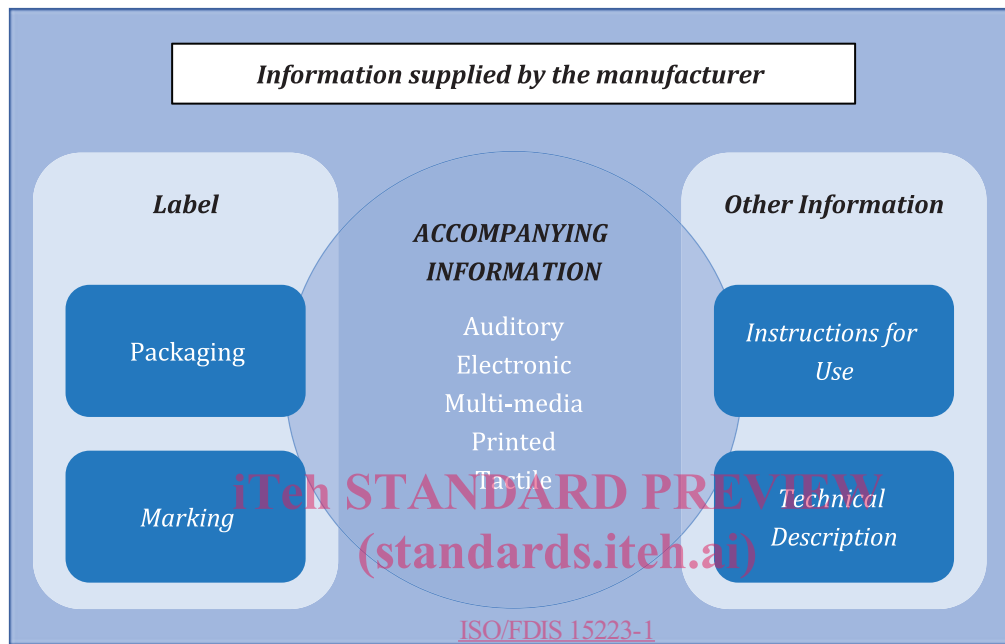

<https://standards.iteh.ai/catalog/standards/sist/a058ba19-d5b4-496a-b6ff-82cdf04529/iso-fdis-15223-1>

**Figure 1 — Relationship of terms used to describe information supplied by the manufacturer**

[SOURCE: ISO 20417:—,<sup>[15]</sup> 3.2 — modified to remove the following text from the graphic: “Scope of ISO 20417”, defined term reference numbers and a side box containing information outside the scope of ISO 20417, and to add Note 8 to entry]

### 3.2 catalogue number

*commercial product name*

*commercial product code*

value given by the *manufacturer* to identify a specific *medical device* or accessory as it relates to its form/fit, function and process (i.e. manufacturing processes requiring differentiation for the end user)

Note 1 to entry: A *catalogue number* shall consist of letters or numbers or a combination of these.

Note 2 to entry: For the purposes of this document, *commercial product code* should not be confused with the US FDA, ‘product code’ or procode classification.

Note 3 to entry: Synonyms for *catalogue number* are ‘reference number’ or ‘reorder number’.

Note 4 to entry: See ISO 20417:—, Figure 2.

[SOURCE: ISO 20417:—,<sup>[15]</sup> 3.3 — modified cross-reference in Note 4 to entry to be external to this document]



### 3.3

#### ***description***

normative text which defines the purpose, the application and the use of the *symbol* (3.20)

[SOURCE: IEC 80416-1:2008,<sup>[19]</sup> 3.2 — modified to remove "and optional product area"]

### 3.4

#### ***distributor***

natural or legal person, different from the *manufacturer* or *importer*, in the supply chain who, on their own behalf, furthers the availability of a *medical device* or accessory to the user

Note 1 to entry: More than one *distributor* may be involved in the supply chain.

Note 2 to entry: For the purposes of this document, persons in the supply chain involved in activities such as storage and transport on behalf of the *manufacturer*, *importer* or *distributor*, are not *distributors*.

Note 3 to entry: Distribution activities alone do not include repackaging or otherwise changing the container, wrapper, or *accompanying information* of the *medical device* or *medical device* package other than providing the identification of the *distributor*.

[SOURCE: ISO 20417:—,<sup>[15]</sup> 3.5]

### 3.5

#### ***importer***

natural or legal person who imports a *medical device* or accessory into a locale that was manufactured in another locale for the purposes of marketing

[SOURCE: ISO 20417:—,<sup>[15]</sup> 3.8]

### 3.6

#### ***information supplied by the manufacturer***

information related to the identification and use of a *medical device* or accessory, in whatever form provided, intended to ensure the safe and effective use of the *medical device* or accessory

Note 1 to entry: For the purposes of this document, e-documentation is included in *information supplied by the manufacturer*.

Note 2 to entry: For the purposes of this document, shipping documents and promotional material are excluded from *information supplied by the manufacturer*. However, some *authorities having jurisdiction* (defined in ISO 16142-1:2016,<sup>[9]</sup> 3.1) can consider such supplemental information as *information supplied by the manufacturer*.

Note 3 to entry: The primary purpose of *information supplied by the manufacturer* is to identify the *medical device* and its *manufacturer*, and provide essential information about its safety, performance, and appropriate use to the user or other relevant persons.

Note 4 to entry: See [Figure 1](#).

Note 5 to entry: There is guidance or rationale related to information supplied by the manufacturer in [Annex A](#).

[SOURCE: ISO 20417:—,<sup>[15]</sup> 3.10 — modified to add a cross-reference in Note 2 to entry and to add Note 5 to entry]

### 3.7

#### ***instructions for use***

##### ***IFU***

##### ***package insert***

portion of the *accompanying information* that is essential for the safe and effective use of a *medical device* or accessory directed to the user of the *medical device*

Note 1 to entry: For the purposes of this document, a user can be either a lay user or professional user with relevant specialized training.

## ISO/FDIS 15223-1:2021(E)

Note 2 to entry: For the purposes of this document, instructions for the professional processing between uses of a *medical device* or accessory can be included in the *instructions for use*.

Note 3 to entry: *The instructions for use*, or portions thereof, can be located on the display of a *medical device* or accessory.

Note 4 to entry: *Medical devices* or accessories that can be used safely and effectively without *instructions for use* are exempted from having *instructions for use* by some authorities with jurisdiction.

Note 5 to entry: See [Figure 1](#).

[SOURCE: ISO 20417:—,<sup>[15]</sup> 3.11]

### 3.8 **label**

<*medical device*, accessory> written, printed or graphic information appearing on the item itself, on the packaging of each item, or on the packaging of multiple items

Note 1 to entry: For the purposes of this document, the term *labelled* is used to designate the corresponding act.

Note 2 to entry: *Label* includes the *marking* on the *medical device* or accessory.

Note 3 to entry: For the purposes of this document, information indicated on a graphical user interface (GUI) is considered as appearing on the item.

Note 4 to entry: See [Figure 1](#).

[SOURCE: ISO 20417:—,<sup>[15]</sup> 3.12]

### 3.9 **lot number batch code**

*batch number*  
*lot code*

production control containing a combination of letters or numbers associated with a single lot or batch

Note 1 to entry: The title of *symbol* 5.1.5 uses the synonym *batch code*.

[SOURCE: ISO 20417:—,<sup>[15]</sup> 3.15 — modified to add Note 1 to entry]

### 3.10 **manufacturer**

natural or legal person with responsibility for the design or manufacture, or both, of a *medical device* with the intention of making the *medical device* available for use, under his or her name; whether or not such a *medical device* is designed or manufactured, or both, by that person themselves or on their behalf by another person(s)

Note 1 to entry: The natural or legal person has ultimate legal responsibility for ensuring compliance with all applicable regulatory requirements for the *medical devices* in the countries or jurisdictions where it is intended to be made available or sold, unless this responsibility is specifically imposed on another person by the Regulatory Authority (RA) within that jurisdiction.

Note 2 to entry: The *manufacturer's* responsibilities are described in other GHTF guidance documents. These responsibilities include meeting both pre-market requirements and post-market requirements, such as adverse event reporting and notification of corrective actions.

Note 3 to entry: "Design or manufacture, or both", may include specification development, production, fabrication, assembly, processing, packaging, repackaging, labelling, relabelling, sterilization, installation, or remanufacturing of a *medical device*; or putting a collection of devices, and possibly other products, together for a medical purpose.

Note 4 to entry: Any person who assembles or adapts a *medical device* that has already been supplied by another person for an individual patient, in accordance with the *instructions for use*, is not the *manufacturer*, provided the assembly or adaptation does not change the intended use of the *medical device*.

Note 5 to entry: Any person who changes the intended use of, or modifies, a *medical device* without acting on behalf of the original *manufacturer* and who makes it available for use under his own name, should be considered the *manufacturer* of the modified *medical device*.

Note 6 to entry: An authorized representative, *distributor* or *importer* who only adds its own address and contact details to the *medical device* or the packaging, without covering or changing the existing labelling, is not considered a *manufacturer*.

Note 7 to entry: To the extent that an accessory is subject to the regulatory requirements of a *medical device*, the person responsible for the design, manufacture, or both, of that accessory is considered to be a *manufacturer*.

[SOURCE: ISO 14971:2019,<sup>[8]</sup> 3.9]

### 3.11

#### **marking**

information, in text or graphical format, durably affixed, printed, etched (or equivalent) to a *medical device* or accessory

Note 1 to entry: For the purposes of this document, the term *marked* is used to designate the corresponding act.

Note 2 to entry: For the purposes of this document, *marking* is different from ‘direct *marking*’ as commonly described in unique device identification (UDI) standards and regulations. A UDI ‘direct *marking*’ is a type of *marking*.

Note 3 to entry: See [Figure 1](#).

[SOURCE: ISO 20417:—,<sup>[15]</sup> 3.16]

### 3.12

#### **medical device**

instrument, apparatus, implement, machine, appliance, implant, reagent for in vitro use, software, material or other similar or related article, intended by the *manufacturer* to be used, alone or in combination, for human beings, for one or more of the specific medical purpose(s) of:

- diagnosis, prevention, monitoring, treatment or alleviation of disease;
- diagnosis, monitoring, treatment, alleviation of or compensation for an injury;
- investigation, replacement, modification, or support of the anatomy or of a physiological process;
- supporting or sustaining life;
- control of conception;
- disinfection of *medical devices*;
- providing information by means of in vitro examination of specimens derived from the human body;

and does not achieve its primary intended action by pharmacological, immunological or metabolic means, in or on the human body, but which may be assisted in its intended function by such means

Note 1 to entry: Products which may be considered to be *medical devices* in some jurisdictions but not in others include:

- disinfection substances;
- aids for persons with disabilities;
- devices incorporating animal or human tissues, or both;
- devices for in vitro fertilization or assisted reproduction technologies.

[SOURCE: ISO 13485:2016,<sup>[7]</sup> 3.11]

**3.13**

**model number**

*model*

letters, numbers or a combination of these assigned by a *manufacturer* to distinguish by function or type, a particular *medical device*, *accessory* or *medical device family* from another

Note 1 to entry: See ISO 20417:—, Figure 2.

[SOURCE: ISO 20417:—, [15] 3.13 — modified cross-reference in Note 1 to entry to be external to this document]

**3.14**

**risk**

combination of the probability of occurrence of harm and the severity of that harm

[SOURCE: ISO 14971:2019, [8] 3.18]

**3.15**

**risk assessment**

overall process comprising a *risk analysis* and a *risk evaluation*

[SOURCE: ISO 14971:2019, [8] 3.20]

**3.16**

**serial number**

production control containing a combination of letters or numbers, selected by the *manufacturer*, intended for quality control and identification purposes to uniquely distinguish an individual *medical device* from other *medical devices* with the same *catalogue number* or *model number*

[SOURCE: ISO 20417:—, [15] 3.22]

**3.17**

**single patient multiple use**

<*medical device*, *accessory*> intended by the *manufacturer* to be reused on an individual patient for multiple uses

Note 1 to entry: A single patient multiple use *medical device* or *accessory* may require processing between uses.

Note 2 to entry: For an implantable *medical device*, the duration of a single use is from implanting to explanting the *medical device*.

[SOURCE: ISO 20417:—, [15] 3.25]

**3.18**

**single use**

**do not re-use**

**use only once**

<*medical device*, *accessory*> intended by the *manufacturer* to be used on an individual *patient* or specimen during a single *procedure* and then disposed of

Note 1 to entry: A single use *medical device* or *accessory* is not intended by its *manufacturer* to be further processed and used again.

[SOURCE: ISO 20417:—, [15] 3.26]

**3.19**

**sterile**

free from viable microorganisms

[SOURCE: ISO 20417:—, [15] 3.28]

**3.20****symbol**

graphical representation appearing on the *label* or associated documentation, or both, of a *medical device* that communicates *characteristic information* without the need for the supplier or receiver of the information to have knowledge of the language of a particular nation or people

Note 1 to entry: The *symbol* can be an abstract pictorial or a graphical representation, or one that uses familiar objects, including alphanumeric characters (with sufficient justification).

[SOURCE: ISO 20417:—, [15] 3.29]

**4 General requirements****4.1 Future symbols**

- a) Future *symbols* proposed for inclusion in this document shall be validated in accordance with ISO 15223-2. *Symbols* registered under ISO 7000, ISO 7010, or IEC 60417 are exempt.
- b) Any *symbol* proposed for inclusion in this document shall be applicable to a range of *medical devices* and have global or regional applicability.

**4.2 Requirements for usage**

- a) When a need to use *symbols* as an appropriate method for conveying information essential for the proper use of a *medical device* is identified, the *symbols* given in [Table 1](#) may be marked on the *medical device*, appear on its packaging or in *information supplied by the manufacturer*.

NOTE ISO and IEC maintain an online database of graphical *symbols* for use on equipment, which contains the complete set of graphical *symbols* included in ISO 7000, ISO 7001 and IEC 60417 available at <https://www.iso.org/obp/ui/#home>. This database shows each graphical *symbol* and identifies it by a reference number and a *title*. The graphical *symbols* are available in different formats (e.g. AI, DWG, EPS) and some additional data, as applicable, is provided.

- b) The *manufacturer* shall determine the appropriate size for the *symbol* to be legible for its intended function.

NOTE 1 This document does not specify colours or minimum size for the *symbols* in [Table 1](#), nor does it specify the relative size of *symbols* and that of indicated information.

NOTE 2 Guidance on the application of graphical *symbols* is found in IEC 80416-3:2002+A1:2011<sup>[20]</sup>.

NOTE 3 Guidance on the use of the general prohibition *symbol* and the negation *symbol* is found in [Annex B](#).

- c) All dates and times presented in association with *symbols* shall use the conventions set out in ISO 8601-1 and ISO 8601-2.

**4.3 Other symbols**

Other standards specify additional *symbols* that are applicable to particular kinds or groups of *medical devices* or to particular situations. The bibliography provides examples of sources for additional *symbols*.

**5 Symbols**

- a) When appropriate, information essential for proper use shall be indicated on the *medical device*, its packaging, or in the *accompanying information* by using the corresponding *symbols* given in [Table 1](#).
- b) A *manufacturer* may use any appropriate *symbol*.

## ISO/FDIS 15223-1:2021(E)

NOTE 1 [Table 1](#) has been organized into *symbol* categories for ease of use. The category into which a *symbol* is grouped does not have any significance as far as usage is concerned. The order of appearance of *symbols* and the categories in which they are placed are not prioritized. Examples of the use of *symbols* can be found in [Annex A](#).



NOTE 2 Each *symbol* in the ISO/IEC *symbols* database (available at <https://www.iso.org/obp/ui/#home>) has a reference number and registration date. This information is given in the final column of [Table 1](#).

## iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO/FDIS 15223-1](#)

<https://standards.iteh.ai/catalog/standards/sist/a058ba19-d5b4-496a-b6ff-82cdf0f04529/iso-fdis-15223-1>

Table 1 — Symbols to convey medical device information

Reference number and graphic	Title	Description	Requirements	Notes	Restrictions of use	ISO/IEC symbol number and registration date
5.1 Manufacturer 5.1.1 	Manufacturer	Indicates the medical device manufacturer	This symbol shall be accompanied by the name and address of the manufacturer adjacent to the symbol.	NOTE 1 This symbol is used to indicate information that is required in Europe and can be required by other authorities having jurisdiction. NOTE 2 For use in Europe the full definition of “manufacturer” is given in EU Regulations 2017/745 <sup>[23]</sup> and 2017/746. <sup>[24]</sup> Other jurisdictions can have unique definitions. NOTE 3 The date of manufacture, as well as the name and address of the manufacturer, can be combined in one symbol.	—	ISO 7000-3082 2011-10-02
5.1.2 	Authorized representative in the European Community/European Union	Indicates the authorized representative in the European Community/European Union	This symbol shall be accompanied by the name and address of the authorized representative, adjacent to the symbol.	NOTE 1 This symbol is used to indicate information that is required in the European Community/European Union. NOTE 2 Additional guidance can be found in ISO 20417 <sup>[15]</sup> , ISO 18113-1 <sup>[10]</sup> , ISO 18113-2 <sup>[11]</sup> , ISO 18113-3 <sup>[12]</sup> , ISO 18113-4 <sup>[13]</sup> and ISO 18113-5 <sup>[14]</sup> . NOTE 3 If multiple symbols (i.e. Authorized Representative, Importer, Distributor, Translation, or Repackaging) identify the same responsible entity, the name and address need not be duplicated, and all applicable symbols can be grouped together next to the single address.	—	N/A