
INTERNATIONAL STANDARD



2782

INTERNATIONAL ORGANIZATION FOR STANDARDIZATION • МЕЖДУНАРОДНАЯ ОРГАНИЗАЦИЯ ПО СТАНДАРТИЗАЦИИ • ORGANISATION INTERNATIONALE DE NORMALISATION

Rubber, vulcanized — Determination of permeability to gases — Constant pressure method

Caoutchouc vulcanisé — Détermination de la perméabilité aux gaz — Méthode de la pression constante

iTeh STANDARD PREVIEW

First edition — 1977-12-01

(standards.iteh.ai)

[ISO 2782:1977](#)

<https://standards.iteh.ai/catalog/standards/sist/1587d3ed-781a-41a4-bafd-c140fcc59f66/iso-2782-1977>

UDC 678.063 : 678.01 : 539.217

Ref. No. ISO 2782-1977 (E)

Descriptors : rubber, vulcanized rubber, tests, gas permeability testing, gas permeability.

Price based on 5 pages

FOREWORD

ISO (the International Organization for Standardization) is a worldwide federation of national standards institutes (ISO member bodies). The work of developing International Standards is carried out through ISO technical committees. Every member body interested in a subject for which a technical committee has been set up has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work.

Draft International Standards adopted by the technical committees are circulated to the member bodies for approval before their acceptance as International Standards by the ISO Council.

International Standard ISO 2782 was developed by Technical Committee ISO/TC 45, *Rubber and rubber products*, and was circulated to the member bodies in March 1976.

It has been approved by the member bodies of the following countries :

Belgium	Hungary	ISO 2782:1977	Sweden
Brazil	India	https://standards.iteh.ai/catalog/standards/sist/1587d3ed-781a-41a4-bafd-c140fcc01726-2782-1977	Switzerland
Canada	Italy		Turkey
Czechoslovakia	Netherlands		United Kingdom
Egypt, Arab Rep. of	Poland		U.S.A.
France	Portugal		Yugoslavia
Germany	Romania		

The member body of the following country expressed disapproval of the document on technical grounds :

U.S.S.R.

Rubber, vulcanized – Determination of permeability to gases – Constant pressure method

0 INTRODUCTION

The measurement of the permeability of rubber to gases is important in the evaluation of compounds for such products as inner tubes, tubeless tyre liners, hoses, balloons or other gas containers, seals, and diaphragms. The measurement is also of theoretical importance in the study of characteristics of diffusion and gas solubility in relation to polymer structure.

1 SCOPE AND FIELD OF APPLICATION

This International Standard gives basic directions for measuring the permeability of rubber to gases at steady state conditions, when a constant pressure is maintained on each of the end faces of the rubber to be tested. Results obtained by this test procedure should not be extrapolated to thicknesses of material considerably different from that of the test piece.

It applies to solid rubber of a hardness not less than 35 IRHD and to gases such as air, nitrogen, oxygen, hydrogen, liquefied petroleum gas (in gaseous form) and coal gas. Errors may be introduced if the gas used appreciably swells the rubber under test.

2 REFERENCES

ISO 471, *Rubber – Standard temperatures, humidities and times for the conditioning and testing of test pieces.*

ISO 1826, *Rubbers – Time-lapse between vulcanization and testing.*

ISO 3383, *Rubber – General directions for achieving elevated or sub-normal temperatures for tests.*

3 DEFINITION

permeability of rubber to gases : The rate of volume flow of gas under steady state conditions referred to standard temperature and pressure, between opposite faces of a unit cube of solid rubber, when subjected to unit pressure difference and controlled temperature.

4 PRINCIPLE

The cavity of a test cell, maintained at a constant temperature, is divided by a disc test piece into a high pressure and a low (atmospheric) pressure side. The high pressure side is connected to a constant pressure gas reservoir or is of such a volume that, once filled, it stays at a practically constant pressure. The gas permeates into the low pressure side, which is of a very low volume and connected to a capillary tube; this is provided for measuring the permeated volume, while keeping or restoring the same low pressure within this side.

Absolute pressure for the high pressure side is maintained in the range 0,3 to 1,5 MPa* and for the low pressure side it is maintained at the prevailing atmospheric pressure.

For normal comparison of permeability of different rubber vulcanizates, the test temperature is a standard laboratory temperature but higher preferred temperatures may be used where conditions are required to approximate to the service temperature of rubber products. Standard laboratory temperature and higher preferred temperatures shall be selected from ISO 471. When higher preferred temperatures are used, directions given in ISO 3383 shall be observed.

WARNING – Because of the dangers connected with high pressure and flammability, handling of gases should be done by experienced personnel only.

* 1 MPa = 1 N/mm²

5 APPARATUS

Examples of suitable apparatus are given in figures 1 and 2.

5.1 Test cell having a means of clamping the test piece round its periphery in a gas-tight manner so as to expose one surface to gas under pressure. The other surface of the test piece shall be supported against the load due to the gas pressure so that no appreciable deformation takes place. For this reason, the low pressure side of the test cell shall be filled with a rigid, very permeable packing piece which may consist of a disc of microporous material such as microporous ebonite, discs of microporous sintered stainless steel or discs of fine wire gauze or filter paper which completely fill the cavity. A means of indicating gas pressure with an error of not more than 1% shall be connected to the high pressure side of the cell.

The volume of the high pressure side of the cell shall be at least $25 \times 10^{-6} \text{ m}^3$ (25 cm^3) to minimize the pressure loss due to diffusion during a test which may last several hours. The internal volume of the test cell on the low pressure (atmospheric) side of the test piece shall be kept to a minimum by the use of permeable packing as described above and by small diameter passages through a dismantable coupling and tubing to the capillary tube. The total free volume between test piece and zero mark shall not exceed $2 \times 10^{-6} \text{ m}^3$ (2 cm^3).

Test cells shall be of metal construction with sufficient mass to assist temperature stability, and shall be provided with a drilled pocket to hold the temperature measuring device (5.2).

5.2 Temperature measuring device, to read accurately to within $\pm 0,2 \text{ }^\circ\text{C}$.

5.3 Barometer.

5.4 Device for the measurement of permeated gas volumes, consisting fundamentally of a capillary tube of known and uniform cross-section over the length used for volume measurements.

Suitable cross-sections are $0,7 \times 10^{-6}$ to $2 \times 10^{-6} \text{ m}^2$ ($0,7$ to 2 mm^2), with an accuracy of within 1% in uniformity.

The capillary tube shall be graduated or a graduated scale shall be held close to it on the long straight portion.

It shall be suitably filled with a non-volatile liquid which does not dissolve the gas [suitable liquids are di-(2 ethyl-hexyl) sebacate or tritolyl phosphate, coloured with Sudan red].

The capillary tube may be mounted on the cell layer or may be provided with a by-pass valve in order to start the volume measurements after a conditioning period.

ISO 2782:1977
<https://standards.iteh.ai/catalog/standards/sist/1587d3ed-781a-41a4-bafd-c140fcc59f66/iso-2782-1977>

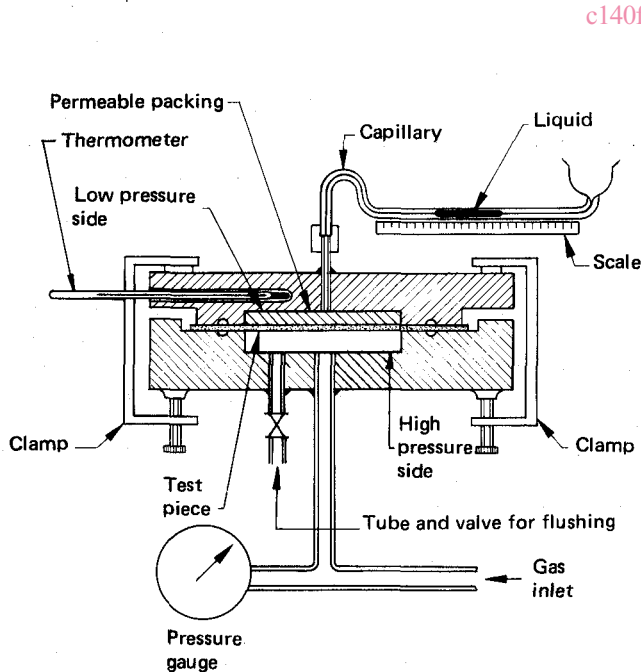


FIGURE 1 – Apparatus with horizontal measuring device

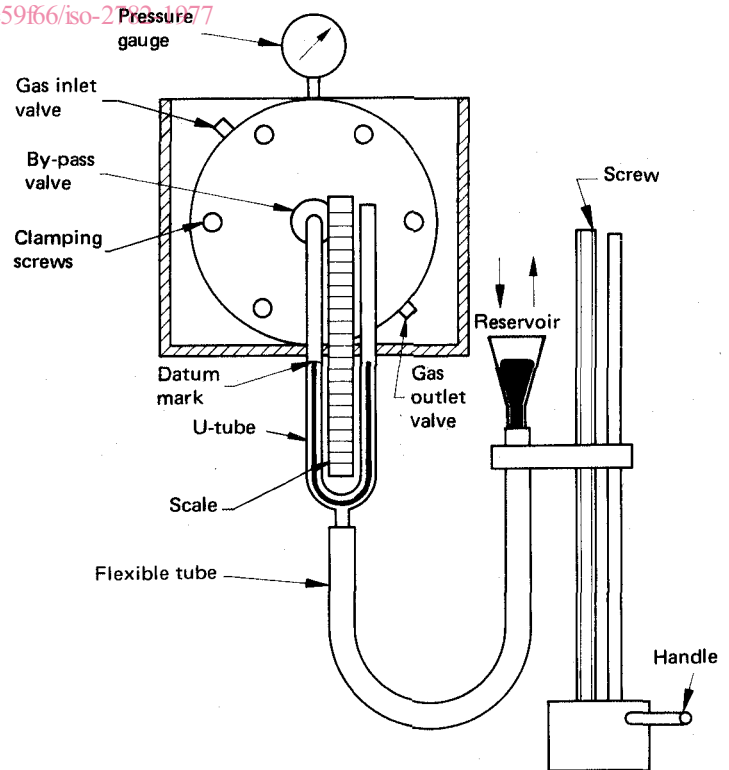


FIGURE 2 – Apparatus with vertical measuring device

The capillary tube may be either horizontally or vertically mounted. In the first case only, a drop of liquid may be used as index of volume variations. In the second case, a vertically adjustable reservoir of liquid connected by a T-piece to the lowest portion of the capillary tube shall be provided to restore the low side pressure.

A microscope or a cathetometer may be used to observe the liquid position.

5.5 Constant temperature bath or other means capable of maintaining the test cell at the required test temperature to within $\pm 1^\circ\text{C}$.

The wall of the bath shall be arranged so that the outlet from the test cell will project through the side, leaving the capillary dismountable coupling accessible.

6 TEST PIECES

6.1 Shape and dimensions

The test piece shall be a disc of uniform thickness and of dimensions to suit those of the test cell, and may be either moulded or cut from a test sheet or a product. It is preferable to use a moulded disc having on each face a circumferential rib or bead to fit into corresponding grooves in the clamping members. Where the test piece is a flat sheet, suitable "O" rings shall be used to fit into grooves in the test cell.

The overall variation in thickness (excluding beads) shall not exceed 10 % of the mean thickness.

Suitable dimensions are 50 to 155 mm diameter with a free testing surface of 800×10^{-6} to $7\,000 \times 10^{-6}$ m² (8 to 70 cm²); thickness may be between 0,25 and 3 mm, the smallest thickness being advantageous for rubbers of low permeability, such as isobutene-isoprene rubber. Imperfections and pinholes shall be absent.

6.2 Number

Duplicate test pieces of each rubber shall be tested.

7 TIME-LAPSE BETWEEN VULCANIZATION AND TESTING

The requirements of ISO 1826 apply.

8 TEMPERATURE OF TEST

For normal comparisons of permeability of different rubber vulcanizates, the test temperature shall be a standard laboratory temperature as given in ISO 471. Higher temperatures may be used where conditions are required to approximate to service temperatures of rubber products.

Such higher temperatures shall be selected from the list of preferred temperatures, as given in ISO 471.

In any given test or series of tests intended to be comparable, the tolerance on the temperature shall be $\pm 1^\circ\text{C}$ for temperatures up to 175°C and it shall be $\pm 2^\circ\text{C}$ for temperatures of 200°C and above.

9 PROCEDURE

9.1 Preparation of test piece

Examine the test piece carefully for pinholes or imperfections within the area of the internal diameter of the cell (which is the effective test area). Care should be taken to avoid contamination of the surface between manufacture and test.

Determine the thickness of the test piece in the test area as the average of six measurements each made to an accuracy of 0,02 mm. Insert the permeable packing in the shallow cavity behind the test piece on the low pressure side. Clamp the test piece securely round its periphery.

NOTE — It is permitted to use a minimum of vacuum grease on the clamping surfaces to ensure gas-tightness. No grease shall be allowed to appear on the central area of the test piece.

Place the test cell in the constant temperature bath and connect to the test gas reservoir at the required pressure of test (0,3 to 1,5 MPa depending on the permeability of the test piece).

Maintain the pressure of gas to within $\pm 2,5\%$ during the test.

9.2 Conditioning of the test piece

The assembled apparatus shall be allowed to remain at the test temperature for a minimum of 16 h, or, where the approximate value of the diffusivity is known, for a minimum time t , in seconds, derived from the following equation :

$$t = \frac{b^2}{2Q} \times S = \frac{b^2}{2D}$$

where

b is the thickness, in metres, of the test piece;

Q is the permeability in metres squared per pascal second [m²/(Pa·s)];

D is the diffusion coefficient in metres squared per second;

S is the solubility constant (the volume of the gas, dissolved per unit volume of the test piece at unit pressure) in reciprocal pascals $\left(\frac{1}{\text{Pa}}\right)$.

This minimum time t ensures that the diffusion of gas through the test piece, and hence the gas flow throughout the test piece, may reach the steady state corresponding

to the right-hand (straight) portion of the curve in figure 3. The left-hand portion of this curve indicates the initial approach to steady conditions due to diffusion through the test piece. The strictly linear portion of the curve only is used for permeability measurement.

9.3 Determination of flow rate

Charge the capillary tube, calibrated as described in the following note, with the non-volatile liquid specified in 5.4. Mount on the test cell and close the by-pass valve, if any. As the gas diffuses through the test piece, the meniscus is displaced. If the capillary tube is mounted vertically as in the apparatus shown in figure 2, compensate the levels in both legs of the U-tube by level modification of the reservoir as often as possible, always directly before reading. Only the levels in the U-tube are to be considered, because the level in the compensator cannot agree with the other levels due to the capillary effect of the U-tube.

Start a stop-watch when the meniscus crosses the zero mark (zero time).

Record readings of the position of the liquid in the capillary tube at intervals of about 2 min throughout the test, which typically has a duration of 10 to 60 min after steady state.

Plot a time-length diagram; it must not show any appreciable departure from linearity after reaching a steady state. If this occurs, the test result shall be rejected and the test repeated.

NOTE – Method for measuring the cross-section of a capillary tube

- 1 Introduce into the capillary tube a quantity of mercury to fill a length of about 20 mm (0,2 to 0,6 g).
- 2 Keeping the tube horizontally mounted, perform the measurement of the length L of the mercury in several positions over the length of the tube (five to ten positions), with an accuracy of 0,02 mm.
- 3 Weigh the capillary tube with and without the mercury, to the nearest milligram.

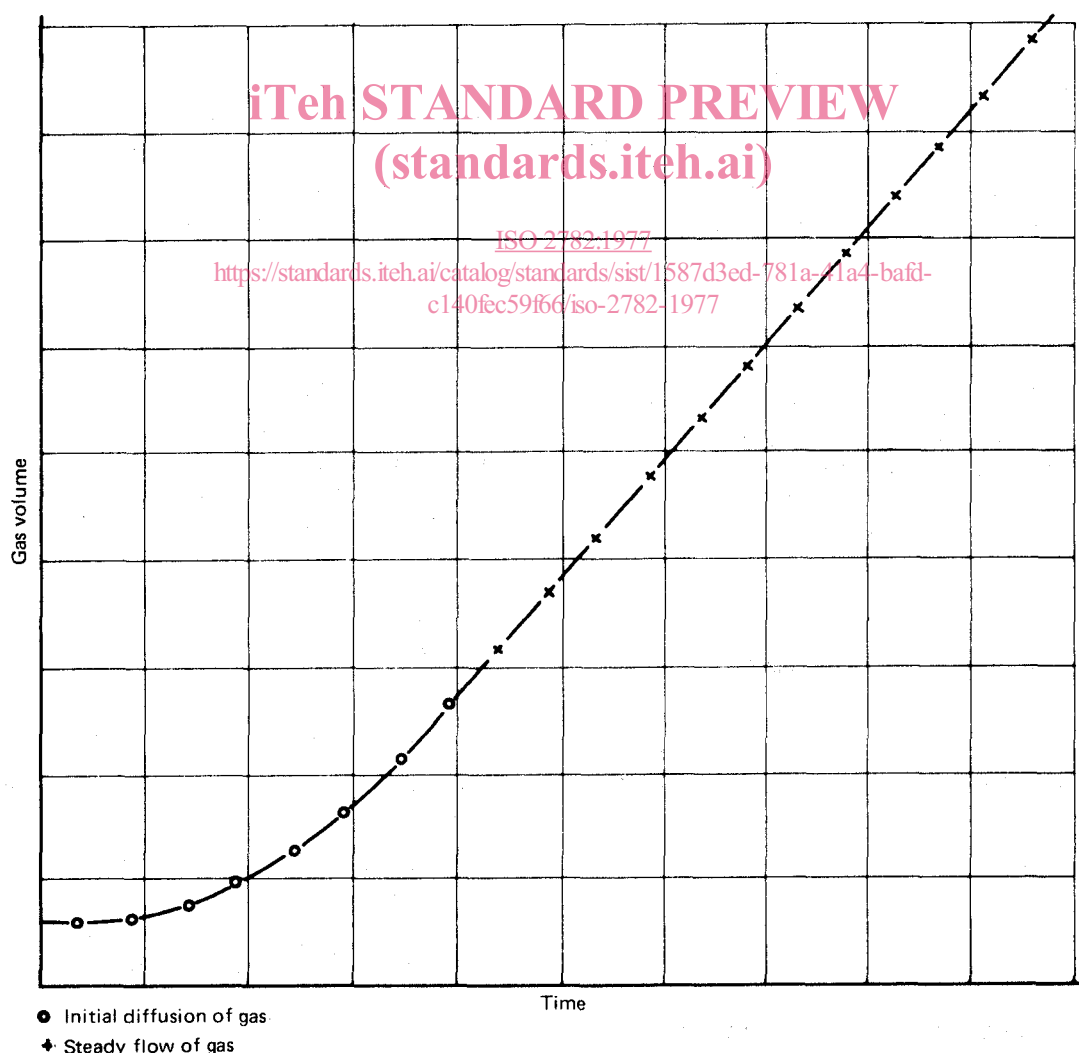


FIGURE 3 – Typical time/gas volume curve

4 The cross-section, A_1 , of the capillary tube in each position is given, in millimetres squared, by the formula

$$A_1 = \frac{m_1 - m_2}{L \rho}$$

where

m_1 is the mass, in milligrams, of the capillary tube with mercury;

m_2 is the mass, in milligrams, of the capillary tube without mercury;

L is the length, in millimetres, of the mercury in the capillary tube;

ρ is the density, in grams per millilitre, of mercury.

The differences between any of the measurements of the cross-section A_1 shall not exceed 1 % of the mean value.

10 EXPRESSION OF RESULTS

The permeability shall be calculated in the following manner. Pressure on the low pressure side shall be deduced from a barometer reading using the following relation :

$$1 \text{ mmHg at } 0^\circ \text{C} = 133,322 \text{ Pa}$$

This may be corrected for thermal expansion of the mercury and the scale, but no sea-level reduction shall be applied.

Pressure on the high pressure side shall be deduced from the manometer reading (if this is relative, p_1 should be added).

Co-ordinates of one pair of points (or averages from many pairs) on the plotted time-length diagram give corresponding Δt and ΔL values.

Permeated volume, reduced to gas reference conditions, is :

$$\begin{aligned} \Delta V &= A_1 \Delta L \frac{273 p_1}{101\,300 T} \\ &= \frac{0,002\,7 A_1 \Delta L p_1}{T} \end{aligned}$$

Permeability may be calculated as follows :

$$\begin{aligned} Q &= \frac{b \Delta V}{\Delta t A_2 (p_2 - p_1)} \\ &= \frac{0,002\,7 b A_1 \Delta L p_1}{\Delta t A_2 T (p_2 - p_1)} \end{aligned}$$

where

A_1 is the cross-section, in square metres, of the capillary tube;

A_2 is the free area, in square metres, of the test piece;

b is the thickness, in metres, of the test piece;

ΔL is the change in length of displacement of meniscus,

in metres, obtained on the linear part of the curve, during time interval Δt seconds;

p_1 is the pressure (absolute), in pascals, on the low pressure side;

p_2 is the pressure (absolute), in pascals, on the high pressure side;

Q is the permeability, in metres squared per pascal second [$\text{m}^2/\text{Pa}\cdot\text{s}$];

T is the test temperature (absolute), in kelvins;

Δt is the time interval, in seconds, for a given change in length of displacement of the meniscus;

ΔV is the permeated volume of gas, at reference conditions, in cubic metres, during the time interval of Δt seconds;

273 is the gas reference temperature (absolute), in kelvins;

101 300 is the gas reference pressure (absolute), in pascals.

For each set of two test pieces, the two values of permeability shall be within $\pm 10\%$ of their mean. If they are not, determine the permeability on a further set of two test pieces and calculate the mean value of the four test results.

11 TEST REPORT

The test report shall include the following information :

a) Sample details :

- 1) a full description of the sample and its origin;
- 2) compound details, cure time and temperature where appropriate;
- 3) method of preparation of test pieces from sample, i.e. whether moulded or cut, and their dimensions.

b) Test method : a reference to this International Standard (ISO 2782).

c) Test details :

- 1) the temperature of test;
- 2) the gas used in the test;
- 3) the gas pressure on the high pressure side.

d) Test results :

- 1) number of test pieces tested;
- 2) the mean value of the permeability.

e) Date of test.