



Designation: F1147 – 05 (Reapproved 2011)

Standard Test Method for Tension Testing of Calcium Phosphate and Metallic Coatings¹

This standard is issued under the fixed designation F1147; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method covers tension testing of calcium phosphate and metallic porous coatings adhering to dense metal substrates at ambient temperatures. It assesses the degree of adhesion of coatings to substrates, or the internal cohesion of a coating in tension normal to the surface plane.

1.2 The values stated in inch-pound units are to be regarded as standard. The values given in parentheses are mathematical conversions to SI units that are provided for information only and are not considered standard.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*²

E4 Practices for Force Verification of Testing Machines
E6 Terminology Relating to Methods of Mechanical Testing
E8 Test Methods for Tension Testing of Metallic Materials
F1501 Test Method for Tension Testing of Calcium Phosphate Coatings (Withdrawn 2000)³

3. Terminology

3.1 The definitions of terms relating to tension testing appearing in Terminology E6 shall be considered as applying to the terms used in this test method.

4. Summary of Test Method

4.1 The tensile test method consists of subjecting a specimen assembly composed of one coated and one uncoated

component to a tensile load. In the case of the calcium phosphate coatings, the components to be tested must be bonded together by use of a polymeric adhesive. In the case of the metallic coatings, the components may either be bonded with the adhesive, or sintered together. The adhesive may be in film form or bulk form, but it must have a minimum bulk tensile strength of 34.5 MPa (5000 psi) or as great as the minimum required adhesion or cohesion strength of the coating, whichever is greater.

4.2 The tensile load must be applied normal to the plane of the coating utilizing a tension machine which is capable of determining the maximum strength of the coating or coating attachment to the substrate interface.

5. Significance and Use

5.1 The tensile test method is recommended for tension testing of calcium phosphate/substrate or porous metal coating/substrate combinations and can provide information on the adhesive or cohesive strength of coatings under (uniaxial) tensile stress.

5.2 The test method may be useful for comparative evaluation of adhesive or cohesive strengths of a variety of types of coatings. Coatings may be applied using a variety of methods, including but not limited to plasma-spraying and sintering. Information developed using this test method may be useful for certain quality control and design purposes.

5.3 The test should not be considered to provide an intrinsic value for utilization directly in making calculations such as determining the ability of a coating to withstand specified environmental stresses.

5.4 Processing variables such as substrate preparation prior to coating, surface texture, coating technique variables or postcoating heat treatment variables may introduce a significant effect on the results of the tension test. The specimen being evaluated must be representative of the actual end use coating.

6. Apparatus

6.1 *Testing Machines*—Machines used for testing shall conform to the requirements of Practices E4. The loads used in determining tensile strength and yield strength shall be within

¹ This test method is under the jurisdiction of ASTM Committee F04 on Medical and Surgical Materials and Devices and is the direct responsibility of Subcommittee F04.15 on Material Test Methods.

Current edition approved Oct. 1, 2011. Published October 2011. Originally approved in 1988. Last previous edition approved in 2005 as F1147 – 05. DOI: 10.1520/F1147-05R11.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ The last approved version of this historical standard is referenced on www.astm.org.

the loading range of the testing machine as defined in Practices E4. See also Test Methods E8.

6.2 Gripping Devices:

6.2.1 *General*—Various types of grips may be used to transmit the load applied to the specimens by the testing machine. To ensure axial tensile stress, it is important that the specimen axis coincide with the centerline of the heads of the testing machine and that the coating test plane be perpendicular to the axial load. Any departure from this requirement (that is, any eccentric loading) will introduce bending stresses that are not included in the usual stress calculation (force/cross-sectional area).

6.2.2 *Yoke and Dowel Pin Grips*—A schematic diagram of a typical gripping device for specimens with holes drilled for pin loading is illustrated in Fig. 1. There should be two perpendicular pins in order to maximize off axis loading.

7. Materials

7.1 *Adhesive Bonding Agent*—A polymeric adhesive bonding agent in film form, or filled viscous adhesive cement, when used, shall be identified and shall meet the following requirements.

7.1.1 The bonding agent shall be capable of bonding the coating on the test specimen components with a tensile strength that is at least 34.5 MPa (5000 psi) or as great as the minimum required adhesion or cohesion strength of the coating.

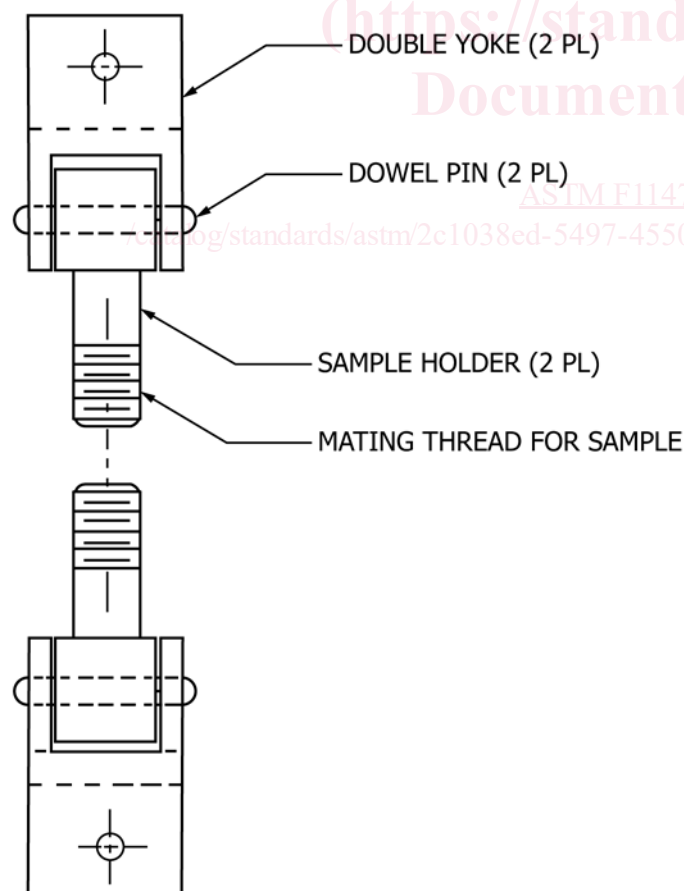


FIG. 1 Yoke and Dowel Pin Grips for Tensile Testing Porous Surfaces

7.1.2 In instances where porosity extends to the coating substrate interface, the bonding agent shall be sufficiently viscous and application to the coating sufficiently careful to assure that it will not penetrate through the coating to the substrate. The FM 1000 Adhesive Film⁴ with a thickness of 0.25 mm (0.01 inc.) has proven satisfactory for this test. If a material other than FM 1000 is used, or the condition of the FM 1000 is unknown, it must be tested to establish its equivalence fresh FM 1000. Testing should be performed without the presence of the coating to establish the performance of the adhesive.

8. Test Specimens

8.1 General:

8.1.1 In order to ensure precision and accuracy in test results, it is important that care be exercised in the preparation of specimens, both in machining and in the case of multi-part specimens, in the assembly. Specimen components must be properly aligned in order that generated stresses be purely axial, that is, normal to the coated surface.

8.1.2 *Tensile-Type Specimens*—Three general types of test specimens are illustrated in Figs. 2 and 3. A complete, assembled test assembly consists either of two solid pieces; one with a coated surface and the other with an uncoated surface or three solid pieces; two with uncoated surfaces and one with a coating applied on one side. The uncoated surface may be roughened to aid in the bonding of the adhesive.

8.1.3 The cross-sectional area of the substrate upon which the coating is applied shall be nominal 5.07 cm² (0.78 in.²). When specimens of another cross-sectional area are used, the data must be demonstrated to be equivalent to a 5.07 cm² standard cross-sectional area, and the specimen size should be reported.

8.1.4 All test specimens for coating characterization shall be prepared from indicative coating lots, using production feed-stock lots and be coated on the same equipment used for actual implants.

8.2 Specimen Coating Preparation:

8.2.1 Coatings may be applied by any one of a number of techniques. The coating should consist of a layer which is mechanically or chemically attached and covers the surface.

8.2.2 All thermal treatments normally performed on the devices should be performed on the test specimens.

8.2.3 If employed, passivation and sterilization techniques should be consistent with those used for actual devices.

8.2.3.1 If the passivation and sterilization processes can be shown not to influence the tensile strength, these steps may be eliminated.

8.2.4 *Inspection*—Before testing, visual inspections should be performed on 100 % of the test specimens. Lack of coating in highly stressed regions, as well as non-uniform coating appearance, shall be cause for specimen rejection.

⁴ The sole source of supply of the apparatus known to the committee at this time is Cytec Engineered Materials, Inc., 1300 Revolution St., Havre de Grace, MD 21078. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee,¹ which you may attend.