



# Standard Specification for Industrial Platinum Resistance Thermometers<sup>1</sup>

This standard is issued under the fixed designation E 1137; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last approval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 This specification covers the requirements for metal-sheathed industrial platinum resistance thermometers (PRT's) suitable for direct immersion temperature measurement. It applies to PRT's with an average temperature coefficient of resistance between 0 and 100°C of 0.385 %/°C and nominal resistance at 0°C of 100  $\Omega$  or other specified value. This specification covers PRT's suitable for all or part of the temperature range -200 to 650°C. The resistance-temperature relationship and tolerances are specified as well as physical, performance, and testing requirements.

1.2 The values of temperature in this specification are based on the International Temperature Scale of 1990 (ITS-90).<sup>2</sup>

## 2. Referenced Documents

### 2.1 ASTM Standards:

A 269 Specification for Seamless and Welded Austenitic Stainless Steel Tubing for General Service<sup>3</sup>

B 167 Specification for Nickel-Chromium-Iron Alloys (UNS N06600, N06601, and N06690) Seamless Pipe and Tube<sup>4</sup>

E 344 Terminology Relating to Thermometry and Hydrometry<sup>5</sup>

E 644 Test Methods for Testing Industrial Resistance Thermometers<sup>5</sup>

E 1652 Specification for Magnesium Oxide and Aluminum Oxide Powder and Crushable Insulators Used in the Manufacture of Metal-Sheathed Platinum Resistance Thermometers and Noble Metal Thermocouples<sup>5</sup>

## 3. Terminology

3.1 *Definitions*—For definitions of terms used in this specification see Terminology E 344.

### 3.2 Definitions of Terms Specific to This Standard:

3.2.1 *cable end closure, n*—moisture barrier at the cable end of the sheath.

3.2.2 *connecting wires, n*—wires that run from the element through the cable end closure and external to the sheath.

3.2.2.1 *Discussion*—The closure does not necessarily constitute a hermetic seal.

3.2.3 *excitation, n*—electrical current passing through the element.

3.2.4 *g-level, n*—acceleration of an object relative to the local acceleration of gravity.

3.2.4.1 *Discussion*—For example, a g-level of 5 is equivalent to an acceleration of approximately  $5 \times 9.8 \text{ m/s}^2 = 49.0 \text{ m/s}^2$ .

3.2.5 *minimum immersion length, n*—depth that a thermometer should be immersed, in a uniform temperature environment, such that further immersion does not produce a change in indicated temperature greater than the specified tolerance.

3.2.6 *PRT design, n*—generic term used to differentiate between different PRT construction details, such as element and connecting wire construction, insulation methods, sealing techniques, and mounting methods (for example, spring loaded or direct mounting).

3.2.7 *self-heating, n*—change in temperature of the element caused by the heating effect of the excitation.

3.2.8 *sheath, n*—cylindrical metal tube with an integral welded closure at the end in which the element is located.

## 4. Significance and Use

4.1 This specification is written to provide common terminology, resistance versus temperature characteristics, accuracy classification, and inspection requirements for a specified configuration of a typical industrial platinum resistance thermometer (PRT).

4.2 This specification may be used as part of the documentation to support negotiations for the purchase and discussion of such thermometers.

## 5. Classification of Tolerances

5.1 The PRT shall conform to the resistance-temperature relation (see 9.2.1) within the following tolerances:

$$\text{Grade A} = \pm[0.13 + 0.0017|t|]^\circ\text{C} \quad (1)$$

<sup>1</sup> This specification is under the jurisdiction of ASTM Committee E-20 on Temperature Measurement and is the direct responsibility of Subcommittee E20.03 on Resistance Thermometers.

Current edition approved Nov. 10, 1997. Published May 1998. Originally published as E 1137 – 87. Last previous edition E 1137 – 95.

<sup>2</sup> Preston-Thomas, H., "The International Temperature Scale of 1990 (ITS-90)," *Metrologia*, Vol 27, No. 1, 1990, pp. 3–10. For errata see *ibid*, Vol 27, No. 2, 1990, p. 107.

<sup>3</sup> *Annual Book of ASTM Standards*, Vol 01.01.

<sup>4</sup> *Annual Book of ASTM Standards*, Vol 02.04.

<sup>5</sup> *Annual Book of ASTM Standards*, Vol 14.03.

$$\text{Grade B} = \pm[0.25 + 0.0042 |t|]^\circ\text{C} \quad (2)$$

where:

$|t|$  = value of temperature without regard to sign, °C.

5.1.1 The tolerances are given in **Table 1** for a PRT with a nominal resistance of 100 Ω at 0°C.

## 6. Ordering Information

6.1 The purchase order documents shall specify the following information to ensure that the PRT is adequately described:

- 6.1.1 The number of this specification,
- 6.1.2 Sheath diameter and overall length (see **Fig. 1**),
- 6.1.3 Sheath material,
- 6.1.4 Minimum and maximum sensed temperature,
- 6.1.5 Maximum temperature at cable end closure,
- 6.1.6 Connection configuration; 2-Wire, 3-Wire, 4-Wire (potentiometric), and compensating loop (4-Wire) (see **Fig. 2**),
- 6.1.7 Tolerance, (Grade A, or Grade B), and
- 6.1.8 Nominal resistance at 0°C (100 Ω unless otherwise specified).

## 7. Materials and Manufacture

7.1 All materials used shall be in accordance with the following requirements:

7.1.1 *Sheath Materials*—For temperatures not exceeding 480°C, austenitic stainless steel tubing, conforming to Specification **A 269**. For temperatures not exceeding 650°C, high-nickel alloy tubing, conforming to Specification **B 167**.

7.1.2 *Sensing Element*—Sensing element shall be platinum.

7.1.3 *Insulation*—The insulating material within the PRT shall be compatible with the temperature range –200 to 650°C or as specified in **6.1.4**. Magnesium oxide (MgO) and aluminum oxide (Al<sub>2</sub>O<sub>3</sub>) Powders and crushable insulators conforming to Specification **E 1652** satisfy this requirement.

7.1.4 *Cable End Potting Materials*—Potting materials shall provide a barrier against water and other liquids and generally prevent the penetration of water vapor. Any potting material used shall be compatible with the ambient temperatures specified for the application.


NOTE 1—Typically, epoxy materials are used for ambient temperatures less than 200°C and moisture impervious ceramic adhesives are used over 200°C, but the cable end potting shall not be limited to these materials if the end seal meets all other requirements of this specification.

**TABLE 1 Classification Tolerances<sup>A, B</sup>**

Temperature, <i>t</i> , °C	Grade A		Grade B	
	°C	Ω	°C	Ω
–200	0.47	0.20	1.1	0.47
–100	0.30	0.12	0.67	0.27
0	0.13	0.05	0.25	0.10
100	0.30	0.11	0.67	0.25
200	0.47	0.17	1.1	0.40
300	0.64	0.23	1.5	0.53
400	0.81	0.28	1.9	0.66
500	0.98	0.33	2.4	0.78
600	1.15	0.37	2.8	0.88
650	1.24	0.40	3.0	0.94

<sup>A</sup> The table represents values for 3-wire and 4-wire PRT's. Caution must be exercised with 2-wire PRT's because of possible errors caused by connecting wires.

<sup>B</sup> Tabulated values are based on elements of 100.0 Ω (nominal) at 0°C.

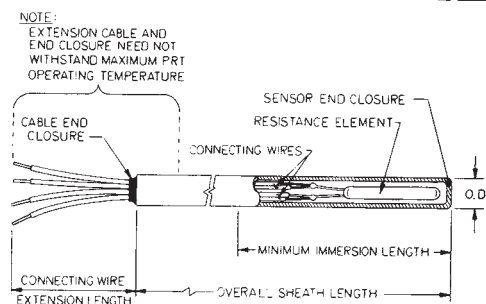

**FIG. 1 Platinum Resistance Thermometer**

7.1.5 *Connecting Wires*—Typically, materials of connecting wires are: nickel plated copper, nickel, platinum, constantan, or manganin. Any material used in joining the connecting wires to the PRT element must withstand the maximum operating temperature of the PRT.

## 8. Other Requirements

8.1 *Pressure*—The PRT shall withstand an external pressure of 21 MPa (3000 psig) and shall be tested in accordance with Test Methods **E 644** pressure test. The PRT shall remain within the tolerance specified in **5.1**.

8.2 *Vibration*:

8.2.1 The PRT shall withstand vibration testing as described in Test Methods **E 644** using the test in **Table 2**.

8.2.2 The PRT shall be mounted by installation in the thermowell or by threaded connection to simulate normal mounting procedure as limited by **Table 2**.

8.2.3 The PRT shall be continuously energized with an oscilloscope-monitored 1.0-mA dc excitation. There shall be no discontinuity of the monitored trace during the test.

8.2.4 After the PRT is tested for vibration the insulation resistance of the PRT shall remain within the tolerance of **Table 3** and the resistance at 0°C within the tolerance specified in **5.1**.

8.3 *Mechanical Shock*:

8.3.1 The PRT shall withstand mechanical shock testing as described in Test Methods **E 644**. The half-sine pulse shall have a peak *g*-level of 50 and duration of 11 ms.

8.3.2 The PRT shall be continuously energized with an oscilloscope-monitored 1.0-mA dc excitation. There shall be no discontinuity of the monitored trace during the test.

8.3.3 After the PRT is tested for mechanical shock the insulation resistance of the PRT shall remain with the tolerance of **Table 3** and the resistance at 0°C within the tolerance in **5.1**.

8.4 *Thermal*:

8.4.1 The PRT shall be capable of continuous operation over the specified temperature range (see **6.1**).


8.4.2 The cable end closure and external connecting wires need not withstand the maximum PRT operating temperature.

## 9. Performance

9.1 *Excitation*:

9.1.1 The PRT must be constructed such that it is usable in ac or dc measurement systems. In ac measuring systems, reactance effects shall be considered.

9.1.2 The PRT shall be capable of operating with continuous excitation of 10 mA. However, excitation of 1 mA or less is

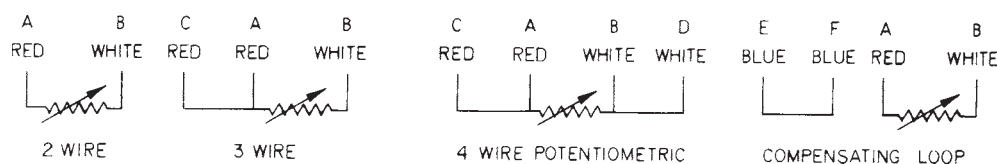

**FIG. 2 Connection Configurations**

**TABLE 2 Vibration Test Parameters**

NOTE 1— The values in Table 2 apply to a PRT mounted in a thermowell with nominal clearance of less than 0.25 mm (0.01 in.) in diameter. If the PRT is not mounted in a thermowell, the values in Table 2 apply to a PRT with an unsupported stem length less than 102 mm (4 in.).

Frequency	5 to 500 Hz
Test Level	1.27-mm (0.05-in.) double amplitude displacement or peak g-level of 3, whichever is less
Resonant Dwell Time	30 min for each resonant point
Cycling Time	3 h per axis less the time spent at resonant dwells at the axis.
Mounting	As normally mounted including the mating thermowell, if applicable.

**TABLE 3 Insulation Resistance**

Applied dc Voltage, Volts dc		Minimum Insulation Resistance	
min	max	°C	MΩ
10	50	25 ± 5	100
10	50	300 ± 10	10
10	50	650 ± 15	2

recommended to minimize measurement errors associated with self-heating (see 9.4).

**9.2 Resistance versus Temperature Relation:**

**9.2.1 Resistance-Temperature Equations**—Within the specified tolerances (see 5.1), the PRT shall have resistance-temperature characteristics defined as follows: for the range  $-200^{\circ}\text{C} \leq t < 0^{\circ}\text{C}$ :

$$R_t = R_o [1 + At + Bt^2 + C(t - 100)r^3] \Omega \tag{3}$$

for the range  $0^{\circ}\text{C} \leq t \leq 650^{\circ}\text{C}$ :

$$R_t = R_o [1 + At + Bt^2] \Omega \tag{4}$$

where:

- $t$  = temperature (ITS-90), °C,
- $R_t$  = resistance at temperature ( $t$ ),
- $R_o$  = resistance at 0°C,
- $A = 3.9083 \times 10^{-3} \text{ }^{\circ}\text{C}^{-1}$ ,
- $B = -5.775 \times 10^{-7} \text{ }^{\circ}\text{C}^{-2}$ , and
- $C = -4.183 \times 10^{-12} \text{ }^{\circ}\text{C}^{-4}$ .

**9.2.2 Resistance Table**—Resistance values of the PRT versus temperature using the equations of 9.2.1 and  $R_o$  of 100 Ω are given in Table 4.

NOTE 2—The resistance versus temperature relationship for a specific thermometer may be computed from measured resistance of that specific thermometer.

**9.2.3 Inverse equations** that may be used to compute values of temperature (°C) as a function of resistance are given in Appendix X1.

**9.3 Insulation Resistance**—The insulation resistance between each connecting wire and the sheath shall meet the

requirements of Table 3 when tested in accordance with Test Methods E 644. The PRT shall be tested with at least the minimum immersion length exposed to the temperature environment.

**9.4 Self-Heating**—A power of at least 33 mW shall be required to produce a self-heating of 1°C when the PRT is tested in water in accordance with Test Methods E 644.

**9.5 Thermal Response Time**—The 63.2 % response time shall not exceed the values in Table 5 when determined in accordance with Test Methods E 644. The step change in temperature shall be from  $20 \pm 5^{\circ}\text{C}$  air to  $77 \pm 5^{\circ}\text{C}$  water flowing at  $0.9 \pm 0.09 \text{ m/s}$  ( $3.0 \pm 0.3 \text{ ft/s}$ ).

**9.6 Thermoelectric Effect**—Wire connections between the PRT sensing element, inner connecting wires, and external connecting wires can generate small voltages when these connection points are exposed to different temperatures. This thermoelectric voltage can add or subtract from the voltage measured across a PRT and cause an unknown variable error in measurement. When tested in accordance with Test Methods E 644, the PRT shall remain within the tolerances specified in 5.1 with an excitation of 1-mA dc, regardless of polarity.

**9.7 Stability**—When tested in accordance with Test Methods E 644, the PRT shall remain within the tolerances specified in 5.1 for a four-week test. During this test, the resistance at 0°C shall be checked at regular intervals (2 times per week).

**9.8 Minimum Immersion Length**—When determined in accordance with Test Methods E 644, the PRT minimum immersion length shall be less than 51 mm (2 in.). The limit of uncertainty shall be 0.13°C and 0.25°C for Grade A and Grade B PRT’s respectively.

**10. Dimensions, Mass, and Permissible Variations**

**10.1** A PRT without a process fitting or other means of attachment is shown in Fig. 1.

**10.2** PRT’s manufactured in accordance with this specification shall be able to pass through the straightness ring gage with the gage sizes listed in Table 6.

**11. Required Tests**

**11.1 Qualification Tests**—The PRT shall be subjected to the tests outlined in Table 7 to demonstrate conformance to this specification. The manufacturer shall perform these tests at least one time to qualify the PRT design. Thereafter, it is recommended these tests be used on a periodic basis to verify process control.

**11.1.1 Qualification Test Report**—The manufacturer shall prepare and retain a qualification test report applicable to the PRT design that documents the model number, test procedure (by reference to Test Methods E 644 and this specification), and the results obtained.